


Data Path : Z:\HPCHEM1\BNA_J\data\BJ060812\
 Data File : BJ000929.D
 Acq On : 8 Jun 2012 11:45
 Operator : HLM
 Sample : DFTPP050
 Misc : DFTPP050 BNA_J HLM
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_J
 ClientSampleId :
 DFTPP050

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_J\method\BJ060812.M
 Title : CWA degradation products by GCMS
 Last Update : Fri Jun 08 15:54:08 2012

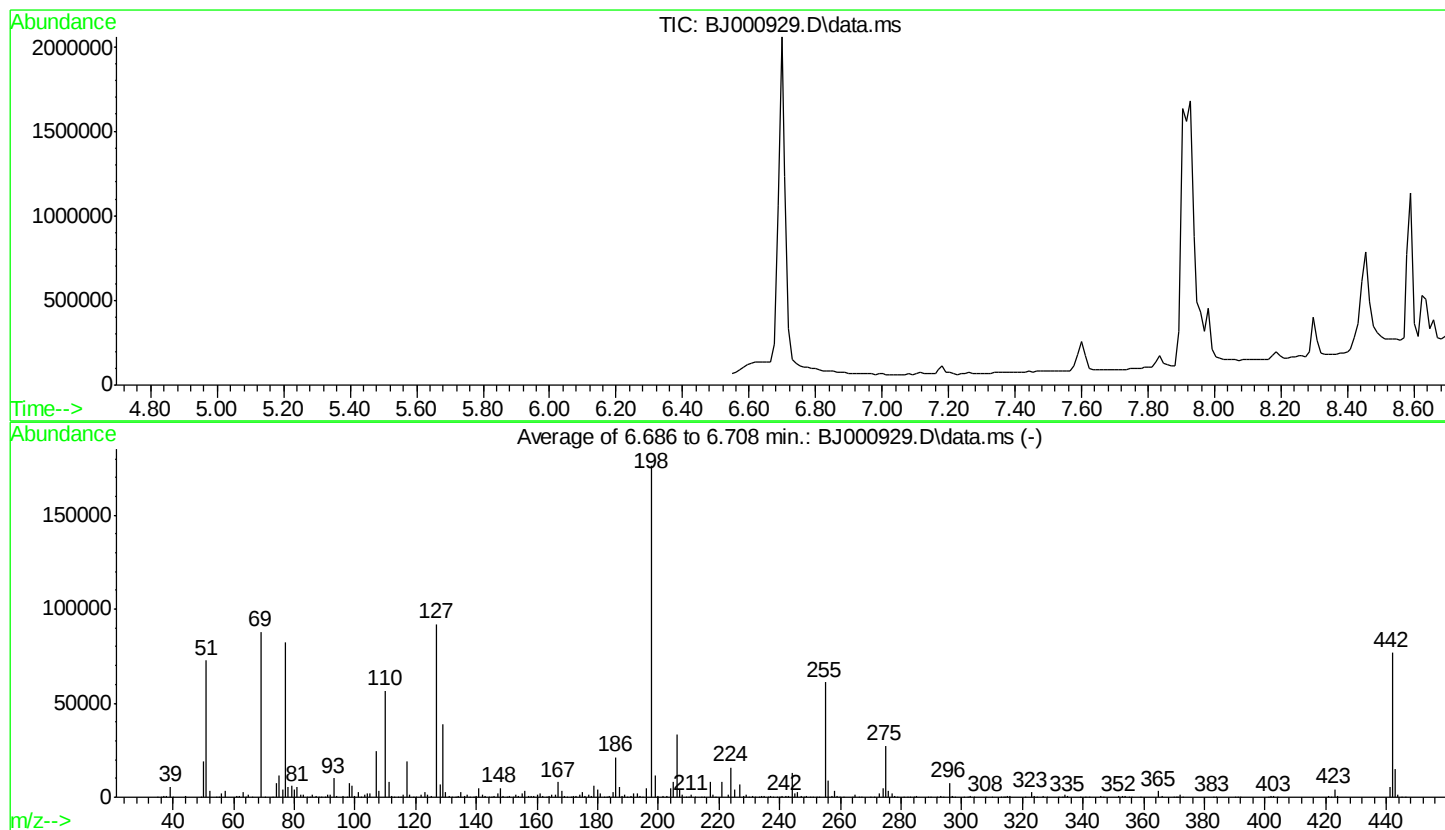

AutoFind: Scans 13, 14, 15; Background Corrected with Scan 7

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	41.2	72608	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	50.0	88072	PASS
70	69	0.00	2	0.4	342	PASS
127	198	40	60	52.3	92158	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	176274	PASS
199	198	5	9	6.4	11337	PASS
275	198	10	30	15.6	27466	PASS
365	198	1	100	1.8	3216	PASS
441	443	0.01	100	35.7	5234	PASS
442	198	40	100	43.5	76725	PASS
443	442	17	23	19.1	14673	PASS