

Data File : H:\VOL1\GCMSDATA\J\120426\BJ000799.D
 Acq On : 26 Apr 2012 20:13
 Sample : PB62574BL
 Misc : WATER BNA J HLM
 MS Integration Params: rteint.p
 Quant Time: Apr 27 11:32 2012

Vial: 15
 Operator: HLM
 Inst : BNA J
 Multiplr: 1.00

Quant Results File: BJ042612.RES

Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ042612.M (RTE Integrator)
 Title : CWA degradation products by GCMS
 Last Update : Fri Apr 27 11:32:02 2012
 Response via : Initial Calibration
 DataAcq Meth : CWAJ

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.75	152	302858	2.00	ug/mL	-0.01
6) Naphthalene-d8	6.06	136	1207333	2.00	ug/mL	0.00
System Monitoring Compounds						
10) Tripropylphosphate	7.11	99	242979	0.59	ug/mL	0.01
Spiked Amount 0.500	Range	70 - 130	Recovery	=	118.00%	
12) 2-Bromothioanisole	7.36	204	396083	5.00	ug/mL	0.00
Spiked Amount 5.000	Range	70 - 130	Recovery	=	100.00%	
Target Compounds						
9) Benzothiazole	6.37	135	5466	0.02	ug/mL#	3
14) p-Chlorophenylmethanesulfon	8.21	111	2475	0.01	ug/mL#	74

Quantitation Report

Data File : H:\VOL1\GCMSDATA\J\120426\BJ000799.D

Vial: 15

Acq On : 26 Apr 2012 20:13

Operator: HLM

Sample : PB62574BL

Inst : BNA J

Misc : WATER BNA J HLM

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Apr 27 11:32 2012


Quant Results File: BJ042612.RES


Method : H:\VOL1\GCMSDATA\J\METHODS\BJ042612.M (RTE Integrator)

Title : CWA degradation products by GCMS

Last Update : Fri Apr 27 11:32:02 2012

Response via : Initial Calibration

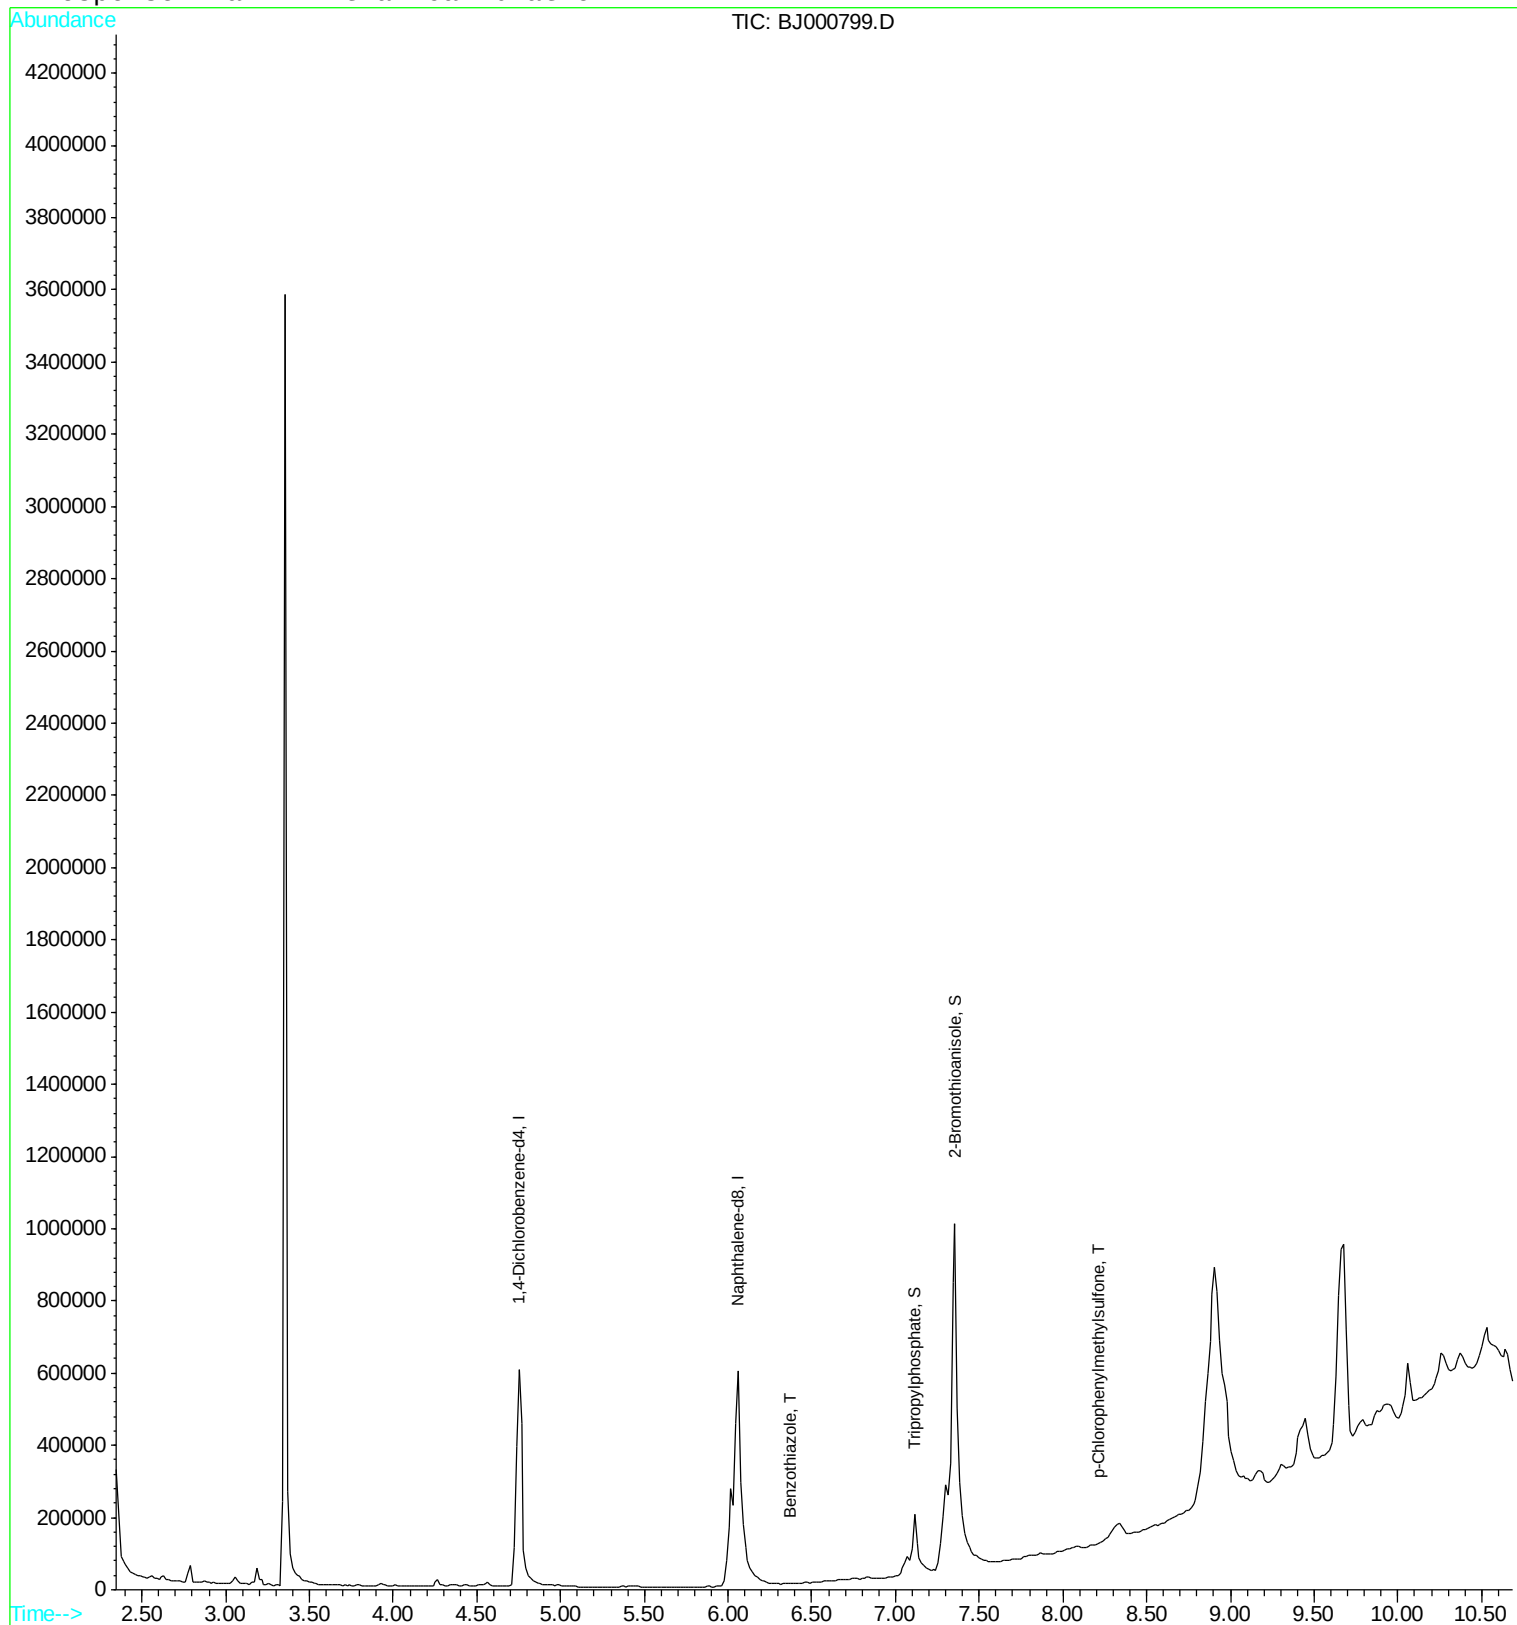

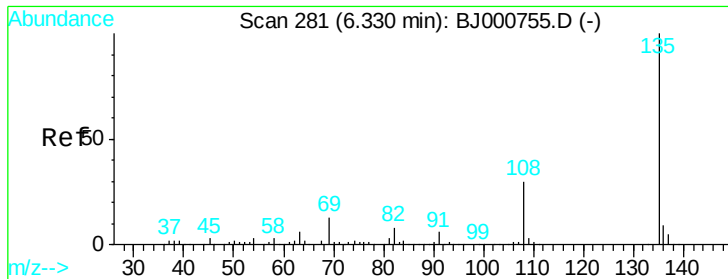

#9

Benzothiazole

Concen: 0.02 ug/mL

RT: 6.37 min Scan# 284

Delta R.T. 0.03 min

Lab File: BJ000799.D

Acq: 26 Apr 2012 20:13


Tgt Ion:135 Resp: 5466

Ion Ratio Lower Upper

135 100

108 0.0 11.1 51.1#

69 89.7 0.0 34.6#



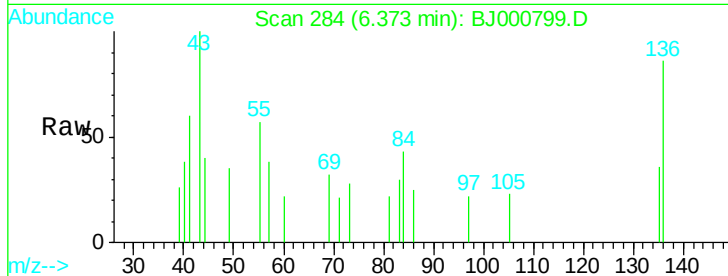


Abundance

Ion 135.00 (134.70 to 135.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 69.00 (68.70 to 69.70): BJ0

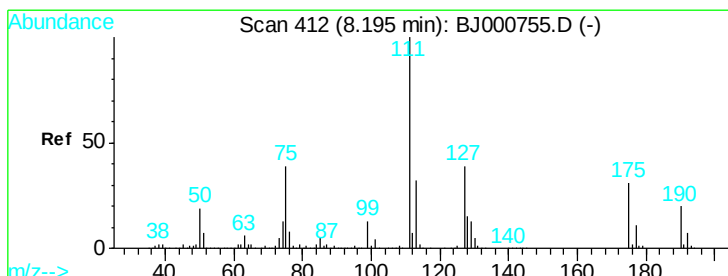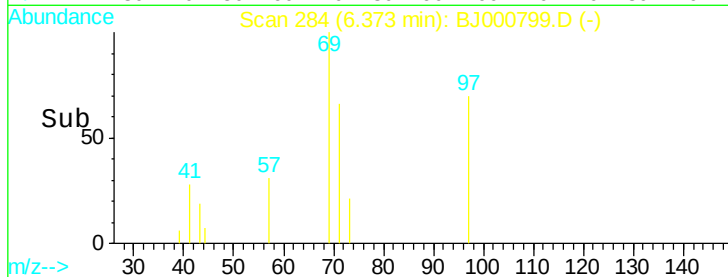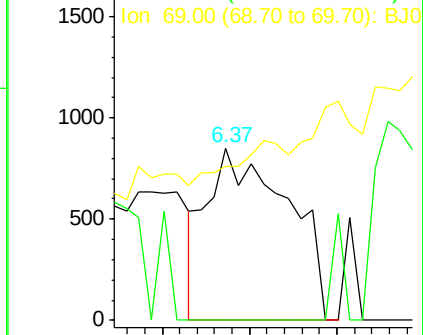

#14

p-Chlorophenylmethylsulfone

Concen: 0.01 ug/mL

RT: 8.21 min Scan# 413

Delta R.T. -0.01 min

Lab File: BJ000799.D

Acq: 26 Apr 2012 20:13

Tgt Ion:111 Resp: 2475


Ion Ratio Lower Upper

111 100

75 46.9 12.8 52.8

127 35.6 21.9 61.9

190 0.0 7.7 47.7#

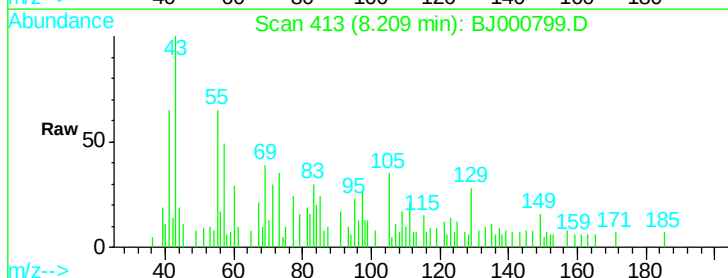

Abundance

Ion 111.00 (110.70 to 111.70): E

Ion 75.00 (74.70 to 75.70): BJ0

Ion 127.00 (126.70 to 127.70): E

Ion 190.00 (189.70 to 190.70): E

