

DFTPP

Data File : H:\VOL1\GCMSDATA\J\120426\BJ000777.D

Vial: 1

Acq On : 26 Apr 2012 12:46

Operator: HLM

Sample : DFTPP050

Inst : BNA_J

Misc : DFTPP050 BNA_J HLM

Multiplr: 1.00

MS Integration Params: rteint.p

Method : H:\VOL1\GCMSDATA\J\METHODS\BJ042612.M (RTE Integrator)



Title : CWA degradation products by GCMS

Instrument :

BNA_J

ClientSampleId :

DFTPP050

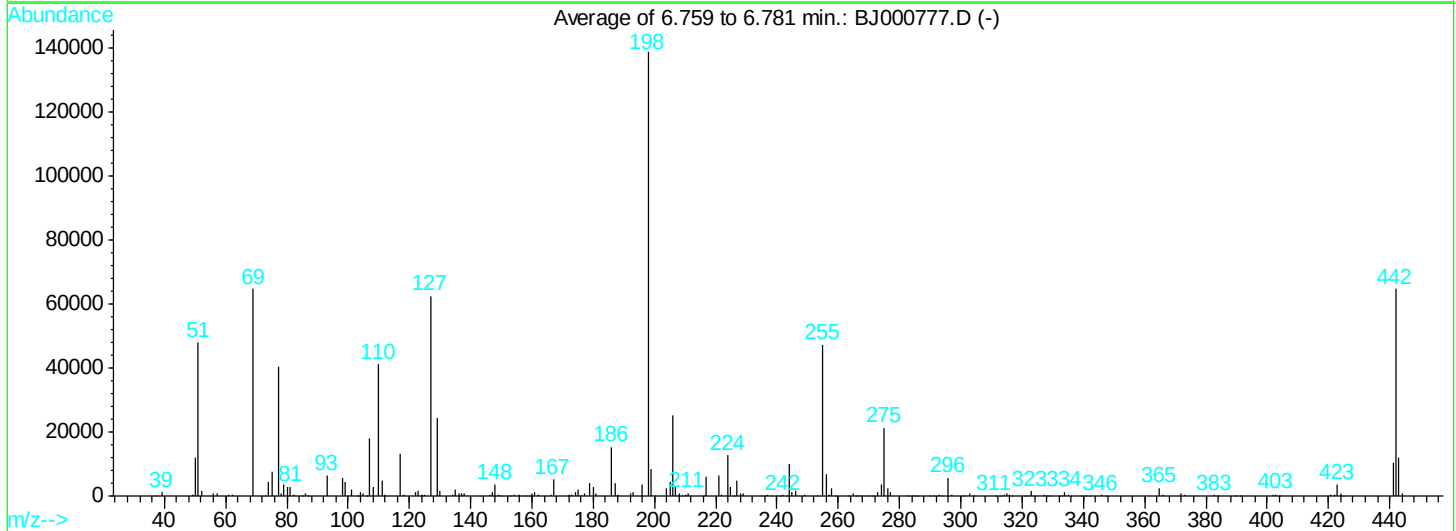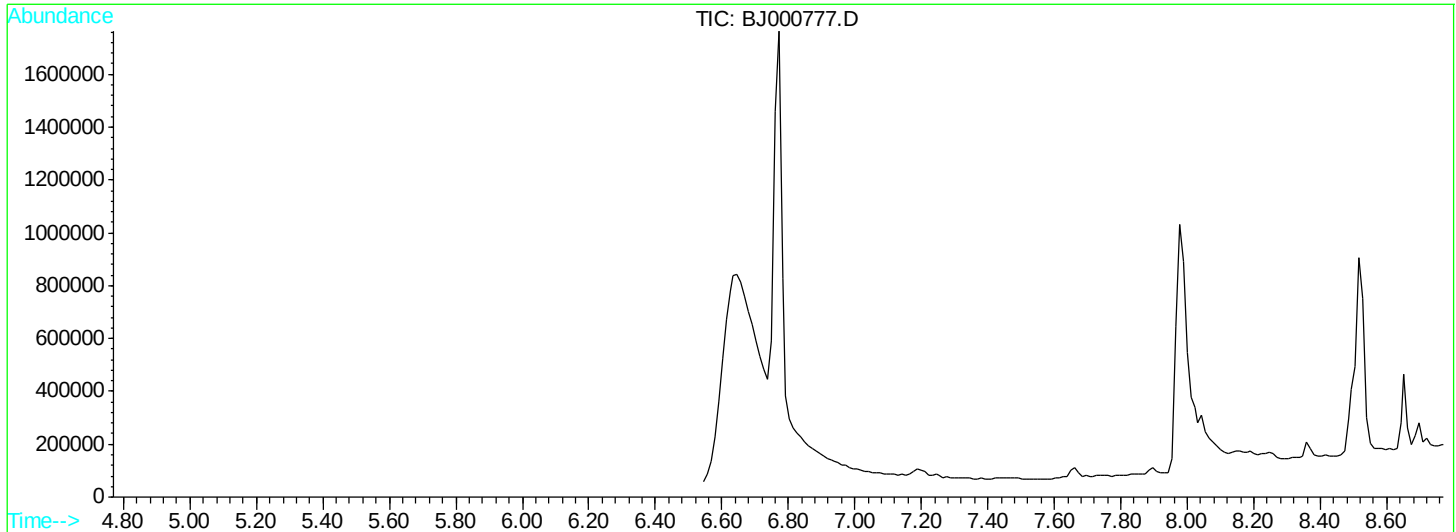

AutoFind: Scans 20, 21, 22; Background Corrected with Scan 14

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	34.5	47883	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.6	64727	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	45.1	62651	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	138823	PASS
199	198	5	9	6.1	8421	PASS
275	198	10	30	15.4	21427	PASS
365	198	1	100	1.8	2440	PASS
441	443	0.01	100	84.9	10244	PASS
442	198	40	100	46.7	64853	PASS
443	442	17	23	18.6	12072	PASS