

DFTPP

Data File : H:\VOL1\GCMSDATA\J\120426\BJ000785.D

Vial: 1

Acq On : 26 Apr 2012 15:52

Operator: HLM

Sample : DFTPP050

Inst : BNA_J

Misc : DFTPP050 BNA_J HLM

Multiplr: 1.00

MS Integration Params: rteint.p

Method : H:\VOL1\GCMSDATA\J\METHODS\BJ042612.M (RTE Integrator)



Title : CWA degradation products by GCMS

Instrument :

BNA_J

ClientSampleId :

DFTPP050

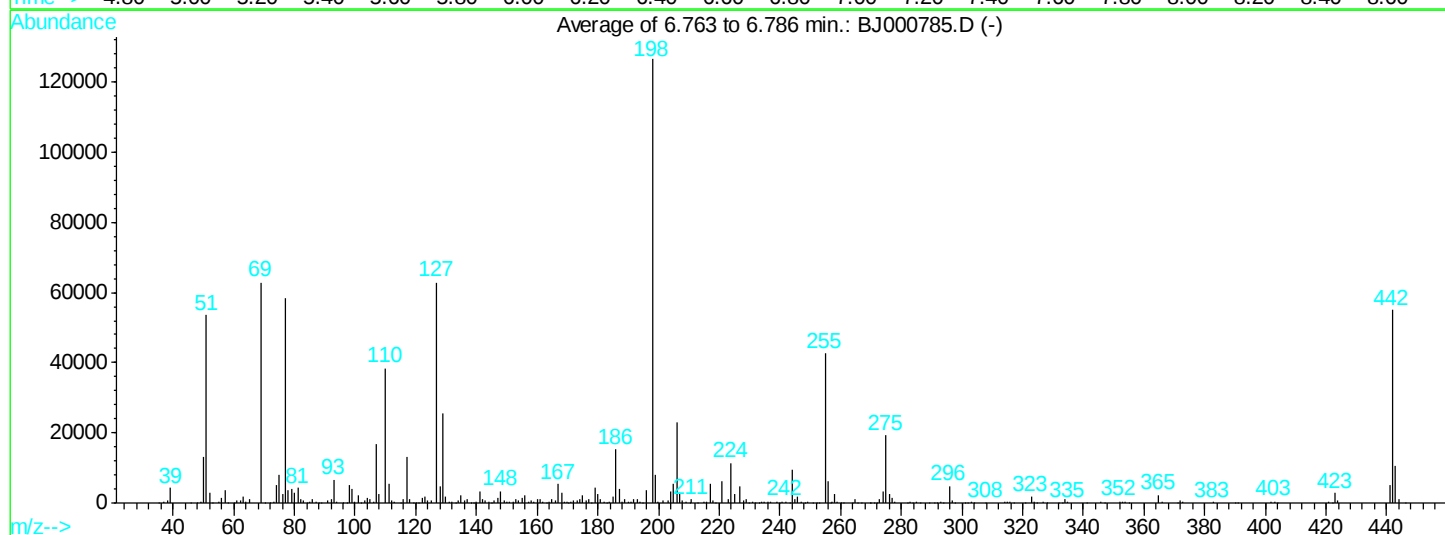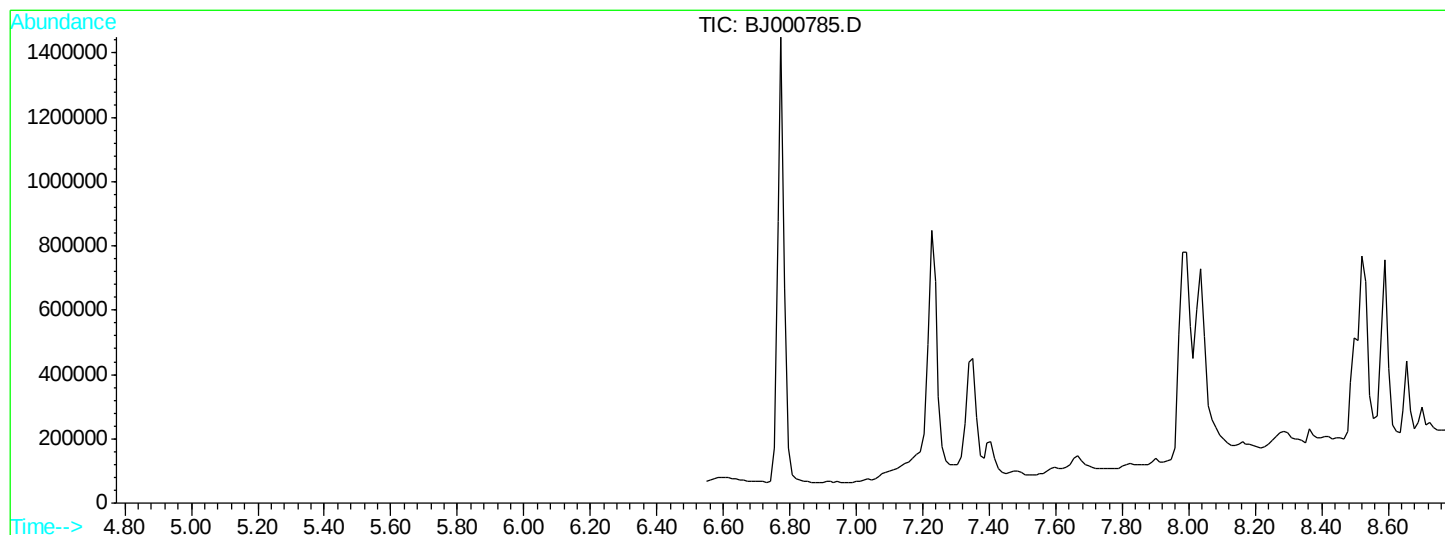

AutoFind: Scans 20, 21, 22; Background Corrected with Scan 15

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	42.4	53585	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	49.7	62887	PASS
70	69	0.00	2	0.2	97	PASS
127	198	40	60	49.6	62780	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	126496	PASS
199	198	5	9	6.4	8144	PASS
275	198	10	30	15.2	19281	PASS
365	198	1	100	1.8	2246	PASS
441	443	0.01	100	48.9	5172	PASS
442	198	40	100	43.5	55061	PASS
443	442	17	23	19.2	10583	PASS