

Data File : H:\VOL1\GCMSDATA\J\120427\BJ000831.D
 Acq On : 27 Apr 2012 20:25
 Sample : PB62691BL
 Misc : WATER BNA J HLM
 MS Integration Params: rteint.p
 Quant Time: Apr 30 10:30 2012

Vial: 10
 Operator: HLM
 Inst : BNA J
 Multiplr: 1.00

Quant Results File: BJ042612.RES

Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ042612.M (RTE Integrator)
 Title : CWA degradation products by GCMS
 Last Update : Mon Apr 30 10:31:38 2012
 Response via : Initial Calibration
 DataAcq Meth : CWAJ

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.74	152	231303	2.00	ug/mL	-0.01
6) Naphthalene-d8	6.05	136	938696	2.00	ug/mL	0.00
System Monitoring Compounds						
10) Tripropylphosphate	7.09	99	146354	0.46	ug/mL	0.00
Spiked Amount 0.500	Range	70 - 130	Recovery	=	92.00%	
12) 2-Bromothioanisole	7.35	204	290309	4.71	ug/mL	0.00
Spiked Amount 5.000	Range	70 - 130	Recovery	=	94.20%	
Target Compounds						Ovalue
11) p-Chlorophenylmethylsulfid	6.61	158	4672	0.03	ug/mL#	79
14) p-Chlorophenylmethylsulfon	8.07	111	2002	0.02	ug/mL#	40


Quantitation Report


Data File : H:\VOL1\GCMSDATA\J\120427\BJ000831.D
Acq On : 27 Apr 2012 20:25
Sample : PB62691BL
Misc : WATER BNA J HLM
MS Integration Params: rteint.p
Quant Time: Apr 30 10:30 2012

Vial: 10
Operator: HLM
Inst : BNA J
Multiplr: 1.00

Quant Results File: BJ042612.RES


Method : H:\VOL1\GCMSDATA\J\METHODS\BJ042612.M (RTE Integrator)
Title : CWA degradation products by GCMS
Last Update : Mon Apr 30 10:31:38 2012
Response via : Initial Calibration

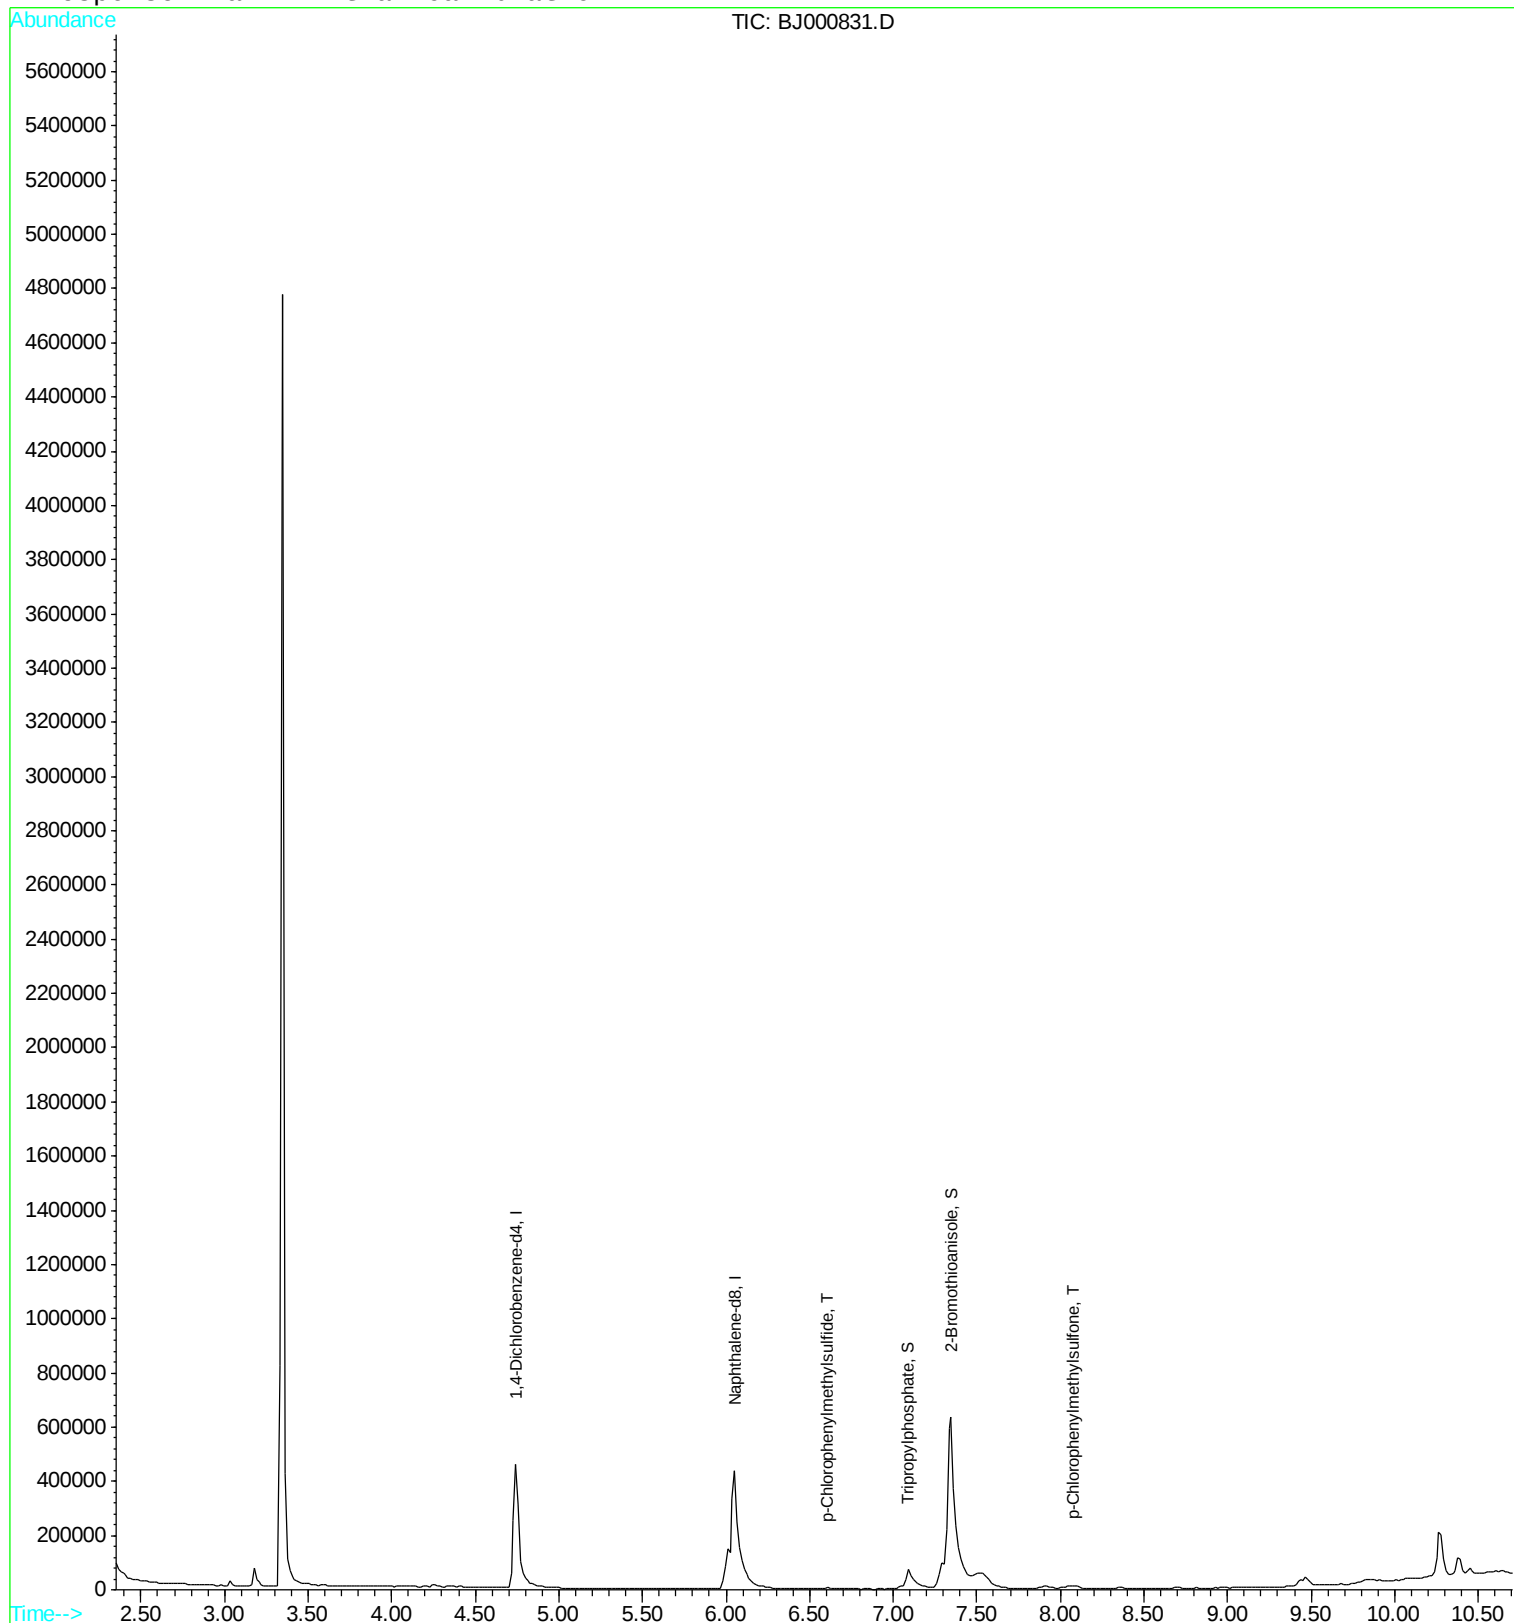

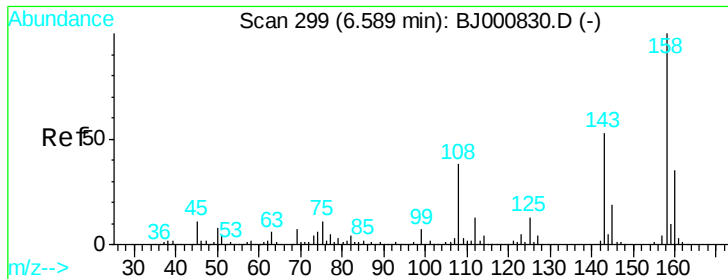

#11
p-Chlorophenylmethylsulfide
Concen: 0.03 ug/mL
RT: 6.61 min Scan# 300
Delta R.T. 0.02 min
Lab File: BJ000831.D
Acq: 27 Apr 2012 20:25

Tgt Ion:158 Resp: 4672
Ion Ratio Lower Upper
158 100
143 49.2 32.7 72.7
108 63.0 18.7 58.7#
45 0.0 0.0 31.9

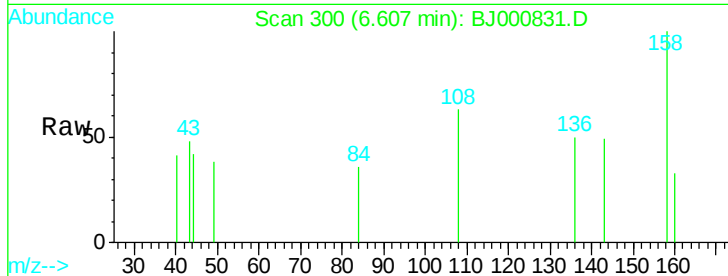




Abundance

Ion 158.00 (157.70 to 158.70): E

Ion 143.00 (142.70 to 143.70): E


Ion 108.00 (107.70 to 108.70): E

Ion 45.00 (44.70 to 45.70): BJ0

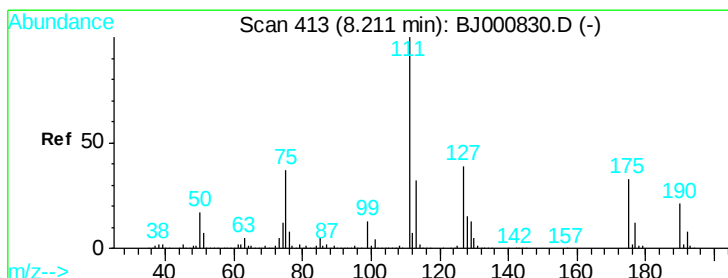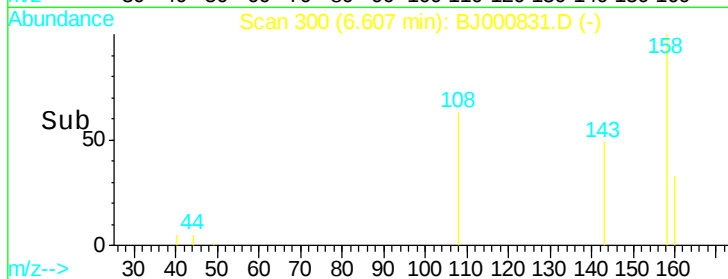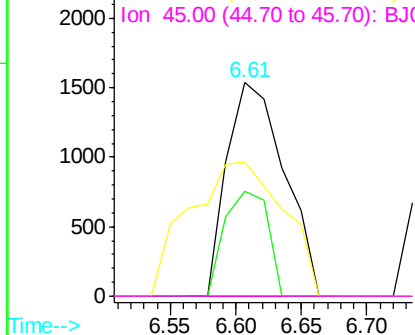

#14
p-Chlorophenylmethylsulfone
Concen: 0.02 ug/mL
RT: 8.07 min Scan# 403
Delta R.T. -0.14 min
Lab File: BJ000831.D
Acq: 27 Apr 2012 20:25

Tgt Ion:111 Resp: 2002
Ion Ratio Lower Upper
111 100
75 0.0 18.5 58.5#
127 0.0 19.3 59.3#
190 0.0 0.9 40.9#

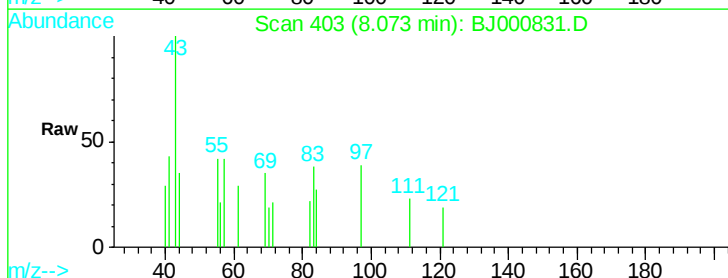

Abundance

Ion 111.00 (110.70 to 111.70): E

Ion 75.00 (74.70 to 75.70): BJ0

Ion 127.00 (126.70 to 127.70): E

Ion 190.00 (189.70 to 190.70): E

