

DFTPP

Data File : H:\VOL1\GCMSDATA\J\120427\BJ000816.D

Vial: 1

Acq On : 27 Apr 2012 11:14

Operator: HLM

Sample : DFTPP050

Inst : BNA_J

Misc : DFTPP050 BNA_J HLM

Multiplr: 1.00

MS Integration Params: rteint.p

Method : H:\VOL1\GCMSDATA\J\METHODS\BJ042612.M (RTE Integrator)



Title : CWA degradation products by GCMS

Instrument :

BNA_J

ClientSampleId :

DFTPP050

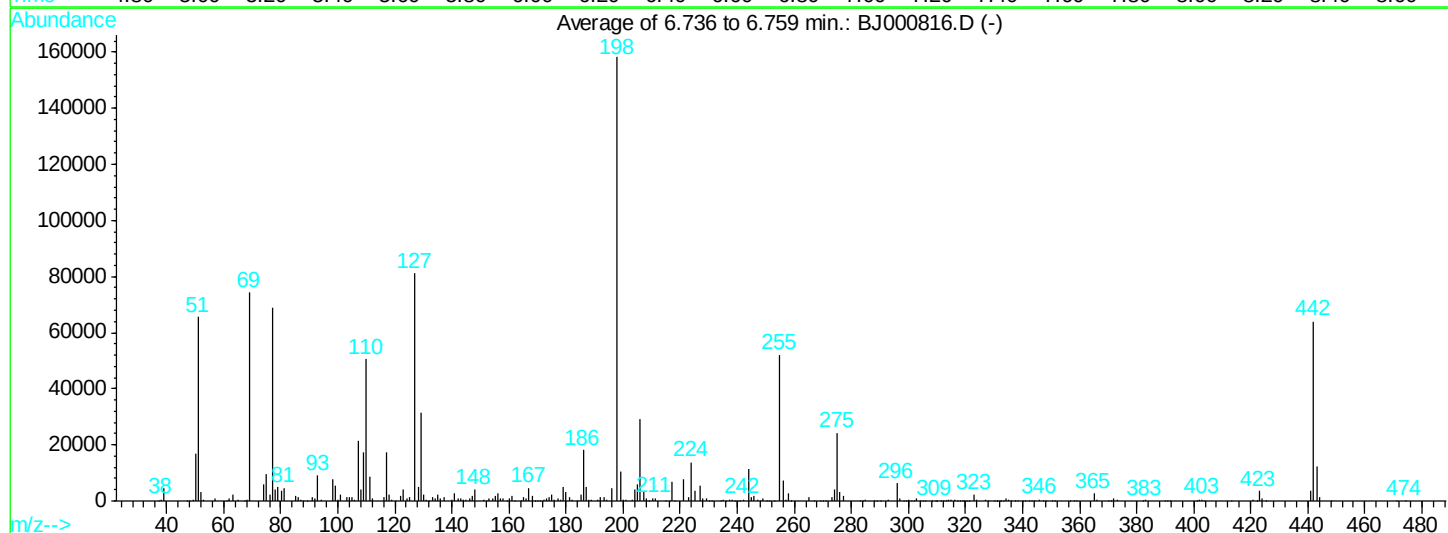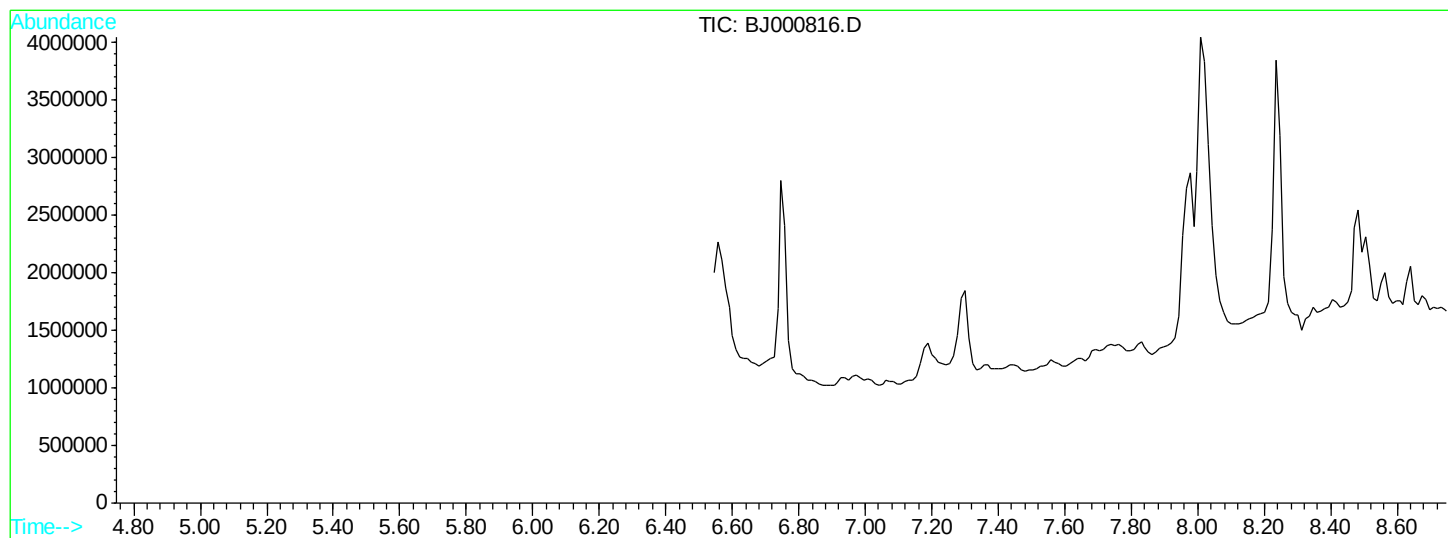

AutoFind: Scans 18, 19, 20; Background Corrected with Scan 11

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	41.5	65690	PASS
68	69	0.00	2	0.4	302	PASS
69	198	0.00	100	46.9	74240	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	51.3	81147	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	158147	PASS
199	198	5	9	6.6	10437	PASS
275	198	10	30	15.3	24223	PASS
365	198	1	100	1.7	2638	PASS
441	443	0.01	100	30.2	3702	PASS
442	198	40	100	40.5	63999	PASS
443	442	17	23	19.1	12250	PASS