

## DFTPP

Data File : H:\VOL1\GCMSDATA\J\120427\BJ000829.D

Vial: 1

Acq On : 27 Apr 2012 19:50

Operator: HLM

Sample : DFTPP050

Inst : BNA\_J

Misc : DFTPP050 BNA\_J HLM

Multiplr: 1.00

MS Integration Params: rteint.p

Method : H:\VOL1\GCMSDATA\J\METHODS\BJ042612.M (RTE Integrator)



Title : CWA degradation products by GCMS

Instrument :

BNA\_J

ClientSampleId :

DFTPP050

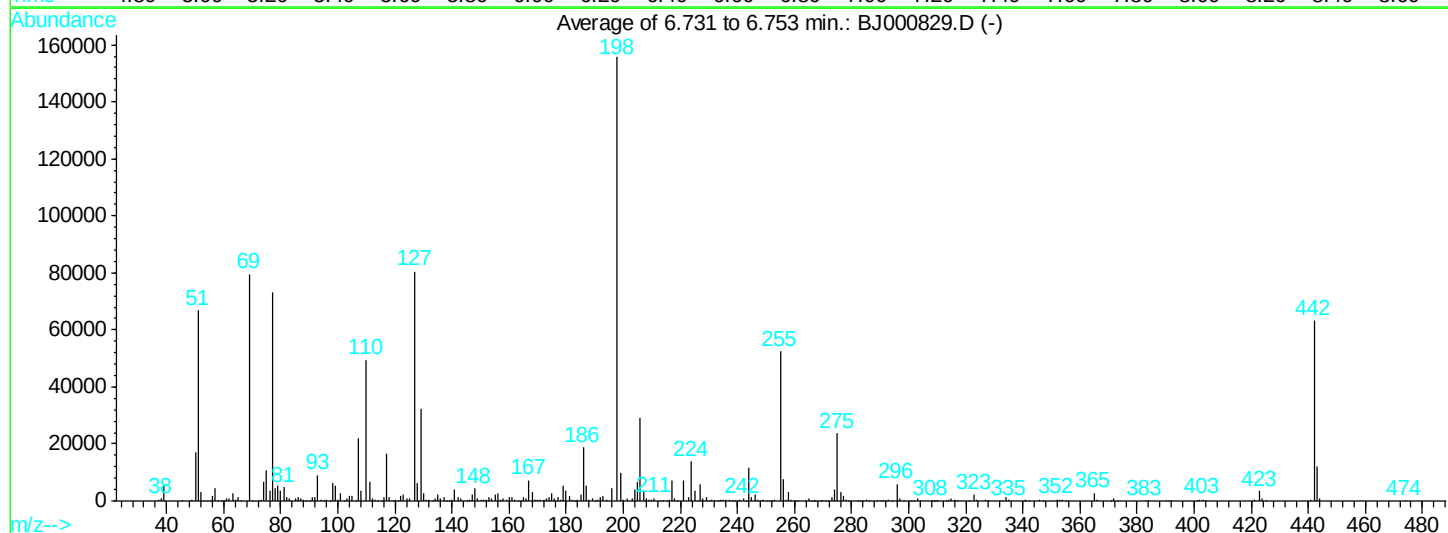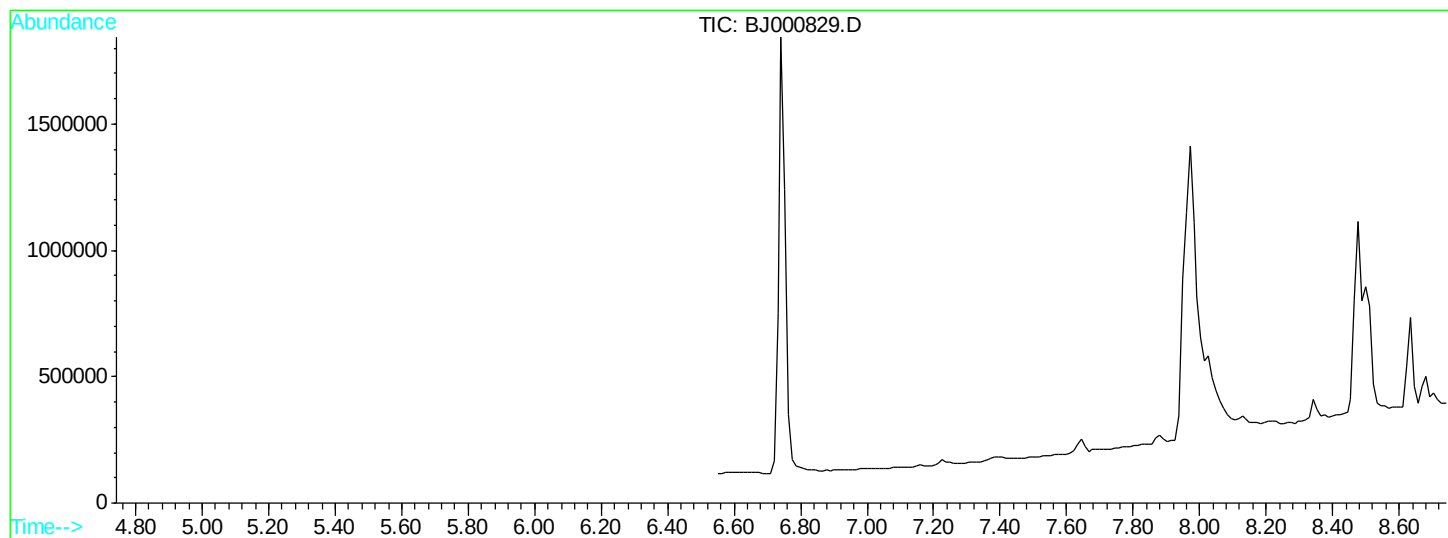

AutoFind: Scans 17, 18, 19; Background Corrected with Scan 13

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 30           | 60           | 42.9      | 66793   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 51.1      | 79498   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.3       | 217     | PASS             |
| 127         | 198          | 40           | 60           | 51.7      | 80502   | PASS             |
| 197         | 198          | 0.00         | 1            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 155651  | PASS             |
| 199         | 198          | 5            | 9            | 6.5       | 10114   | PASS             |
| 275         | 198          | 10           | 30           | 15.3      | 23767   | PASS             |
| 365         | 198          | 1            | 100          | 1.7       | 2721    | PASS             |
| 441         | 443          | 0.01         | 100          | 4.7       | 585     | PASS             |
| 442         | 198          | 40           | 100          | 40.6      | 63195   | PASS             |
| 443         | 442          | 17           | 23           | 19.5      | 12321   | PASS             |