

DFTPP

Data File : H:\VOL1\GCMSDATA\J\120501\BJ000880.D

Vial: 1

Acq On : 1 May 2012 13:34

Operator: HLM

Sample : DFTPP050

Inst : BNA_J

Misc : DFTPP050 BNA_J HLM

Multiplr: 1.00

MS Integration Params: rteint.p

Method : H:\VOL1\GCMSDATA\J\METHODS\BJ042612.M (RTE Integrator)



Title : CWA degradation products by GCMS

Instrument :

BNA_J

ClientSampleId :

DFTPP050

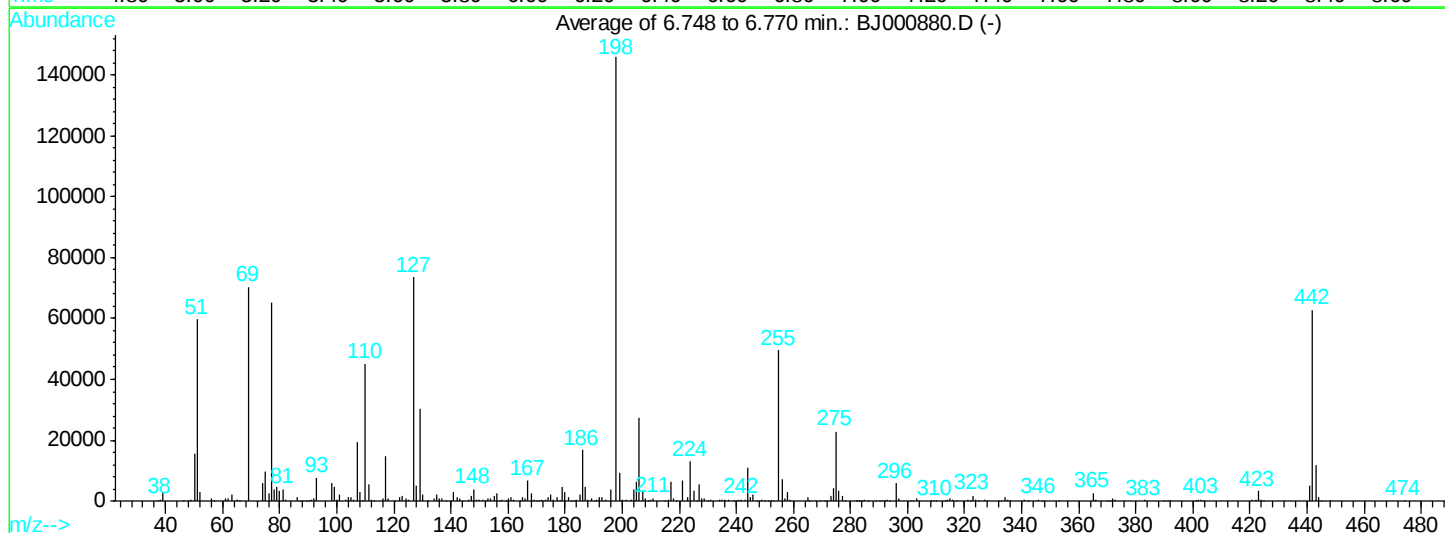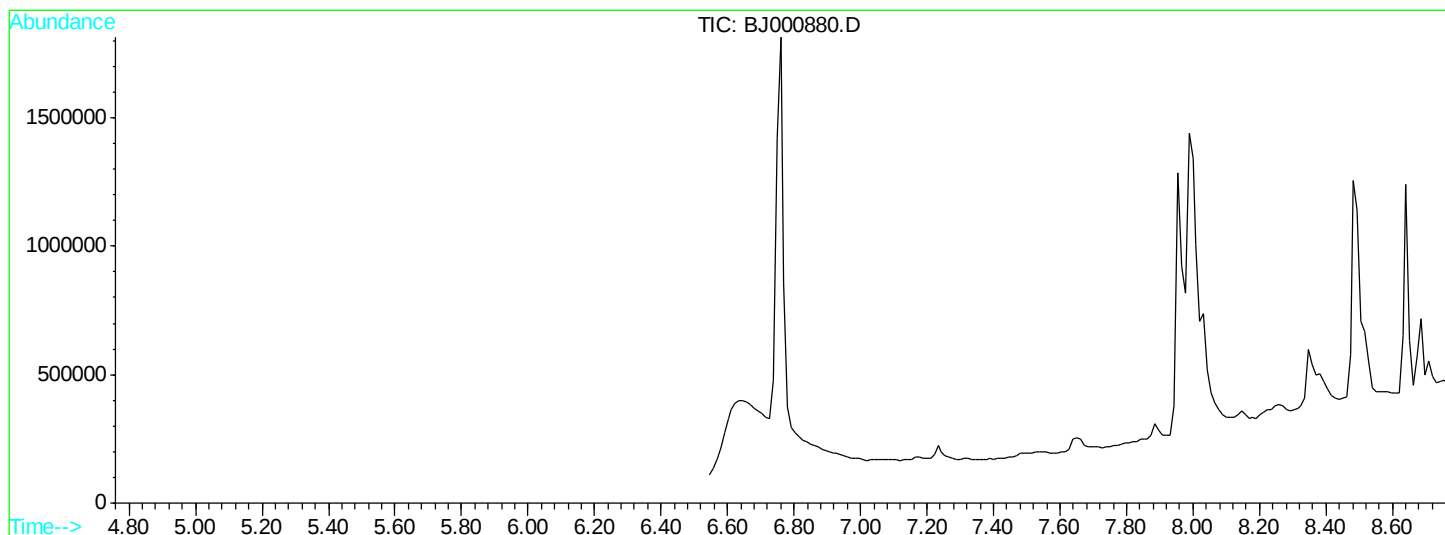

Spectrum Information: Average of 6.748 to 6.770 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	40.8	59604	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	48.2	70359	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	50.4	73612	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	145915	PASS
199	198	5	9	6.5	9431	PASS
275	198	10	30	15.6	22748	PASS
365	198	1	100	1.8	2666	PASS
441	443	0.01	100	41.3	4932	PASS
442	198	40	100	43.1	62824	PASS
443	442	17	23	19.0	11948	PASS