

Data File : H:\VOL1\GCMSDATA\J\120627\BJ000967.D
 Acq On : 27 Jun 2012 16:38
 Sample : D3152-06
 Misc : WATER BNA J HLM
 MS Integration Params: rteint.p
 Quant Time: Jun 28 10:47 2012

Vial: 11
 Operator: HLM
 Inst : BNA J
 Multiplr: 1.00

Quant Results File: BJ060812.RES

Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ060812.M (RTE Integrator)
 Title : CWA degradation products by GCMS
 Last Update : Thu Jun 28 10:45:59 2012
 Response via : Initial Calibration
 DataAcq Meth : CWAJ

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.68	152	200450	2.00	ug/mL	0.00
6) Naphthalene-d8	5.98	136	821641	2.00	ug/mL	0.00
System Monitoring Compounds						
10) Tripropylphosphate	7.03	99	171815	0.54	ug/mL	0.01
Spiked Amount 0.500	Range	70 - 130	Recovery	=	108.00%	
12) 2-Bromothioanisole	7.27	204	237661	4.24	ug/mL	0.00
Spiked Amount 5.000	Range	70 - 130	Recovery	=	84.80%	
Target Compounds						Ovalue
4) DIMP	5.00	97	6479	0.04	ug/mL#	1
8) Thiodiglycol	5.87	61	480	1.45	ug/mL#	1
14) p-Chlorophenylmethanesulfon	8.07	111	5117	0.04	ug/mL#	69


Quantitation Report




Data File : H:\VOL1\GCMSDATA\J\120627\BJ000967.D
 Acq On : 27 Jun 2012 16:38
 Sample : D3152-06
 Misc : WATER BNA J HLM
 MS Integration Params: rteint.p
 Quant Time: Jun 28 10:47 2012

Vial: 11
 Operator: HLM
 Inst : BNA J
 Multiplr: 1.00

Quant Results File: BJ060812.RES

Method : H:\VOL1\GCMSDATA\J\METHODS\BJ060812.M (RTE Integrator)
 Title : CWA degradation products by GCMS
 Last Update : Thu Jun 28 10:45:59 2012
 Response via : Initial Calibration

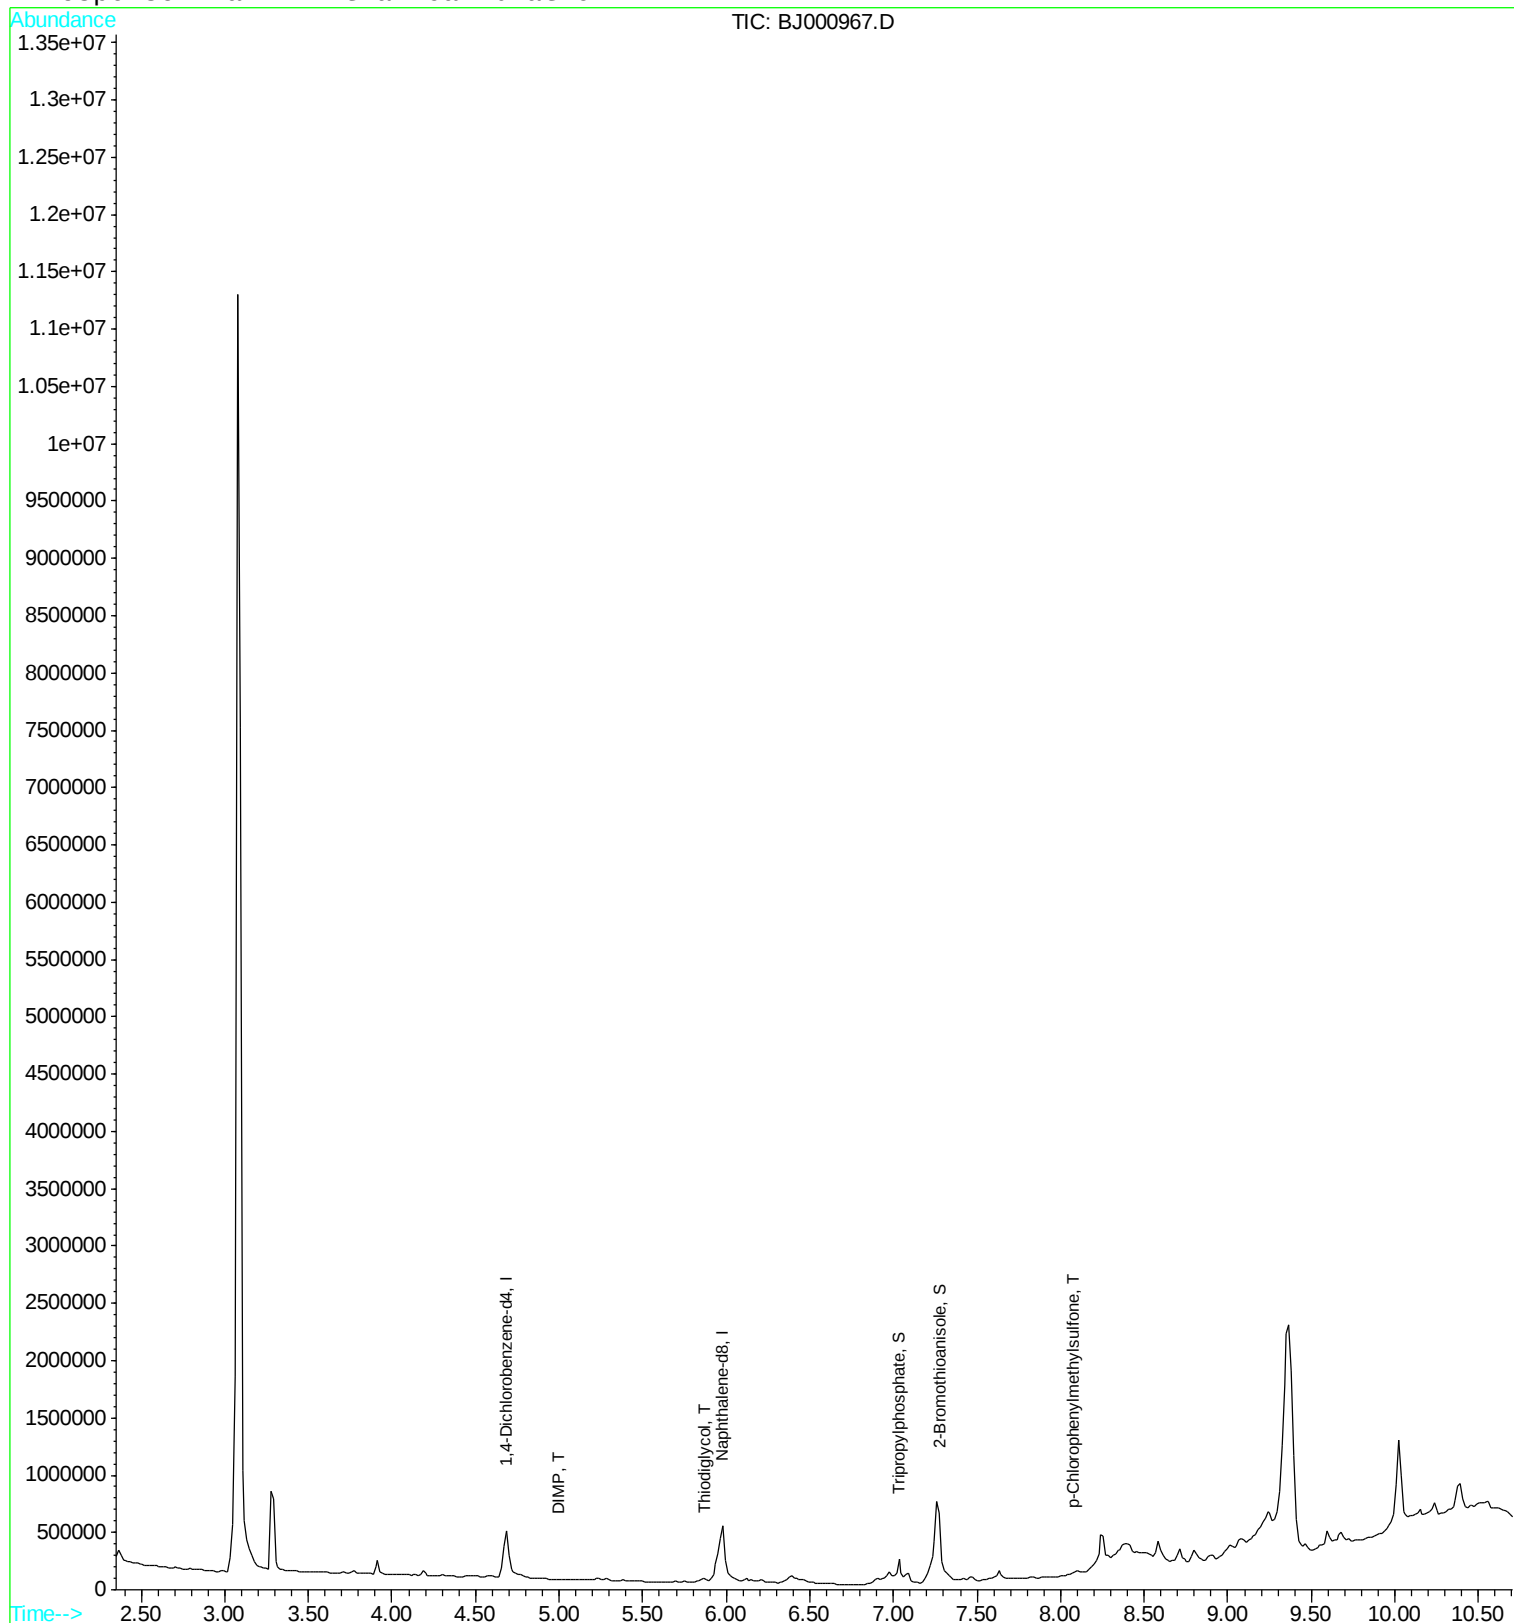

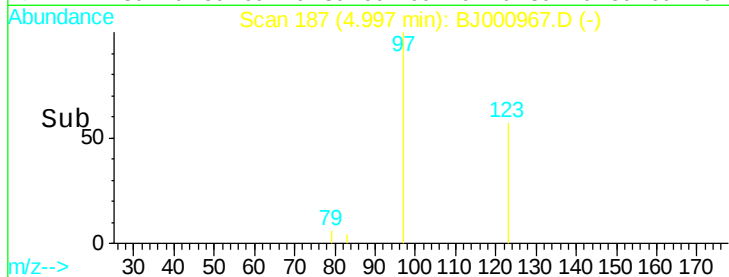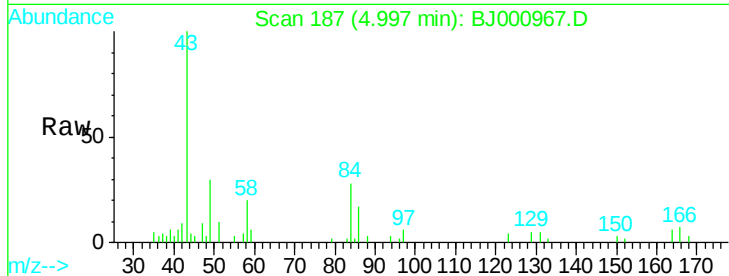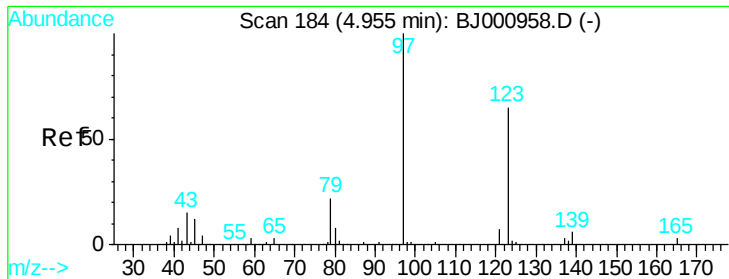

#4

DIMP

Concen: 0.04 ug/mL

RT: 5.00 min Scan# 187

Delta R.T. 0.04 min





Lab File: BJ000967.D

Acq: 27 Jun 2012 16:38

Tgt Ion: 97 Resp: 6479

Ion Ratio Lower Upper

97	100		
123	57.4	45.3	85.3
43	1560.0	0.0	35.5#
41	99.9	0.0	27.9#

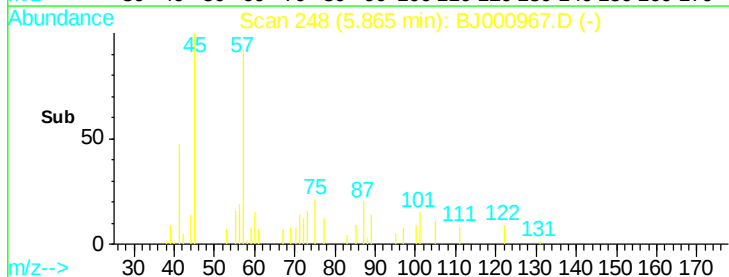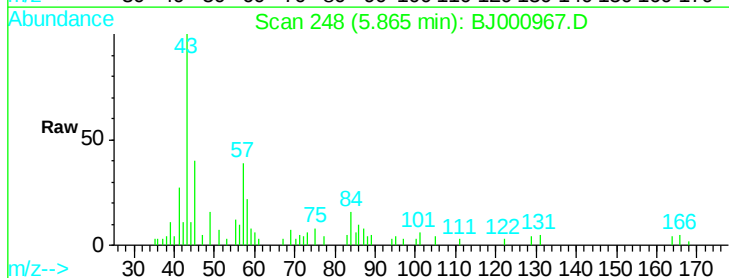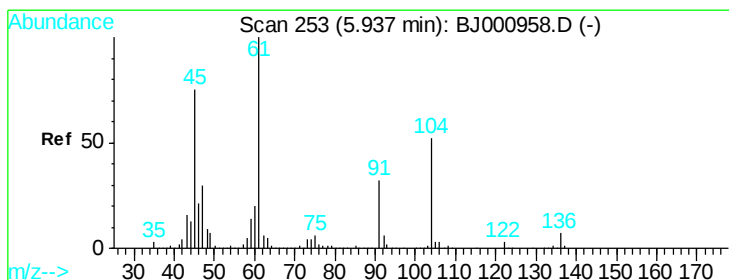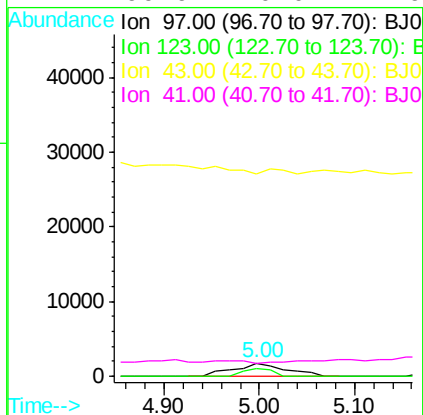

#8

Thiodiglycol

Concen: 1.45 ug/mL

RT: 5.87 min Scan# 248

Delta R.T. -0.07 min


Lab File: BJ000967.D


Acq: 27 Jun 2012 16:38

Tgt Ion: 61 Resp: 480

Ion Ratio Lower Upper


61	100		
45	1512.3	55.5	95.5#
47	172.6	10.4	50.4#

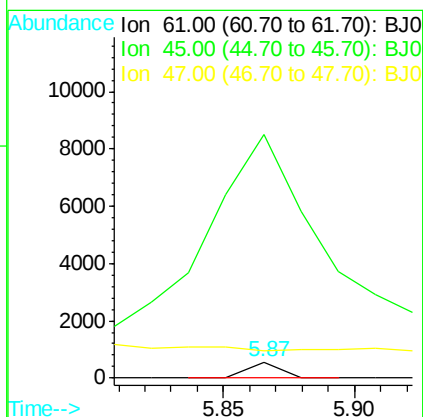

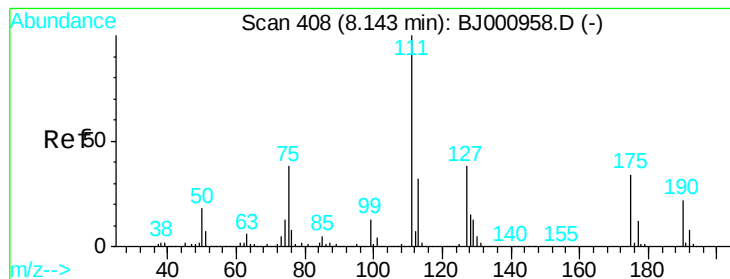

#14
 p-Chlorophenylmethylsulfone
 Concen: 0.04 ug/mL
 RT: 8.07 min Scan# 403
 Delta R.T. -0.07 min
 Lab File: BJ000967.D
 Acq: 27 Jun 2012 16:38

Tgt Ion:	111	Resp:	5117
Ion Ratio	Lower	Upper	
111	100		
75	18.9	19.3	59.3#
127	25.8	18.4	58.4
190	0.0	1.5	41.5#

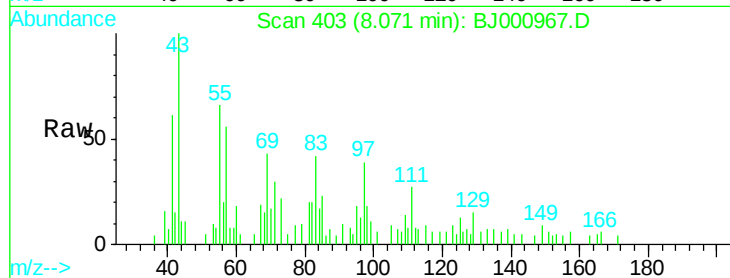

Abundance

Ion 111.00 (110.70 to 111.70): E

Ion 75.00 (74.70 to 75.70): BJ0

Ion 127.00 (126.70 to 127.70): E

Ion 190.00 (189.70 to 190.70): E

