


Data Path : Z:\HPCHEM1\BNA_J\data\BJ062712\
 Data File : BJ000957.D
 Acq On : 27 Jun 2012 13:25
 Operator : HLM
 Sample : DFTPP050
 Misc : DFTPP050 BNA_J HLM
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_J
 ClientSampleId :
 DFTPP050

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_J\method\BJ060812.M
 Title : CWA degradation products by GCMS
 Last Update : Fri Jun 08 15:54:08 2012

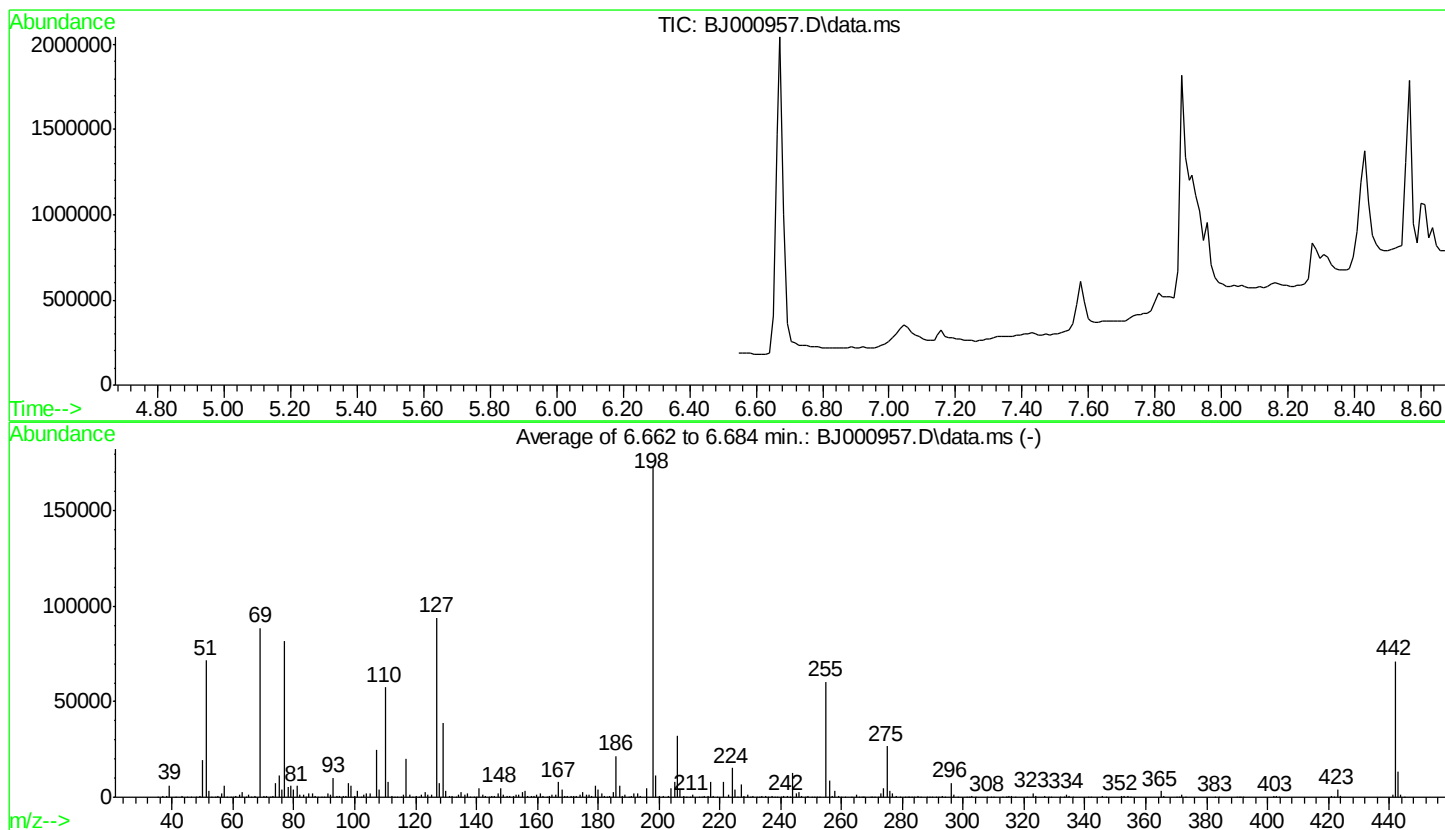

AutoFind: Scans 11, 12, 13; Background Corrected with Scan 5

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	41.3	71663	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	51.1	88703	PASS
70	69	0.00	2	0.7	594	PASS
127	198	40	60	54.1	93967	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	173662	PASS
199	198	5	9	6.5	11286	PASS
275	198	10	30	15.4	26666	PASS
365	198	1	100	1.8	3157	PASS
441	443	0.01	100	11.9	1607	PASS
442	198	40	100	41.1	71389	PASS
443	442	17	23	18.9	13481	PASS

Average of 6.662 to 6.684 min.: BJ000957.D\data.ms

DFTPP050

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.05	139	51.00	71663	62.05	1043	74.00	7649
37.00	369	52.05	3553	63.00	2848	75.00	11603
38.00	1016	53.00	173	64.10	339	76.05	3836
39.10	6253	54.10	140	65.00	1303	77.05	81871
41.10	130	55.10	977	66.00	68	78.00	5444
43.10	440	56.10	2054	67.10	524	79.00	5992
45.00	65	57.10	6016	69.00	88703	80.00	4383
46.25	36	58.05	66	70.10	594	81.00	5757
47.95	24	59.05	95	71.00	706	82.05	1171
49.05	439	60.05	2	72.05	173	83.10	1622
50.05	19594	61.05	868	73.00	428	84.10	320

Instrument :

BNA_J

ClientSampleId :

DFTPP050

Average of 6.662 to 6.684 min.: BJ000957.D\data.ms

DFTPP050

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
85.05	1808	96.10	449	108.00	3929	120.00	383
86.00	1907	97.10	709	110.00	57388	121.05	272
86.95	699	98.00	7587	111.00	8173	121.95	1654
87.95	257	98.95	6248	112.05	857	123.00	2721
88.95	131	100.00	559	113.05	275	124.00	1302
90.05	48	100.95	3303	114.00	61	125.05	1460
91.05	1793	101.95	113	115.00	19	126.95	93967
92.00	1625	102.95	1137	116.00	1599	127.95	7087
93.00	10131	103.95	2244	116.95	19900	128.95	39048
94.00	542	105.05	2241	118.00	1413	129.95	3110
95.10	423	107.00	25131	119.05	186	130.95	417

Average of 6.662 to 6.684 min.: BJ000957.D\data.ms

DFTPP050

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
131.95	395	142.95	1025	154.00	1128	165.00	1619
133.05	286	144.00	242	154.95	2594	166.00	1311
134.00	1096	145.00	445	155.95	3579	167.00	7993
135.00	2876	146.00	856	156.95	825	168.00	3740
136.00	1076	147.00	2299	157.90	835	168.95	661
137.00	1725	147.90	4993	159.00	561	169.95	404
138.05	357	149.00	1074	159.95	1545	170.95	382
139.05	194	150.00	362	161.00	1990	171.95	705
140.05	309	151.05	862	161.95	532	172.95	877
140.95	4693	152.00	419	163.00	117	174.00	1635
141.95	1524	153.00	1562	163.95	521	175.00	2874

Average of 6.662 to 6.684 min.: BJ000957.D\data.ms

DFTPP050

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
175.95	1037	186.95	6037	199.95	848	213.00	88
177.00	1406	188.05	720	201.45	892	214.00	92
178.00	608	188.95	1408	202.95	951	214.95	442
178.90	6228	189.95	193	203.95	4623	216.00	744
180.00	3898	191.00	619	205.00	7752	216.95	8022
181.00	2040	191.90	1716	205.95	32275	217.90	977
182.00	436	193.00	1930	207.00	4102	219.00	26
183.05	157	194.00	376	208.00	961	221.00	7809
183.90	453	196.00	4923	209.05	272	223.00	1659
184.95	2835	197.90	173662	210.15	323	223.95	15418
185.95	21677	198.95	11286	210.95	1206	224.95	3843

Average of 6.662 to 6.684 min.: BJ000957.D\data.ms

DFTPP050

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
225.85	124	237.00	573	247.95	132	259.95	148
226.95	6850	238.00	132	248.90	364	261.05	159
227.90	1031	238.90	306	250.10	168	263.20	64
228.95	1254	240.00	270	251.05	174	264.95	1339

Instrument :
BNA_J
ClientSampleId :
DFTPP050

Modified:subtracted

Modified:subtracted

Page: 3