

## DFTPP

Data File : H:\VOL1\GCMSDATA\J\120828\BJ001084.D

Vial: 1

Acq On : 28 Aug 2012 14:30

Operator: HLM

Sample : DFTPP050

Inst : BNA\_J


Misc : DFTPP050 BNA\_J HLM

Multiplr: 1.00

MS Integration Params: RTEINT.P

Method : H:\VOL1\GCMSDATA\J\METHODS\BJ082812.M (RTE Integrator)

Title : P4 by SOP M.5

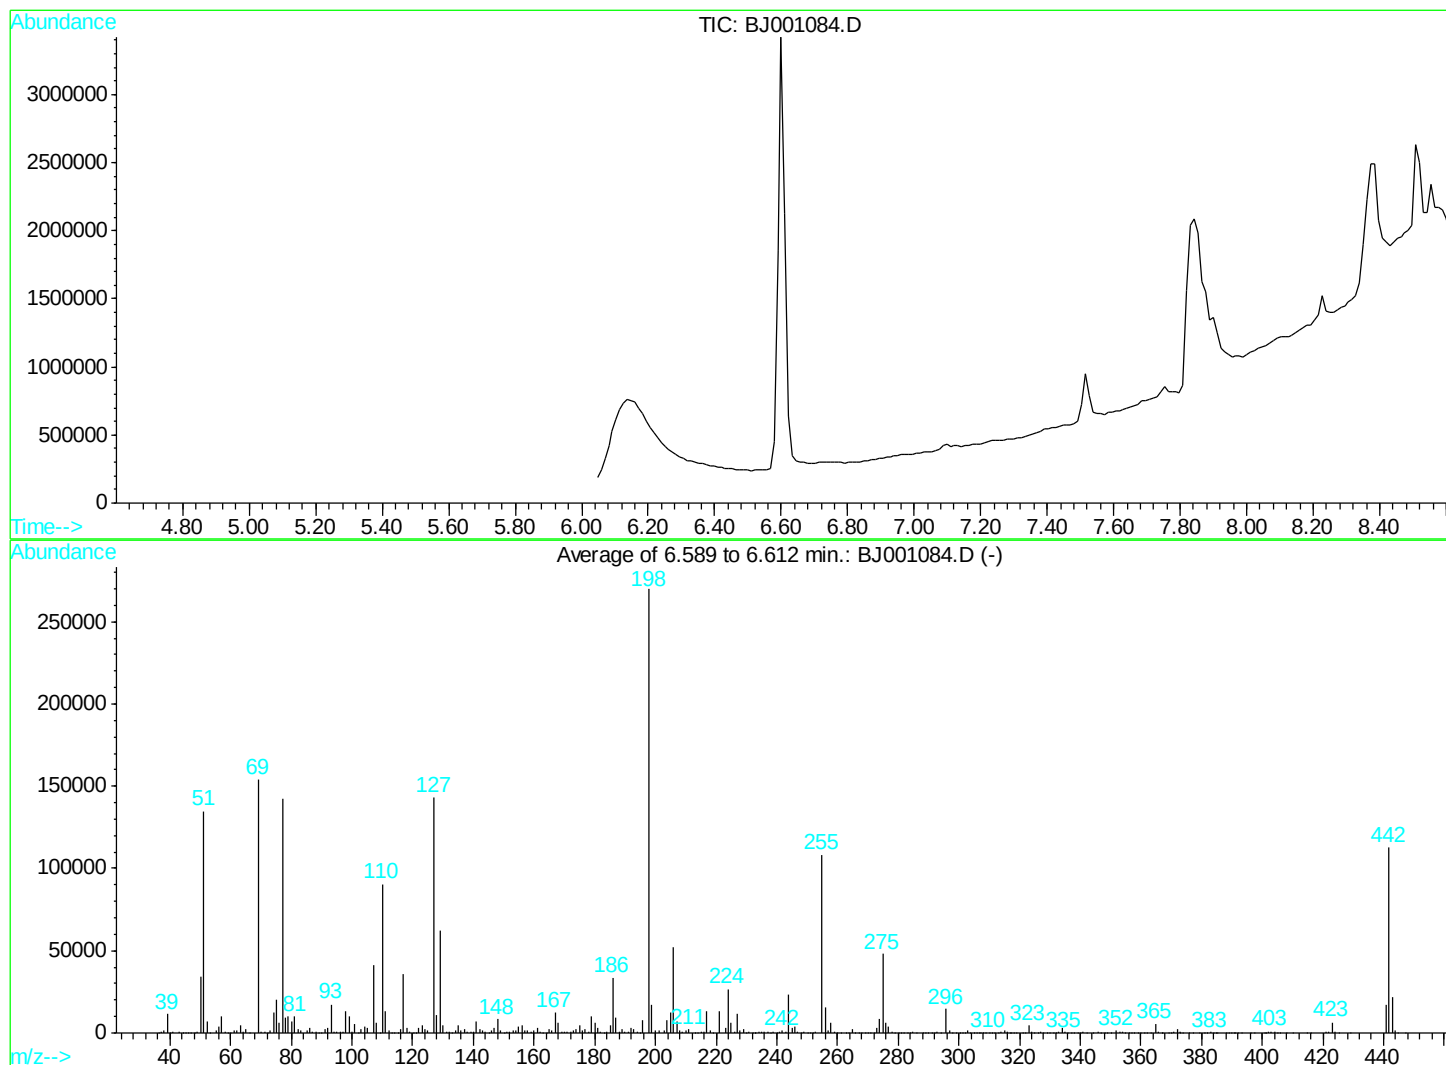

AutoFind: Scans 49, 50, 51; Background Corrected with Scan 44

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 30           | 60           | 49.9      | 134688  | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 57.0      | 153701  | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 835     | PASS             |
| 127         | 198          | 40           | 60           | 53.0      | 143009  | PASS             |
| 197         | 198          | 0.00         | 1            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 269691  | PASS             |
| 199         | 198          | 5            | 9            | 6.5       | 17441   | PASS             |
| 275         | 198          | 10           | 30           | 17.9      | 48196   | PASS             |
| 365         | 198          | 1            | 100          | 2.2       | 5844    | PASS             |
| 441         | 443          | 0.01         | 100          | 77.9      | 16985   | PASS             |
| 442         | 198          | 40           | 100          | 41.7      | 112571  | PASS             |
| 443         | 442          | 17           | 23           | 19.4      | 21795   | PASS             |