


Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ091112\
 Data File : BJ001102.D
 Acq On : 11 Sep 2012 12:55
 Operator : HLM
 Sample : DFTPP050
 Misc : DFTPP050 BNA_J HLM
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_J
 ClientSampleId :
 DFTPP050

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_J\METHOD\BJ091112.M
 Title : CWA degradation products by GCMS
 Last Update : Tue Sep 11 15:38:38 2012

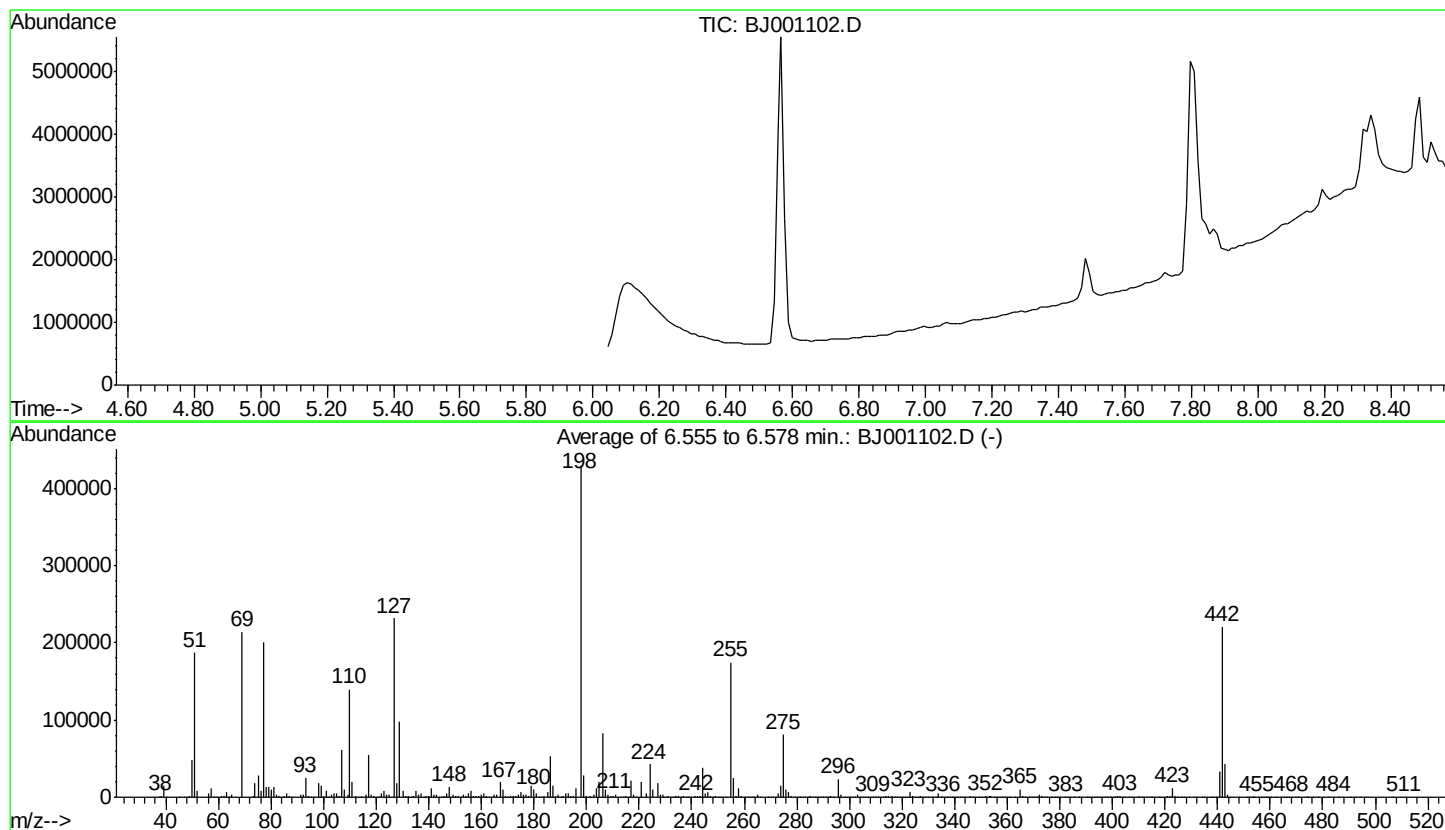

AutoFind: Scans 46, 47, 48; Background Corrected with Scan 39

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	43.6	187366	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	49.8	214016	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	53.9	231551	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	429544	PASS
199	198	5	9	6.5	27989	PASS
275	198	10	30	18.7	80509	PASS
365	198	1	100	2.4	10294	PASS
441	443	0.01	100	78.0	33208	PASS
442	198	40	100	51.4	220965	PASS
443	442	17	23	19.3	42570	PASS