


Data Path : Z:\HPCHEM1\BNA_L\data\BL021512\
 Data File : BL000556.D
 Acq On : 15 Feb 2012 10:18
 Operator : HLM
 Sample : DFTPP050
 Misc : DFTPP050 HLM
 ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_L\METHODS\BL021512.M
 Title : CWA degradation products by GCMS
 Last Update : Fri Feb 17 10:16:01 2012

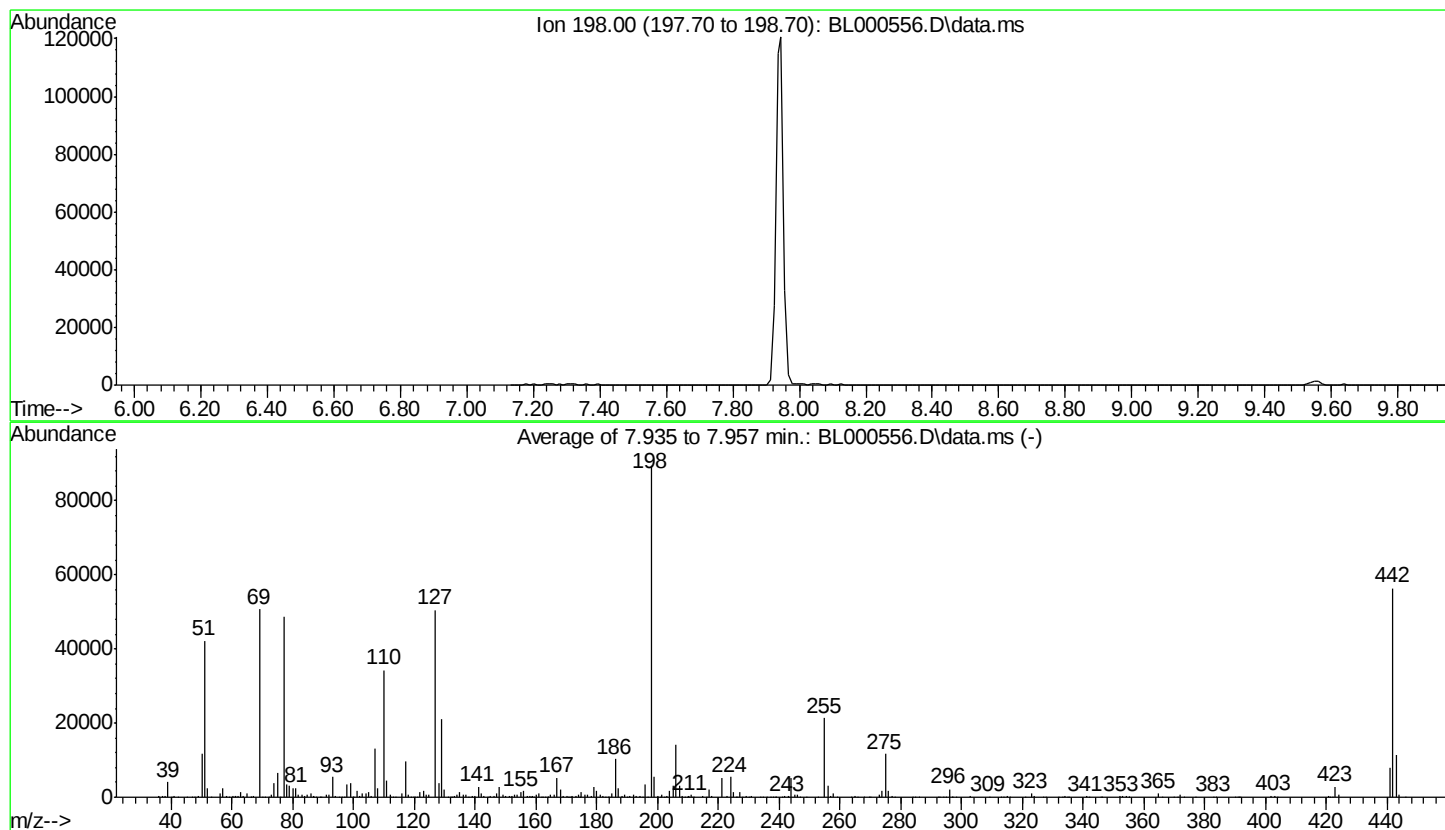

AutoFind: Scans 72, 73, 74; Background Corrected with Scan 67

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	47.1	42145	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	56.6	50618	PASS
70	69	0.00	2	0.2	83	PASS
127	198	40	60	56.5	50549	PASS
197	198	0.00	1	0.1	133	PASS
198	198	100	100	100.0	89456	PASS
199	198	5	9	6.1	5493	PASS
275	198	10	30	13.0	11664	PASS
365	198	1	100	1.1	1018	PASS
441	443	0.01	100	67.6	7832	PASS
442	198	40	100	62.9	56301	PASS
443	442	17	23	20.6	11578	PASS