


Data Path : Z:\HPCHEM1\BNA_L\data\BL021612\
 Data File : BL000564.D
 Acq On : 16 Feb 2012 14:24
 Operator : HLM
 Sample : DFTPP050
 Misc : DFTPP050 HLM
 ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_L\METHODS\BL021512.M
 Title : CWA degradation products by GCMS
 Last Update : Fri Feb 17 10:16:01 2012

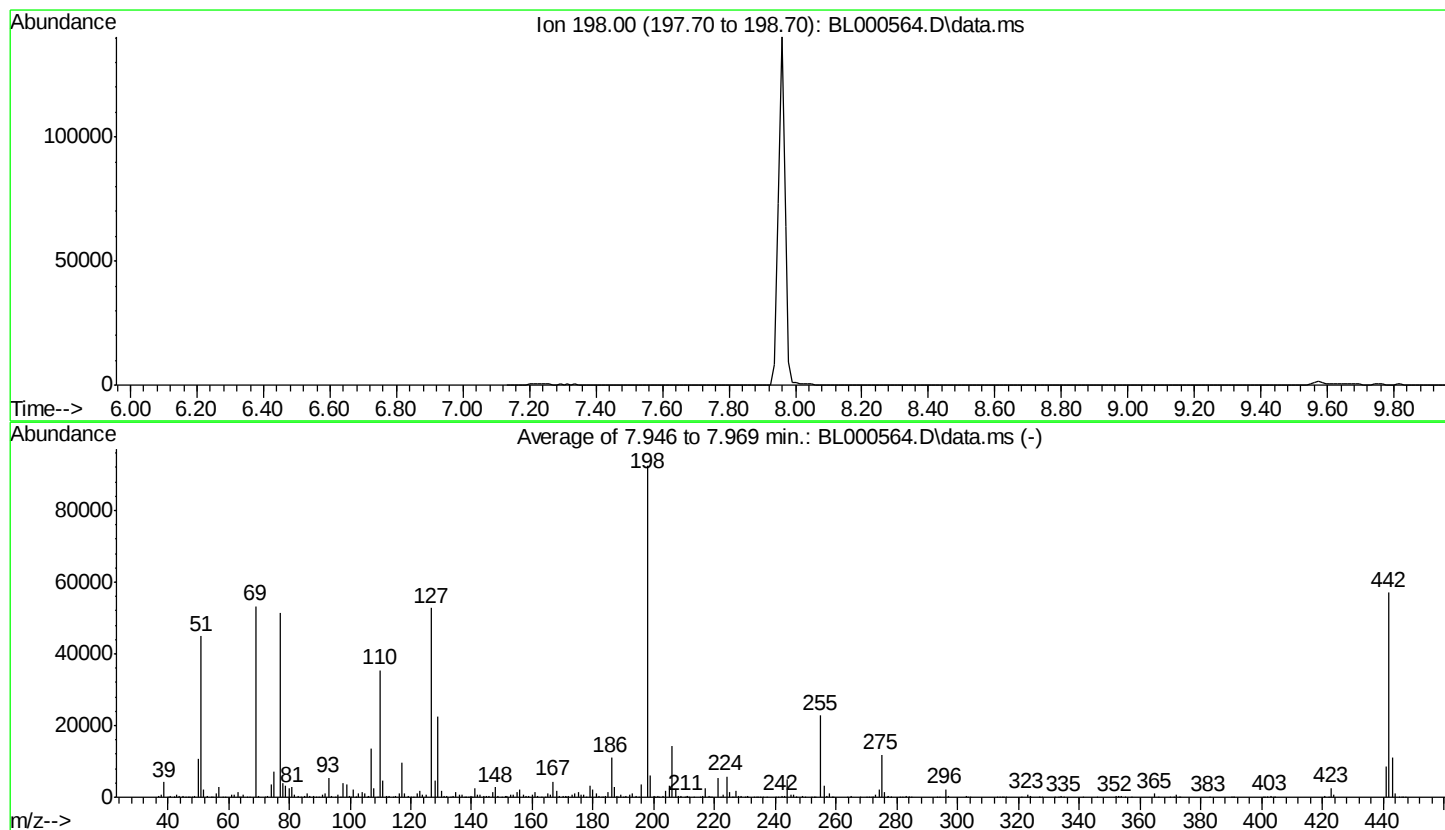

AutoFind: Scans 73, 74, 75; Background Corrected with Scan 68

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	48.5	44869	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	57.7	53324	PASS
70	69	0.00	2	0.4	236	PASS
127	198	40	60	57.1	52818	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	92472	PASS
199	198	5	9	6.6	6087	PASS
275	198	10	30	12.7	11785	PASS
365	198	1	100	1.0	954	PASS
441	443	0.01	100	76.8	8400	PASS
442	198	40	100	61.8	57109	PASS
443	442	17	23	19.1	10932	PASS