

Data File : H:\VOL1\GCMSDATA\L\120725\BL000654.D

Vial: 14

Acq On : 26 Jul 2012 3:24

Operator: HLM

Sample : BENZIDINE010

Inst : BNA L

Misc : HLM

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Jul 26 11:13 2012

Quant Results File: BL0725A2.RES

Instrument :

BNA_L


ClientSampleId :


Method : H:\VOL1\GCMSDATA\L\METHODS\BL0725A2.M (RTE Integrator)

Title : SW-846 Method 8270

Last Update : Thu Jul 26 11:14:39 2012

Response via : Initial Calibration

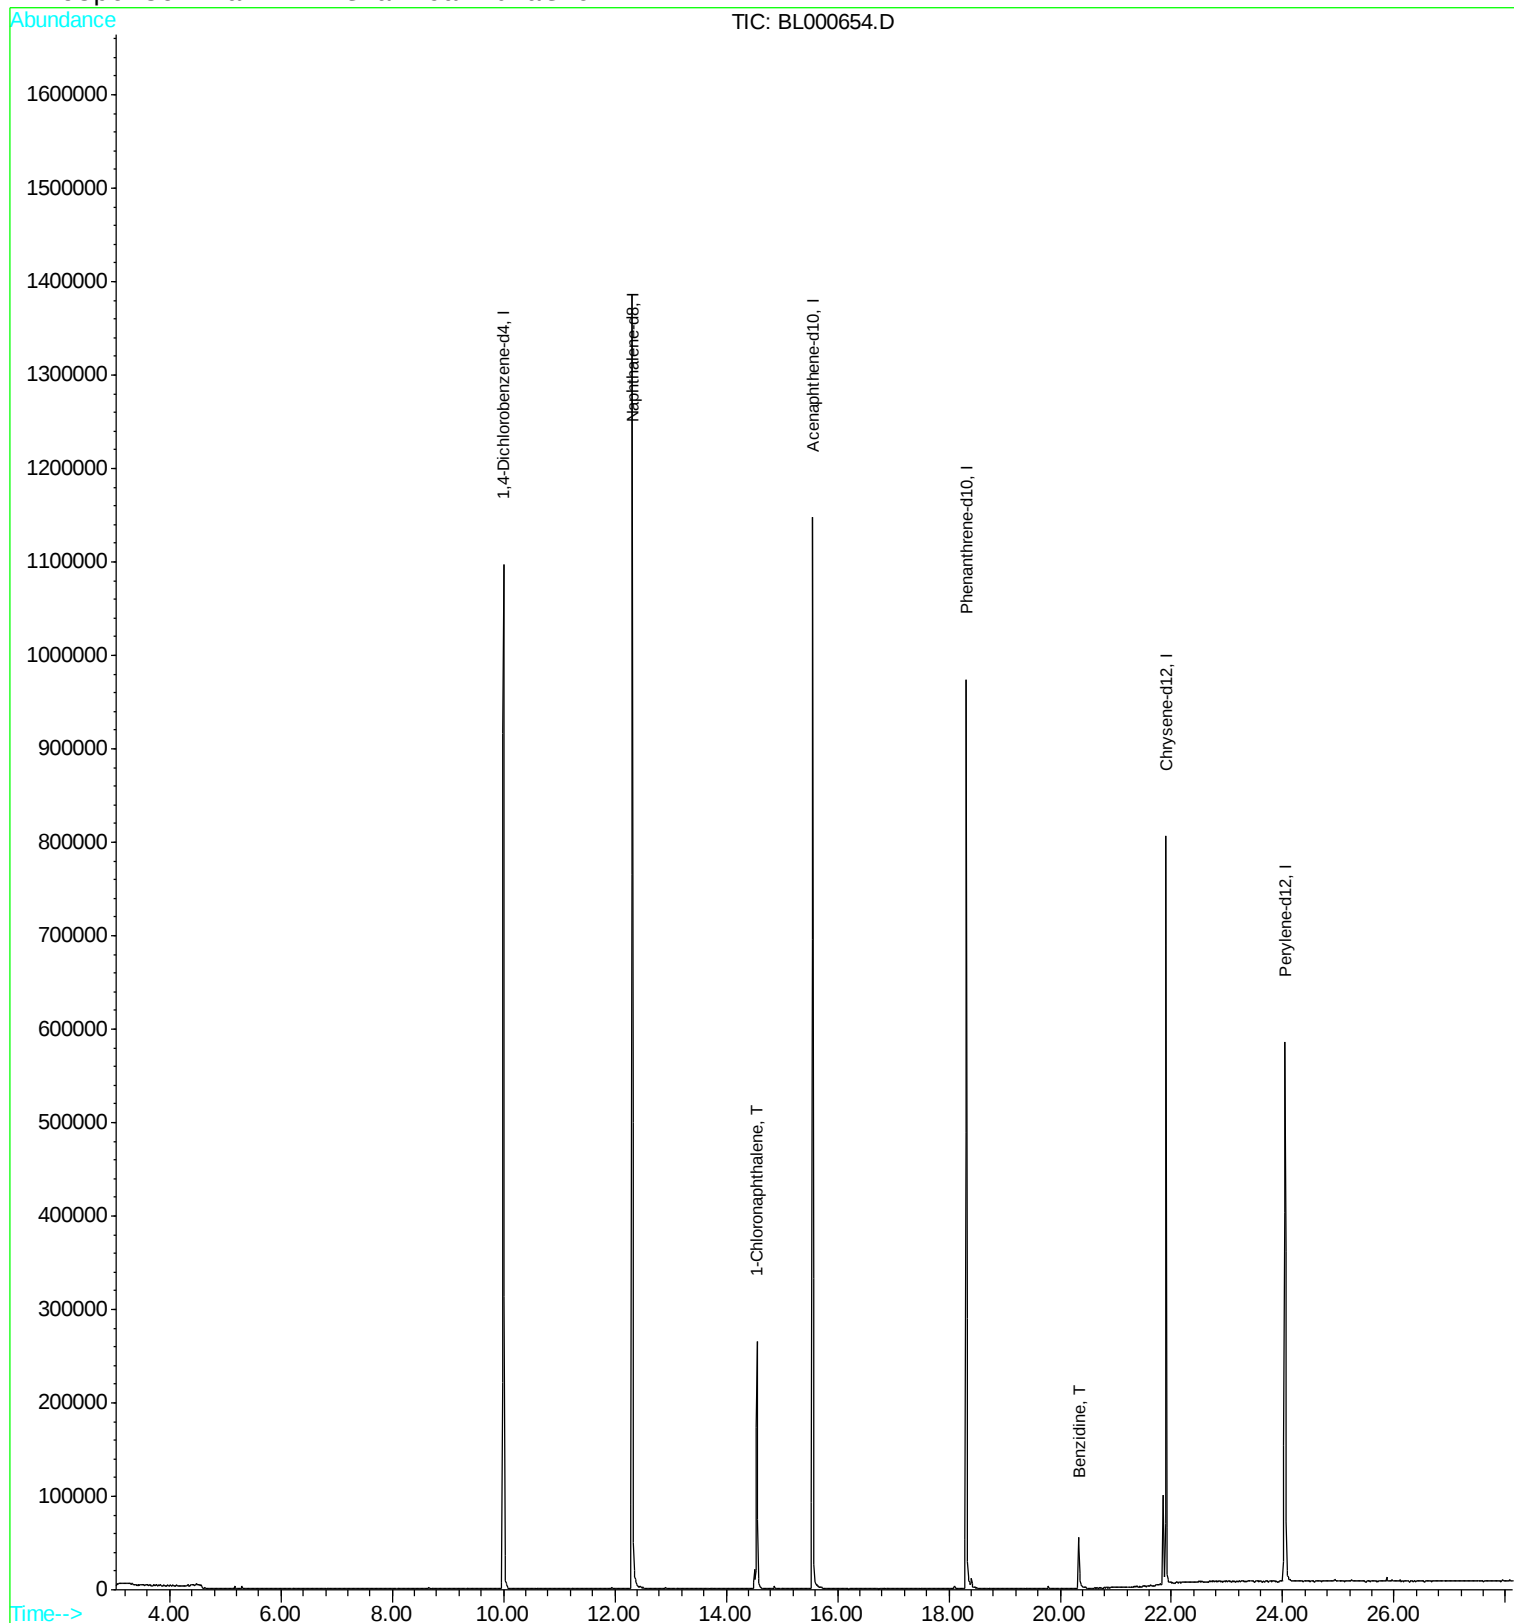

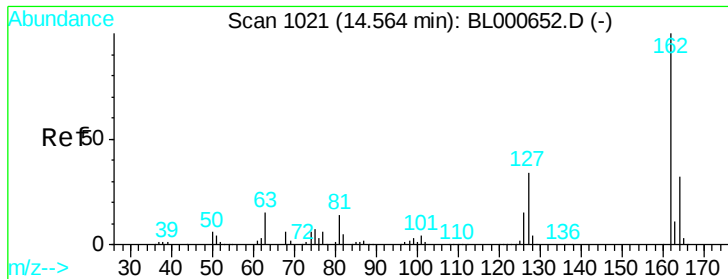

#4

1-Chloronaphthalene

Concen: 7.04 ug/ml

RT: 14.56 min Scan# 1021

Delta R.T. -0.01 min

Lab File: BL000654.D

Acq: 26 Jul 2012 3:24

Instrument :

BNA_L

ClientSampled :


Tgt Ion:162 Resp: 141299

Ion Ratio Lower Upper

162 100

164 32.8 11.9 51.9

127 32.5 13.6 53.6

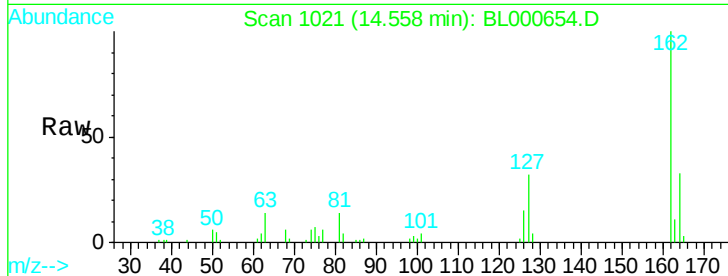

Abundance

Ion 162.00 (161.70 to 162.70): E

120000

Ion 164.00 (163.70 to 164.70): E

100000

Ion 127.00 (126.70 to 127.70): E




80000

60000

40000

20000

0

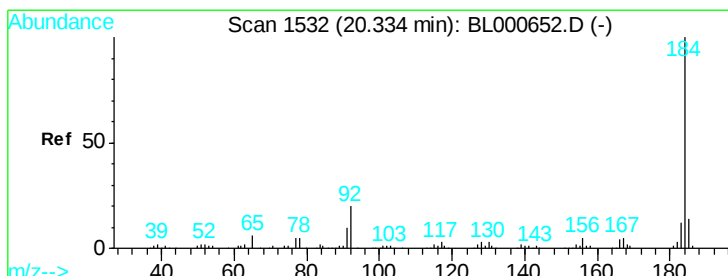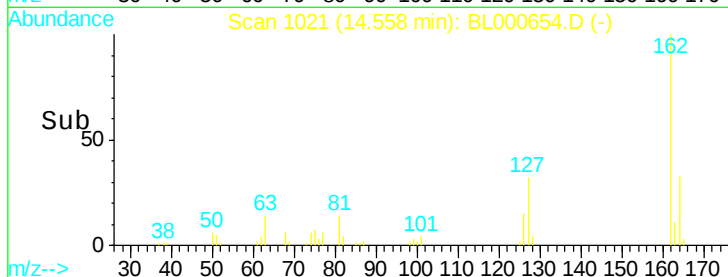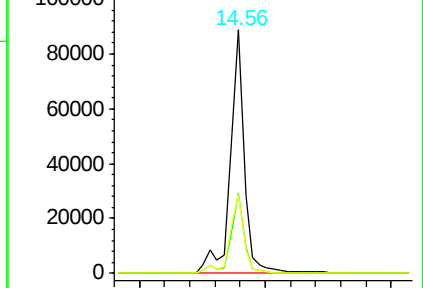

#6

Benzidine

Concen: 10.77 ug/ml


RT: 20.34 min Scan# 1533

Delta R.T. 0.01 min

Lab File: BL000654.D

Acq: 26 Jul 2012 3:24

Tgt Ion:184 Resp: 54792

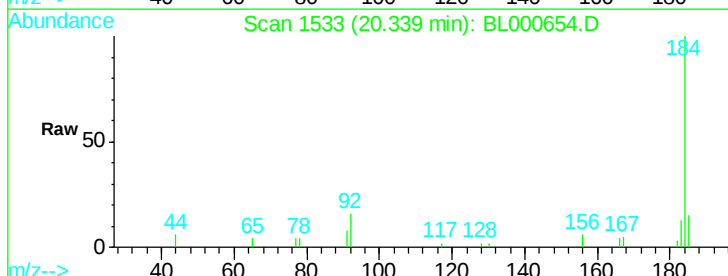

Abundance

Ion 184.00 (183.70 to 184.70): E

30000

25000



20000

15000

10000

5000

0

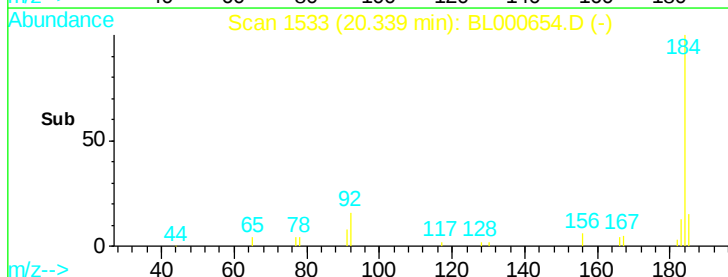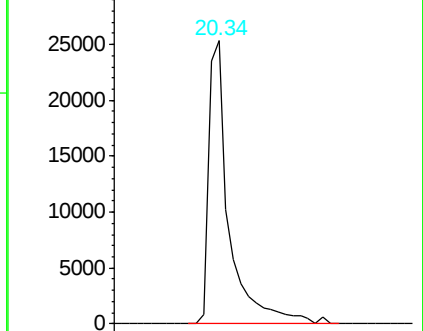

Data File : H:\VOL1\GCMSDATA\L\120725\BL000654.D

Vial: 14

Acq On : 26 Jul 2012 3:24

Operator: HLM

Sample : BENZIDINE010

Inst : BNA L

Misc : HLM

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Jul 26 11:13 2012

Quant Results File: BL0725A2.RES

Instrument :

BNA_L

ClientSampleId :

Quant Method : H:\VOL1\GCMSDATA\L\METHODS\BL0725A2.M (RTE Integrator)

Title : SW-846 Method 8270

Last Update : Thu Jul 26 11:14:39 2012

Response via : Initial Calibration

DataAcq Meth : 8270L

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	10.01	152	313418	40.00	ug/ml	0.00
2) Naphthalene-d8	12.31	136	957674	40.00	ug/ml	0.00
3) Acenaphthene-d10	15.55	164	368476	40.00	ug/ml	0.00
5) Phenanthrene-d10	18.32	188	491842	40.00	ug/ml	0.00
7) Chrysene-d12	21.91	240	389334	40.00	ug/ml	0.00
8) Perylene-d12	24.04	264	361972	40.00	ug/ml	0.00

System Monitoring Compounds

Target Compounds						Ovalue
4) 1-Chloronaphthalene	14.56	162	141299	7.04	ug/ml	98
6) Benzidine	20.34	184	54792	10.77	ug/ml	100