


Method : H:\VOL1\GCMSDATA\L\METHODS\BL0725A2.M (RTE Integrator)
Title : SW-846 Method 8270
Last Update : Thu Jul 26 11:16:39 2012
Response via : Initial Calibration

Calibration Files

50 =BL000652.D 160 =BL000649.D 10 =BL000654.D
20 =BL000653.D 80 =BL000651.D 120 =BL000650.D

	Compound	50	160	10	20	80	120	Avg	%RSD
1) I	1,4-Dichlorobenzene-d	-----ISTD-----							
2) I	Naphthalene-d8	-----ISTD-----							
3) I	Acenaphthene-d10	-----ISTD-----							
4) T	1-Chloronaphthalene	1.132	1.020	1.534	1.416	1.139	1.038	1.213	17.45
5) I	Phenanthrene-d10	-----ISTD-----							
6) T	Benzidine	0.452	0.462	0.446	0.447	0.378	0.437	0.437	6.86
7) I	Chrysene-d12	-----ISTD-----							
8) I	Perylene-d12	-----ISTD-----							

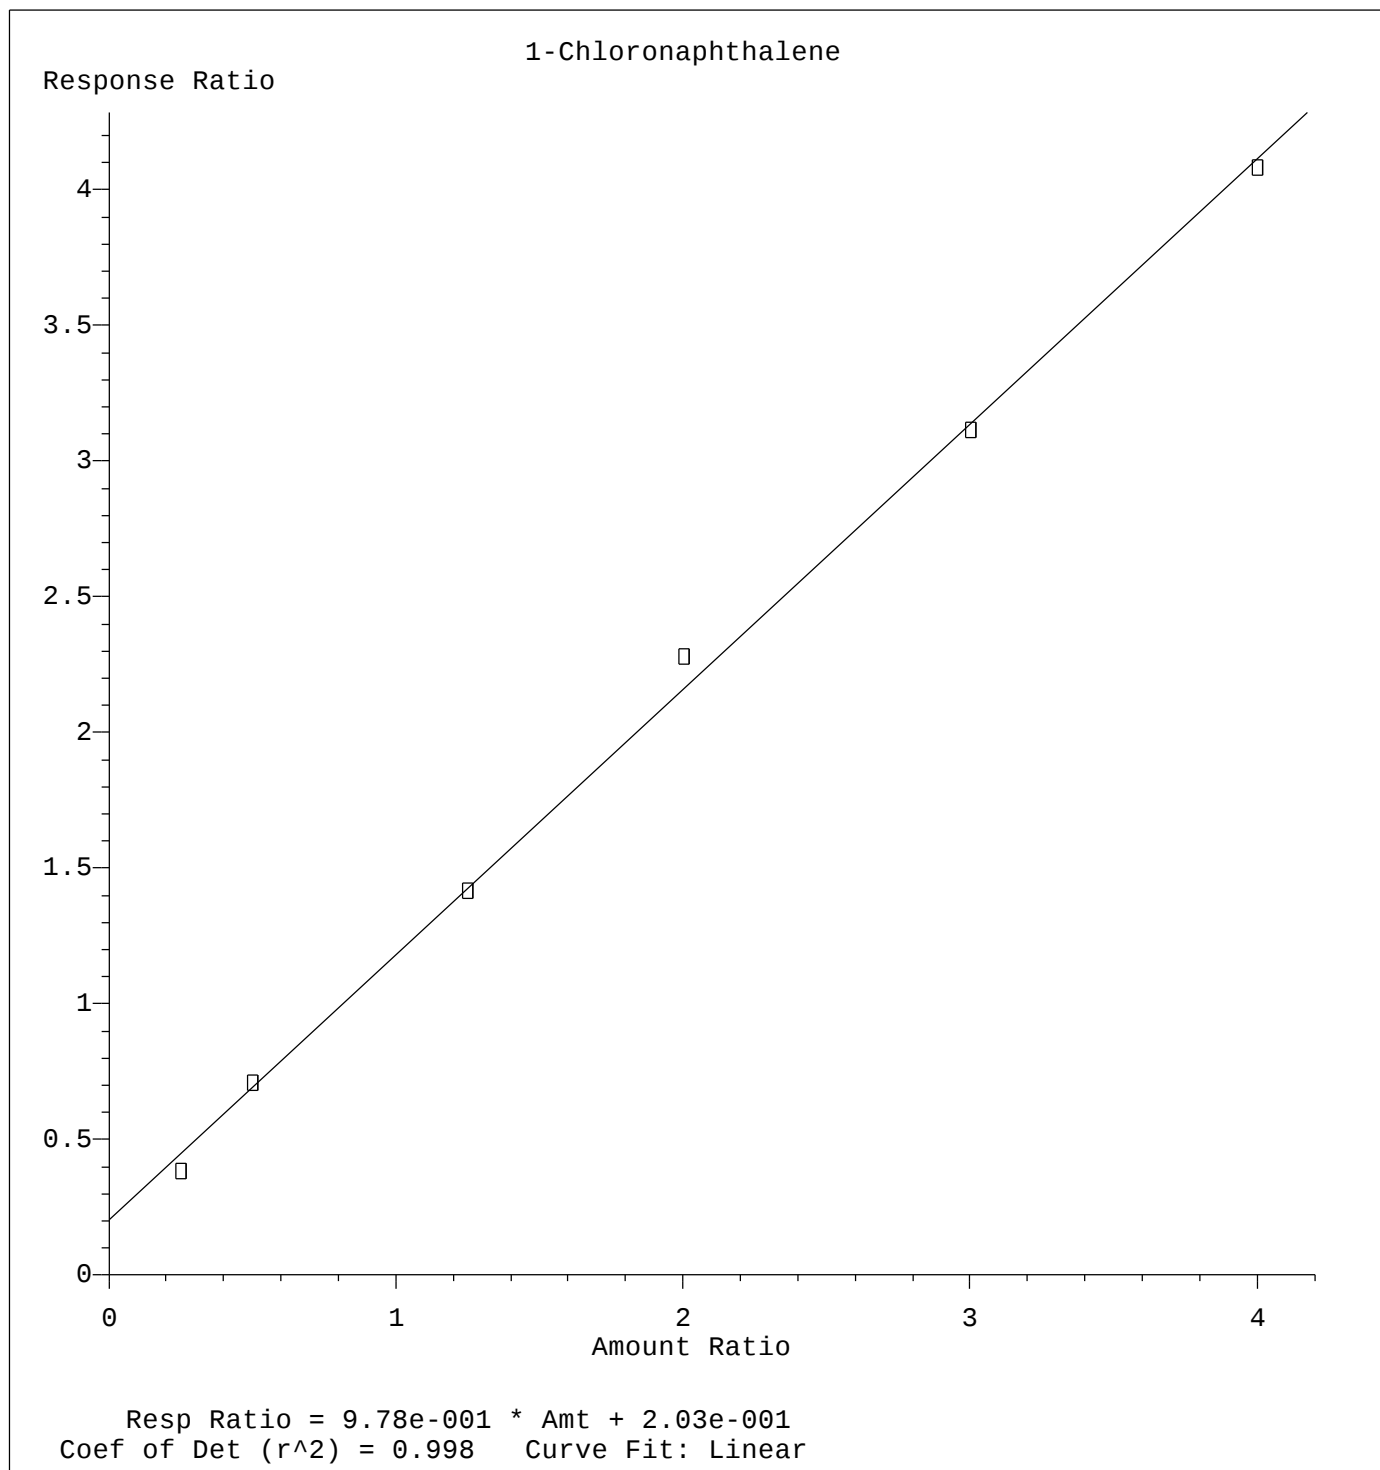

Method Name: H:\VOL1\GCMSDATA\L\METHODS\BL0725A2.M
Calibration Table Last Updated: Thu Jul 26 11:17:04 2012