

Data File : H:\VOL1\GCMSDATA\L\120725\BL000650.D

Vial: 10

Acq On : 26 Jul 2012 00:52

Operator: HLM

Sample : BENZIDINE120

Inst : BNA L

Misc : HLM

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Jul 26 11:13 2012

Quant Results File: BL0725A2.RES

Instrument :

BNA_L


ClientSampleId :


Method : H:\VOL1\GCMSDATA\L\METHODS\BL0725A2.M (RTE Integrator)

Title : SW-846 Method 8270

Last Update : Thu Jul 26 11:17:04 2012

Response via : Initial Calibration

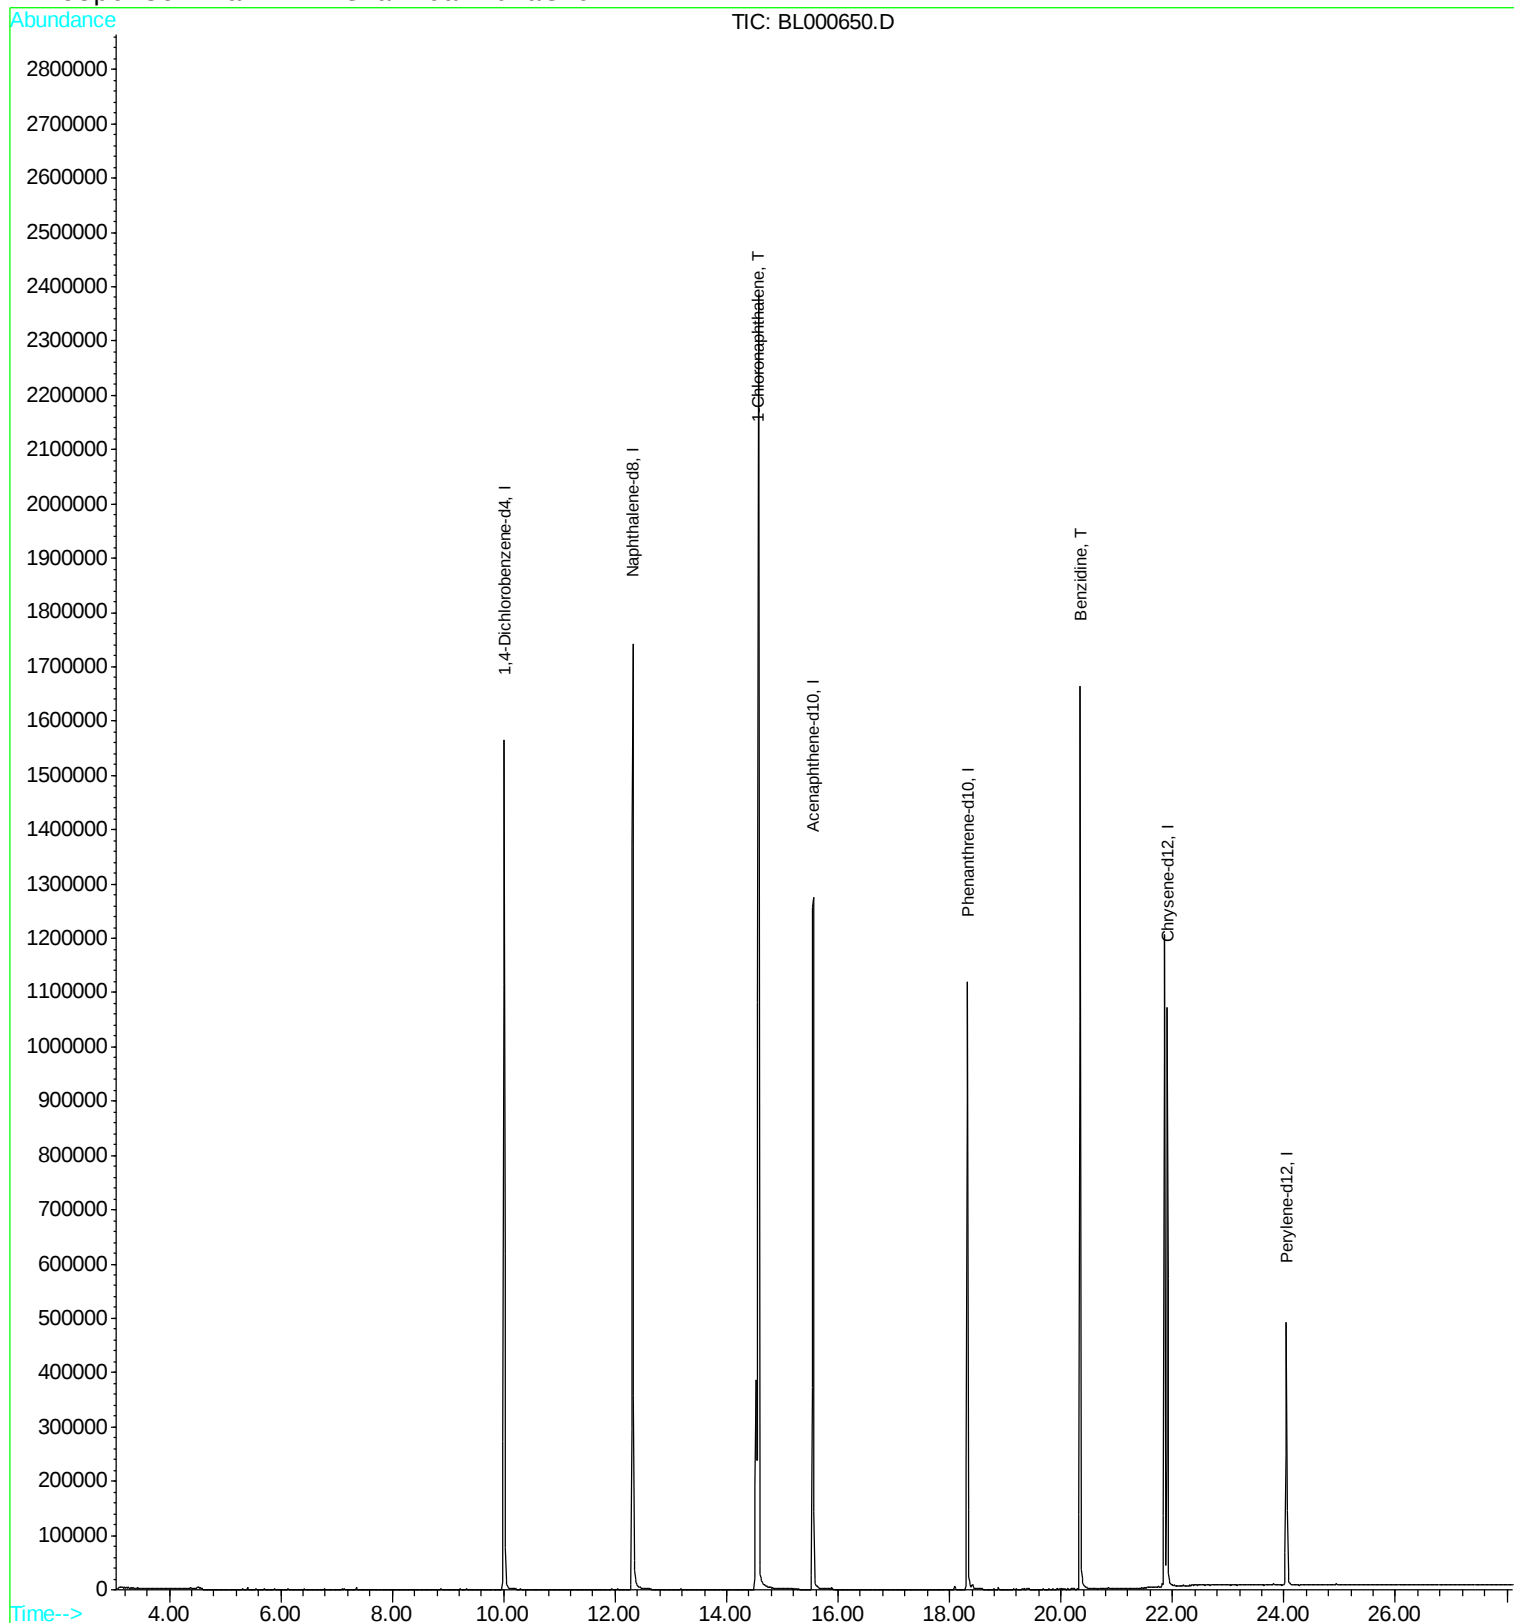

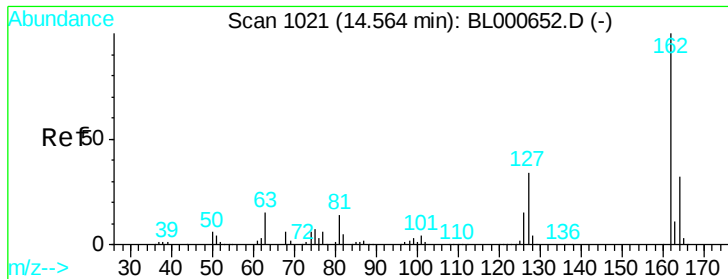

#4

1-Chloronaphthalene

Concen: 114.80 ug/ml

RT: 14.57 min Scan# 1022

Delta R.T. 0.01 min

Lab File: BL000650.D

Acq: 26 Jul 2012 00:52

Instrument :

BNA_L

ClientSampleId :


Tgt Ion:162 Resp: 1574963

Ion Ratio Lower Upper

162 100

164 32.8 11.9 51.9

127 33.2 13.6 53.6



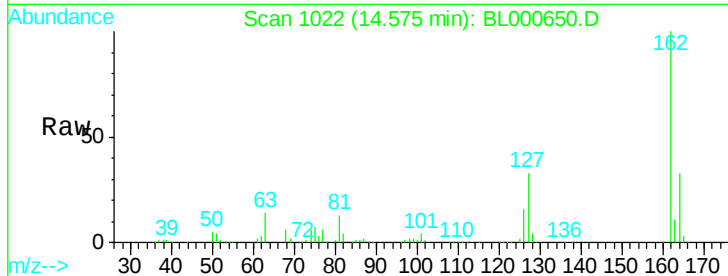


Abundance

Ion 162.00 (161.70 to 162.70): E

Ion 164.00 (163.70 to 164.70): E

Ion 127.00 (126.70 to 127.70): E

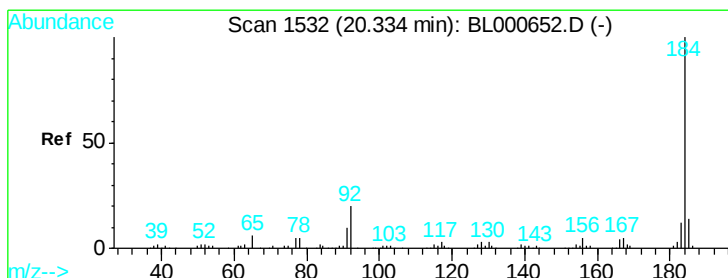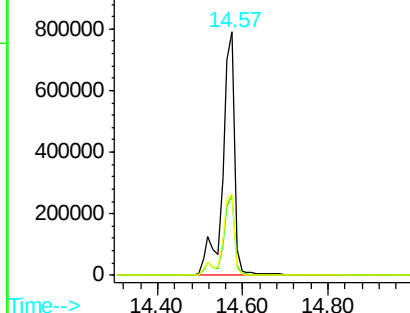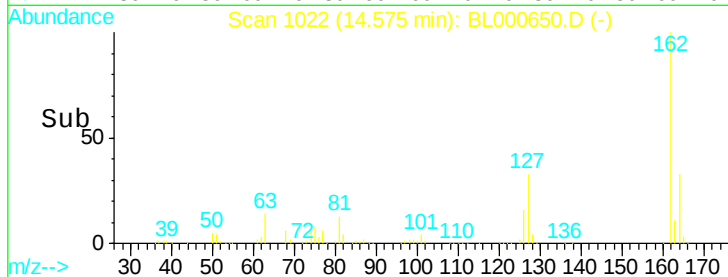

#6

Benzidine

Concen: 115.95 ug/ml


RT: 20.34 min Scan# 1533

Delta R.T. 0.01 min

Lab File: BL000650.D



Acq: 26 Jul 2012 00:52

Tgt Ion:184 Resp: 846164

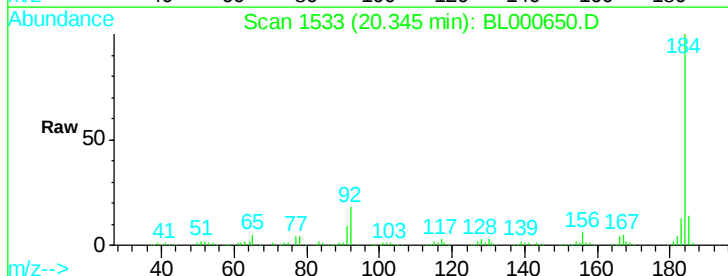

Abundance

Ion 184.00 (183.70 to 184.70): E

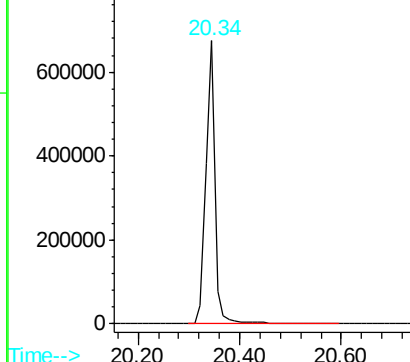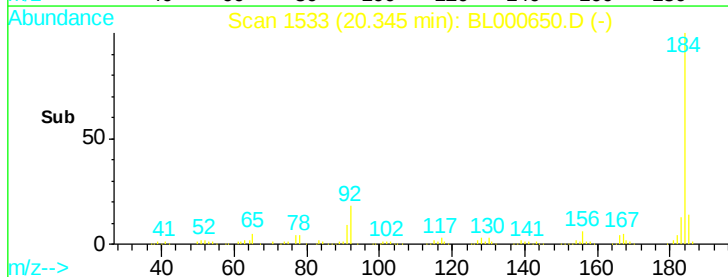

Data File : H:\VOL1\GCMSDATA\L\120725\BL000650.D

Vial: 10

Acq On : 26 Jul 2012 00:52

Operator: HLM

Sample : BENZIDINE120

Inst : BNA L

Misc : HLM

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Jul 26 11:13 2012

Quant Results File: BL0725A2.RES

Instrument :

BNA_L

ClientSampleId :

Quant Method : H:\VOL1\GCMSDATA\L\METHODS\BL0725A2.M (RTE Integrator)

Title : SW-846 Method 8270

Last Update : Thu Jul 26 11:14:39 2012

Response via : Initial Calibration

DataAcq Meth : 8270L

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	10.01	152	441674	40.00	ug/ml	0.01
2) Naphthalene-d8	12.32	136	1289373	40.00	ug/ml	0.01
3) Acenaphthene-d10	15.56	164	505788	40.00	ug/ml	0.00
5) Phenanthrene-d10	18.32	188	646001	40.00	ug/ml	0.00
7) Chrysene-d12	21.90	240	443386	40.00	ug/ml	0.00
8) Perylene-d12	24.05	264	327760	40.00	ug/ml	0.00

System Monitoring Compounds

Target Compounds						Ovalue
4) 1-Chloronaphthalene	14.57	162	1574963	114.80	ug/ml	99
6) Benzidine	20.34	184	846164	115.95	ug/ml	100