

Quantitation Report

Data File : H:\VOL1\GCMSDATA\L\120725\BL000655.D

Vial: 15

Acq On : 26 Jul 2012 4:01

Operator: HLM

Sample : BENZIDINE050ICV

Inst : BNA L

Misc : HLM

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Jul 26 11:15 2012

Quant Results File: BL0725A2.RES

Instrument :

BNA_L


ClientSampleId :


Method : H:\VOL1\GCMSDATA\L\METHODS\BL0725A2.M (RTE Integrator)

Title : SW-846 Method 8270

Last Update : Thu Jul 26 11:17:04 2012

Response via : Initial Calibration

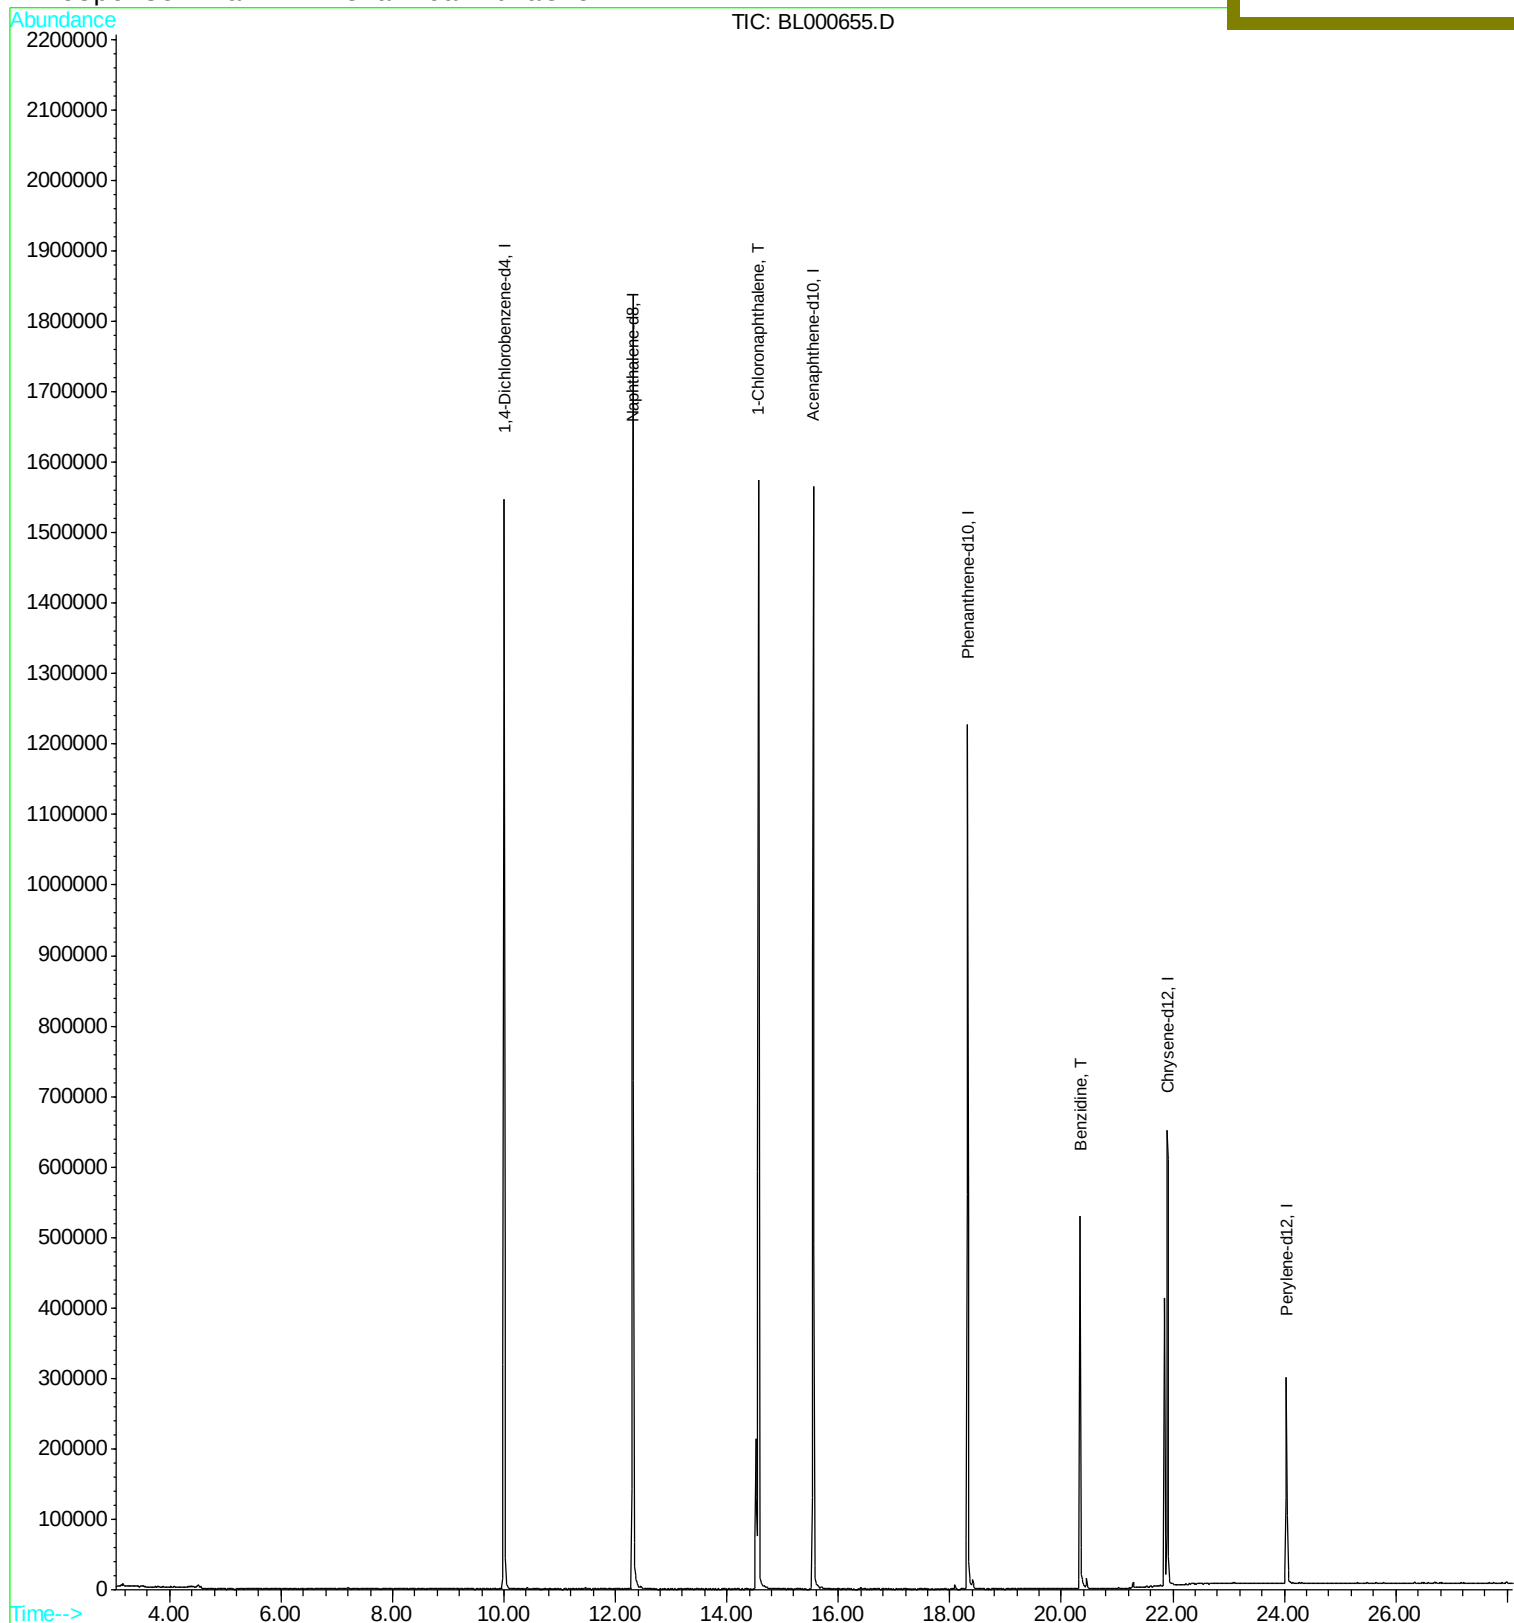Manual Integrations
APPROVEDAHPatel
9/6/2012 6:41:53 AM

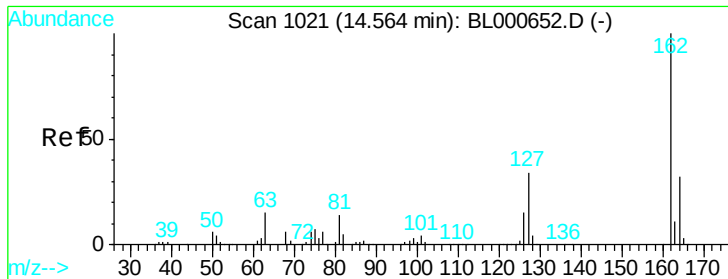

#4

1-Chloronaphthalene

Concen: 54.18 ug/ml m

RT: 14.56 min Scan# 1021

Delta R.T. -0.00 min


Lab File: BL000655.D

Acq: 26 Jul 2012 4:01

Instrument :

BNA_L

ClientSampled :

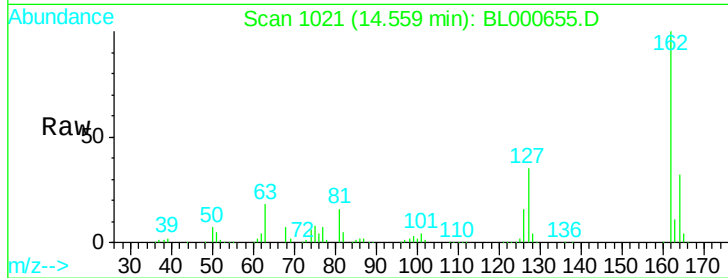

Tgt Ion:162 Resp: 759872

Ion Ratio Lower Upper


162 100

164 31.8 11.9 51.9

127 35.3 13.6 53.6

Manual Integrations
APPROVED

AHPatel
9/6/2012 6:41:53 AM


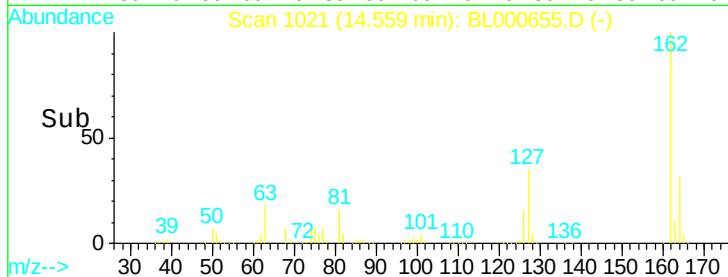


Abundance

Ion 162.00 (161.70 to 162.70): E

Ion 164.00 (163.70 to 164.70): E

Ion 127.00 (126.70 to 127.70): E

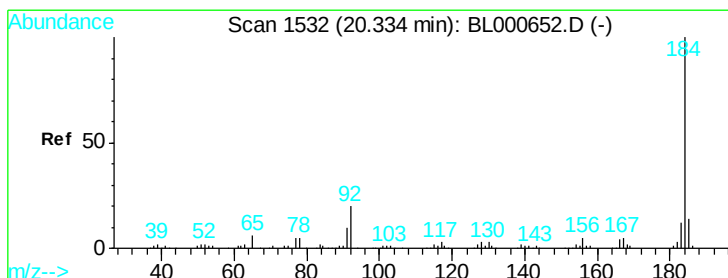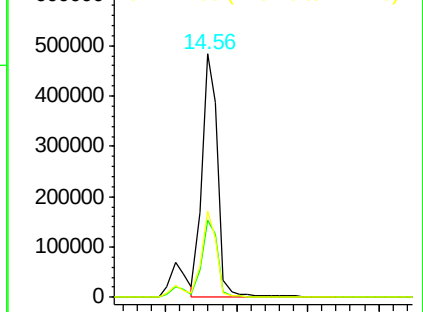

#6

Benidine

Concen: 53.45 ug/ml



RT: 20.34 min Scan# 1533

Delta R.T. 0.01 min

Lab File: BL000655.D


Acq: 26 Jul 2012 4:01

Tgt Ion:184 Resp: 345630

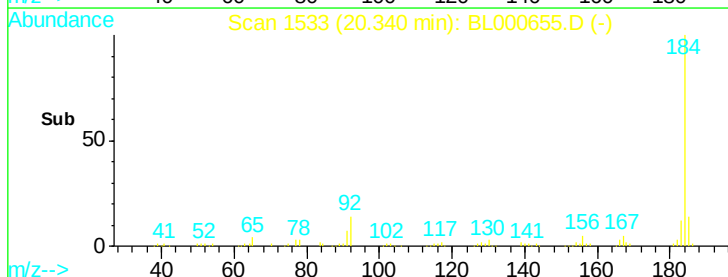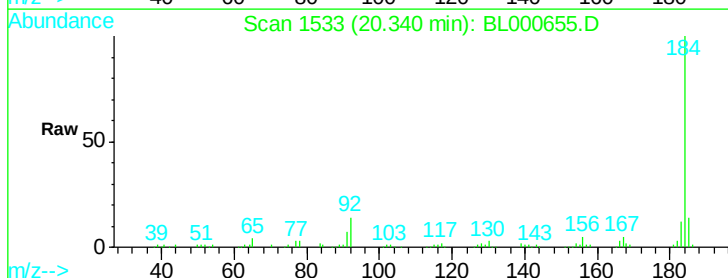

Abundance

Ion 184.00 (183.70 to 184.70): E

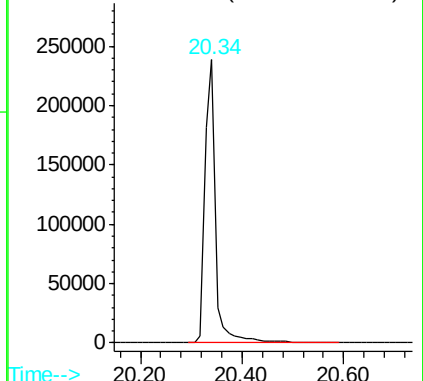

Data File : H:\VOL1\GCMSDATA\L\120725\BL000655.D

Vial: 15

Acq On : 26 Jul 2012 4:01

Operator: HLM

Sample : BENZIDINE050ICV

Inst : BNA L

Misc : HLM

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Jul 26 11:15 2012

Quant Results File: BL0725A2.RES

Instrument :

BNA_L

ClientSampleId :

Quant Method : H:\VOL1\GCMSDATA\L\METHODS\BL0725A2.M (RTE Integrator)

Title : SW-846 Method 8270

Last Update : Thu Jul 26 11:17:04 2012

Response via : Initial Calibration

DataAcq Meth : 8270L

Manual Integrations
APPROVEDAHPatel
9/6/2012 6:41:53 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	10.01	152	440658	40.00	ug/ml	0.00
2) Naphthalene-d8	12.31	136	1288653	40.00	ug/ml	0.00
3) Acenaphthene-d10	15.55	164	497309	40.00	ug/ml	0.00
5) Phenanthrene-d10	18.32	188	647166	40.00	ug/ml	0.00
7) Chrysene-d12	21.91	240	326100	40.00	ug/ml	0.00
8) Perylene-d12	24.04	264	199136	40.00	ug/ml	0.00

System Monitoring Compounds

Target Compounds						Ovalue
4) 1-Chloronaphthalene	14.56	162	759872m	54.18	ug/ml	
6) Benzidine	20.34	184	345630	53.45	ug/ml	100