


Data Path : S:\HPCHEM1\BNA_L\data\BL072512\
 Data File : BL000639.D
 Acq On : 25 Jul 2012 18:03
 Operator : HLM
 Sample : DFTPP050
 Misc : DFTPP050 HLM
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_L
 ClientSampleId :
 DFTPP050

Integration File: rteint.p

Method : S:\HPCHEM1\BNA_L\method\BL072512.M
 Title : SW-846 Method 8270
 Last Update : Thu Jul 26 11:02:15 2012

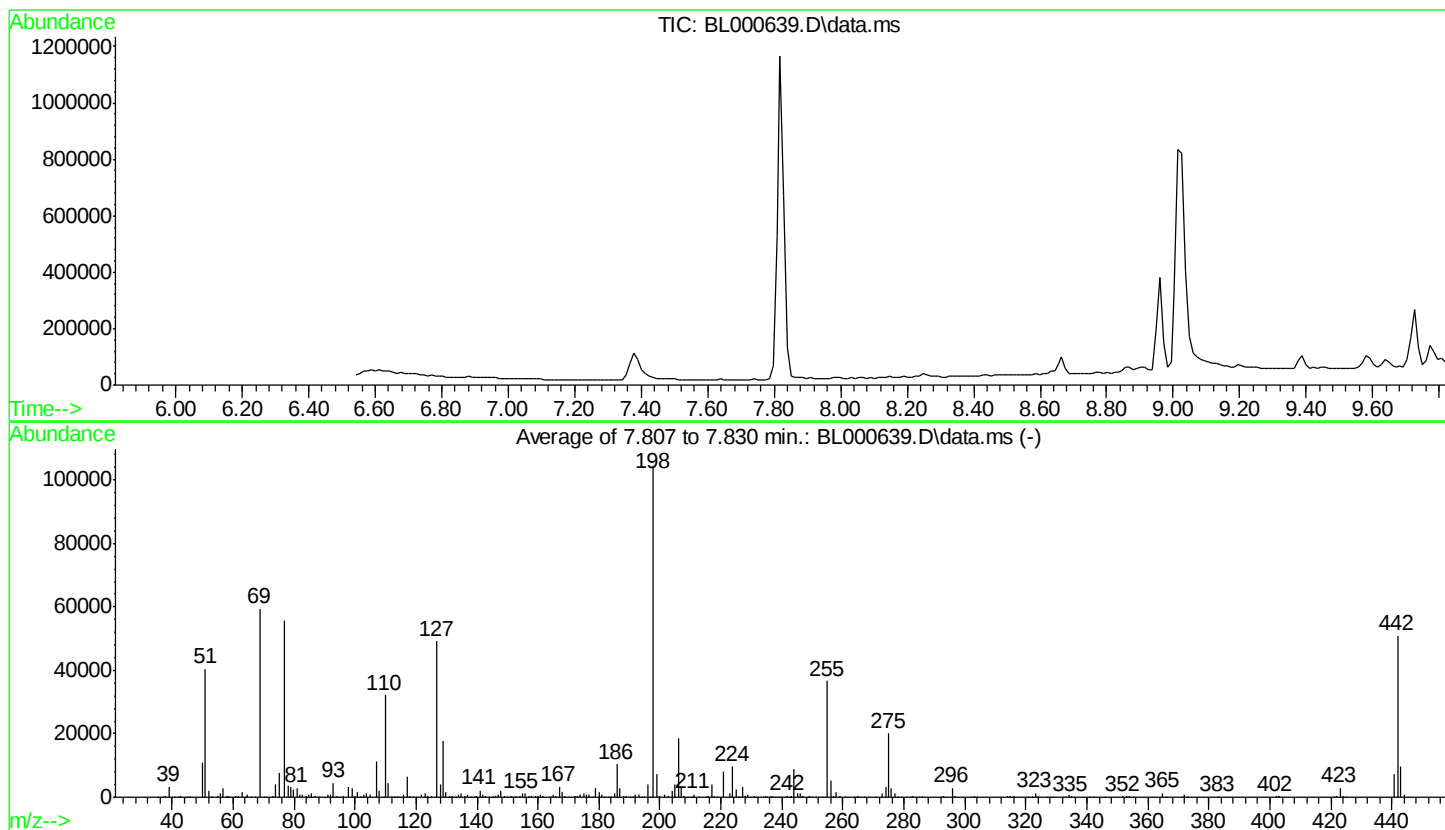

AutoFind: Scans 113, 114, 115; Background Corrected with Scan 109

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	38.8	40544	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	56.8	59408	PASS
70	69	0.00	2	0.3	183	PASS
127	198	40	60	47.1	49194	PASS
197	198	0.00	1	0.2	195	PASS
198	198	100	100	100.0	104533	PASS
199	198	5	9	6.8	7136	PASS
275	198	10	30	19.2	20059	PASS
365	198	1	100	1.2	1285	PASS
441	443	0.01	100	72.9	7178	PASS
442	198	40	100	48.8	51051	PASS
443	442	17	23	19.3	9845	PASS