

Quantitation Report

Data File : H:\VOL1\GCMSDATA\L\120726\BL000658.D

Vial: 3

Acq On : 26 Jul 2012 11:51

Operator: HLM

Sample : BENZIDINE050

Inst : BNA L

Misc : HLM

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Jul 26 12:09 2012

Quant Results File: BL0725A2.RES

Instrument :

BNA_L


ClientSampleId :


Method : H:\VOL1\GCMSDATA\L\METHODS\BL0725A2.M (RTE Integrator)

Title : SW-846 Method 8270

Last Update : Thu Jul 26 11:16:39 2012

Response via : Initial Calibration

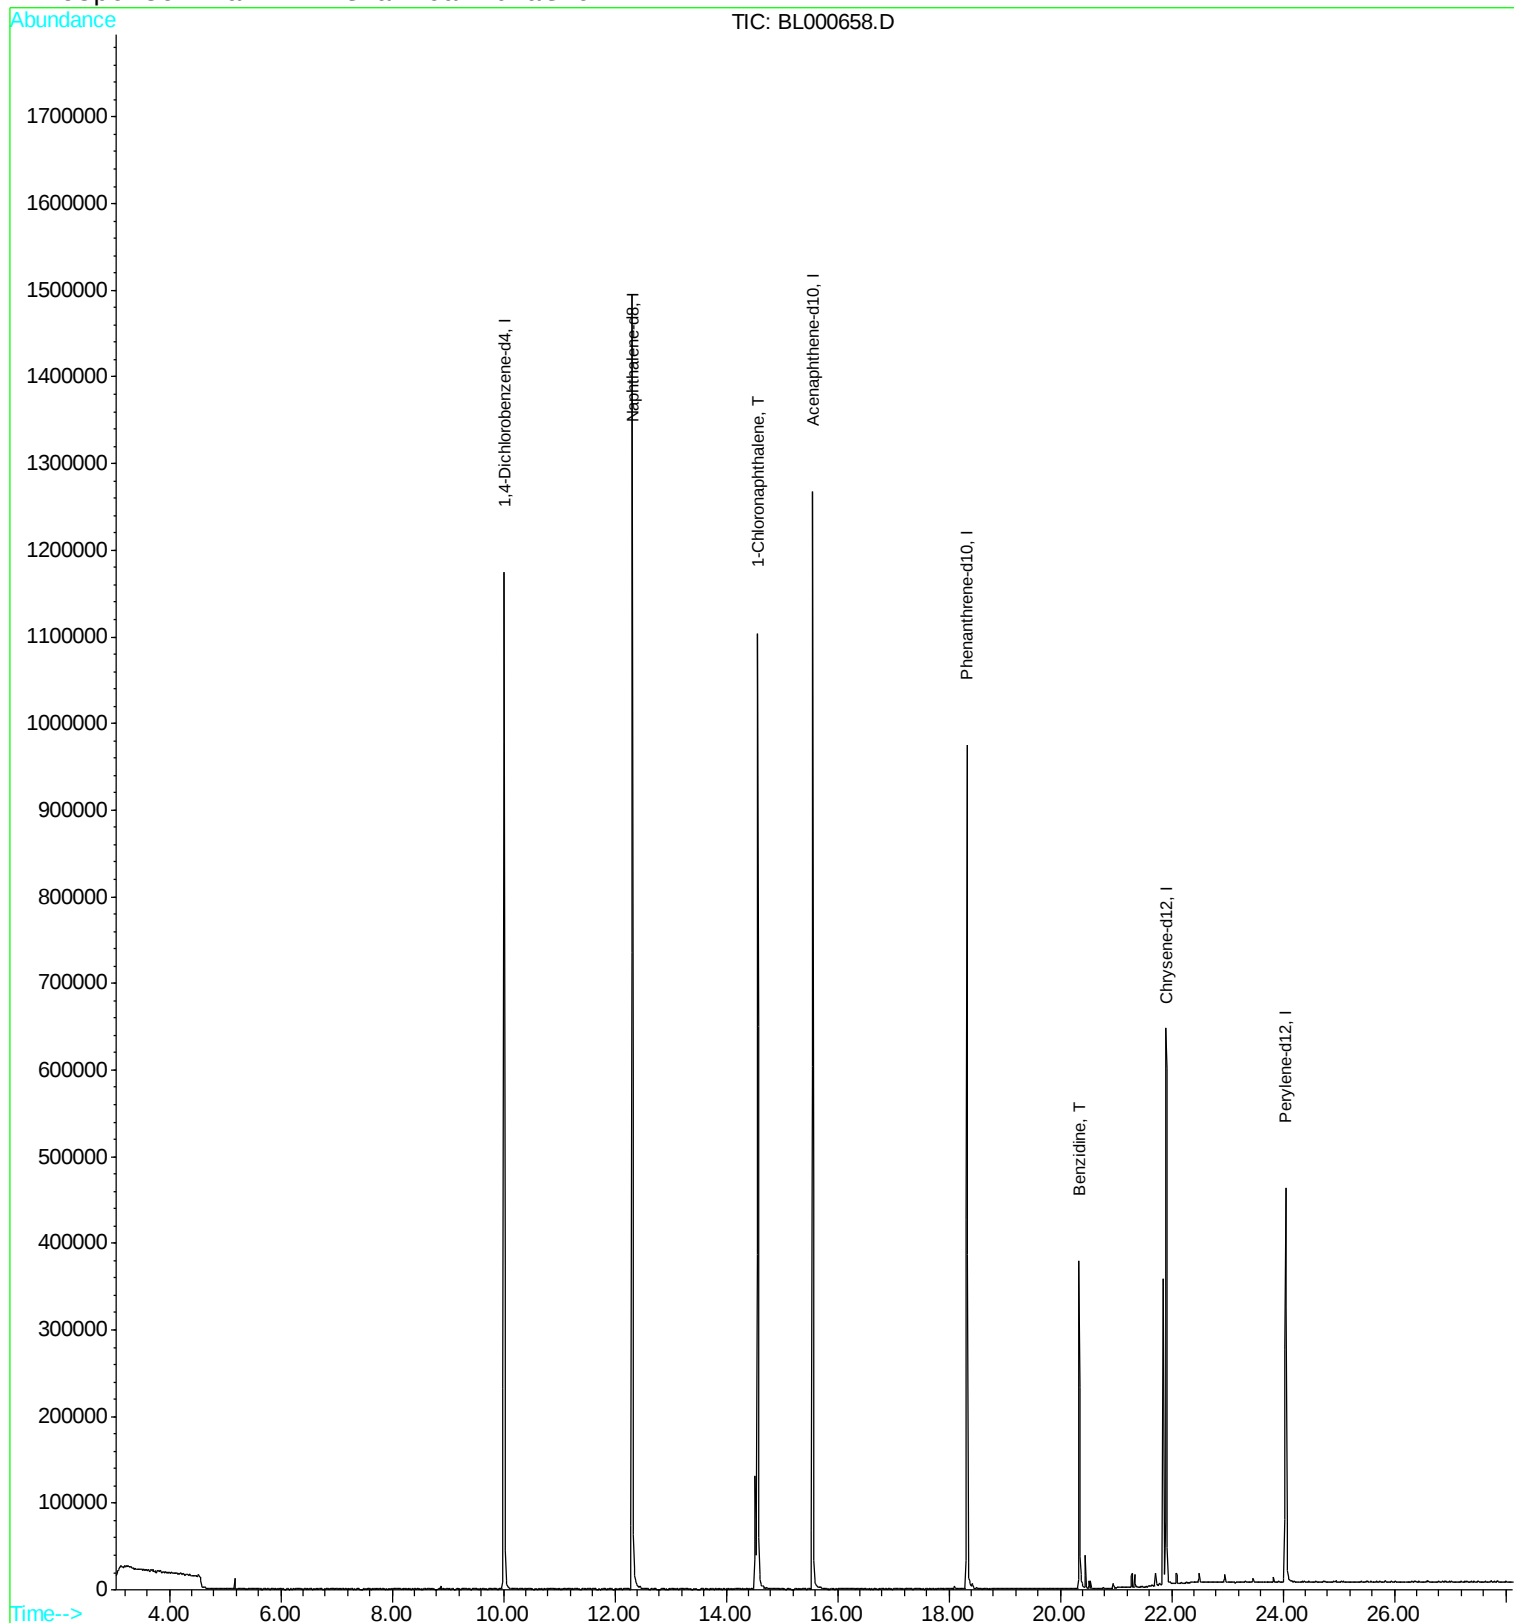

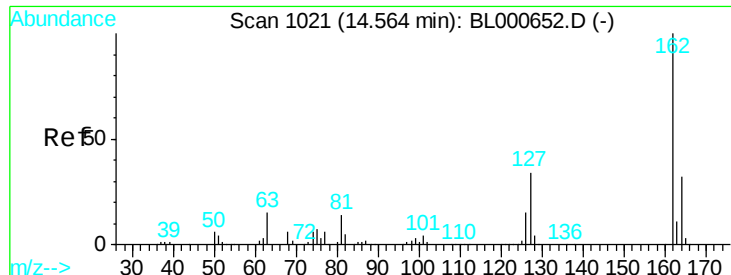

#4

1-Chloronaphthalene

Concen: 50.60 ug/ml

RT: 14.56 min Scan# 1021

Delta R.T. 0.00 min

Lab File: BL000658.D

Acq: 26 Jul 2012 11:51

Instrument :

BNA_L

ClientSampleId :


Tgt Ion:162 Resp: 563241

Ion Ratio Lower Upper

162 100

164 31.9 11.9 51.9

127 35.9 13.6 53.6



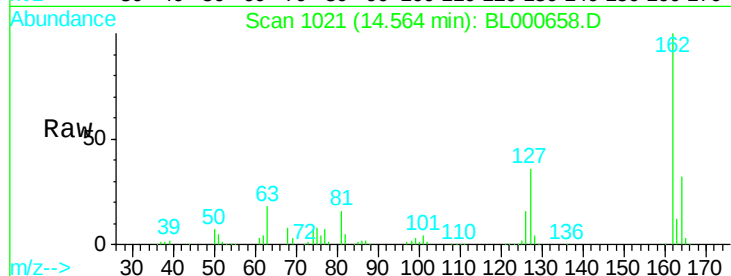


Abundance

Ion 162.00 (161.70 to 162.70): E

Ion 164.00 (163.70 to 164.70): E

Ion 127.00 (126.70 to 127.70): E

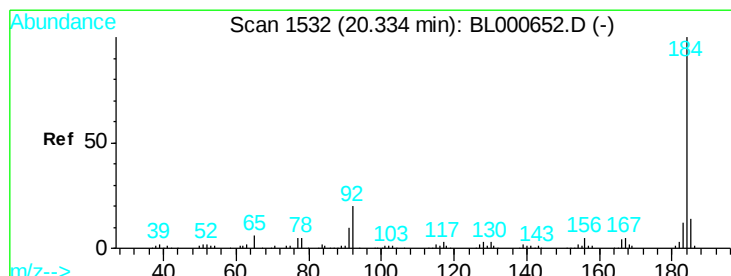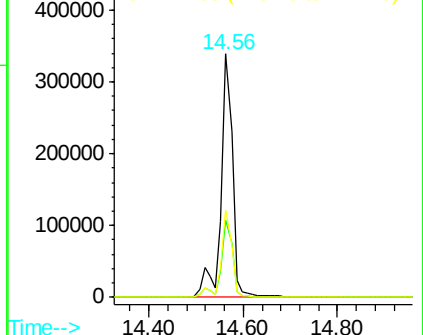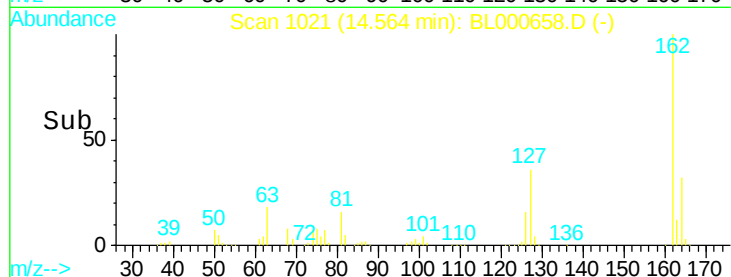

#6

Benzidine

Concen: 43.08 ug/ml




RT: 20.33 min Scan# 1532

Delta R.T. -0.00 min

Lab File: BL000658.D

Acq: 26 Jul 2012 11:51

Tgt Ion:184 Resp: 212109

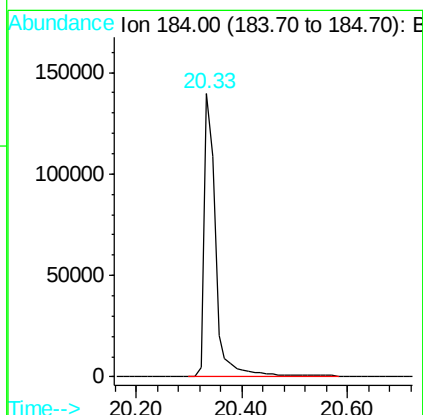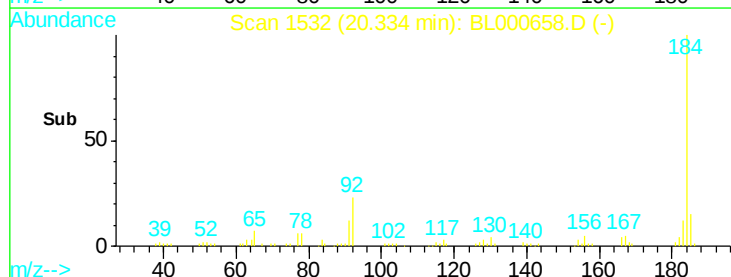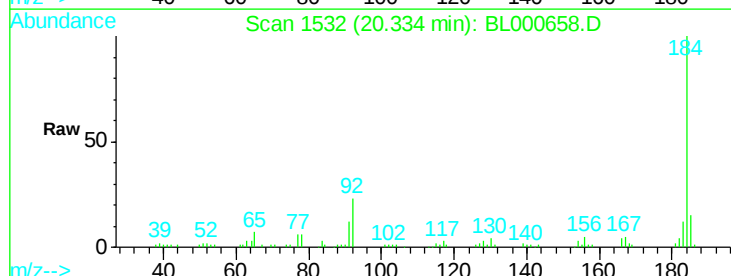

Data File : H:\VOL1\GCMSDATA\L\120726\BL000658.D

Vial: 3

Acq On : 26 Jul 2012 11:51

Operator: HLM

Sample : BENZIDINE050

Inst : BNA L

Misc : HLM

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Jul 26 12:09 2012

Quant Results File: BL0725A2.RES

Instrument :

BNA_L

ClientSampleId :

Quant Method : H:\VOL1\GCMSDATA\L\METHODS\BL0725A2.M (RTE Integrator)

Title : SW-846 Method 8270

Last Update : Thu Jul 26 11:17:04 2012

Response via : Initial Calibration

DataAcq Meth : 8270L

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	10.01	152	339965	40.00	ug/ml	0.01
2) Naphthalene-d8	12.32	136	1005538	40.00	ug/ml	0.01
3) Acenaphthene-d10	15.56	164	391021	40.00	ug/ml	0.00
5) Phenanthrene-d10	18.32	188	491612	40.00	ug/ml	0.00
7) Chrysene-d12	21.91	240	323457	40.00	ug/ml	0.01
8) Perylene-d12	24.05	264	271147	40.00	ug/ml	0.00

System Monitoring Compounds

Target Compounds						Ovalue
4) 1-Chloronaphthalene	14.56	162	563241	50.60	ug/ml	98
6) Benzidine	20.33	184	212109	43.08	ug/ml	100