

#3

N-Nitrosodimethylamine

Concen: 48.43 ug/ml

RT: 3.450 min Scan# 37

Delta R.T. 0.092 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29

Instrument :

BNA_L

ClientSampleId :





ICVBL072512

Tgt Ion: 74 Resp: 707424

Ion Ratio Lower Upper

74 100

43 23.4 2.3 42.3

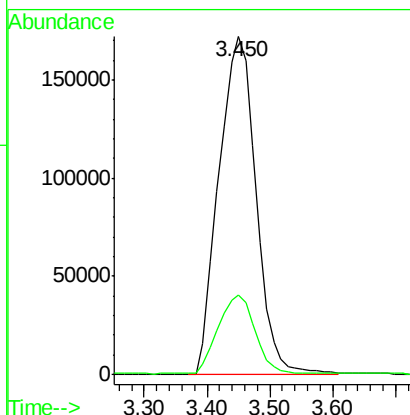

#4

Pyridine

Concen: 47.69 ug/ml

RT: 3.540 min Scan# 45

Delta R.T. 0.081 min

Lab File: BL000659.D




Acq: 26 Jul 2012 12:29


Tgt Ion: 79 Resp: 1063489

Ion Ratio Lower Upper

79 100

52 67.3 47.6 87.6





#6

Benzaldehyde

Concen: 197.22 ug/ml

RT: 9.220 min Scan# 54

Delta R.T. 0.024 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29

Instrument :

BNA_L

ClientSampleId :

ICVBL072512





Tgt Ion: 77 Resp: 646649

Ion Ratio Lower Upper

77 100

105 92.6 70.4 110.4

106 92.8 70.4 110.4

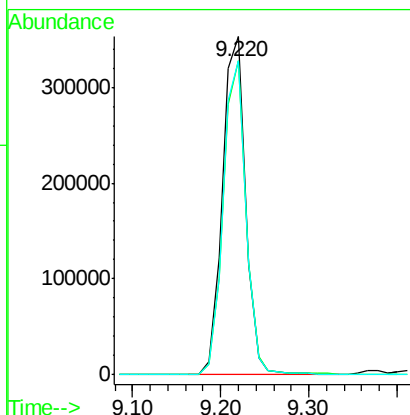

#7

Aniline

Concen: 34.31 ug/ml

RT: 9.412 min Scan# 565

Delta R.T. 0.002 min

Lab File: BL000659.D




Acq: 26 Jul 2012 12:29


Tgt Ion: 93 Resp: 729654

Ion Ratio Lower Upper

93 100

66 39.1 30.6 46.0









#8
 bis(2-Chloroethyl)ether
 Concen: 47.69 ug/ml
 RT: 9.536 min Scan# 576
 Delta R.T. 0.013 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29




Instrument :
 BNA_L
 ClientSampleId :
 ICVBL072512


Tgt Ion:	93	Resp:	679894
Ion	Ratio	Lower	Upper
93	100		
63	75.4	58.9	98.9
95	32.4	11.9	51.9



#10
 Phenol
 Concen: 48.35 ug/ml
 RT: 9.378 min Scan# 562
 Delta R.T. 0.013 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29

Tgt Ion:	94	Resp:	920289
Ion	Ratio	Lower	Upper
94	100		
65	19.8	1.6	41.6
66	22.6	4.3	44.3



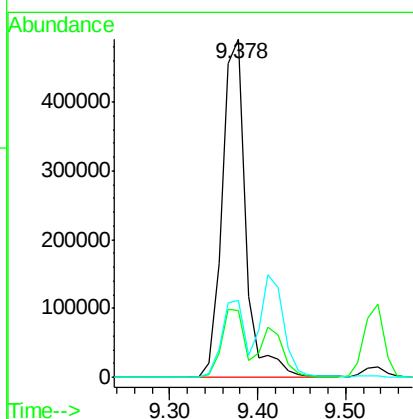



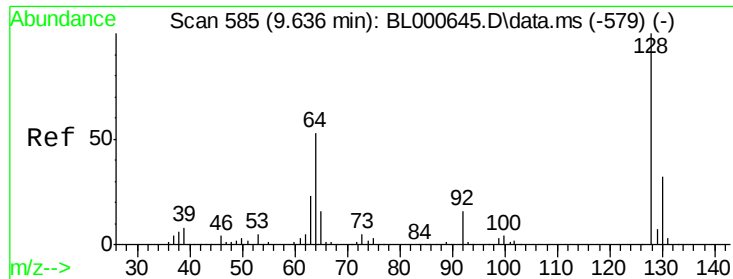

#11
 2-Chlorophenol
 Concen: 47.70 ug/ml
 RT: 9.638 min Scan# 58
 Delta R.T. 0.013 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29




Instrument :
 BNA_L
 ClientSampleId :
 ICVBL072512


Tgt Ion:128 Resp: 561066
 Ion Ratio Lower Upper
 128 100
 64 56.2 37.3 77.3
 130 32.5 12.4 52.4

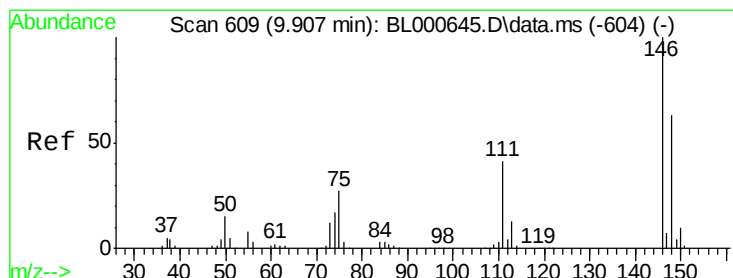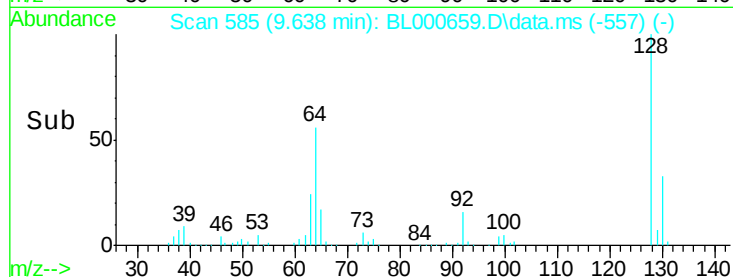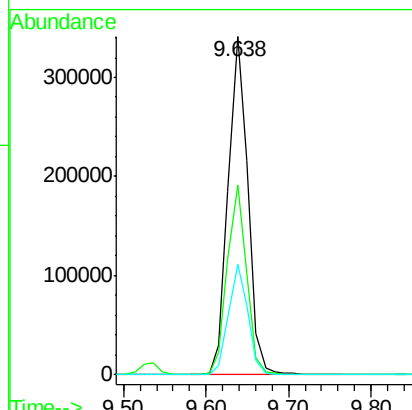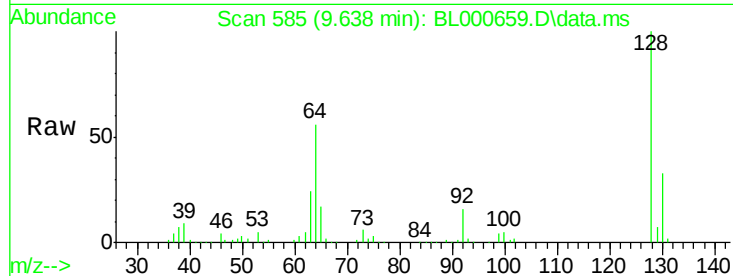

#12
 1,3-Dichlorobenzene
 Concen: 47.73 ug/ml
 RT: 9.920 min Scan# 610
 Delta R.T. 0.013 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29

Tgt Ion:146 Resp: 568161
 Ion Ratio Lower Upper
 146 100
 148 64.8 44.0 84.0
 113 12.5 0.0 32.5


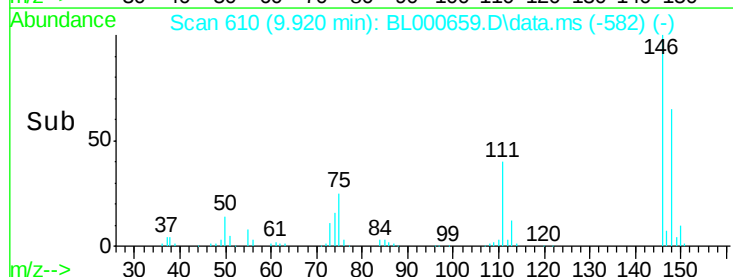
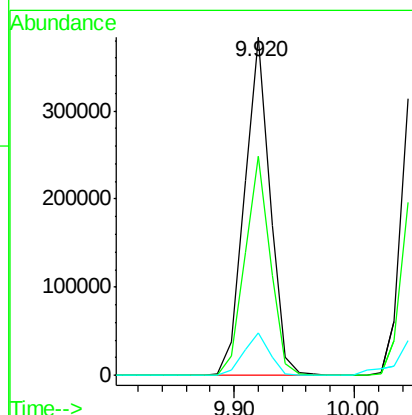
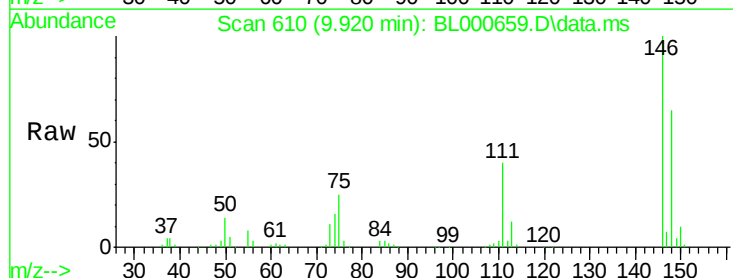




#13
 1,4-Dichlorobenzene
 Concen: 47.84 ug/ml
 RT: 10.056 min Scan# 62
 Delta R.T. 0.013 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29




Instrument :
 BNA_L
 ClientSampleId :
 ICVBL072512


Tgt Ion	Ratio	Lower	Upper
146	100		
148	64.5	44.6	84.6
113	11.9	0.0	32.8

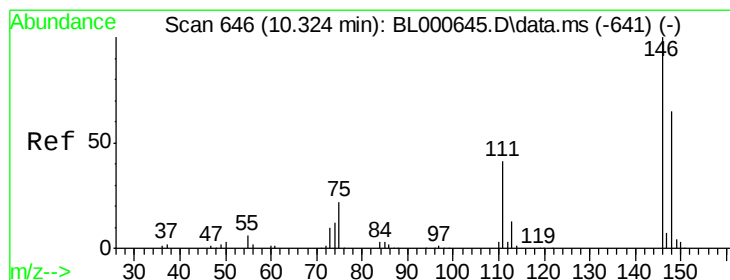

#14
 1,2-Dichlorobenzene
 Concen: 48.42 ug/ml
 RT: 10.327 min Scan# 646
 Delta R.T. 0.013 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29

Tgt Ion	Ratio	Lower	Upper
146	100		
148	64.8	44.0	84.0
113	13.3	0.0	33.6

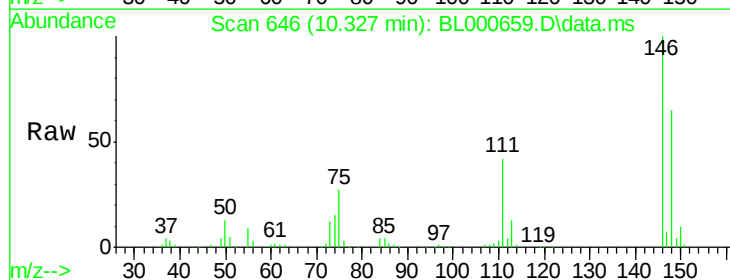

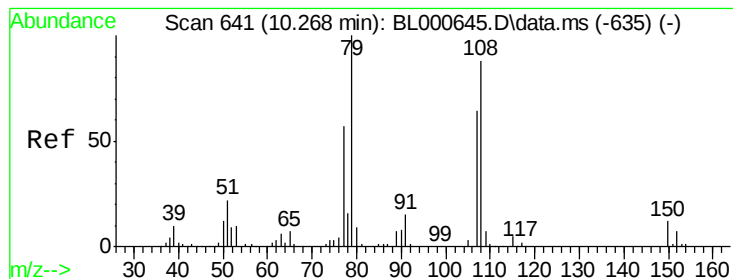

#15

Benzyl alcohol

Concen: 48.26 ug/ml

RT: 10.270 min Scan# 641

Delta R.T. 0.013 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29

Instrument :

BNA_L

ClientSampleId :

ICVBL072512





Tgt Ion: 108 Resp: 367826

Ion Ratio Lower Upper

108 100

79 112.0 94.5 134.5

77 63.8 43.7 83.7

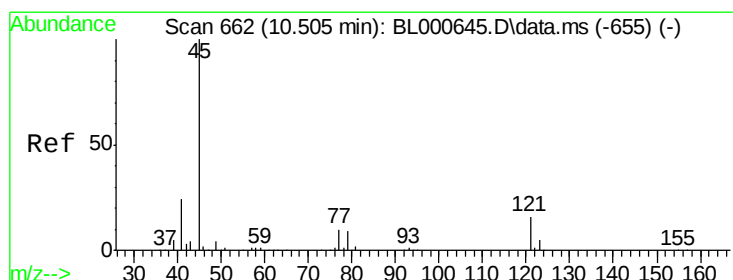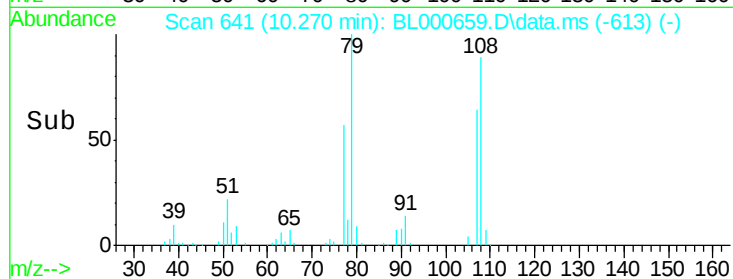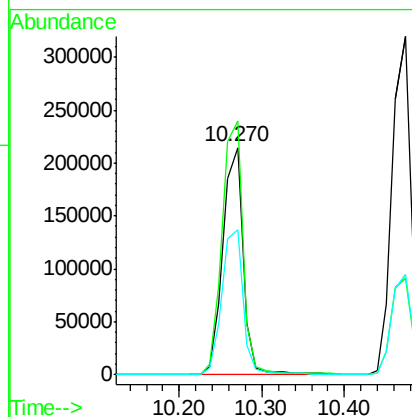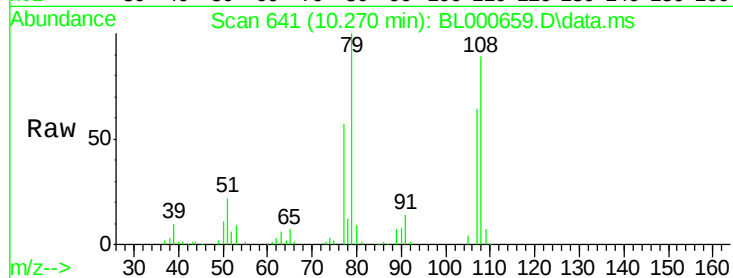

#16

2,2-oxybis(1-chloropropane)

Concen: 48.57 ug/ml

RT: 10.507 min Scan# 662

Delta R.T. 0.013 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29




Tgt Ion: 45 Resp: 1072343


Ion Ratio Lower Upper

45 100

77 9.6 0.0 30.0

79 8.7 0.0 28.9


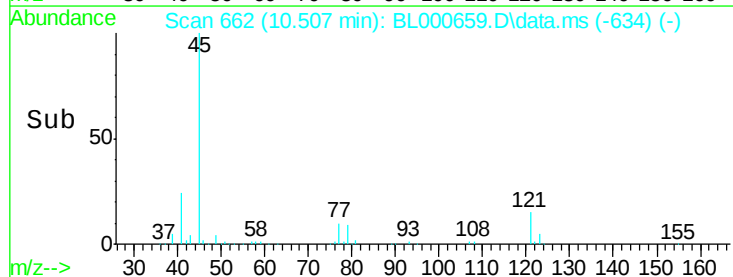
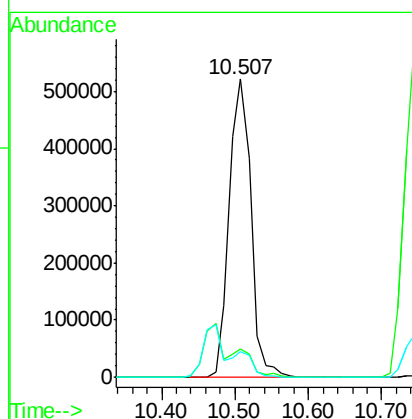
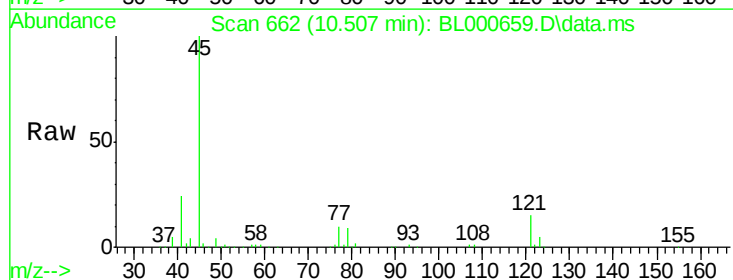




#17
2-Methylphenol
Concen: 46.61 ug/ml
RT: 10.474 min Scan# 65
Delta R.T. 0.024 min
Lab File: BL000659.D
Acq: 26 Jul 2012 12:29




Instrument :
BNA_L
ClientSampleId :
ICVBL072512


Tgt Ion:108 Resp: 509923
Ion Ratio Lower Upper
108 100
107 89.5 67.8 107.8



#18
Acetophenone
Concen: 90.04 ug/ml
RT: 10.745 min Scan# 683
Delta R.T. 0.014 min
Lab File: BL000659.D
Acq: 26 Jul 2012 12:29

Tgt Ion:105 Resp: 1153675
Ion Ratio Lower Upper
105 100
71 5.7 0.0 27.0
51 32.0 16.6 56.6

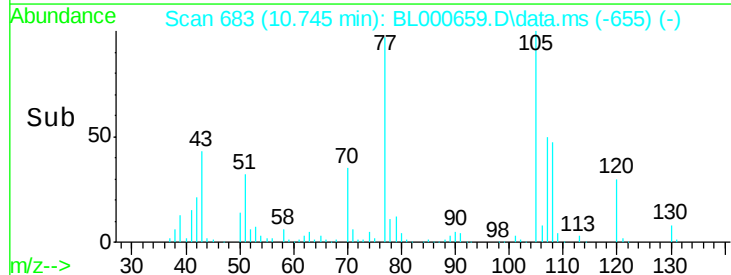



#19

Hexachloroethane

Concen: 46.63 ug/ml

RT: 10.937 min Scan# 700

Delta R.T. 0.002 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29

Instrument :

BNA_L

ClientSampleId :

ICVBL072512





Tgt Ion: 117 Resp: 214891

Ion Ratio Lower Upper

117 100

200 0.0 0.0 20.0

199 42.4 21.2 61.2

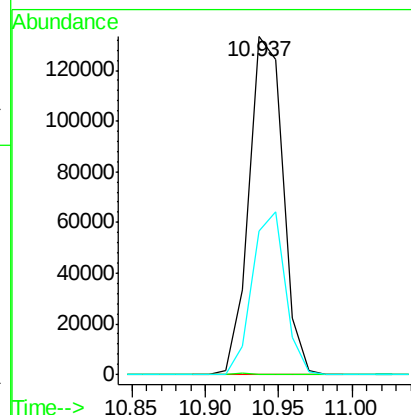

#20

N-Nitroso-di-n-propylamine

Concen: 44.71 ug/ml

RT: 10.745 min Scan# 683

Delta R.T. 0.002 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29




Tgt Ion: 70 Resp: 367950


Ion Ratio Lower Upper

70 100

42 59.2 32.8 72.8

130 22.4 3.0 43.0



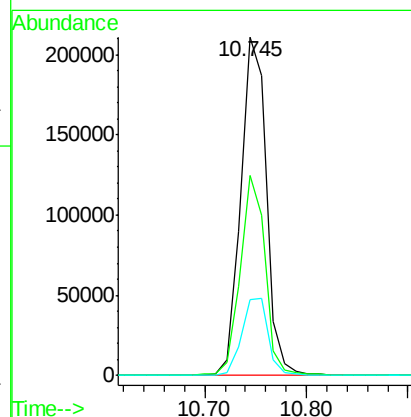



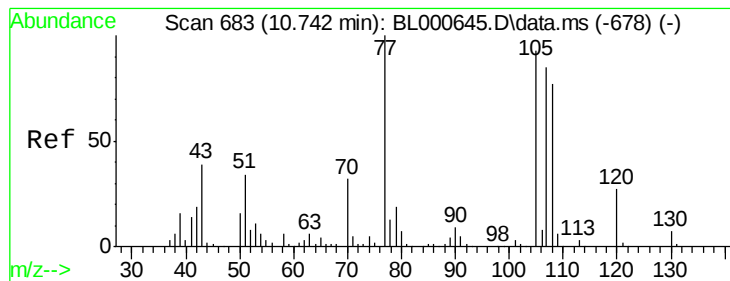

#21
 4-Methylphenol
 Concen: 45.67 ug/ml
 RT: 10.745 min Scan# 68
 Delta R.T. 0.013 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29




Instrument :
 BNA_L
 ClientSampleId :
 ICVBL072512


Tgt Ion: 108 Resp: 468008
 Ion Ratio Lower Upper
 108 100
 107 105.3 86.9 126.9

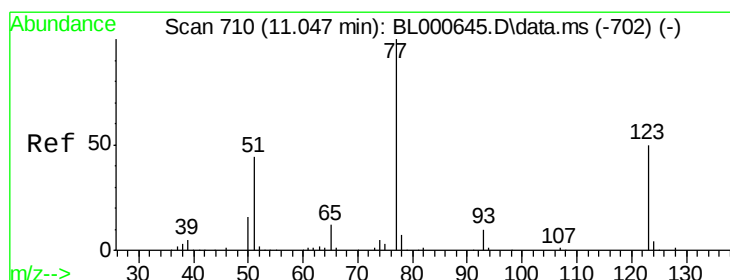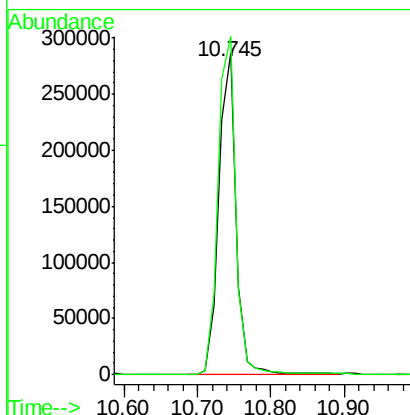

#24
 Nitrobenzene
 Concen: 46.48 ug/ml
 RT: 11.049 min Scan# 710
 Delta R.T. 0.002 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29

Tgt Ion: 77 Resp: 518040
 Ion Ratio Lower Upper
 77 100
 123 52.5 26.9 66.9
 65 12.1 0.0 32.1

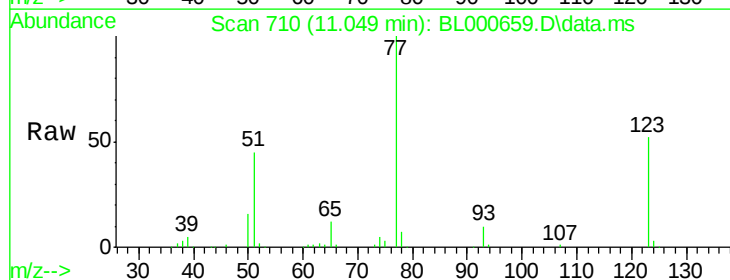

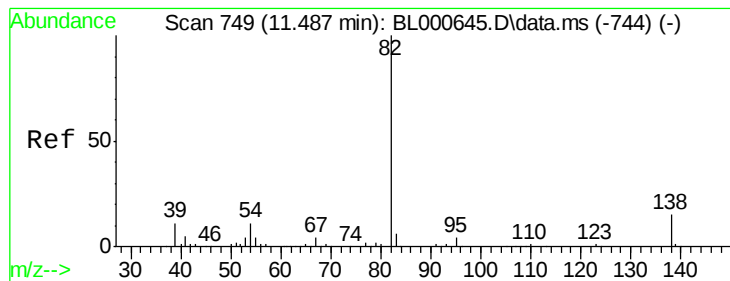

#25

Isophorone

Concen: 47.22 ug/ml

RT: 11.490 min Scan# 749

Delta R.T. 0.013 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29

Instrument :

BNA_L

ClientSampleId :





ICVBL072512

Tgt Ion: 82 Resp: 1013227

Ion Ratio Lower Upper

82 100

138 16.1 0.0 35.5

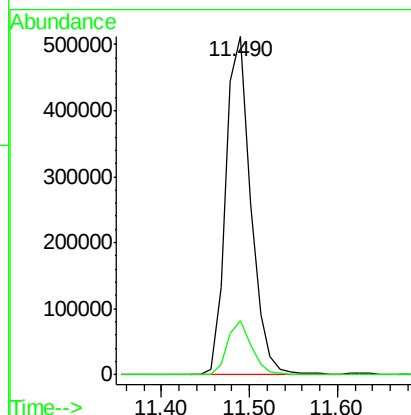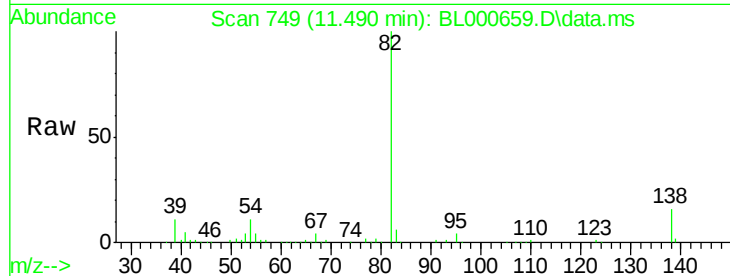

#26

2-Nitrophenol

Concen: 47.89 ug/ml

RT: 11.625 min Scan# 761

Delta R.T. 0.002 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29




Tgt Ion: 139 Resp: 270809


Ion Ratio Lower Upper

139 100

65 39.4 20.8 60.8

109 13.5 0.0 33.5


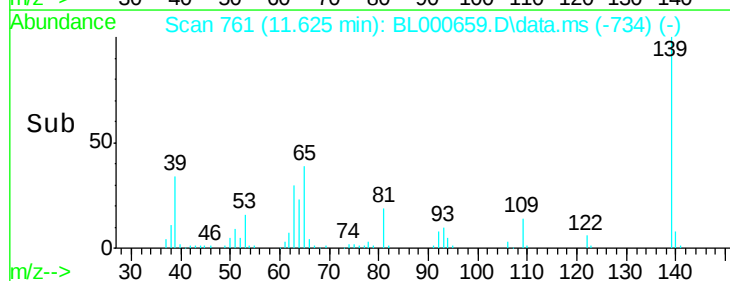
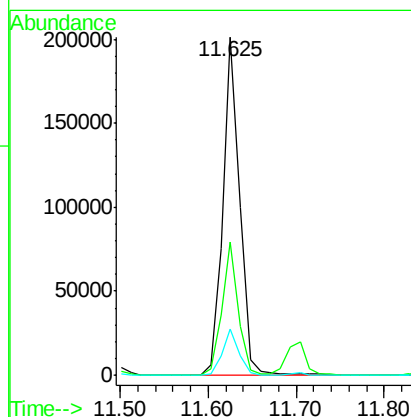



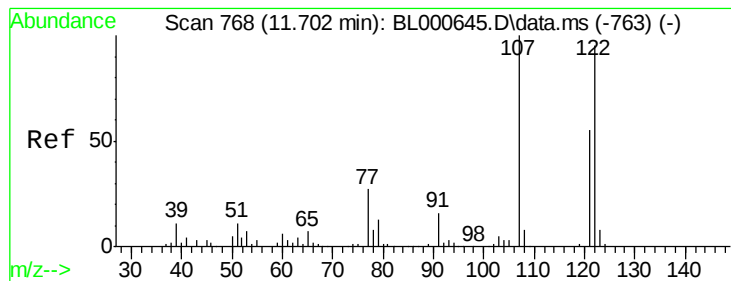

#27
 2,4-Dimethylphenol
 Concen: 48.14 ug/ml
 RT: 11.704 min Scan# 76
 Delta R.T. 0.013 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29




Instrument :
 BNA_L
 ClientSampleId :
 ICVBL072512


Tgt Ion:107 Resp: 412178
 Ion Ratio Lower Upper
 107 100
 121 55.2 33.2 73.2
 122 97.5 75.9 115.9

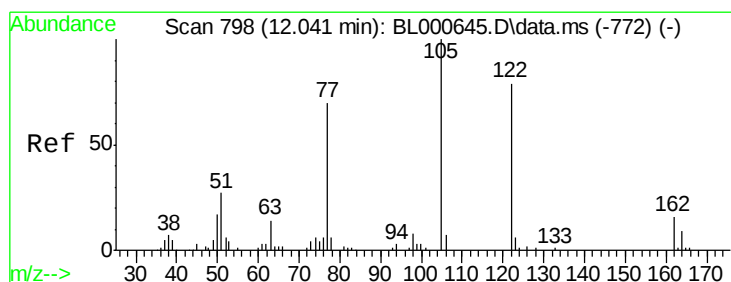

#28
 Benzoic Acid
 Concen: 90.71 ug/ml
 RT: 11.987 min Scan# 793
 Delta R.T. -0.009 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29

Tgt Ion:105 Resp: 601022
 Ion Ratio Lower Upper
 105 100
 77 73.8 52.0 92.0
 122 84.9 61.6 101.6



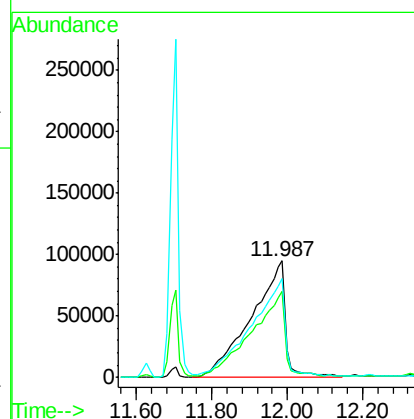
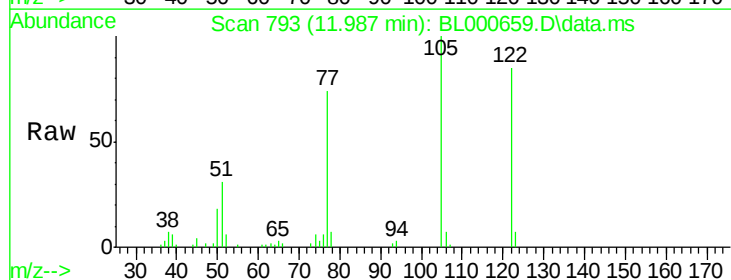




#29
 bis(2-Chloroethoxy)methane
 Concen: 48.25 ug/ml
 RT: 11.874 min Scan# 783
 Delta R.T. 0.013 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29




Instrument :
 BNA_L
 ClientSampleId :
 ICVBL072512


Tgt Ion: 93 Resp: 617704
 Ion Ratio Lower Upper
 93 100
 95 32.2 11.6 51.6
 123 11.0 0.0 30.8

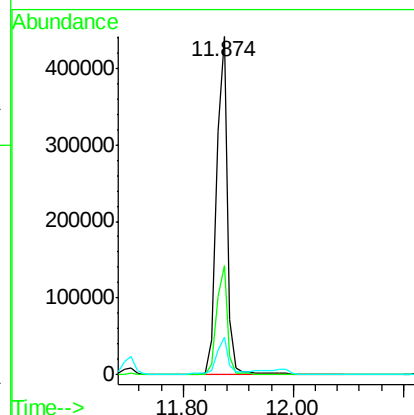

#30
 2,4-Dichlorophenol
 Concen: 48.57 ug/ml
 RT: 12.066 min Scan# 800
 Delta R.T. 0.013 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29

Tgt Ion: 162 Resp: 334482
 Ion Ratio Lower Upper
 162 100
 164 64.4 43.5 83.5
 98 36.4 19.5 59.5


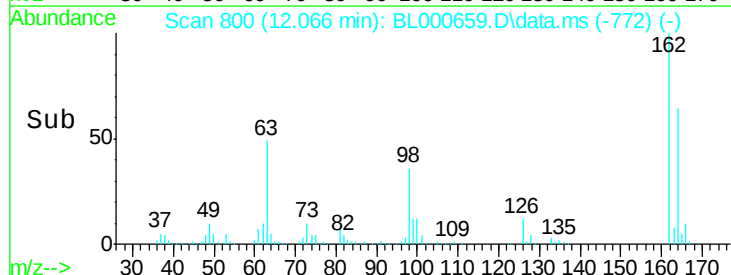






#32
1,2,4-Trichlorobenzene
Concen: 48.26 ug/ml
RT: 12.224 min Scan# 81
Delta R.T. 0.013 min
Lab File: BL000659.D
Acq: 26 Jul 2012 12:29




Instrument :
BNA_L
ClientSampleId :
ICVBL072512


Tgt Ion:180 Resp: 366049
Ion Ratio Lower Upper
180 100
182 96.5 75.6 115.6
145 27.5 8.3 48.3

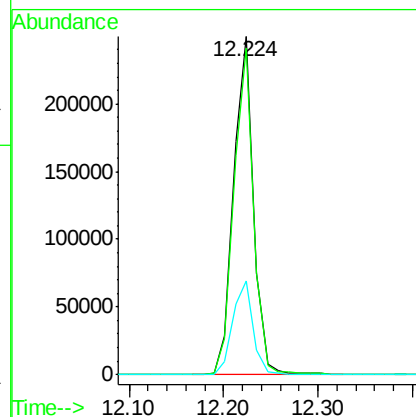

#33
Naphthalene
Concen: 48.07 ug/ml
RT: 12.359 min Scan# 826
Delta R.T. 0.002 min
Lab File: BL000659.D
Acq: 26 Jul 2012 12:29

Tgt Ion:128 Resp: 1170778
Ion Ratio Lower Upper
128 100
129 11.1 0.0 30.7
127 12.8 0.0 33.1



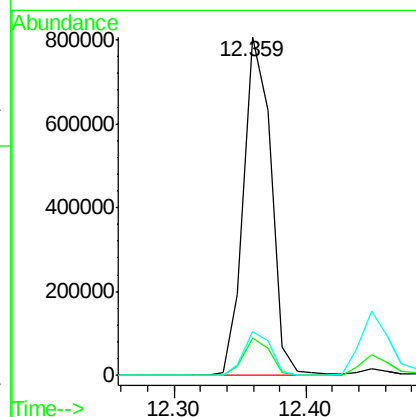





#34
4-Chloroaniline
Concen: 26.50 ug/ml
RT: 12.450 min Scan# 83
Delta R.T. 0.002 min
Lab File: BL000659.D
Acq: 26 Jul 2012 12:29




Instrument :
BNA_L
ClientSampleId :
ICVBL072512


Tgt Ion:127 Resp: 273583
Ion Ratio Lower Upper
127 100
129 31.3 12.1 52.1

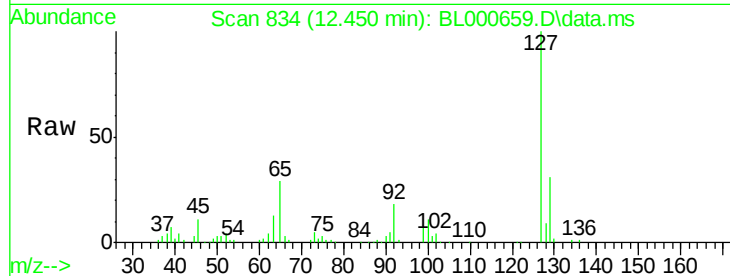

#35
Hexachlorobutadiene
Concen: 48.27 ug/ml
RT: 12.596 min Scan# 847
Delta R.T. 0.002 min
Lab File: BL000659.D
Acq: 26 Jul 2012 12:29

Tgt Ion:225 Resp: 156412
Ion Ratio Lower Upper
225 100
223 61.5 41.7 81.7
227 61.2 45.2 85.2









#37
4-Chloro-3-methylphenol
Concen: 49.84 ug/ml
RT: 13.330 min Scan# 91
Delta R.T. -0.009 min
Lab File: BL000659.D
Acq: 26 Jul 2012 12:29




Instrument :
BNA_L
ClientSampleId :
ICVBL072512


Tgt Ion:107 Resp: 320692
Ion Ratio Lower Upper
107 100
144 27.3 9.7 49.7
142 83.9 71.3 111.3



#38
2-Methylnaphthalene
Concen: 48.64 ug/ml
RT: 13.624 min Scan# 938
Delta R.T. 0.002 min
Lab File: BL000659.D
Acq: 26 Jul 2012 12:29

Tgt Ion:142 Resp: 659136
Ion Ratio Lower Upper
142 100
141 84.2 64.5 104.5


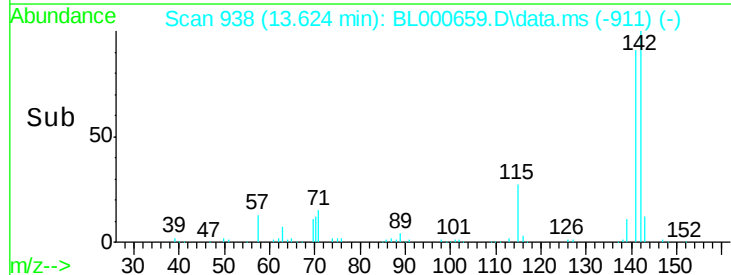




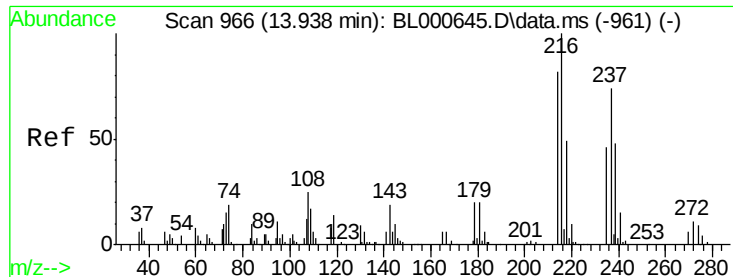

#40
Hexachlorocyclopentadiene
Concen: 40.09 ug/ml
RT: 13.940 min Scan# 96
Delta R.T. 0.013 min
Lab File: BL000659.D
Acq: 26 Jul 2012 12:29




Instrument :
BNA_L
ClientSampleId :
ICVBL072512


Tgt Ion:237 Resp: 125044
Ion Ratio Lower Upper
237 100
235 63.4 42.1 82.1
272 14.9 0.0 35.7

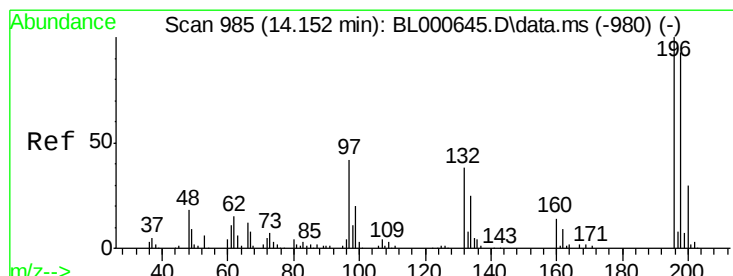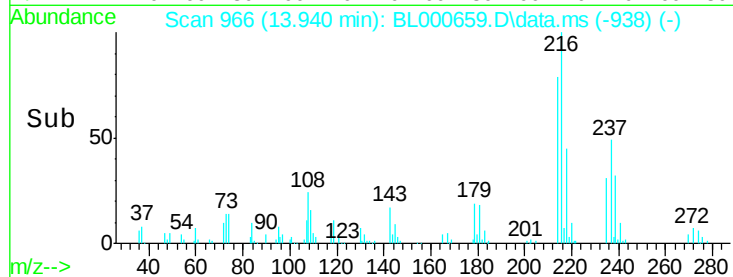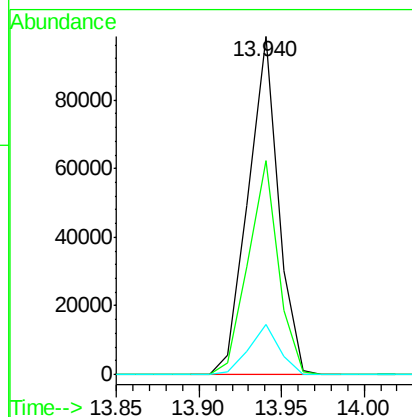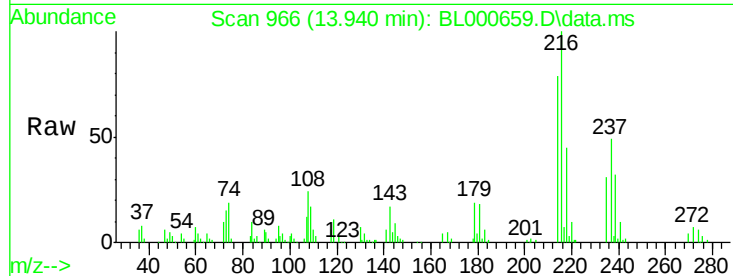

#41
2,4,6-Trichlorophenol
Concen: 46.77 ug/ml
RT: 14.155 min Scan# 985
Delta R.T. 0.013 min
Lab File: BL000659.D
Acq: 26 Jul 2012 12:29

Tgt Ion:196 Resp: 184917
Ion Ratio Lower Upper
196 100
198 97.3 73.1 113.1
200 31.6 9.7 49.7

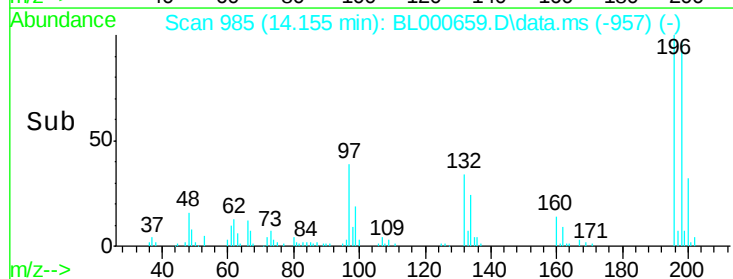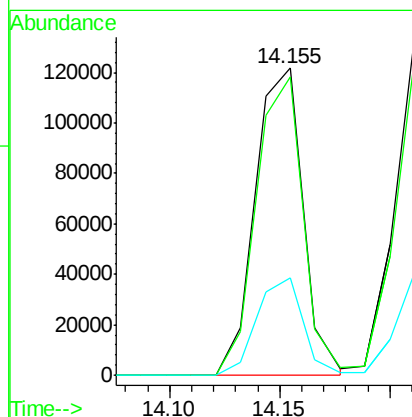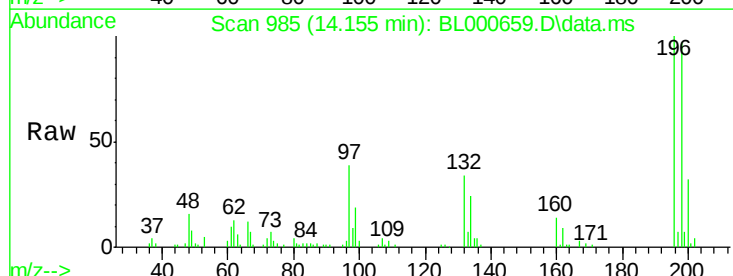

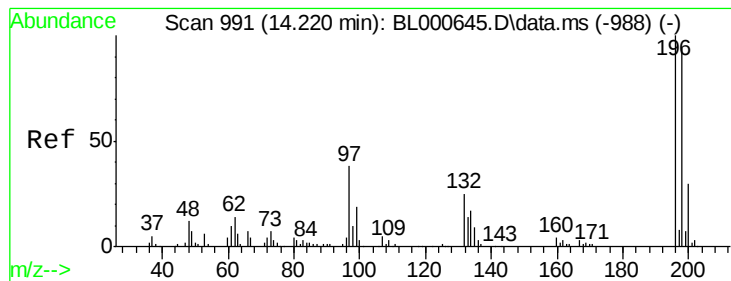

#42

2,4,5-Trichlorophenol

Concen: 47.51 ug/ml

RT: 14.211 min Scan# 991

Delta R.T. 0.002 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29

Instrument :

BNA_L

ClientSampleId :

ICVBL072512





Tgt Ion:196 Resp: 204887

Ion Ratio Lower Upper

196 100

198 93.6 74.5 114.5

200 30.4 10.8 50.8



#44

1,1-Biphenyl

Concen: 84.52 ug/ml

RT: 14.493 min Scan# 1015

Delta R.T. 0.002 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29




Tgt Ion:154 Resp: 1284380


Ion Ratio Lower Upper

154 100

153 40.7 19.9 59.9

76 30.0 3.3 43.3







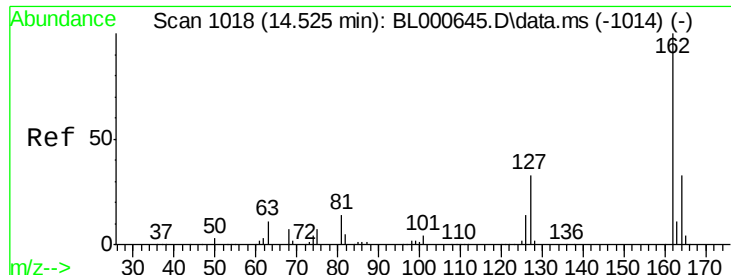

#45
 2-Chloronaphthalene
 Concen: 45.09 ug/ml
 RT: 14.527 min Scan# 1018
 Delta R.T. 0.002 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29




Instrument :
 BNA_L
 ClientSampleId :
 ICVBL072512


Tgt Ion	Ratio	Lower	Upper
162	100		
164	32.9	12.8	52.8
127	34.2	10.9	50.9

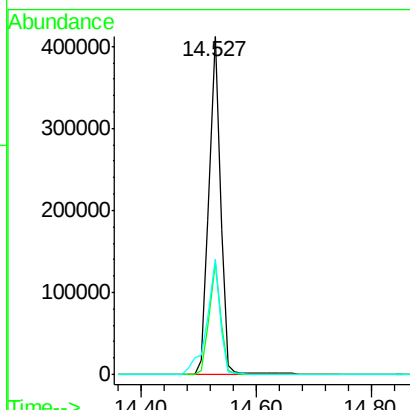

#46
 2-Nitroaniline
 Concen: 47.84 ug/ml
 RT: 14.719 min Scan# 1035
 Delta R.T. 0.013 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29

Tgt Ion	Ratio	Lower	Upper
65	100		
92	68.6	49.2	89.2
138	131.7	102.4	142.4









#47
 Acenaphthylene
 Concen: 45.74 ug/ml
 RT: 15.295 min Scan# 1086
 Delta R.T. 0.002 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29




Instrument :
 BNA_L
 ClientSampleId :
 ICVBL072512


Tgt Ion	Ratio	Lower	Upper
152	100		
151	20.0	0.0	39.9
153	13.3	0.0	32.6



#48
 Dimethylphthalate
 Concen: 46.43 ug/ml
 RT: 15.069 min Scan# 1066
 Delta R.T. 0.002 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29

Tgt Ion	Ratio	Lower	Upper
163	100		
194	5.6	0.0	25.9
164	9.8	0.0	29.6


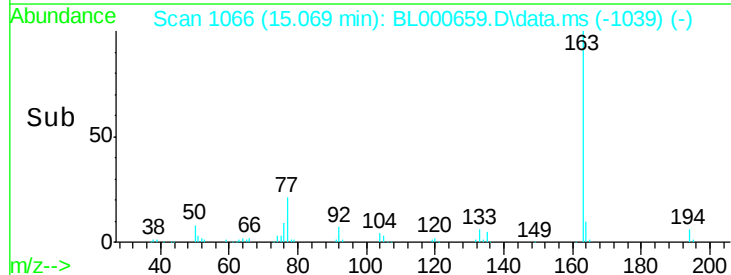






#49
2,6-Dinitrotoluene
Concen: 46.06 ug/ml
RT: 15.171 min Scan# 10
Delta R.T. 0.002 min
Lab File: BL000659.D
Acq: 26 Jul 2012 12:29




Instrument :
BNA_L
ClientSampleId :
ICVBL072512


Tgt Ion	Ratio	Lower	Upper
165	100		
89	35.7	19.2	59.2
121	15.5	0.0	36.2

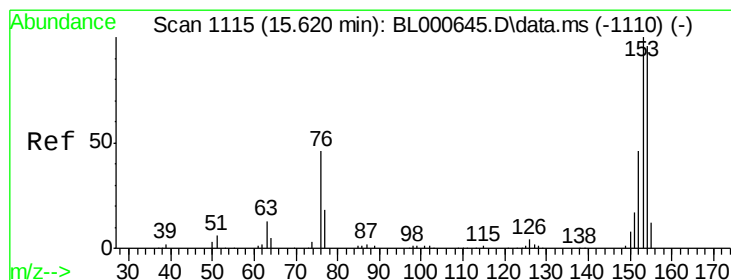

#50
Acenaphthene
Concen: 47.72 ug/ml
RT: 15.623 min Scan# 1115
Delta R.T. 0.002 min
Lab File: BL000659.D
Acq: 26 Jul 2012 12:29

Tgt Ion	Ratio	Lower	Upper
153	100		
152	46.0	25.1	65.1
154	96.5	75.9	115.9

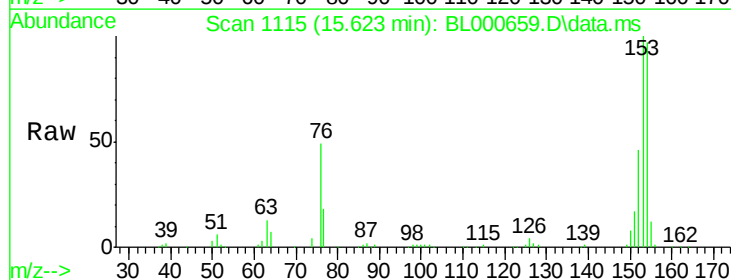



#51

3-Nitroaniline

Concen: 33.98 ug/ml

RT: 15.476 min Scan# 11

Delta R.T. 0.002 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29

Instrument :

BNA_L

ClientSampleId :

ICVBL072512





Tgt Ion:138 Resp: 105689

Ion Ratio Lower Upper

138 100

108 9.2 0.0 30.0

92 102.6 81.9 121.9

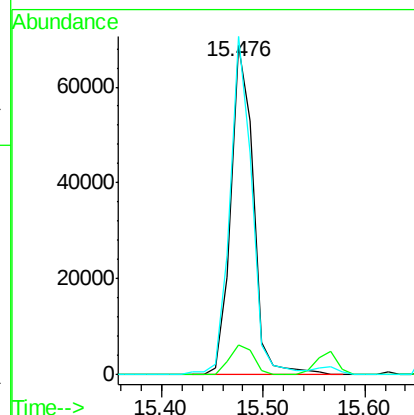

#52

2,4-Dinitrophenol

Concen: 41.14 ug/ml

RT: 15.668 min Scan# 1119

Delta R.T. 0.003 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29




Tgt Ion:184 Resp: 70163


Ion Ratio Lower Upper

184 100

63 44.0 11.7 51.7

154 28.1 6.0 46.0





#53

Dibenzenofuran

Concen: 47.80 ug/ml

RT: 15.950 min Scan# 1144

Delta R.T. 0.013 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29

Instrument :

BNA_L

ClientSampleId :





ICVBL072512

Tgt Ion:168 Resp: 674281

Ion Ratio Lower Upper

168 100

139 26.1 7.3 47.3



#54

2,4-Dinitrotoluene

Concen: 48.76 ug/ml

RT: 15.916 min Scan# 1141

Delta R.T. 0.002 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29




Tgt Ion:165 Resp: 174512


Ion Ratio Lower Upper

165 100

63 37.7 13.1 53.1

182 5.6 0.0 26.1









#55
4-Nitrophenol
Concen: 45.31 ug/ml
RT: 15.792 min Scan# 1131
Delta R.T. 0.002 min
Lab File: BL000659.D
Acq: 26 Jul 2012 12:29




Instrument :
BNA_L
ClientSampleId :
ICVBL072512


Tgt Ion	Ratio	Lower	Upper
139	100		
65	74.7	44.1	84.1
109	30.3	6.8	46.8

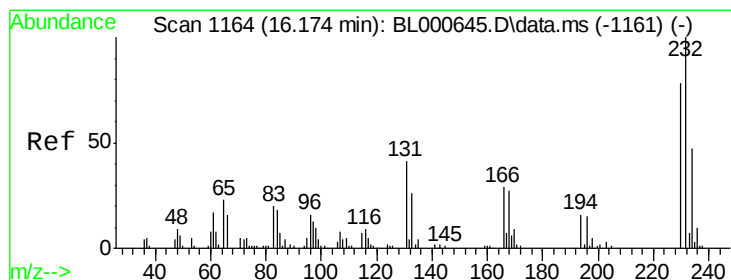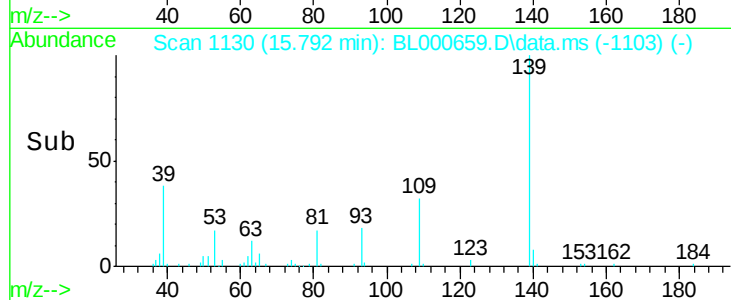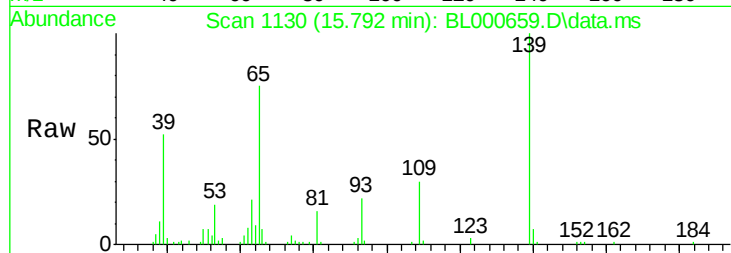

#56
2,3,4,6-Tetrachlorophenol
Concen: 47.72 ug/ml
RT: 16.176 min Scan# 1164
Delta R.T. 0.002 min
Lab File: BL000659.D
Acq: 26 Jul 2012 12:29

Tgt Ion	Ratio	Lower	Upper
232	100		
230	78.3	64.6	96.8
131	33.9	29.2	43.8
166	25.1	20.6	30.8

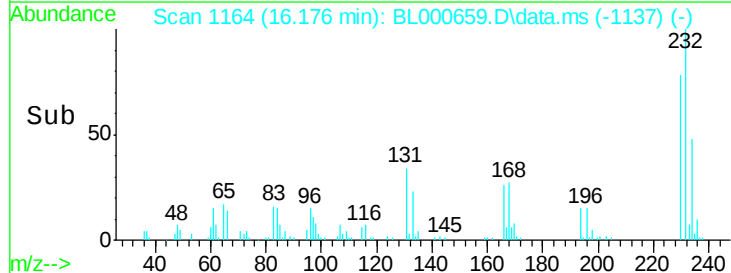



#57

Fluorene

Concen: 48.22 ug/ml

RT: 16.582 min Scan# 1200

Delta R.T. 0.002 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29

Instrument :

BNA_L

ClientSampleId :

ICVBL072512





Tgt Ion:166 Resp: 489975

Ion Ratio Lower Upper

166 100

165 92.2 72.3 112.3

167 13.5 0.0 33.1

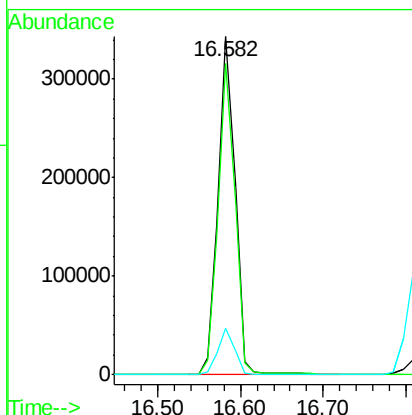

#58

4-Chlorophenyl-phenylether

Concen: 47.36 ug/ml

RT: 16.594 min Scan# 1201

Delta R.T. 0.014 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29




Tgt Ion:204 Resp: 219140


Ion Ratio Lower Upper

204 100

206 32.6 12.0 52.0

141 40.9 26.4 66.4



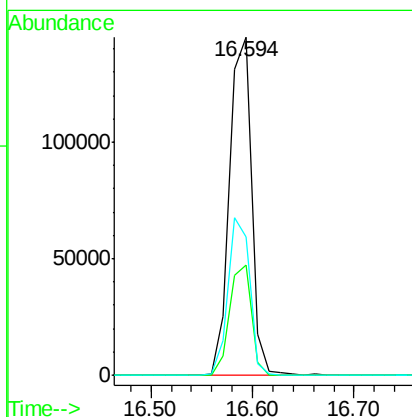





#59
 Diethylphthalate
 Concen: 47.44 ug/ml
 RT: 16.391 min Scan# 11
 Delta R.T. 0.002 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29




Instrument :
 BNA_L
 ClientSampleId :
 ICVBL072512


Tgt Ion	Ratio	Lower	Upper
149	100		
177	22.3	1.3	41.3
150	11.4	0.0	31.6

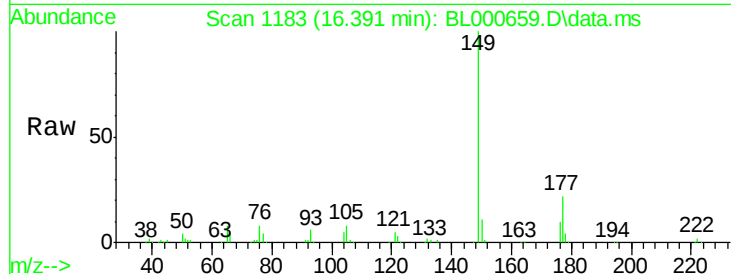

#60
 4-Nitroaniline
 Concen: 41.90 ug/ml
 RT: 16.616 min Scan# 1203
 Delta R.T. 0.002 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29

Tgt Ion	Ratio	Lower	Upper
138	100		
92	40.7	16.5	56.5
108	29.2	8.1	48.1



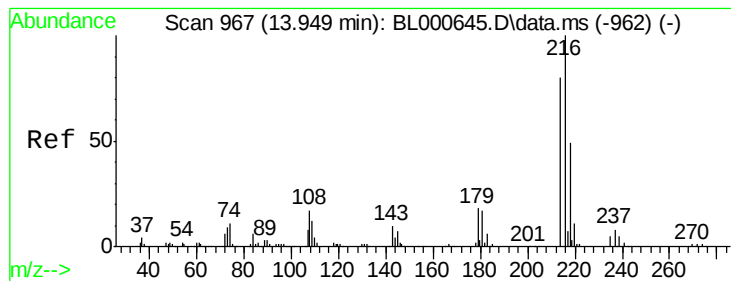

#63

1,2,4,5-Tetrachlorobenzene

Concen: 86.55 ug/ml

RT: 13.951 min Scan# 96

Delta R.T. 0.013 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29

Instrument :

BNA_L

ClientSampleId :

ICVBL072512

Tgt Ion:216 Resp: 506847





Ion Ratio Lower Upper

216 100

214 78.5 64.0 96.0

179 18.2 14.6 22.0

218 47.3 38.6 57.8

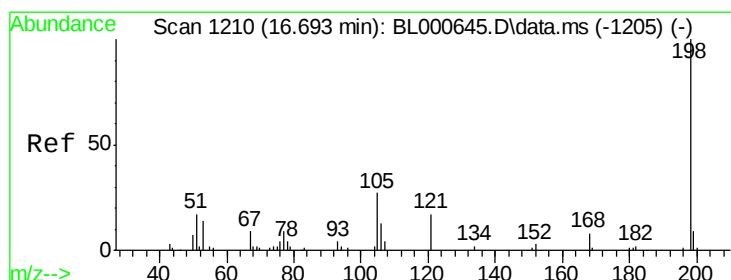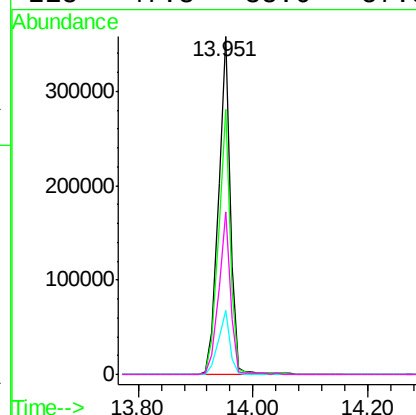

#64

4,6-Dinitro-2-methylphenol

Concen: 44.80 ug/ml




RT: 16.684 min Scan# 1209


Delta R.T. 0.002 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29

Tgt Ion:198 Resp: 91336



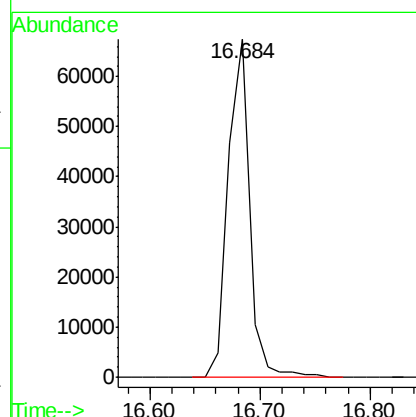
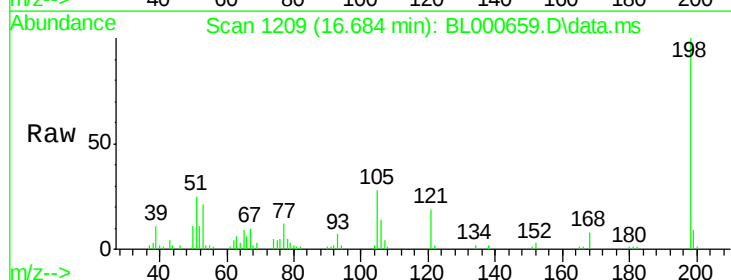




#65
 n-Nitrosodiphenylamine
 Concen: 47.65 ug/ml
 RT: 16.808 min Scan# 1221
 Delta R.T. 0.002 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29




Instrument :
 BNA_L
 ClientSampleId :
 ICVBL072512


Tgt Ion	Ratio	Lower	Upper
169	100		
168	62.6	40.9	80.9
167	32.8	12.5	52.5



#66
 1,2-Diphenylhydrazine
 Concen: 48.36 ug/ml
 RT: 16.887 min Scan# 1227
 Delta R.T. 0.013 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29

Tgt Ion	Ratio	Lower	Upper
77	100		
182	23.0	0.0	39.4
105	15.2	0.0	34.5









#67
 4-Bromophenyl-phenylether
 Concen: 47.69 ug/ml
 RT: 17.508 min Scan# 1282
 Delta R.T. 0.013 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29




Instrument :
 BNA_L
 ClientSampleId :
 ICVBL072512


Tgt Ion	Ratio	Lower	Upper
248	100		
250	99.0	78.2	118.2
141	44.9	34.7	74.7



#68
 Hexachlorobenzene
 Concen: 48.64 ug/ml
 RT: 17.633 min Scan# 1293
 Delta R.T. 0.013 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29

Tgt Ion	Ratio	Lower	Upper
284	100		
142	26.1	14.3	54.3
249	25.0	6.7	46.7


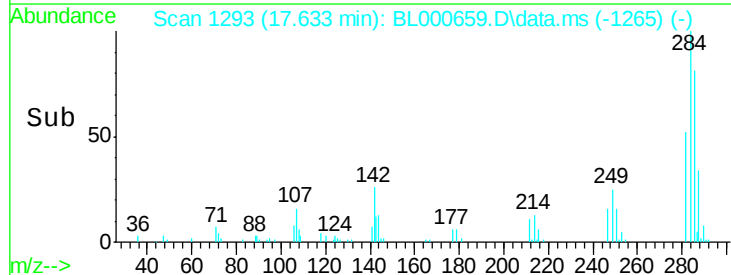






#70
 Pentachlorophenol
 Concen: 42.33 ug/ml
 RT: 17.994 min Scan# 1325
 Delta R.T. 0.014 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29




Instrument :
 BNA_L
 ClientSampleId :
 ICVBL072512


Tgt Ion:266 Resp: 61641
 Ion Ratio Lower Upper
 266 100
 264 63.1 44.5 84.5
 268 64.0 45.0 85.0

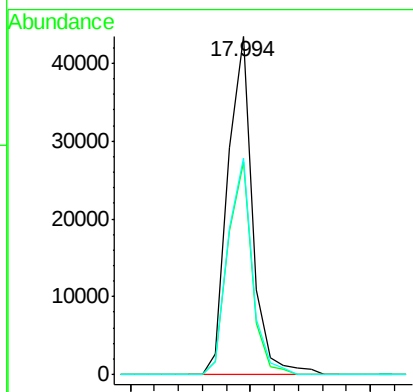

#73
 Phenanthrene
 Concen: 47.34 ug/ml
 RT: 18.367 min Scan# 1358
 Delta R.T. 0.002 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29

Tgt Ion:178 Resp: 554415
 Ion Ratio Lower Upper
 178 100
 179 15.7 0.0 35.3
 176 18.6 0.0 38.6









#74
 Anthracene
 Concen: 47.71 ug/ml
 RT: 18.457 min Scan# 1366
 Delta R.T. 0.002 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29




Instrument :
 BNA_L
 ClientSampleId :
 ICVBL072512


Tgt Ion:178 Resp: 575297
 Ion Ratio Lower Upper
 178 100
 179 15.6 0.0 34.9
 176 18.0 0.0 37.0



#75
 Carbazole
 Concen: 47.14 ug/ml
 RT: 18.728 min Scan# 1390
 Delta R.T. 0.002 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29

Tgt Ion:167 Resp: 487662
 Ion Ratio Lower Upper
 167 100
 167 100.0 80.0 120.0

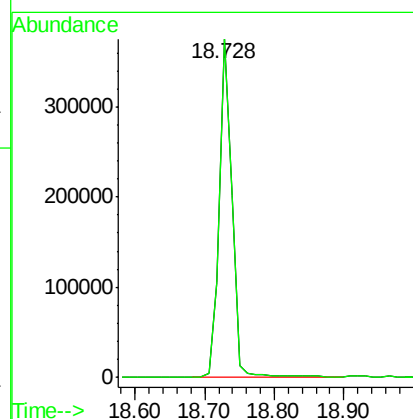

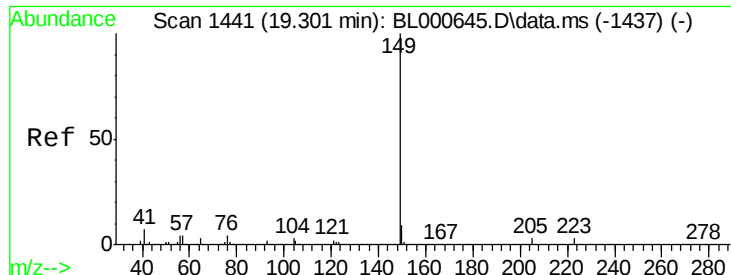

#76

Di-n-butylphthalate

Concen: 45.67 ug/ml

RT: 19.304 min Scan# 14

Delta R.T. 0.002 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29

Instrument :

BNA_L

ClientSampleId :

ICVBL072512





Tgt Ion:149 Resp: 626523

Ion Ratio Lower Upper

149 100

150 9.2 0.0 29.4

104 3.4 0.0 23.7

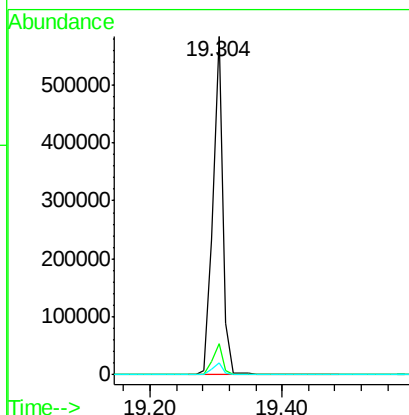

#77

Fluoranthene

Concen: 45.74 ug/ml

RT: 20.162 min Scan# 1517

Delta R.T. 0.002 min

Lab File: BL000659.D




Acq: 26 Jul 2012 12:29


Tgt Ion:202 Resp: 453318

Ion Ratio Lower Upper

202 100

101 31.5 5.5 45.5



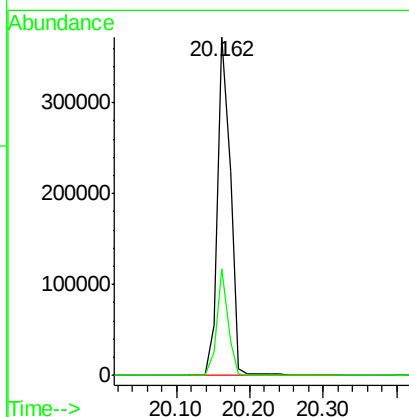





#79
 Pyrene
 Concen: 49.12 ug/ml
 RT: 20.456 min Scan# 151
 Delta R.T. 0.002 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29




Instrument :
 BNA_L
 ClientSampleId :
 ICVBL072512


Tgt Ion	Ratio	Lower	Upper
202	100		
101	38.0	11.7	51.7
100	31.0	6.0	46.0

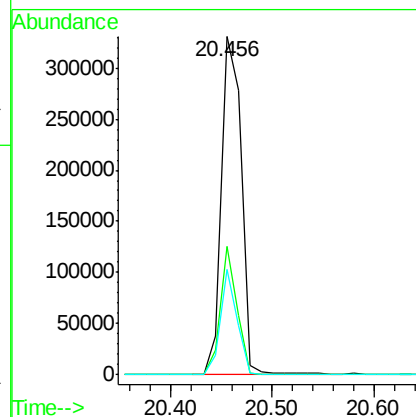

#81
 Butylbenzylphthalate
 Concen: 46.10 ug/ml
 RT: 21.235 min Scan# 1612
 Delta R.T. 0.013 min
 Lab File: BL000659.D
 Acq: 26 Jul 2012 12:29

Tgt Ion	Ratio	Lower	Upper
149	100		
91	56.5	51.8	91.8
206	20.9	0.0	36.6

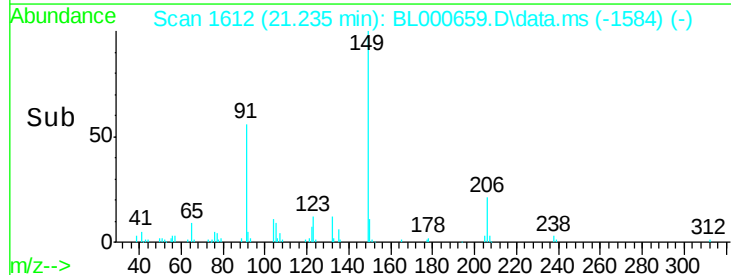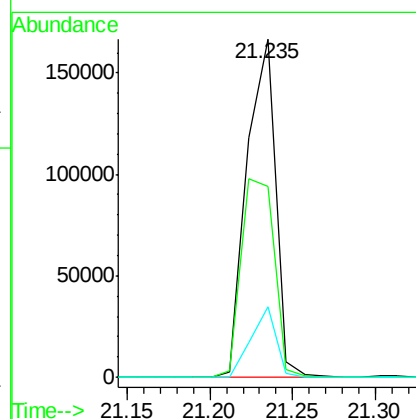



#83

Benzo[a]anthracene

Concen: 47.15 ug/ml

RT: 21.901 min Scan# 16

Delta R.T. 0.013 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29

Instrument :

BNA_L

ClientSampleId :

ICVBL072512





Tgt Ion:228 Resp: 328123

Ion Ratio Lower Upper

228 100

229 19.4 0.0 39.4

226 24.5 5.2 45.2

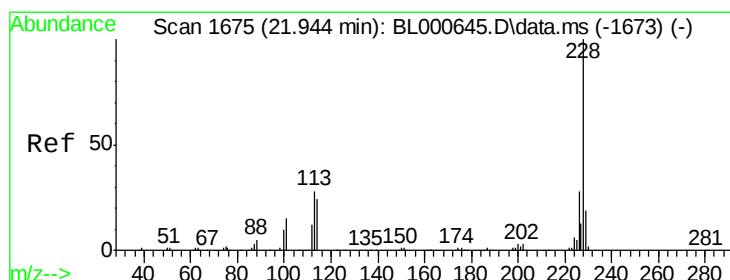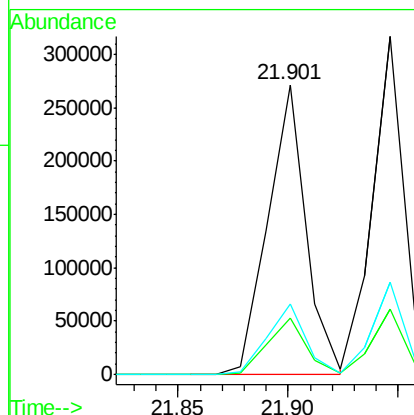

#84

Chrysene

Concen: 49.49 ug/ml

RT: 21.946 min Scan# 1675

Delta R.T. 0.002 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29




Tgt Ion:228 Resp: 326271


Ion Ratio Lower Upper

228 100

226 27.4 6.9 46.9

229 19.2 0.0 39.1



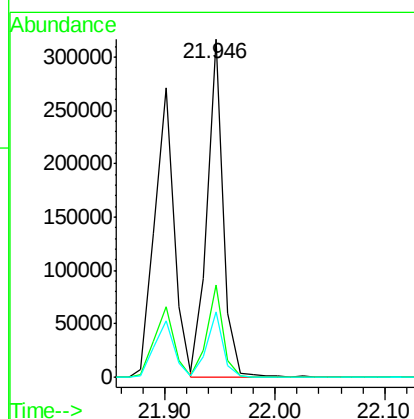





#85
bis(2-Ethylhexyl)phthalate
Concen: 44.45 ug/ml
RT: 21.878 min Scan# 1669
Delta R.T. 0.002 min
Lab File: BL000659.D
Acq: 26 Jul 2012 12:29




Instrument :
BNA_L
ClientSampleId :
ICVBL072512


Tgt Ion	Ratio	Resp	Lower	Upper
149	100	282847		
167	32.1	9.1	49.1	
279	6.1	0.0	24.0	

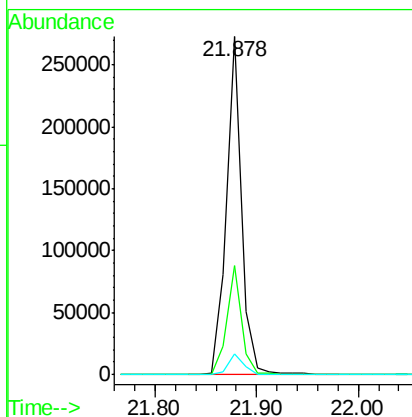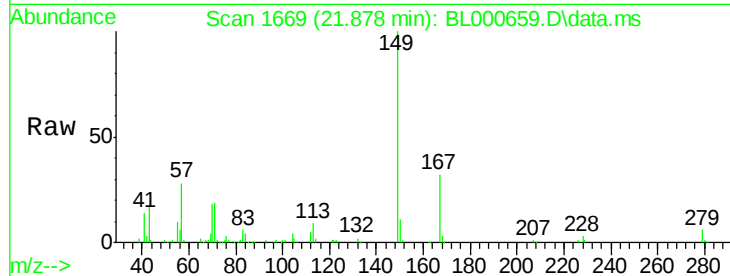

#87
Di-n-octylphthalate
Concen: 43.70 ug/ml
RT: 22.691 min Scan# 1741
Delta R.T. 0.002 min
Lab File: BL000659.D
Acq: 26 Jul 2012 12:29

Tgt Ion	Ratio	Resp	Lower	Upper
149	100	440599		
150	9.6	0.0	29.4	


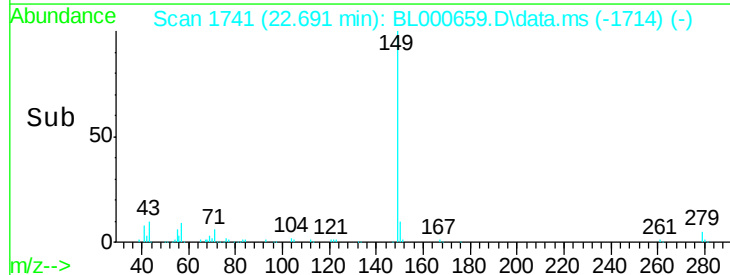
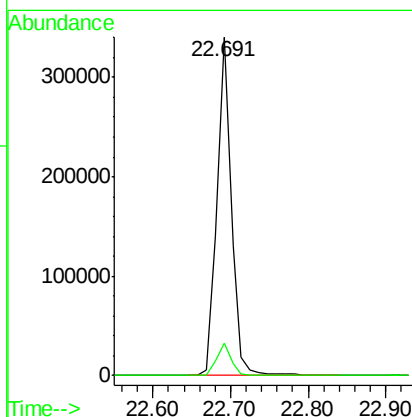





#88
Benzo[b]fluoranthene
Concen: 46.29 ug/ml
RT: 23.391 min Scan# 1803
Delta R.T. 0.013 min
Lab File: BL000659.D
Acq: 26 Jul 2012 12:29




Instrument :
BNA_L
ClientSampleId :
ICVBL072512


Tgt Ion:	252	Resp:	292501
Ion Ratio	Lower	Upper	
252	100		
253	21.5	1.5	41.5
125	25.0	1.4	41.4

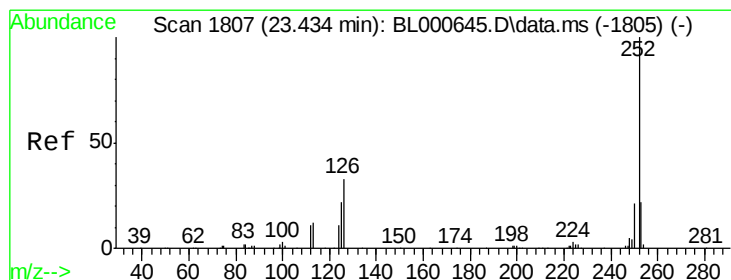

#89
Benzo[k]fluoranthene
Concen: 47.15 ug/ml
RT: 23.437 min Scan# 1807
Delta R.T. 0.013 min
Lab File: BL000659.D
Acq: 26 Jul 2012 12:29

Tgt Ion:	252	Resp:	274885
Ion Ratio	Lower	Upper	
252	100		
253	22.9	2.6	42.6
125	24.4	7.4	47.4

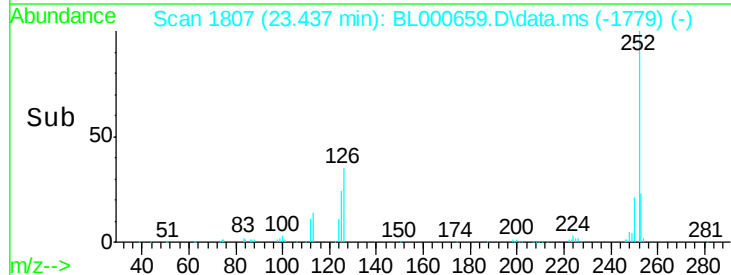



#90

Benzo[a]pyrene

Concen: 45.57 ug/ml

RT: 23.956 min Scan# 18

Delta R.T. 0.013 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29

Instrument :

BNA_L

ClientSampleId :

ICVBL072512





Tgt Ion:252 Resp: 264390

Ion Ratio Lower Upper

252 100

253 21.5 1.8 41.8

125 25.1 8.0 48.0



#91

Indeno[1,2,3-cd]pyrene

Concen: 47.70 ug/ml

RT: 26.361 min Scan# 2066

Delta R.T. 0.024 min

Lab File: BL000659.D




Acq: 26 Jul 2012 12:29


Tgt Ion:276 Resp: 272562

Ion Ratio Lower Upper

276 100

138 56.4 37.7 77.7

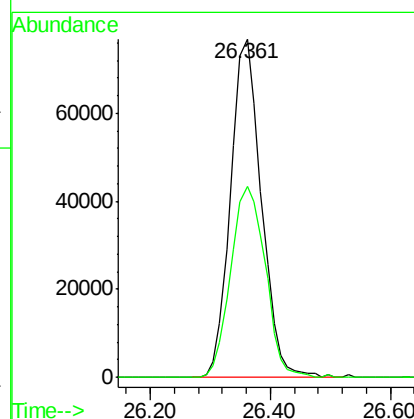

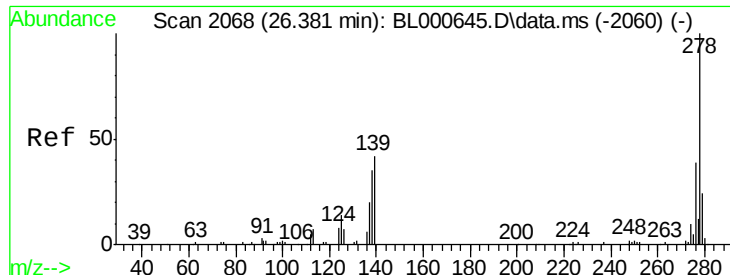

#92

Dibenz[a,h]anthracene

Concen: 46.54 ug/ml

RT: 26.384 min Scan# 20

Delta R.T. 0.014 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29

Instrument :

BNA_L

ClientSampleId :

ICVBL072512





Tgt Ion:278 Resp: 222379

Ion Ratio Lower Upper

278 100

139 42.9 18.8 58.8

279 24.7 4.5 44.5

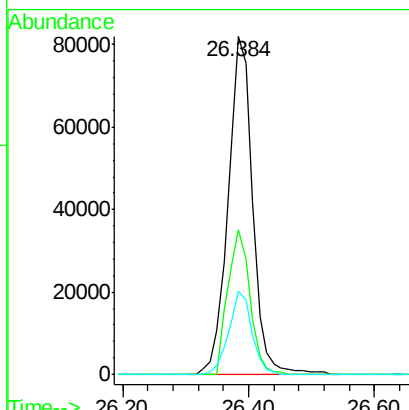

#93

Benzo[g,h,i]perylene

Concen: 47.53 ug/ml

RT: 27.073 min Scan# 2129

Delta R.T. 0.013 min

Lab File: BL000659.D

Acq: 26 Jul 2012 12:29




Tgt Ion:276 Resp: 236465

Ion Ratio Lower Upper

276 100

138 52.6 36.8 76.8

277 23.3 4.5 44.5

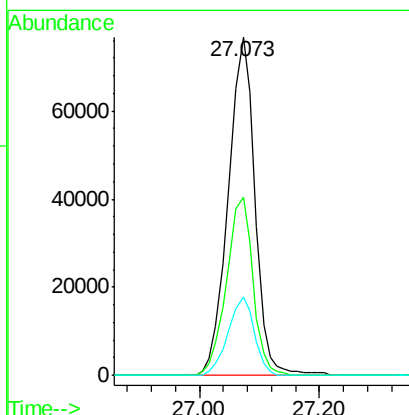

Data Path : S:\HPCHEM1\BNA_L\data\BL072612\
 Data File : BL000659.D
 Acq On : 26 Jul 2012 12:29
 Operator : HLM
 Sample : SST050ICV
 Misc : SST050ICV HLM
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_L
 ClientSampleId :
 ICVBL072512

Quant Time: Sep 06 06:45:36 2012
 Quant Method : H:\VOL1\GCMSDATA\L\METHODS\BL072512.M
 Quant Title : SW-846 Method 8270
 QLast Update : Thu Jul 26 11:02:15 2012
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	10.022	152	454450	40.00	ug/ml	0.01
22) Naphthalene-d8	12.325	136	1412639	40.00	ug/ml	0.01
39) Acenaphthene-d10	15.566	164	559876	40.00	ug/ml	0.01
62) Phenanthrene-d10	18.333	188	692205	40.00	ug/ml	0.01
78) Chrysene-d12	21.912	240	384611	40.00	ug/ml	0.00
86) Perylene-d12	24.058	264	299416	40.00	ug/ml	0.01

System Monitoring Compounds

5) 2-Fluorophenol	0.000	112	0	0.00	ug/ml	
Spiked Amount	200.000	Range	20 - 110	Recovery	=	0.00%#
9) Phenol-d5	0.000	99	0	0.00	ug/ml	
Spiked Amount	200.000	Range	10 - 115	Recovery	=	0.00%#
23) Nitrobenzene-d5	10.937	82	41871	3.90	ug/ml	-0.07
Spiked Amount	100.000	Range	40 - 110	Recovery	=	3.90%#
43) 2-Fluorobiphenyl	0.000	172	0	0.00	ug/ml	
Spiked Amount	100.000	Range	50 - 110	Recovery	=	0.00%#
61) 2,4,6-Tribromophenol	0.000	330	0	0.00	ug/ml	
Spiked Amount	200.000	Range	40 - 125	Recovery	=	0.00%#
80) Terphenyl-d14	0.000	244	0	0.00	ug/ml	
Spiked Amount	100.000	Range	50 - 135	Recovery	=	0.00%#

Target Compounds

						Qvalue
3) N-Nitrosodimethylamine	3.450	74	707424	48.43	ug/ml	98
4) Pyridine	3.540	79	1063489	47.69	ug/ml	100
6) Benzaldehyde	9.220	77	646649	197.22	ug/ml	98
7) Aniline	9.412	93	729654	34.31	ug/ml	99
8) bis(2-Chloroethyl)ether	9.536	93	679894	47.69	ug/ml	97
10) Phenol	9.378	94	920289	48.35	ug/ml	96
11) 2-Chlorophenol	9.638	128	561066	47.70	ug/ml	99
12) 1,3-Dichlorobenzene	9.920	146	568161	47.73	ug/ml	99
13) 1,4-Dichlorobenzene	10.056	146	569288	47.84	ug/ml	99
14) 1,2-Dichlorobenzene	10.327	146	527010	48.42	ug/ml	99
15) Benzyl alcohol	10.270	108	367826	48.26	ug/ml	98
16) 2,2-oxybis(1-chloropro...	10.507	45	1072343	48.57	ug/ml	99
17) 2-Methylphenol	10.474	108	509923	46.61	ug/ml	98
18) Acetophenone	10.745	105	1153675	90.04	ug/ml	93
19) Hexachloroethane	10.937	117	214891	46.63	ug/ml	98
20) N-Nitroso-di-n-propyla...	10.745	70	367950	44.71	ug/ml	93
21) 4-Methylphenol	10.745	108	468008	45.67	ug/ml	98
24) Nitrobenzene	11.049	77	518040	46.48	ug/ml	93
25) Isophorone	11.490	82	1013227	47.22	ug/ml	99
26) 2-Nitrophenol	11.625	139	270809	47.89	ug/ml	98
27) 2,4-Dimethylphenol	11.704	107	412178	48.14	ug/ml	98
28) Benzoic Acid	11.987	105	601022	90.71	ug/ml	97
29) bis(2-Chloroethoxy)met...	11.874	93	617704	48.25	ug/ml	99
30) 2,4-Dichlorophenol	12.066	162	334482	48.57	ug/ml	97
32) 1,2,4-Trichlorobenzene	12.224	180	366049	48.26	ug/ml	99
33) Naphthalene	12.359	128	1170778	48.07	ug/ml	99
34) 4-Chloroaniline	12.450	127	273583	26.50	ug/ml	99

Data Path : S:\HPCHEM1\BNA_L\data\BL072612\
 Data File : BL000659.D
 Acq On : 26 Jul 2012 12:29
 Operator : HLM
 Sample : SSTD050ICV
 Misc : SSTD050ICV HLM
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_L
 ClientSampleId :
 ICVBL072512

Quant Time: Sep 06 06:45:36 2012
 Quant Method : H:\VOL1\GCMSDATA\L\METHODS\BL072512.M
 Quant Title : SW-846 Method 8270
 QLast Update : Thu Jul 26 11:02:15 2012
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) Hexachlorobutadiene	12.596	225	156412	48.27	ug/ml	97
37) 4-Chloro-3-methylphenol	13.330	107	320692	49.84	ug/ml	93
38) 2-Methylnaphthalene	13.624	142	659136	48.64	ug/ml	100
40) Hexachlorocyclopentadiene	13.940	237	125044	40.09	ug/ml	98
41) 2,4,6-Trichlorophenol	14.155	196	184917	46.77	ug/ml	96
42) 2,4,5-Trichlorophenol	14.211	196	204887	47.51	ug/ml	99
44) 1,1-Biphenyl	14.493	154	1284380	84.52	ug/ml	94
45) 2-Chloronaphthalene	14.527	162	559779	45.09	ug/ml	97
46) 2-Nitroaniline	14.719	65	182153	47.84	ug/ml	94
47) Acenaphthylene	15.295	152	818620	45.74	ug/ml	99
48) Dimethylphthalate	15.069	163	570235	46.43	ug/ml	99
49) 2,6-Dinitrotoluene	15.171	165	149081	46.06	ug/ml	96
50) Acenaphthene	15.623	153	506668	47.72	ug/ml	99
51) 3-Nitroaniline	15.476	138	105689	33.98	ug/ml	99
52) 2,4-Dinitrophenol	15.668	184	70163	41.14	ug/ml	86
53) Dibenzofuran	15.950	168	674281	47.80	ug/ml	98
54) 2,4-Dinitrotoluene	15.916	165	174512	48.76	ug/ml	93
55) 4-Nitrophenol	15.792	139	112560	45.31	ug/ml	89
56) 2,3,4,6-Tetrachlorophenol	16.176	232	124631	47.72	ug/ml	97
57) Fluorene	16.582	166	489975	48.22	ug/ml	100
58) 4-Chlorophenyl-phenyle...	16.594	204	219140	47.36	ug/ml	95
59) Diethylphthalate	16.391	149	483312	47.44	ug/ml	98
60) 4-Nitroaniline	16.616	138	98188	41.90	ug/ml	95
63) 1,2,4,5-Tetrachloroben...	13.951	216	506847	86.55	ug/ml	99
64) 4,6-Dinitro-2-methylph...	16.684	198	91336	44.80	ug/ml	100
65) n-Nitrosodiphenylamine	16.808	169	417941	47.65	ug/ml	98
66) 1,2-Diphenylhydrazine	16.887	77	640978	48.36	ug/ml	95
67) 4-Bromophenyl-phenylether	17.508	248	121636	47.69	ug/ml	95
68) Hexachlorobenzene	17.633	284	130547	48.64	ug/ml	90
70) Pentachlorophenol	17.994	266	61641	42.33	ug/ml	98
73) Phenanthrene	18.367	178	554415	47.34	ug/ml	100
74) Anthracene	18.457	178	575297	47.71	ug/ml	98
75) Carbazole	18.728	167	487662	47.14	ug/ml	100
76) Di-n-butylphthalate	19.304	149	626523	45.67	ug/ml	99
77) Fluoranthene	20.162	202	453318	45.74	ug/ml	88
79) Pyrene	20.456	202	451574	49.12	ug/ml	89
81) Butylbenzylphthalate	21.235	149	200921	46.10	ug/ml	83
83) Benzo[a]anthracene	21.901	228	328123	47.15	ug/ml	99
84) Chrysene	21.946	228	326271	49.49	ug/ml	99
85) bis(2-Ethylhexyl)phtha...	21.878	149	282847	44.45	ug/ml	94
87) Di-n-octylphthalate	22.691	149	440599	43.70	ug/ml	100
88) Benzo[b]fluoranthene	23.391	252	292501	46.29	ug/ml	96
89) Benzo[k]fluoranthene	23.437	252	274885	47.15	ug/ml	97
90) Benzo[a]pyrene	23.956	252	264390	45.57	ug/ml	97
91) Indeno[1,2,3-cd]pyrene	26.361	276	272562	47.70	ug/ml	98
92) Dibenz[a,h]anthracene	26.384	278	222379	46.54	ug/ml	96
93) Benzo[g,h,i]perylene	27.073	276	236465	47.53	ug/ml	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed