


Data Path : S:\HPCHEM1\BNA_L\data\BL072612\
 Data File : BL000656.D
 Acq On : 26 Jul 2012 10:55
 Operator : HLM
 Sample : DFTPP050
 Misc : DFTPP050 HLM
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_L
 ClientSampleId :
 DFTPP050

Integration File: rteint.p

Method : S:\HPCHEM1\BNA_L\method\BL072512.M
 Title : SW-846 Method 8270
 Last Update : Thu Jul 26 11:02:15 2012

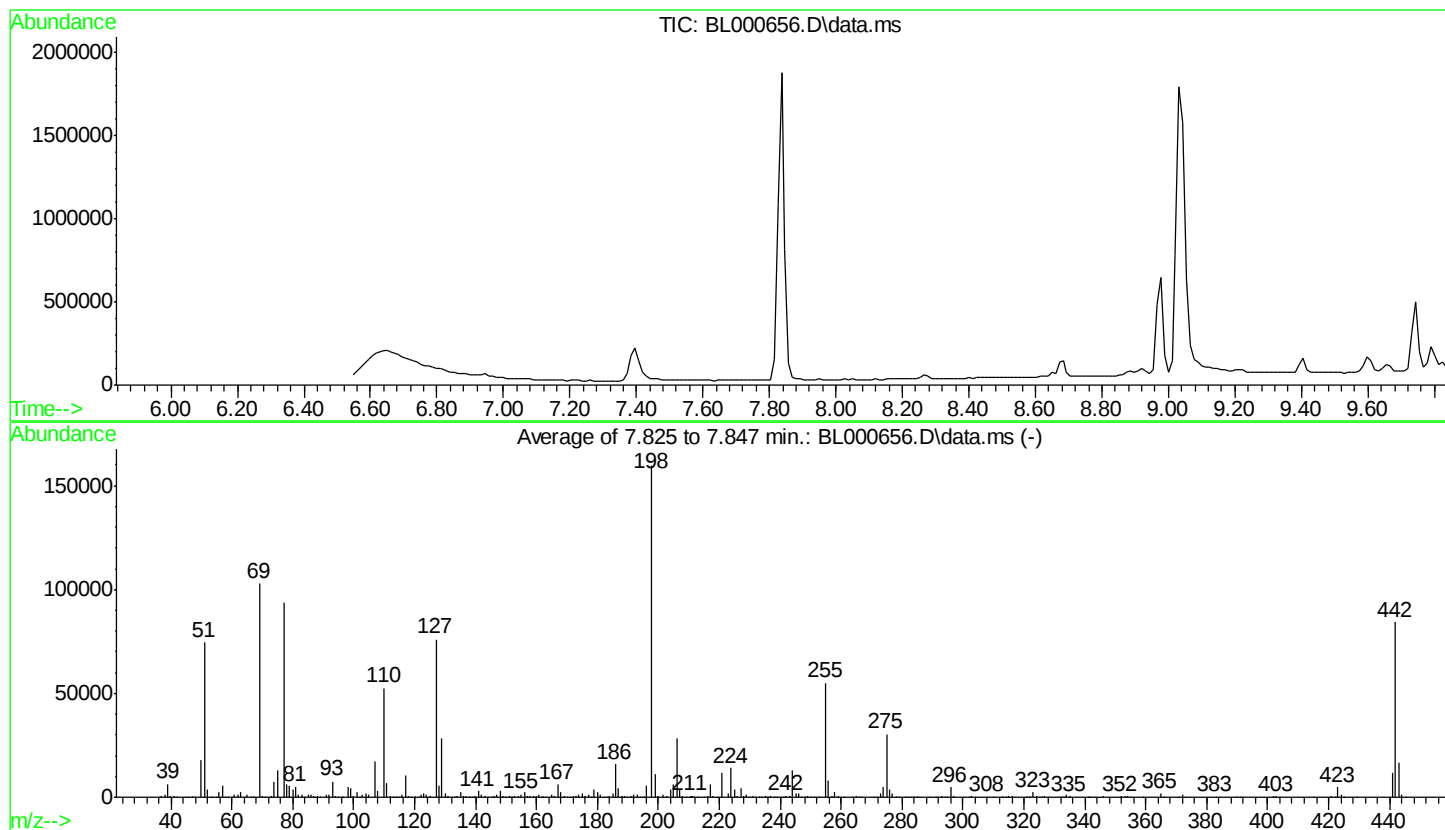

AutoFind: Scans 114, 115, 116; Background Corrected with Scan 109

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	46.6	74358	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	64.4	102791	PASS
70	69	0.00	2	0.4	406	PASS
127	198	40	60	47.5	75893	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	159634	PASS
199	198	5	9	6.8	10826	PASS
275	198	10	30	19.1	30525	PASS
365	198	1	100	1.2	1853	PASS
441	443	0.01	100	72.3	11929	PASS
442	198	40	100	52.8	84237	PASS
443	442	17	23	19.6	16491	PASS