

DFTPP

Data File : H:\VOL1\GCMSDATA\L\110621\BL000311.D

Vial: 1

Acq On : 21 Jun 2011 14:08

Operator: HLM/JCSA

Sample : DFTPP050

Inst : BNA L


Misc : DFTPP050 HLM

Multiplr: 1.00

MS Integration Params: rteint.p

Method : H:\VOL1\GCMSDATA\L\METHODS\DFTPP.M (RTE Integrator)

Title :

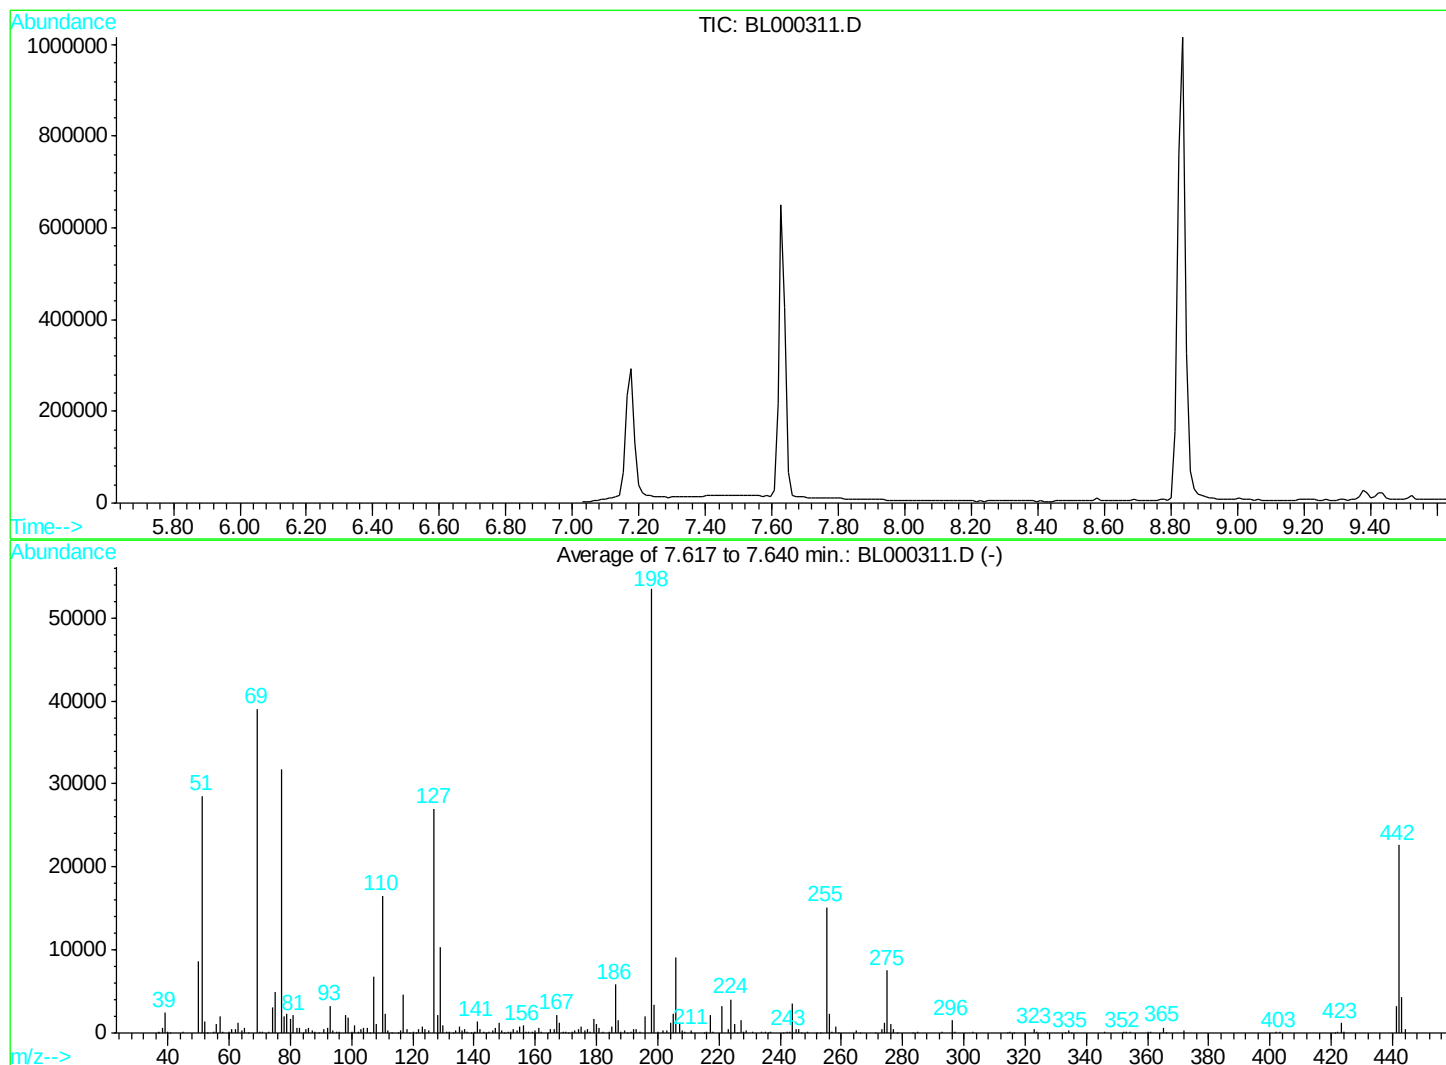



AutoFind: Scans 53, 54, 55; Background Corrected with Scan 49

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	53.4	28571	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	73.1	39076	PASS
70	69	0.00	2	0.3	134	PASS
127	198	40	60	50.5	26995	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	53461	PASS
199	198	5	9	6.5	3452	PASS
275	198	10	30	14.1	7523	PASS
365	198	1	100	1.2	645	PASS
441	443	0.01	100	76.0	3279	PASS
442	198	40	100	42.4	22661	PASS
443	442	17	23	19.1	4317	PASS

Quantitation Report

Data File : H:\VOL1\GCMSDATA\L\110621\BL000311.D Vial: 1
 Acq On : 21 Jun 2011 14:08 Operator: HLM/JCSA
 Sample : DFTPP050 Inst : BNA L
 Misc : DFTPP050 HLM Multiplr: 1.00
 Quant Time: Jun 24 12:10 2011 Quant Results File: temp.res

Method : H:\VOL1\GCMSDATA\L\METHODS\DFTPP.M (RTE Integrator)
 Title :
 Last Update : Thu Jun 09 16:36:07 2011
 Response via : Single Level Calibration

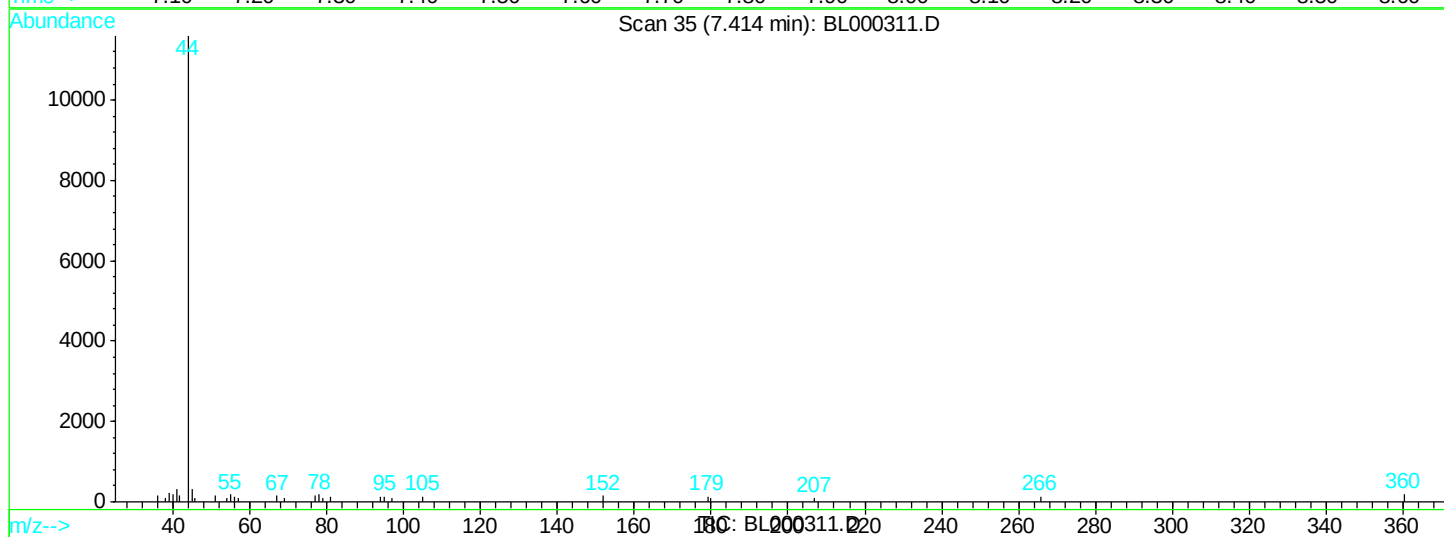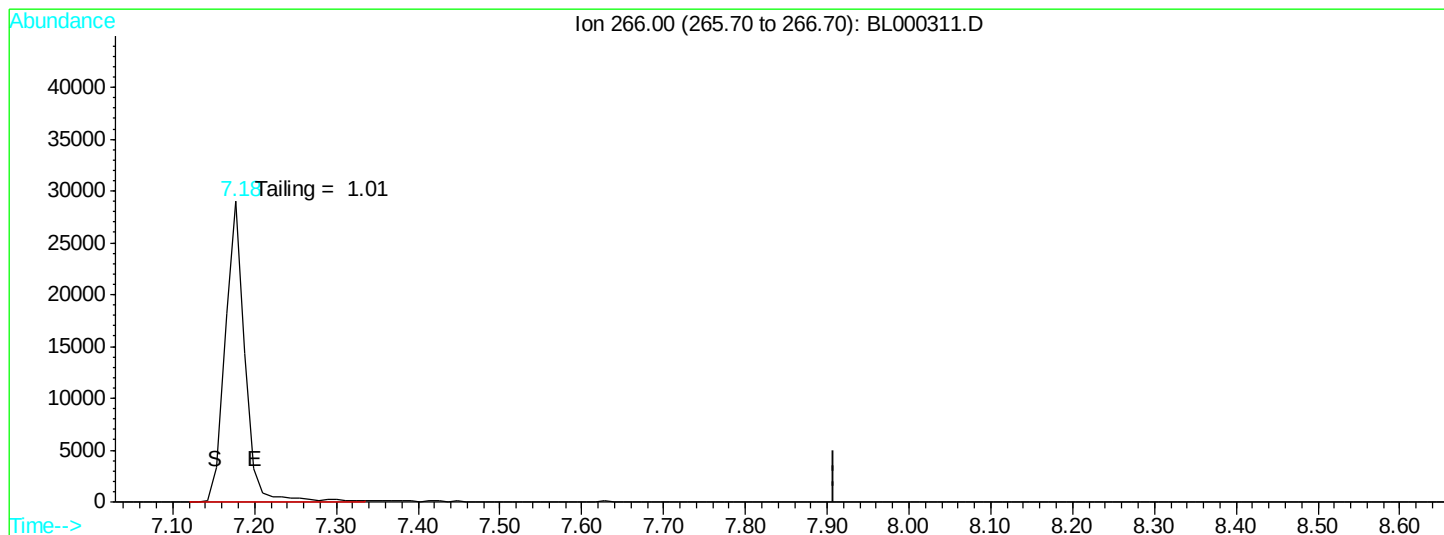

(1) Pentachlorophenol (T)

7.41min 0.00ug/ml



response 0

Ion	Exp%	Act%
266.00	100	0.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report

Data File : H:\VOL1\GCMSDATA\L\110621\BL000311.D Vial: 1
 Acq On : 21 Jun 2011 14:08 Operator: HLM/JCSA
 Sample : DFTPP050 Inst : BNA L
 Misc : DFTPP050 HLM Multiplr: 1.00
 Quant Time: Jun 24 12:10 2011 Quant Results File: temp.res

Method : H:\VOL1\GCMSDATA\L\METHODS\DFTPP.M (RTE Integrator)
 Title :
 Last Update : Thu Jun 09 16:36:07 2011
 Response via : Single Level Calibration

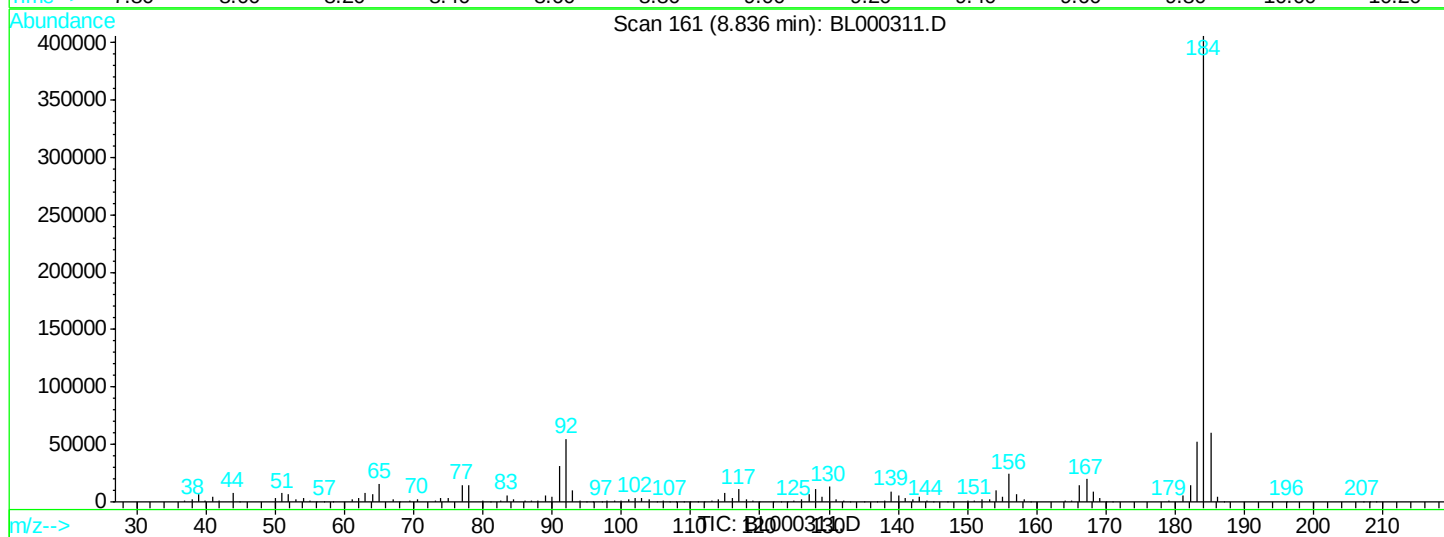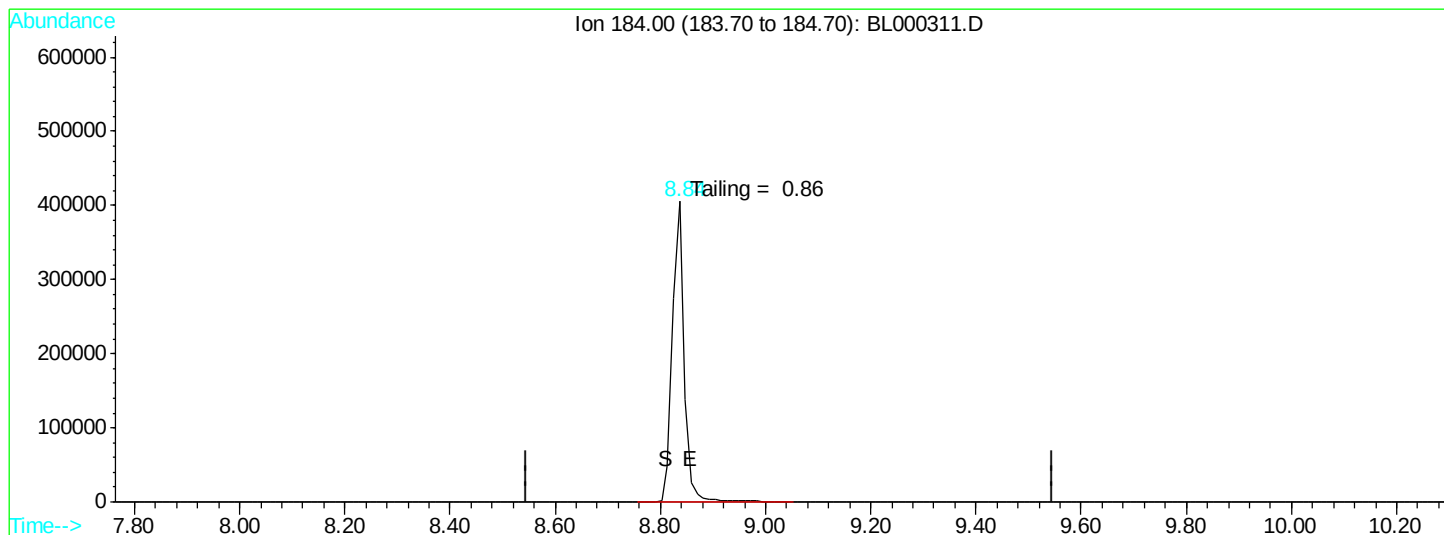

(3) Benzidine (T)

8.84min 62.02ug/ml



response 632726

Ion	Exp%	Act%
184.00	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report

Data File : H:\VOL1\GCMSDATA\L\110621\BL000311.D Vial: 1
 Acq On : 21 Jun 2011 14:08 Operator: HLM/JCSA
 Sample : DFTPP050 Inst : BNA L
 Misc : DFTPP050 HLM Multiplr: 1.00
 Quant Time: Jun 24 12:10 2011 Quant Results File: temp.res

Method : H:\VOL1\GCMSDATA\L\METHODS\DFTPP.M (RTE Integrator)
 Title :
 Last Update : Thu Jun 09 16:36:07 2011
 Response via : Single Level Calibration

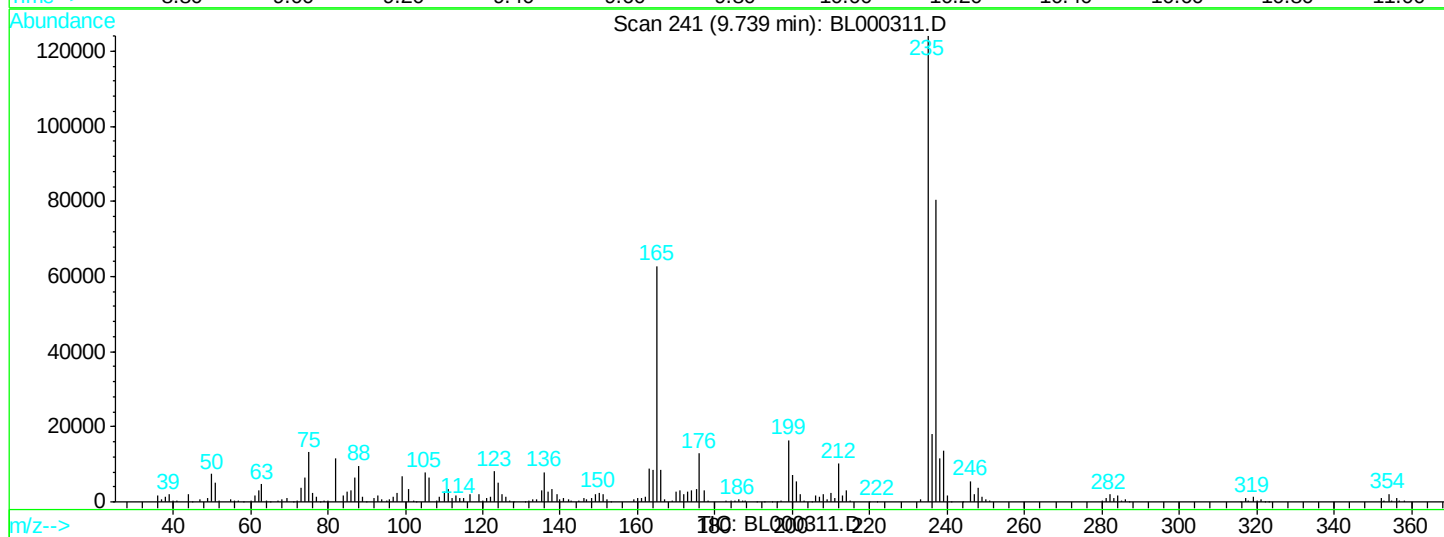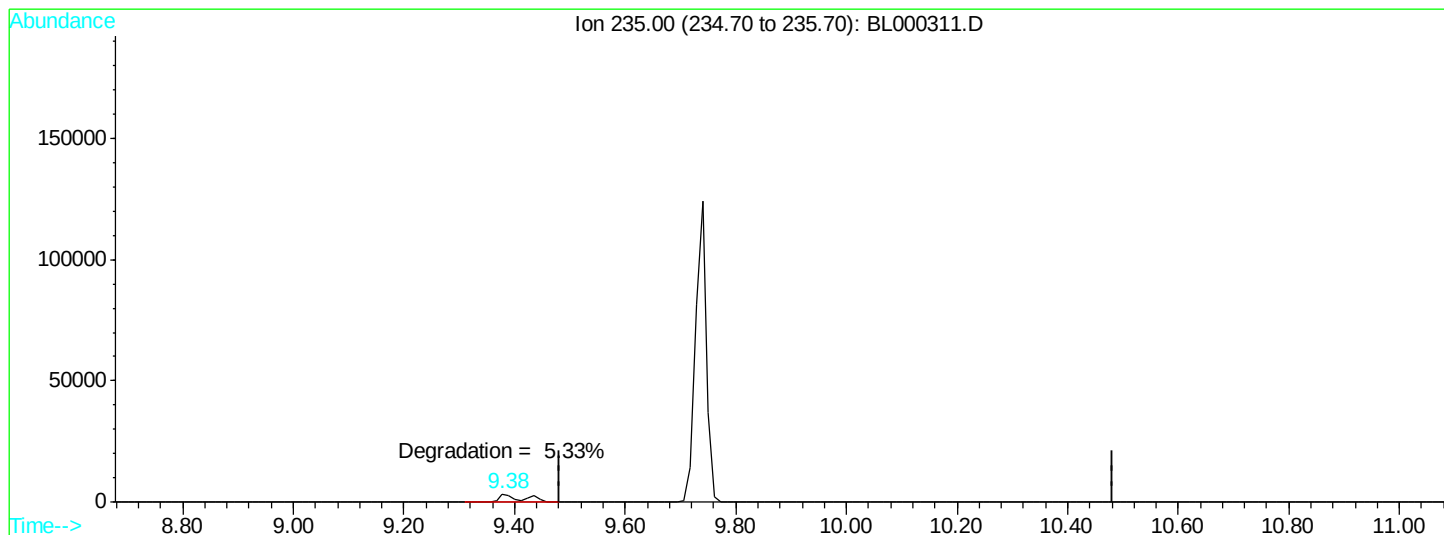

(4) DDT (T)

9.74min 41.87ug/ml

response 175979

Ion	Exp%	Act%
235.00	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00