

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010121\
 Data File : BM028327.D
 Acq On : 01 Jan 2021 08:10
 Operator : JU/CG
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Jan 01 08:42:39 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-SIM-BM010121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 31 16:18:03 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.135	152	930	0.40	ng	0.00
7) Naphthalene-d8	10.947	136	3731	0.40	ng	#-0.01
13) Acenaphthene-d10	14.764	164	1928	0.40	ng	0.00
19) Phenanthrene-d10	17.481	188	3815	0.40	ng	# 0.00
27) Chrysene-d12	21.601	240	3770	0.40	ng	#-0.01
34) Perylene-d12	23.931	264	3550	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.638	112	1128	0.35	ng	0.00
5) Phenol-d6	7.273	99	1535	0.36	ng	0.00
8) Nitrobenzene-d5	9.299	82	1166	0.34	ng	0.00
11) 2-Methylnaphthalene-d10	12.531	152	2268	0.35	ng	0.00
14) 2,4,6-Tribromophenol	16.237	330	337	0.33	ng	0.00
15) 2-Fluorobiphenyl	13.390	172	2942	0.37	ng	0.00
25) Fluoranthene-d10	19.486	212	4022	0.34	ng	0.00
29) Terphenyl-d14	20.061	244	2931	0.32	ng	-0.01
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.408	88	438	0.33	ng	# 86
3) n-Nitrosodimethylamine	3.762	42	705	0.36	ng	# 92
6) bis(2-Chloroethyl)ether	7.547	93	1113	0.37	ng	96
9) Naphthalene	10.997	128	3818	0.35	ng	99
10) Hexachlorobutadiene	11.289	225	739	0.36	ng	# 99
12) 2-Methylnaphthalene	12.602	142	2553	0.35	ng	95
16) Acenaphthylene	14.481	152	2901	0.34	ng	100
17) Acenaphthene	14.824	154	2247	0.36	ng	96
18) Fluorene	15.794	166	2746	0.35	ng	100
20) Hexachlorobenzene	16.790	284	908	0.35	ng	94
21) Atrazine	19.516	200	876	0.34	ng	# 36
22) Pentachlorophenol	17.130	266	334	0.31	ng	97
23) Phenanthrene	17.523	178	4142	0.35	ng	100
24) Anthracene	17.608	178	3515	0.34	ng	99
26) Fluoranthene	19.516	202	4485	0.34	ng	# 97
28) Pyrene	19.874	202	4805	0.37	ng	100
30) Benzo(a)anthracene	21.590	228	4431	0.35	ng	96
31) Chrysene	21.643	228	4600	0.35	ng	97
32) Bis(2-ethylhexyl)phtha...	21.494	149	2090	0.35	ng	95
33) Indeno(1,2,3-cd)pyrene	26.303	276	5028	0.36	ng	# 91
35) Benzo(b)fluoranthene	23.222	252	4850	0.37	ng	# 94
36) Benzo(k)fluoranthene	23.270	252	4504	0.36	ng	# 91
37) Benzo(a)pyrene	23.825	252	4233	0.38	ng	# 92
38) Dibenzo(a,h)anthracene	26.317	278	4394	0.36	ng	# 93
39) Benzo(g,h,i)perylene	27.032	276	4368	0.36	ng	# 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010121\
Data File : BM028327.D
Acq On : 01 Jan 2021 08:10
Operator : JU/CG
Sample : SSTDCCC0.4
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTDCCC0.4

Quant Time: Jan 01 08:42:39 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-SIM-BM010121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 31 16:18:03 2020
Response via : Initial Calibration




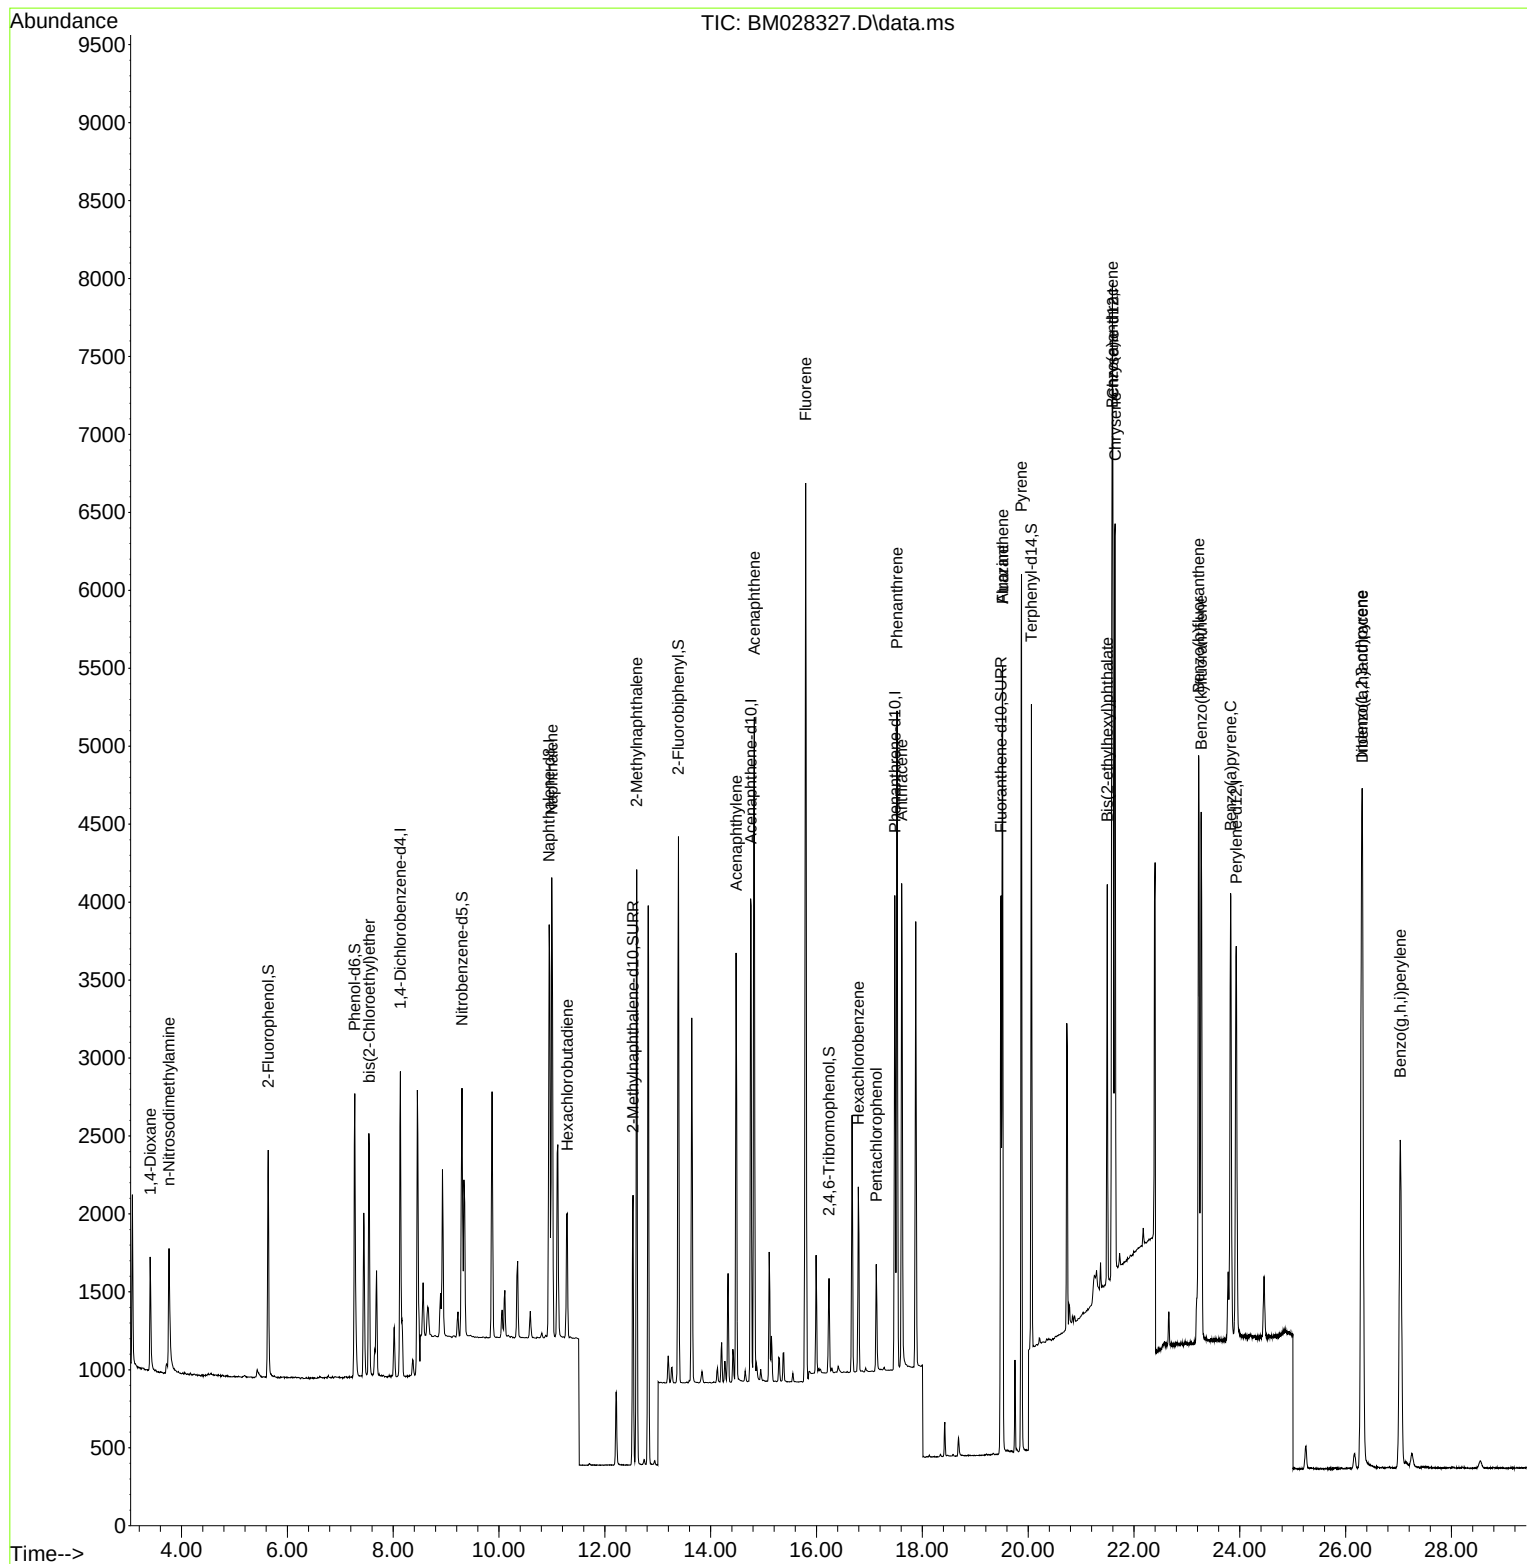




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 8.135 min Scan# 634
 Delta R.T. -0.008 min
 Lab File: BM028327.D
 Acq: 01 Jan 2021 08:10




Instrument :
 BNA_M
 ClientSampled :
 SSTDCCC0.4

Tgt Ion:152 Resp: 930
 Ion Ratio Lower Upper
 152 100
 150 152.5 116.6 174.8
 115 66.2 52.9 79.3

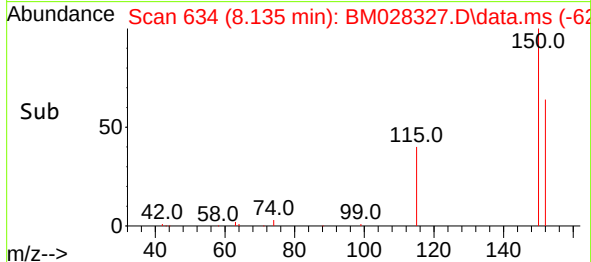


#2
 1,4-Dioxane
 Concen: 0.33 ng
 RT: 3.408 min Scan# 47
 Delta R.T. -0.008 min
 Lab File: BM028327.D
 Acq: 01 Jan 2021 08:10

Tgt Ion: 88 Resp: 438
 Ion Ratio Lower Upper
 88 100
 58 91.6 59.4 89.2#
 43 42.2 32.3 48.5

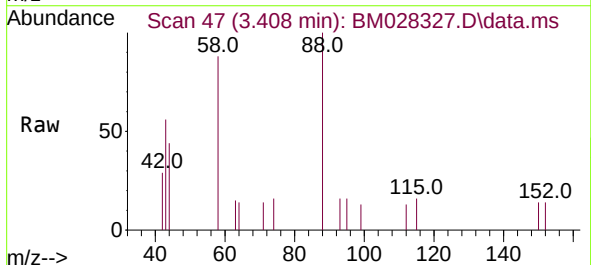

Abundance Scan 92 (3.770 min): BM028303.D\data.ms (-84)

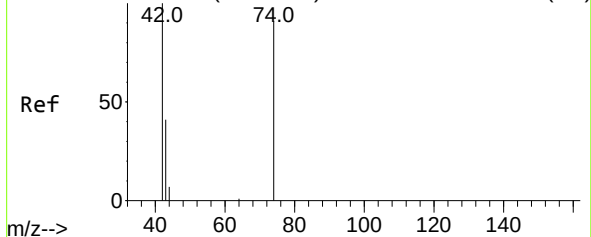

#3

n-Nitrosodimethylamine

Concen: 0.36 ng

RT: 3.762 min Scan# 91

Delta R.T. -0.008 min

Lab File: BM028327.D

Acq: 01 Jan 2021 08:10



Tgt Ion: 42 Resp: 705

Ion Ratio Lower Upper


42 100

74 87.7 64.4 96.6


44 4.4 2.8 4.2#

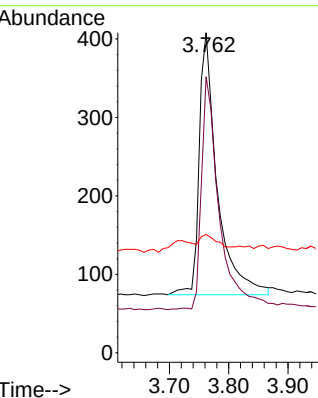

Abundance Scan 91 (3.762 min): BM028327.D\data.ms (-80)

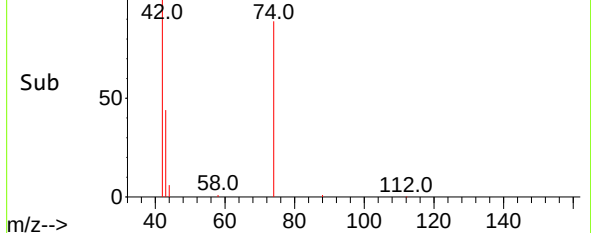

Abundance Scan 325 (5.646 min): BM028303.D\data.ms (-30)

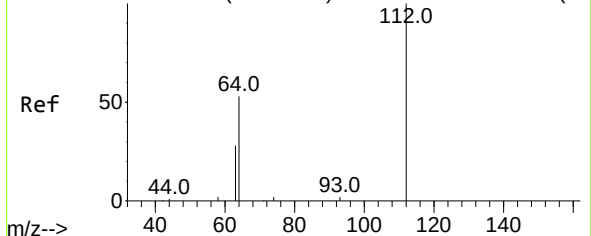

#4

2-Fluorophenol

Concen: 0.35 ng

RT: 5.638 min Scan# 324

Delta R.T. -0.008 min

Lab File: BM028327.D

Acq: 01 Jan 2021 08:10



Tgt Ion: 112 Resp: 1128

Ion Ratio Lower Upper


112 100


64 64.5 49.5 74.3

63 36.3 32.0 48.0

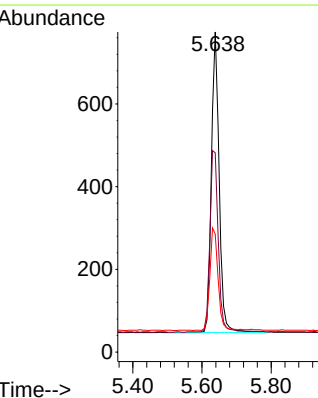

Abundance Scan 324 (5.638 min): BM028327.D\data.ms (-30)




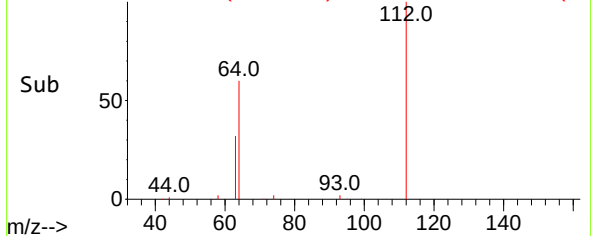




#5
Phenol-d6
Concen: 0.36 ng
RT: 7.273 min Scan# 527
Delta R.T. -0.008 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10




Instrument :
BNA_M
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	99	Resp:	1535
Ion	Ratio	Lower	Upper
99	100		
42	26.7	22.4	33.6
71	37.3	37.8	56.6#

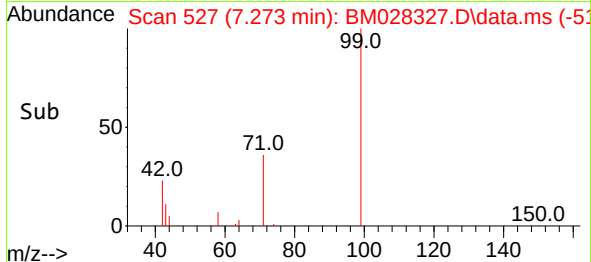

#6
bis(2-Chloroethyl)ether
Concen: 0.37 ng
RT: 7.547 min Scan# 561
Delta R.T. 0.000 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10

Tgt Ion:	93	Resp:	1113
Ion	Ratio	Lower	Upper
93	100		
63	84.0	63.1	94.7
95	31.9	26.1	39.1









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.947 min Scan# 873
Delta R.T. -0.013 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10




Instrument :
BNA_M
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	136	Resp:	3731
Ion Ratio	Lower	Upper	
136	100		
137	13.2	10.6	15.8
54	13.8	8.6	12.8#
68	8.9	5.7	8.5#



#8
Nitrobenzene-d5
Concen: 0.34 ng
RT: 9.299 min Scan# 743
Delta R.T. 0.000 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10

Tgt Ion:	82	Resp:	1166
Ion Ratio	Lower	Upper	
82	100		
128	41.9	30.6	46.0
54	64.1	48.3	72.5


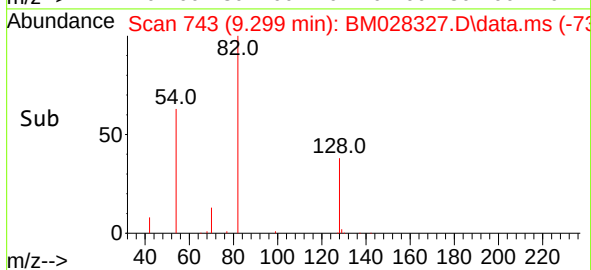






#9
Naphthalene
Concen: 0.35 ng
RT: 10.997 min Scan# 877
Delta R.T. -0.013 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10




Instrument :
BNA_M
ClientSampleId :
SSTDCCC0.4


Tgt Ion:128 Resp: 3818
Ion Ratio Lower Upper
128 100
129 12.7 9.8 14.8
127 14.9 12.2 18.4

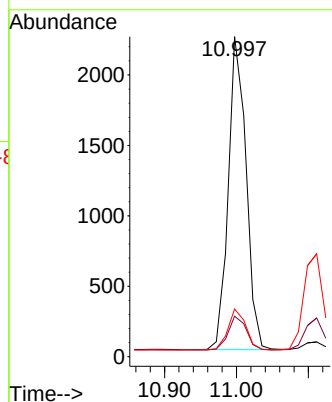

#10
Hexachlorobutadiene
Concen: 0.36 ng
RT: 11.289 min Scan# 900
Delta R.T. 0.000 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10

Tgt Ion:225 Resp: 739
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.2 51.0 76.6


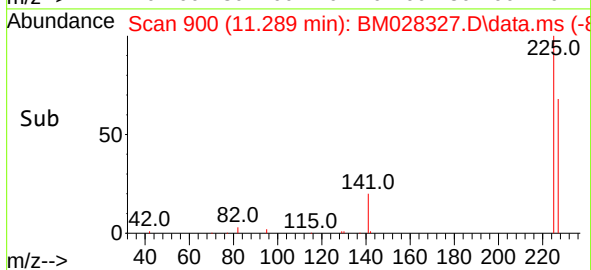






#11
2-Methylnaphthalene-d10
Concen: 0.35 ng
RT: 12.531 min Scan# 1146
Delta R.T. -0.004 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10




Instrument :
BNA_M
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 2268
Ion Ratio Lower Upper
152 100
151 20.4 16.7 25.1

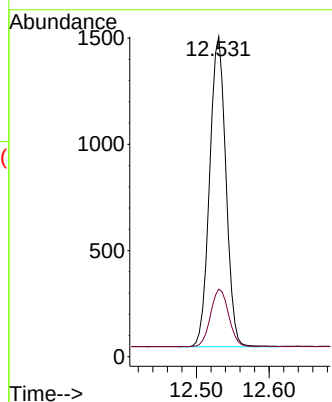

#12
2-Methylnaphthalene
Concen: 0.35 ng
RT: 12.602 min Scan# 1162
Delta R.T. -0.004 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10

Tgt Ion:142 Resp: 2553
Ion Ratio Lower Upper
142 100
141 89.9 69.4 104.2
115 38.6 35.7 53.5


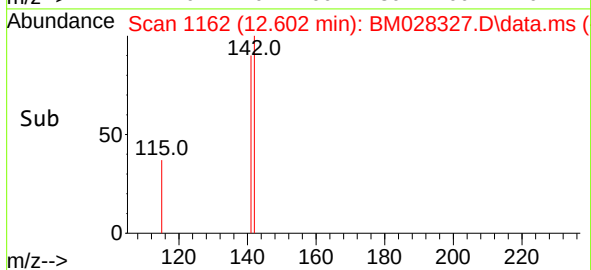






#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.764 min Scan# 1427
Delta R.T. 0.000 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10




Instrument :
BNA_M
ClientSampleId :
SSTDCCC0.4


Tgt Ion:164	Resp:	1928
Ion Ratio	Lower	Upper
164	100	
162	100.0	80.6 120.8
160	45.0	39.5 59.3

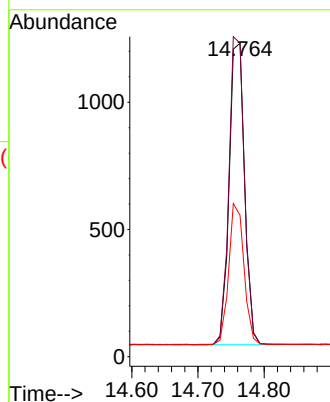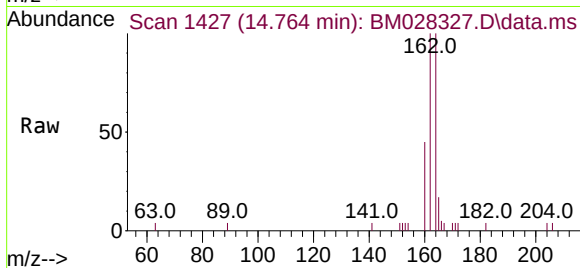

#14
2,4,6-Tribromophenol
Concen: 0.33 ng
RT: 16.237 min Scan# 1571
Delta R.T. 0.000 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10

Tgt Ion:330	Resp:	337
Ion Ratio	Lower	Upper
330	100	
332	97.3	0.0 0.0#
141	37.4	34.4 51.6


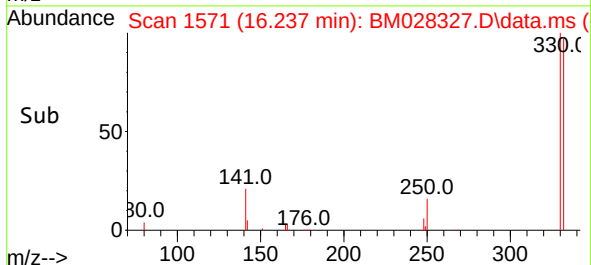

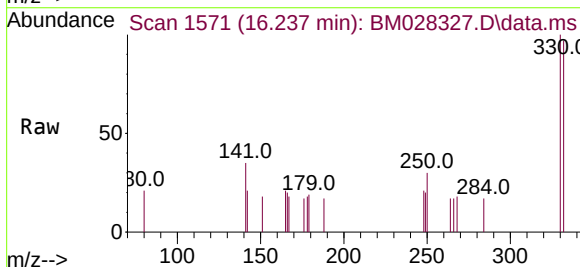




#15
2-Fluorobiphenyl
Concen: 0.37 ng
RT: 13.390 min Scan# 1291
Delta R.T. 0.000 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10




Instrument :
BNA_M
ClientSampleId :
SSTDCCC0.4


Tgt Ion:172	Resp:	2942
Ion Ratio	Lower	Upper
172	100	
171	36.2	28.2 42.4
170	24.3	20.0 30.0

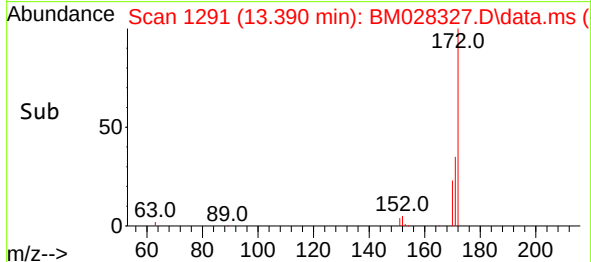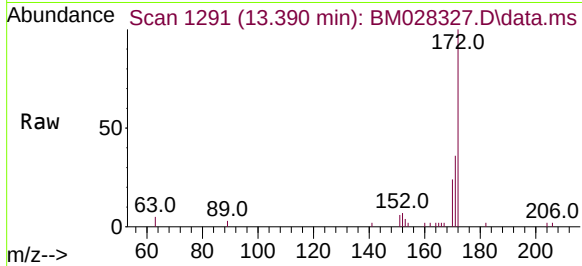

#16
Acenaphthylene
Concen: 0.34 ng
RT: 14.481 min Scan# 1399
Delta R.T. -0.010 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10

Tgt Ion:152	Resp:	2901
Ion Ratio	Lower	Upper
152	100	
151	20.0	15.8 23.8
153	13.1	10.6 16.0




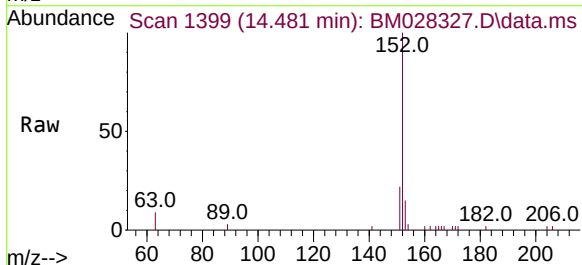




#17
Acenaphthene
Concen: 0.36 ng
RT: 14.824 min Scan# 1433
Delta R.T. 0.000 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10




Instrument :
BNA_M
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	154	Resp:	2247
Ion	Ratio	Lower	Upper
154	100		
153	110.1	83.6	125.4
152	53.4	43.9	65.9

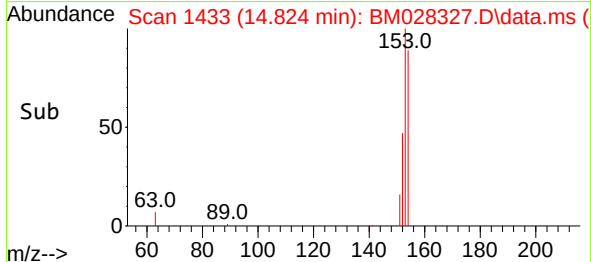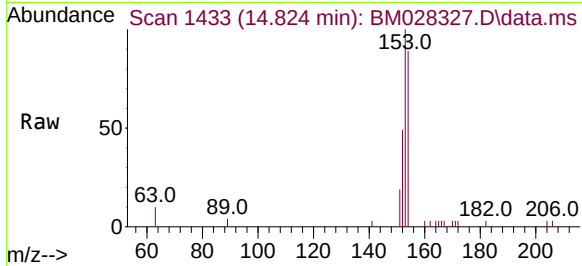

#18
Fluorene
Concen: 0.35 ng
RT: 15.794 min Scan# 1529
Delta R.T. -0.010 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10

Tgt Ion:	166	Resp:	2746
Ion	Ratio	Lower	Upper
166	100		
165	98.3	78.6	118.0
167	13.1	10.7	16.1




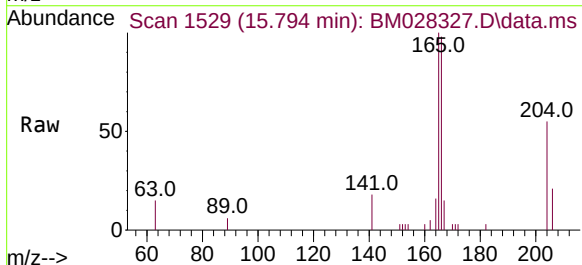




#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.481 min Scan# 1688
Delta R.T. 0.000 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10




Instrument :
BNA_M
ClientSampleId :
SSTDCCC0.4


Tgt Ion:188 Resp: 3815
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.4 5.0 7.4#

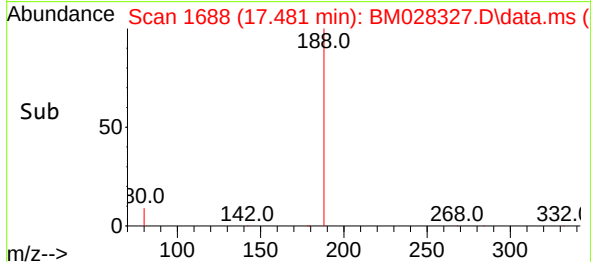

#20
Hexachlorobenzene
Concen: 0.35 ng
RT: 16.790 min Scan# 1623
Delta R.T. -0.011 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10

Tgt Ion:284 Resp: 908
Ion Ratio Lower Upper
284 100
142 34.5 32.0 48.0
249 32.7 27.0 40.6




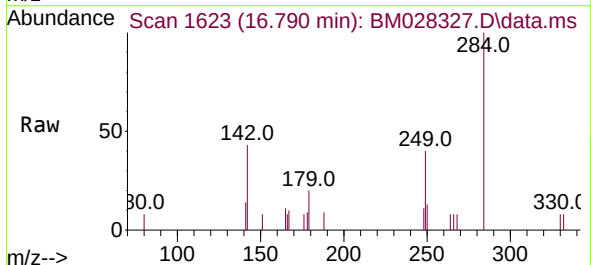




#21
Atrazine
Concen: 0.34 ng
RT: 19.516 min Scan# 2041
Delta R.T. 0.000 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10




Instrument :
BNA_M
ClientSampleId :
SSTDCCC0.4


Tgt Ion:200 Resp: 876
Ion Ratio Lower Upper
200 100
173 0.0 22.8 34.2#
215 0.0 38.1 57.1#

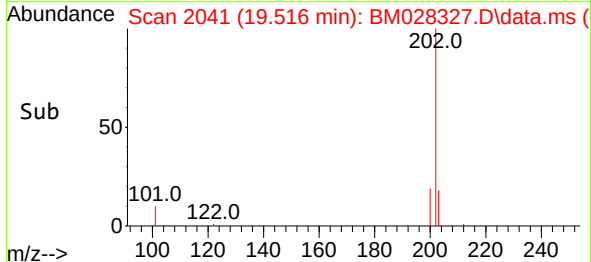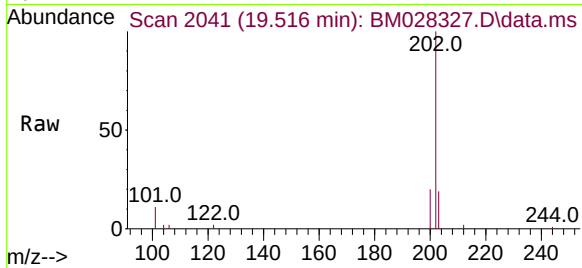

#22
Pentachlorophenol
Concen: 0.31 ng
RT: 17.130 min Scan# 1655
Delta R.T. -0.011 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10

Tgt Ion:266 Resp: 334
Ion Ratio Lower Upper
266 100
264 62.0 50.9 76.3
268 66.8 51.5 77.3




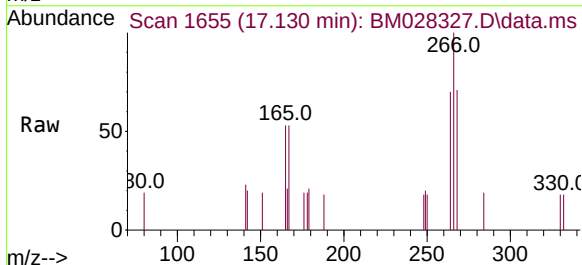




#23
Phenanthrene
Concen: 0.35 ng
RT: 17.523 min Scan# 1692
Delta R.T. 0.000 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10




Instrument :
BNA_M
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	178	Resp:	4142
Ion Ratio	Lower	Upper	
178	100		
176	18.6	14.8	22.2
179	15.6	12.4	18.6

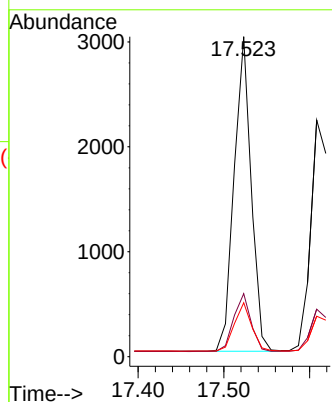

#24
Anthracene
Concen: 0.34 ng
RT: 17.608 min Scan# 1700
Delta R.T. -0.011 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10

Tgt Ion:	178	Resp:	3515
Ion Ratio	Lower	Upper	
178	100		
176	18.1	14.8	22.2
179	15.3	12.5	18.7


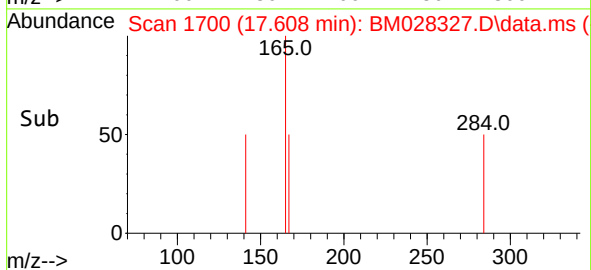






#25
Fluoranthene-d10
Concen: 0.34 ng
RT: 19.486 min Scan# 2035
Delta R.T. -0.005 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10




Instrument :
BNA_M
ClientSampleId :
SSTDCCC0.4


Tgt Ion:212 Resp: 4022
Ion Ratio Lower Upper
212 100
106 12.5 6.8 10.2#
104 7.2 4.1 6.1#

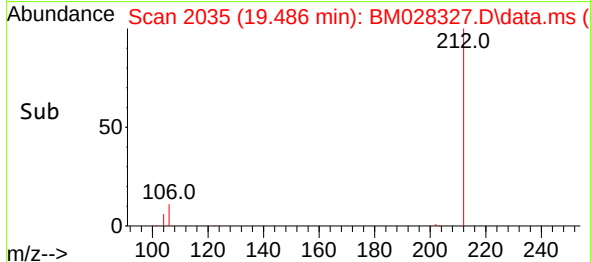

#26
Fluoranthene
Concen: 0.34 ng
RT: 19.516 min Scan# 2041
Delta R.T. 0.000 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10

Tgt Ion:202 Resp: 4485
Ion Ratio Lower Upper
202 100
101 10.9 5.8 8.6#
203 17.2 13.7 20.5


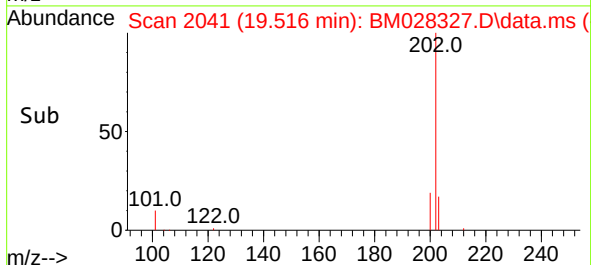
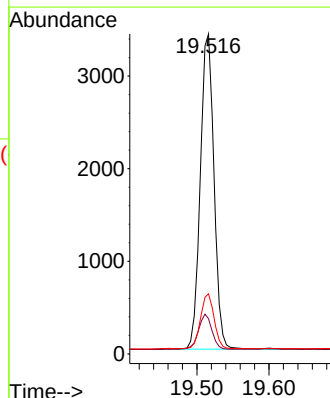
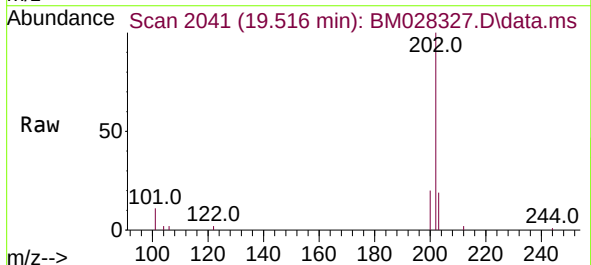


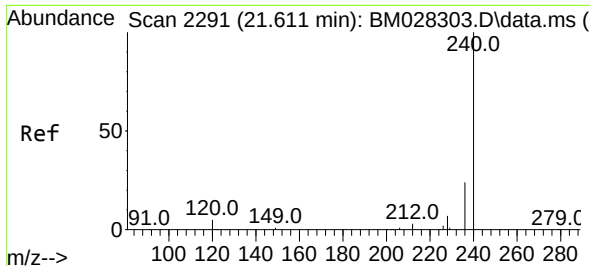

#27
Chrysene-d12
Concen: 0.40 ng
RT: 21.601 min Scan# 2290
Delta R.T. -0.011 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10




Instrument :
BNA_M
ClientSampleId :
SSTDCCC0.4


Tgt Ion:240 Resp: 3770
Ion Ratio Lower Upper
240 100
120 11.2 5.3 7.9#
236 26.3 21.8 32.8

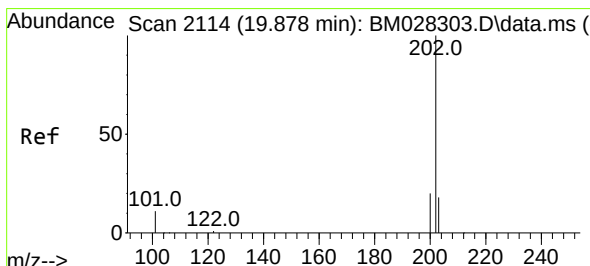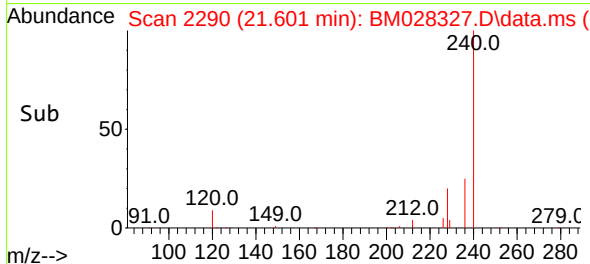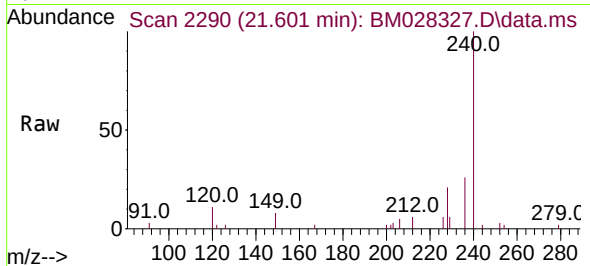

#28
Pyrene
Concen: 0.37 ng
RT: 19.874 min Scan# 2113
Delta R.T. -0.005 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10

Tgt Ion:202 Resp: 4805
Ion Ratio Lower Upper
202 100
200 20.6 16.6 24.8
203 17.6 13.8 20.8


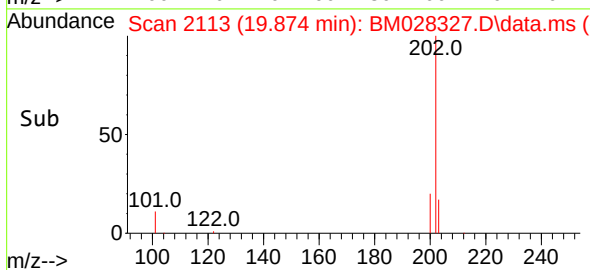

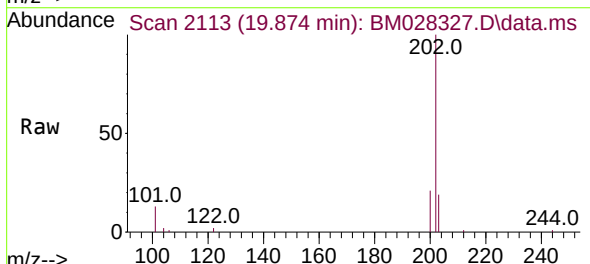




#29
 Terphenyl-d14
 Concen: 0.32 ng
 RT: 20.061 min Scan# 2145
 Delta R.T. -0.011 min
 Lab File: BM028327.D
 Acq: 01 Jan 2021 08:10




Instrument :
 BNA_M
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:244 Resp: 2931
 Ion Ratio Lower Upper
 244 100
 212 8.7 7.3 10.9
 122 10.4 7.3 10.9

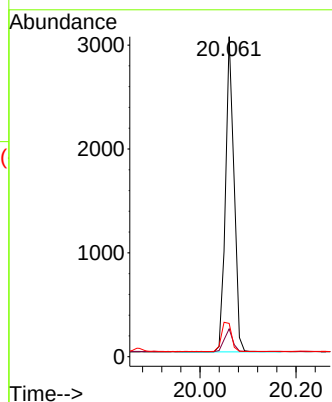

#30
 Benzo(a)anthracene
 Concen: 0.35 ng
 RT: 21.590 min Scan# 2289
 Delta R.T. 0.000 min
 Lab File: BM028327.D
 Acq: 01 Jan 2021 08:10

Tgt Ion:228 Resp: 4431
 Ion Ratio Lower Upper
 228 100
 226 25.9 22.3 33.5
 229 21.6 15.7 23.5


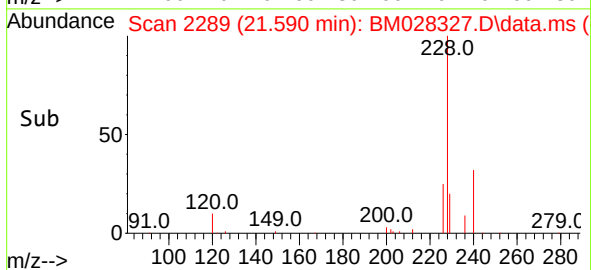






#31
Chrysene
Concen: 0.35 ng
RT: 21.643 min Scan# 2294
Delta R.T. 0.000 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10




Instrument :
BNA_M
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	228	Resp:	4600
Ion Ratio	Lower	Upper	
228	100		
226	28.5	24.2	36.2
229	21.2	15.7	23.5

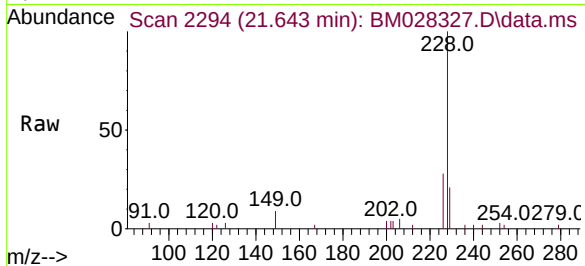

#32
Bis(2-ethylhexyl)phthalate
Concen: 0.35 ng
RT: 21.494 min Scan# 2280
Delta R.T. 0.000 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10

Tgt Ion:	149	Resp:	2090
Ion Ratio	Lower	Upper	
149	100		
167	26.3	23.2	34.8
279	4.4	3.9	5.9




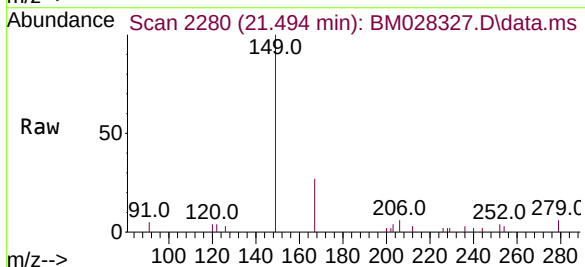




#33
Indeno(1,2,3-cd)pyrene
Concen: 0.36 ng
RT: 26.303 min Scan# 3504
Delta R.T. -0.010 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10




Instrument :
BNA_M
ClientSampleId :
SSTDCCC0.4


Tgt Ion:276 Resp: 5028
Ion Ratio Lower Upper
276 100
138 25.9 13.3 19.9#
277 25.5 20.2 30.4

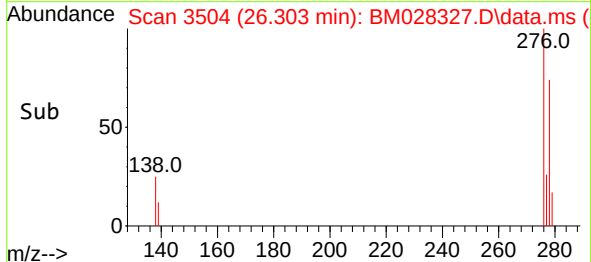

#34
Perylene-d12
Concen: 0.40 ng
RT: 23.931 min Scan# 2811
Delta R.T. -0.007 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10

Tgt Ion:264 Resp: 3550
Ion Ratio Lower Upper
264 100
260 24.5 19.8 29.6
265 55.4 51.4 77.0


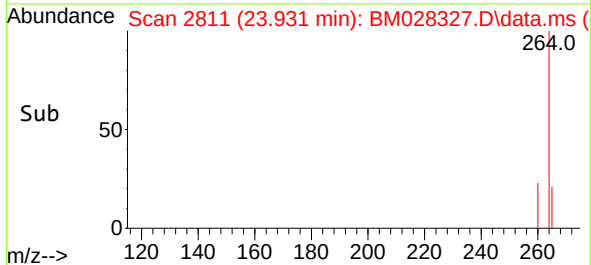






#35
Benzo(b)fluoranthene
Concen: 0.37 ng
RT: 23.222 min Scan# 2604
Delta R.T. -0.010 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10




Instrument :
BNA_M
ClientSampleId :
SSTDCCC0.4


Tgt Ion:252 Resp: 4850
Ion Ratio Lower Upper
252 100
253 26.3 20.1 30.1
125 15.5 7.2 10.8#

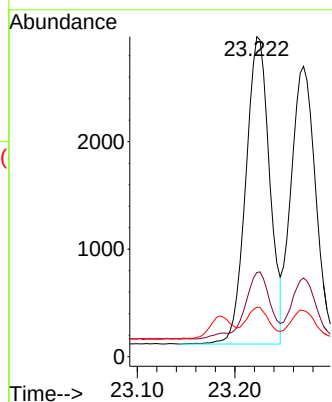

#36
Benzo(k)fluoranthene
Concen: 0.36 ng
RT: 23.270 min Scan# 2618
Delta R.T. -0.007 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10

Tgt Ion:252 Resp: 4504
Ion Ratio Lower Upper
252 100
253 27.1 19.8 29.8
125 15.9 7.1 10.7#


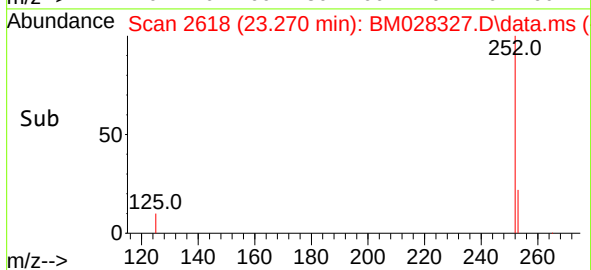






#37
Benzo(a)pyrene
Concen: 0.38 ng
RT: 23.825 min Scan# 2780
Delta R.T. -0.010 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10




Instrument :
BNA_M
ClientSampleId :
SSTDCCC0.4


Tgt Ion:252	Resp:	4233
Ion Ratio	Lower	Upper
252	100	
253	28.0	21.3 31.9
125	18.3	8.3 12.5#



#38
Dibenzo(a,h)anthracene
Concen: 0.36 ng
RT: 26.317 min Scan# 3508
Delta R.T. -0.010 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10

Tgt Ion:278	Resp:	4394
Ion Ratio	Lower	Upper
278	100	
139	19.5	9.3 13.9#
279	28.0	21.6 32.4

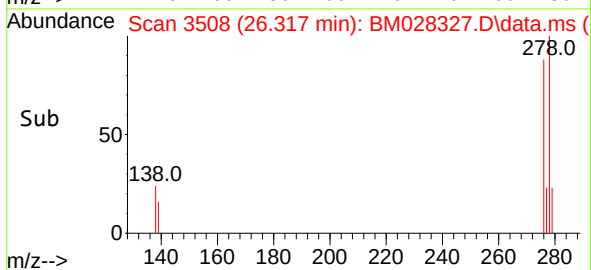



#39
Benzo(g,h,i)perylene
Concen: 0.36 ng
RT: 27.032 min Scan# 3717
Delta R.T. -0.017 min
Lab File: BM028327.D
Acq: 01 Jan 2021 08:10

Instrument :
BNA_M
ClientSampleId :
SSTDCCC0.4

Tgt Ion:276 Resp: 4368
Ion Ratio Lower Upper
276 100
277 26.8 19.8 29.8
138 25.4 11.7 17.5#

