
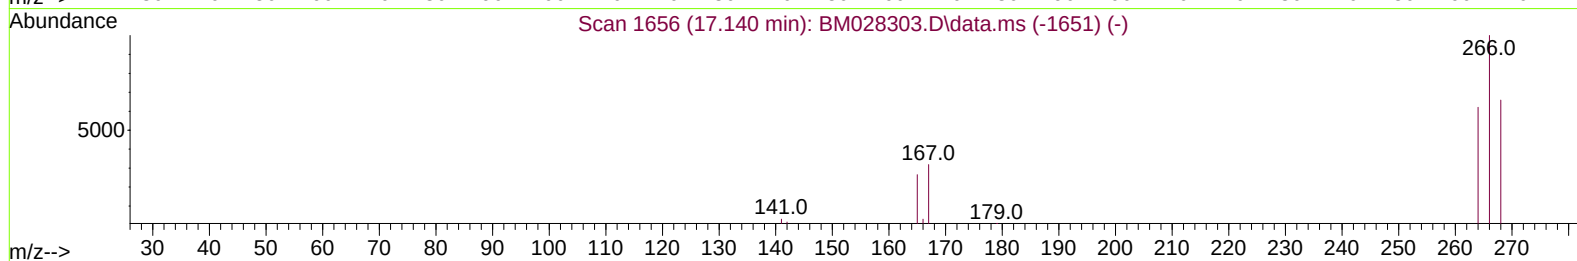
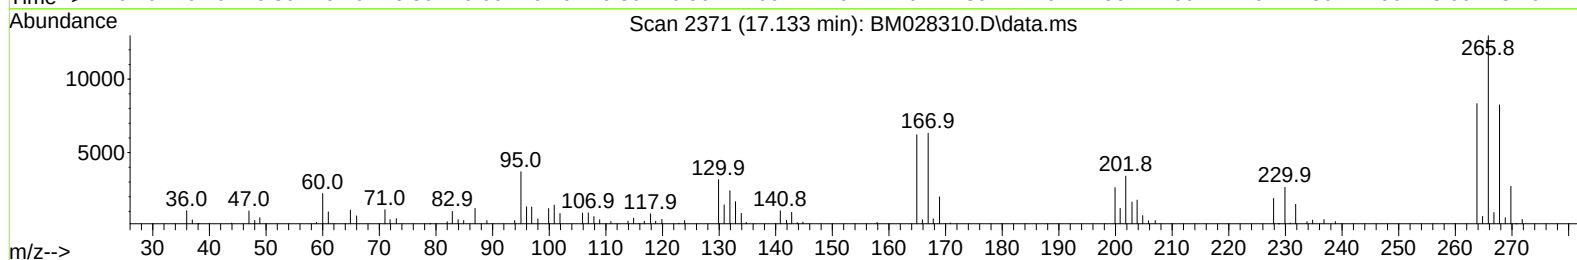


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010121\
 Data File : BM028310.D
 Acq On : 31 Dec 2020 18:02
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 01 01:51:21 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-SIM-BM010121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 31 16:18:03 2020
 Response via : Initial Calibration

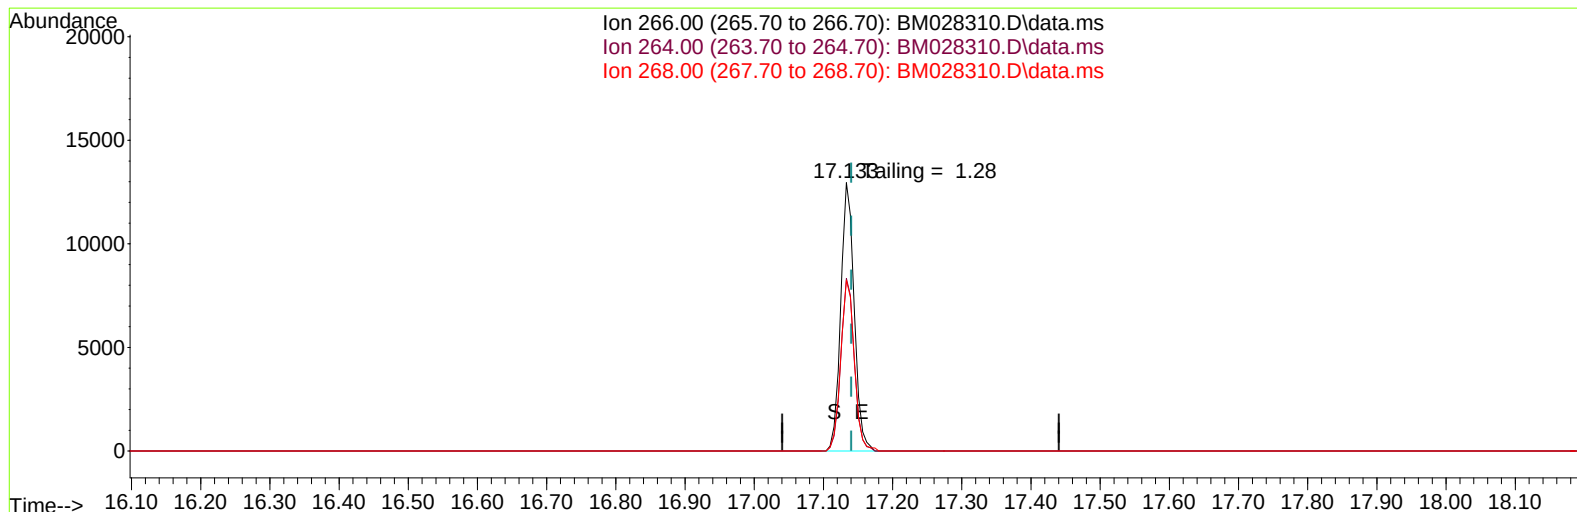

TIC: BM028310.D\data.ms

(22) Pentachlorophenol

17.133min (-0.007) 0.00 ng

response 17440

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	63.60	63.80
268.00	64.40	64.58
0.00	0.00	0.00