
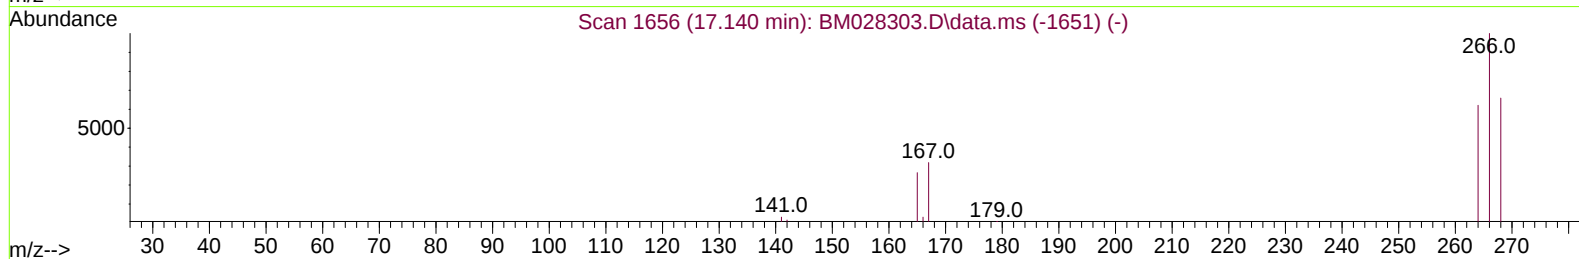
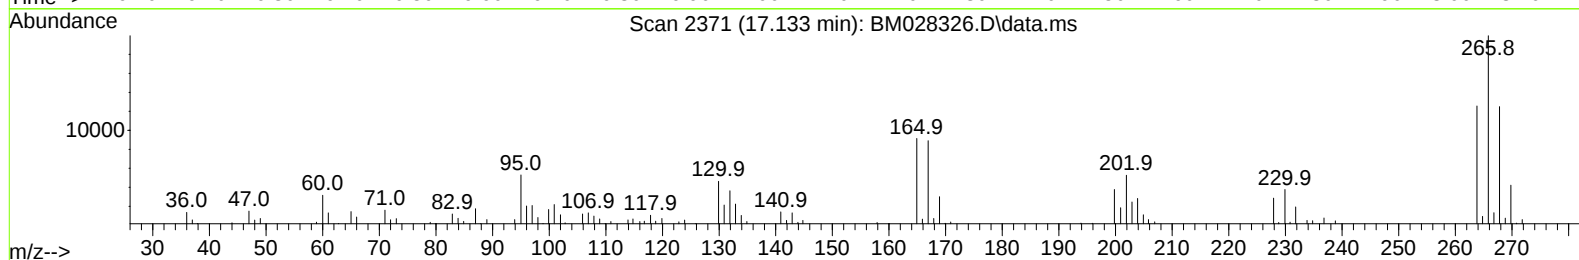


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010121\
Data File : BM028326.D
Acq On : 01 Jan 2021 07:34
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 02 08:07:17 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-SIM-BM010121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 31 16:18:03 2020
Response via : Initial Calibration

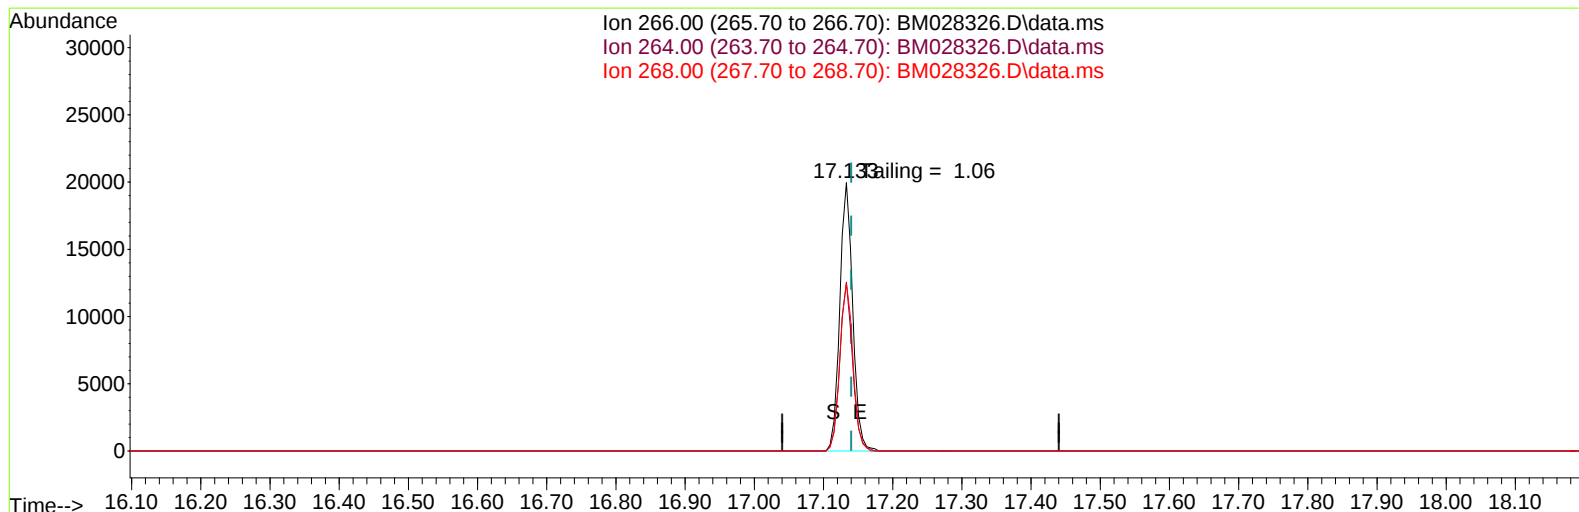

TIC: BM028326.D\data.ms

(22) Pentachlorophenol

17.133min (-0.007) 0.00 ng

response 25747

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	63.60	62.14
268.00	64.40	63.61
0.00	0.00	0.00