

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010121\
 Data File : BM028317.D
 Acq On : 31 Dec 2020 22:15
 Operator : JU/CG
 Sample : PB133674BS
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB133674BS

Quant Time: Jan 01 00:01:26 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-SIM-BM010121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 31 16:18:03 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.135	152	671	0.40	ng	0.00
7) Naphthalene-d8	10.959	136	2663	0.40	ng	0.00
13) Acenaphthene-d10	14.764	164	1392	0.40	ng	0.00
19) Phenanthrene-d10	17.481	188	2736	0.40	ng	# 0.00
27) Chrysene-d12	21.601	240	2676	0.40	ng	#-0.01
34) Perylene-d12	23.934	264	2475	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.638	112	819	0.36	ng	0.00
5) Phenol-d6	7.273	99	1105	0.36	ng	0.00
8) Nitrobenzene-d5	9.299	82	852	0.35	ng	0.00
11) 2-Methylnaphthalene-d10	12.531	152	1626	0.35	ng	0.00
14) 2,4,6-Tribromophenol	16.237	330	245	0.34	ng	0.00
15) 2-Fluorobiphenyl	13.390	172	2110	0.36	ng	0.00
25) Fluoranthene-d10	19.486	212	2841	0.34	ng	0.00
29) Terphenyl-d14	20.061	244	2618	0.40	ng	-0.01
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.408	88	324	0.34	ng	# 88
3) n-Nitrosodimethylamine	3.762	42	502	0.36	ng	# 91
6) bis(2-Chloroethyl)ether	7.547	93	797	0.37	ng	95
9) Naphthalene	11.010	128	2740	0.36	ng	98
10) Hexachlorobutadiene	11.289	225	529	0.36	ng	# 98
12) 2-Methylnaphthalene	12.606	142	1836	0.35	ng	95
16) Acenaphthylene	14.481	152	2145	0.34	ng	99
17) Acenaphthene	14.824	154	1572	0.35	ng	96
18) Fluorene	15.804	166	1975	0.35	ng	99
20) Hexachlorobenzene	16.800	284	667	0.36	ng	93
21) Atrazine	19.516	200	611	0.33	ng	# 36
22) Pentachlorophenol	17.130	266	248	0.32	ng	96
23) Phenanthrene	17.523	178	2971	0.35	ng	100
24) Anthracene	17.619	178	2531	0.34	ng	99
26) Fluoranthene	19.516	202	3147	0.33	ng	# 97
28) Pyrene	19.874	202	3165	0.35	ng	99
30) Benzo(a)anthracene	21.590	228	3042	0.34	ng	97
31) Chrysene	21.643	228	3256	0.35	ng	97
32) Bis(2-ethylhexyl)phtha...	21.494	149	1454	0.35	ng	94
33) Indeno(1,2,3-cd)pyrene	26.310	276	3541	0.35	ng	# 91
35) Benzo(b)fluoranthene	23.226	252	3443	0.37	ng	# 89
36) Benzo(k)fluoranthene	23.274	252	3147	0.36	ng	# 89
37) Benzo(a)pyrene	23.828	252	2932	0.37	ng	# 86
38) Dibenzo(a,h)anthracene	26.320	278	3076	0.37	ng	# 89
39) Benzo(g,h,i)perylene	27.042	276	3090	0.37	ng	# 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010121\
Data File : BM028317.D
Acq On : 31 Dec 2020 22:15
Operator : JU/CG
Sample : PB133674BS
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB133674BS

Quant Time: Jan 01 00:01:26 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-SIM-BM010121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 31 16:18:03 2020
Response via : Initial Calibration







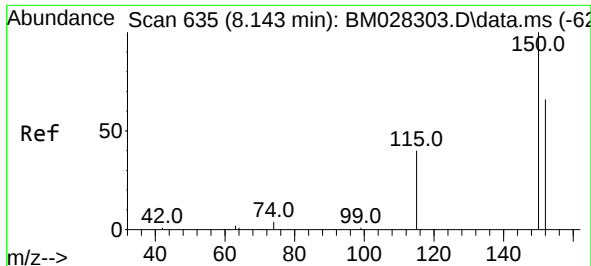

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 8.135 min Scan# 634
 Delta R.T. -0.008 min
 Lab File: BM028317.D
 Acq: 31 Dec 2020 22:15




Instrument :
 BNA_M
 ClientSampleId :
 PB133674BS


Tgt Ion:152 Resp: 671
 Ion Ratio Lower Upper
 152 100
 150 153.7 116.6 174.8
 115 69.8 52.9 79.3



#2
 1,4-Dioxane
 Concen: 0.34 ng
 RT: 3.408 min Scan# 47
 Delta R.T. -0.008 min
 Lab File: BM028317.D
 Acq: 31 Dec 2020 22:15

Tgt Ion: 88 Resp: 324
 Ion Ratio Lower Upper
 88 100
 58 90.4 59.4 89.2#
 43 40.1 32.3 48.5









#3
n-Nitrosodimethylamine
Concen: 0.36 ng
RT: 3.762 min Scan# 91
Delta R.T. -0.008 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15




Instrument :
BNA_M
ClientSampleId :
PB133674BS


Tgt Ion:	42	Resp:	502
Ion	Ratio	Lower	Upper
42	100		
74	87.8	64.4	96.6
44	11.2	2.8	4.2#



#4
2-Fluorophenol
Concen: 0.36 ng
RT: 5.638 min Scan# 324
Delta R.T. -0.008 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15

Tgt Ion:	112	Resp:	819
Ion	Ratio	Lower	Upper
112	100		
64	64.0	49.5	74.3
63	35.2	32.0	48.0









#5
Phenol-d6
Concen: 0.36 ng
RT: 7.273 min Scan# 527
Delta R.T. -0.008 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15




Instrument :
BNA_M
ClientSampleId :
PB133674BS


Tgt Ion:	99	Resp:	1105
Ion	Ratio	Lower	Upper
99	100		
42	28.1	22.4	33.6
71	37.6	37.8	56.6#



#6
bis(2-Chloroethyl)ether
Concen: 0.37 ng
RT: 7.547 min Scan# 561
Delta R.T. 0.000 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15

Tgt Ion:	93	Resp:	797
Ion	Ratio	Lower	Upper
93	100		
63	85.3	63.1	94.7
95	32.1	26.1	39.1









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.959 min Scan# 874
Delta R.T. 0.000 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15




Instrument :
BNA_M
ClientSampleId :
PB133674BS


Tgt Ion:	136	Resp:	2663
Ion Ratio	Lower	Upper	
136	100		
137	13.8	10.6	15.8
54	8.8	8.6	12.8
68	6.7	5.7	8.5



#8
Nitrobenzene-d5
Concen: 0.35 ng
RT: 9.299 min Scan# 743
Delta R.T. 0.000 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15

Tgt Ion:	82	Resp:	852
Ion Ratio	Lower	Upper	
82	100		
128	41.4	30.6	46.0
54	69.9	48.3	72.5









#9
Naphthalene
Concen: 0.36 ng
RT: 11.010 min Scan# 878
Delta R.T. 0.000 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15




Instrument :
BNA_M
ClientSampleId :
PB133674BS


Tgt Ion:	128	Resp:	2740
Ion	Ratio	Lower	Upper
128	100		
129	13.8	9.8	14.8
127	15.4	12.2	18.4



#10
Hexachlorobutadiene
Concen: 0.36 ng
RT: 11.289 min Scan# 900
Delta R.T. 0.000 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15

Tgt Ion:	225	Resp:	529
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	65.0	51.0	76.6









#11
2-Methylnaphthalene-d10
Concen: 0.35 ng
RT: 12.531 min Scan# 1146
Delta R.T. -0.004 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15




Instrument :
BNA_M
ClientSampleId :
PB133674BS


Tgt Ion:152 Resp: 1626
Ion Ratio Lower Upper
152 100
151 20.6 16.7 25.1



#12
2-Methylnaphthalene
Concen: 0.35 ng
RT: 12.606 min Scan# 1163
Delta R.T. 0.000 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15


Tgt Ion:142 Resp: 1836
Ion Ratio Lower Upper
142 100
141 89.6 69.4 104.2
115 38.8 35.7 53.5








#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.764 min Scan# 1427
Delta R.T. 0.000 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15


Instrument :
BNA_M
ClientSampleId :
PB133674BS





Tgt Ion:164	Resp:	1392
Ion	Ratio	Lower Upper
164	100	
162	99.5	80.6 120.8
160	47.1	39.5 59.3




#14
2,4,6-Tribromophenol
Concen: 0.34 ng
RT: 16.237 min Scan# 1571
Delta R.T. 0.000 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15



Tgt Ion:330	Resp:	245
Ion	Ratio	Lower Upper
330	100	
332	97.6	0.0 0.0#
141	37.6	34.4 51.6









#15
2-Fluorobiphenyl
Concen: 0.36 ng
RT: 13.390 min Scan# 1291
Delta R.T. 0.000 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15




Instrument :
BNA_M
ClientSampleId :
PB133674BS


Tgt Ion:172	Resp:	2110
Ion Ratio	Lower	Upper
172	100	
171	37.1	28.2 42.4
170	25.2	20.0 30.0



#16
Acenaphthylene
Concen: 0.34 ng
RT: 14.481 min Scan# 1399
Delta R.T. -0.010 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15

Tgt Ion:152	Resp:	2145
Ion Ratio	Lower	Upper
152	100	
151	19.5	15.8 23.8
153	13.1	10.6 16.0









#17
Acenaphthene
Concen: 0.35 ng
RT: 14.824 min Scan# 1433
Delta R.T. 0.000 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15




Instrument :
BNA_M
ClientSampleId :
PB133674BS


Tgt Ion:154 Resp: 1572
Ion Ratio Lower Upper
154 100
153 111.3 83.6 125.4
152 54.6 43.9 65.9



#18
Fluorene
Concen: 0.35 ng
RT: 15.804 min Scan# 1530
Delta R.T. 0.000 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15

Tgt Ion:166 Resp: 1975
Ion Ratio Lower Upper
166 100
165 97.5 78.6 118.0
167 13.1 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.481 min Scan# 1688
Delta R.T. 0.000 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15




Instrument :
BNA_M
ClientSampleId :
PB133674BS


Tgt Ion:188 Resp: 2736
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.7 5.0 7.4#



#20
Hexachlorobenzene
Concen: 0.36 ng
RT: 16.800 min Scan# 1624
Delta R.T. 0.000 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15

Tgt Ion:284 Resp: 667
Ion Ratio Lower Upper
284 100
142 34.2 32.0 48.0
249 31.8 27.0 40.6









#21
Atrazine
Concen: 0.33 ng
RT: 19.516 min Scan# 2041
Delta R.T. 0.000 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15




Instrument :
BNA_M
ClientSampleId :
PB133674BS


Tgt Ion:200 Resp: 611
Ion Ratio Lower Upper
200 100
173 0.0 22.8 34.2#
215 0.0 38.1 57.1#



#22
Pentachlorophenol
Concen: 0.32 ng
RT: 17.130 min Scan# 1655
Delta R.T. -0.010 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15

Tgt Ion:266 Resp: 248
Ion Ratio Lower Upper
266 100
264 59.7 50.9 76.3
268 66.5 51.5 77.3









#23
Phenanthrene
Concen: 0.35 ng
RT: 17.523 min Scan# 1692
Delta R.T. 0.000 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15




Instrument :
BNA_M
ClientSampleId :
PB133674BS


Tgt Ion:	178	Resp:	2971
Ion Ratio	Lower	Upper	
178	100		
176	18.6	14.8	22.2
179	15.3	12.4	18.6



#24
Anthracene
Concen: 0.34 ng
RT: 17.619 min Scan# 1701
Delta R.T. 0.000 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15

Tgt Ion:	178	Resp:	2531
Ion Ratio	Lower	Upper	
178	100		
176	18.2	14.8	22.2
179	15.2	12.5	18.7









#25
Fluoranthene-d10
Concen: 0.34 ng
RT: 19.486 min Scan# 2035
Delta R.T. -0.005 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15




Instrument :
BNA_M
ClientSampleId :
PB133674BS


Tgt Ion:212 Resp: 2841
Ion Ratio Lower Upper
212 100
106 12.3 6.8 10.2#
104 7.0 4.1 6.1#



#26
Fluoranthene
Concen: 0.33 ng
RT: 19.516 min Scan# 2041
Delta R.T. 0.000 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15

Tgt Ion:202 Resp: 3147
Ion Ratio Lower Upper
202 100
101 11.0 5.8 8.6#
203 17.2 13.7 20.5









#27
Chrysene-d12
Concen: 0.40 ng
RT: 21.601 min Scan# 2290
Delta R.T. -0.010 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15




Instrument :
BNA_M
ClientSampleId :
PB133674BS


Tgt Ion:240 Resp: 2676
Ion Ratio Lower Upper
240 100
120 15.2 5.3 7.9#
236 28.0 21.8 32.8



#28
Pyrene
Concen: 0.35 ng
RT: 19.874 min Scan# 2113
Delta R.T. -0.005 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15

Tgt Ion:202 Resp: 3165
Ion Ratio Lower Upper
202 100
200 19.9 16.6 24.8
203 17.5 13.8 20.8





#29

Terphenyl-d14

Concen: 0.40 ng

RT: 20.061 min Scan# 2145

Delta R.T. -0.010 min

Lab File: BM028317.D

Acq: 31 Dec 2020 22:15

Tgt Ion:244 Resp: 2618

Ion Ratio Lower Upper

244 100

212 9.6 7.3 10.9





122 12.8 7.3 10.9#

Instrument :

BNA_M

ClientSampleId :

PB133674BS



#30

Benzo(a)anthracene

Concen: 0.34 ng

RT: 21.590 min Scan# 2289

Delta R.T. 0.000 min

Lab File: BM028317.D

Acq: 31 Dec 2020 22:15




Tgt Ion:228 Resp: 3042


Ion Ratio Lower Upper

228 100

226 26.7 22.3 33.5

229 21.5 15.7 23.5





#31

Chrysene

Concen: 0.35 ng

RT: 21.643 min Scan# 2294

Delta R.T. 0.000 min

Lab File: BM028317.D

Acq: 31 Dec 2020 22:15





Tgt Ion:228	Resp:	3256
Ion Ratio	Lower	Upper
228	100	
226	28.8	24.2 36.2
229	21.1	15.7 23.5

Instrument :

BNA_M

ClientSampleId :

PB133674BS



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.35 ng




RT: 21.494 min Scan# 2280


Delta R.T. 0.000 min

Lab File: BM028317.D

Acq: 31 Dec 2020 22:15


Tgt Ion:149	Resp:	1454
Ion Ratio	Lower	Upper
149	100	
167	25.5	23.2 34.8
279	4.6	3.9 5.9








#33
Indeno(1,2,3-cd)pyrene
Concen: 0.35 ng
RT: 26.310 min Scan# 3506
Delta R.T. -0.003 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15


Instrument :
BNA_M
ClientSampleId :
PB133674BS





Tgt Ion:276 Resp: 3541
Ion Ratio Lower Upper
276 100
138 26.0 13.3 19.9#
277 25.5 20.2 30.4




#34
Perylene-d12
Concen: 0.40 ng
RT: 23.934 min Scan# 2812
Delta R.T. -0.003 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15



Tgt Ion:264 Resp: 2475
Ion Ratio Lower Upper
264 100
260 25.1 19.8 29.6
265 67.6 51.4 77.0









#35
Benzo(b)fluoranthene
Concen: 0.37 ng
RT: 23.226 min Scan# 2605
Delta R.T. -0.007 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15




Instrument :
BNA_M
ClientSampleId :
PB133674BS


Tgt Ion:252 Resp: 3443
Ion Ratio Lower Upper
252 100
253 28.3 20.1 30.1
125 17.4 7.2 10.8#



#36
Benzo(k)fluoranthene
Concen: 0.36 ng
RT: 23.274 min Scan# 2619
Delta R.T. -0.003 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15

Tgt Ion:252 Resp: 3147
Ion Ratio Lower Upper
252 100
253 28.1 19.8 29.8
125 17.7 7.1 10.7#









#37
Benzo(a)pyrene
Concen: 0.37 ng
RT: 23.828 min Scan# 2781
Delta R.T. -0.007 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15




Instrument :
BNA_M
ClientSampleId :
PB133674BS


Tgt Ion:252	Resp:	2932
Ion Ratio	Lower	Upper
252	100	
253	30.8	21.3 31.9
125	21.4	8.3 12.5#



#38
Dibenzo(a,h)anthracene
Concen: 0.37 ng
RT: 26.320 min Scan# 3509
Delta R.T. -0.007 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15


Tgt Ion:278	Resp:	3076
Ion Ratio	Lower	Upper
278	100	
139	19.9	9.3 13.9#
279	30.1	21.6 32.4





#39
Benzo(g,h,i)perylene
Concen: 0.37 ng
RT: 27.042 min Scan# 3720
Delta R.T. -0.007 min
Lab File: BM028317.D
Acq: 31 Dec 2020 22:15

Instrument :
BNA_M
ClientSampleId :
PB133674BS



Tgt Ion: 276 Resp: 3090
Ion Ratio Lower Upper
276 100
277 28.0 19.8 29.8
138 26.0 11.7 17.5#

