
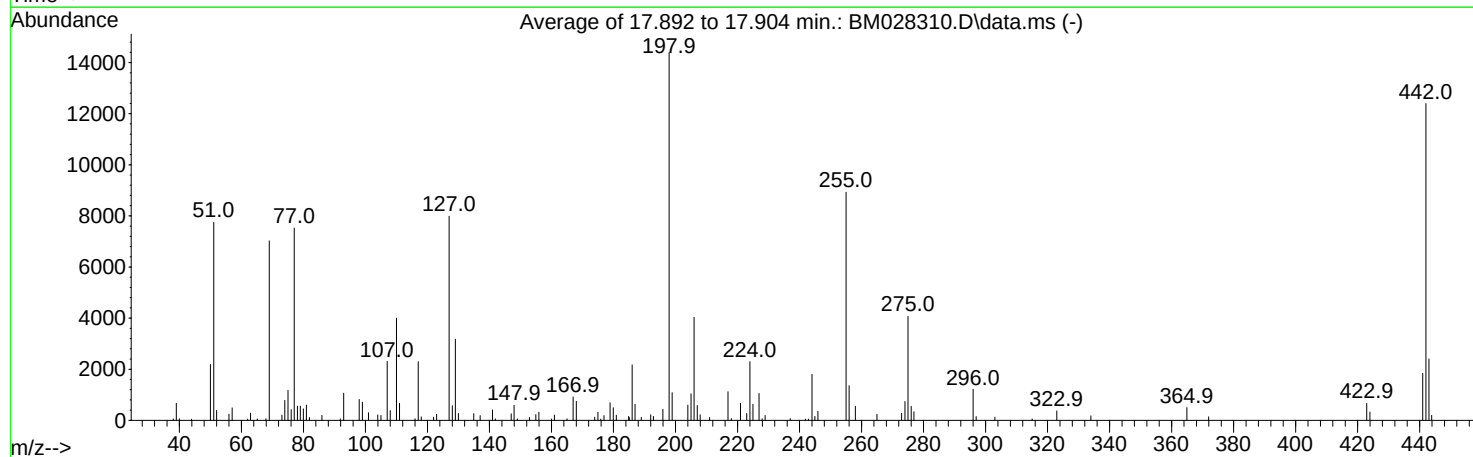


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010121\
 Data File : BM028310.D
 Acq On : 31 Dec 2020 18:02
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-SIM-BM010121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 31 16:18:03 2020

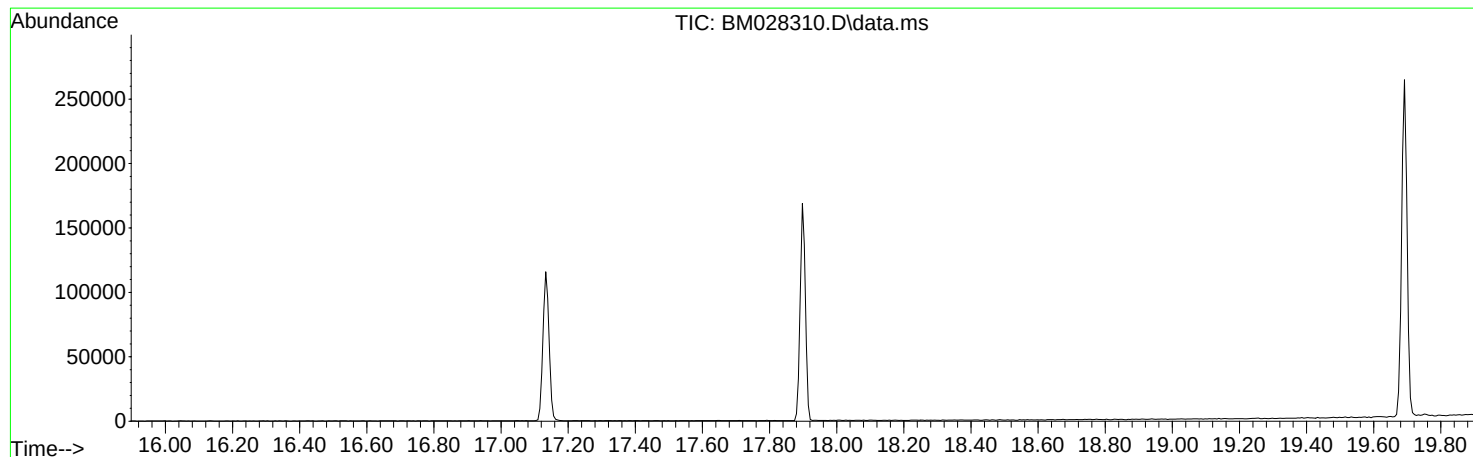

AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.9	7753	PASS
68	69	0.00	2	0.9	62	PASS
69	198	0.00	100	48.8	7022	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.5	7987	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14392	PASS
199	198	5	9	7.5	1085	PASS
275	198	10	60	28.3	4070	PASS
365	198	1	100	3.5	504	PASS
441	198	0.01	100	12.8	1840	PASS
442	442	50	100	100.0	12397	PASS
443	442	15	24	19.4	2404	PASS