


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010423\
Data File : BM038361.D
Acq On : 04 Jan 2023 09:05
Operator : CG/JU
Sample : DFTPP099
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP099

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Title : SVOA CALIBRATION
Last Update : Thu Jan 05 02:11:50 2023

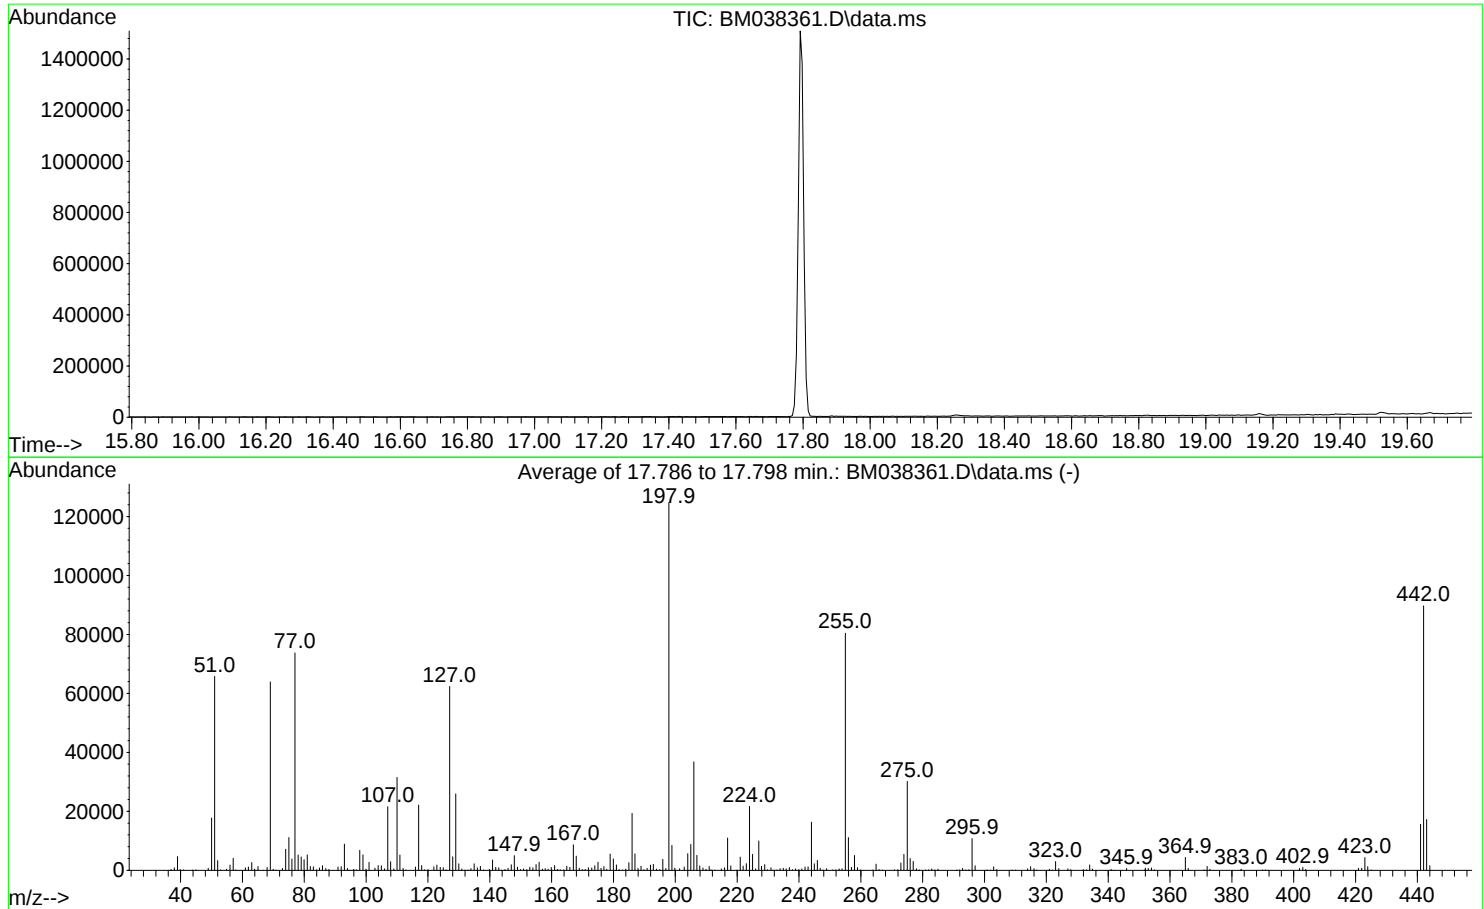

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.7	65765	PASS
68	69	0.00	2	1.5	945	PASS
69	198	0.00	100	51.2	63899	PASS
70	69	0.00	2	0.6	367	PASS
127	198	10	80	49.9	62320	PASS
197	198	0.00	2	0.5	652	PASS
198	198	100	100	100.0	124779	PASS
199	198	5	9	6.8	8433	PASS
275	198	10	60	24.2	30147	PASS
365	198	1	100	3.5	4356	PASS
441	198	0.01	100	12.5	15635	PASS
442	198	50	100	71.9	89691	PASS
443	442	15	24	19.2	17221	PASS

m/z	Abundance
39.90	158.0
44.00	242.0
73.00	337.0
77.10	272.0
192.90	251.0
206.90	1100.0
207.90	180.0
281.00	161.0

Instrument :

BNA_M

ClientSampleId :

DFTPP099

m/z	Abundance
36.90	322.0
37.90	678.0
39.00	3707.0
39.90	571.0
41.00	222.0
43.80	181.0
48.90	637.0
50.00	14226.0
51.00	53192.0
52.00	2821.0
54.90	310.0
55.90	1381.0
57.00	3297.0
57.80	172.0
60.90	582.0
61.90	905.0
63.00	1914.0
63.90	281.0
65.00	938.0
68.00	909.0
69.00	47608.0
69.90	265.0
73.00	1003.0
74.00	5504.0
75.00	8071.0
76.00	2903.0
77.00	56264.0
78.00	4261.0
79.00	3458.0
80.00	3015.0
81.00	4024.0
82.00	858.0
82.90	905.0
84.00	175.0
84.90	627.0
85.90	1218.0
87.00	402.0
87.90	341.0
90.90	812.0
92.00	877.0
92.90	6750.0
93.90	385.0
95.90	285.0
96.90	183.0
97.90	4863.0
98.90	3835.0
100.00	340.0
101.00	1868.0
102.80	551.0
103.90	1036.0
104.90	1111.0
105.90	428.0
107.00	15773.0
107.90	2107.0
108.90	328.0
110.00	22712.0
111.00	3725.0
112.00	455.0
116.00	721.0
117.00	16728.0
118.00	1119.0
118.90	249.0
119.90	181.0
121.90	863.0
122.90	1348.0
124.00	601.0
125.00	563.0
127.00	43616.0
128.00	3363.0
129.00	18672.0
130.00	1540.0
130.90	299.0
133.00	160.0
134.00	251.0
134.90	1507.0
135.90	520.0
137.00	961.0
139.90	186.0
140.90	2335.0
142.00	735.0
142.90	589.0
144.80	152.0
145.80	416.0
146.90	1298.0
147.90	3385.0
148.90	748.0
149.90	157.0
150.90	262.0
152.00	162.0
153.00	579.0
154.00	488.0
154.90	1243.0

Instrument :
BNA_M
ClientSampleId :
DFTPP099

155.90	1616.0
157.00	257.0
157.90	349.0
158.90	330.0
159.80	371.0
160.90	1174.0
161.80	273.0
162.90	181.0
164.90	910.0
165.90	718.0
167.00	5762.0
167.90	3273.0
168.90	446.0
169.90	191.0
170.80	216.0
171.90	463.0
172.90	588.0
173.90	991.0
175.00	1928.0
175.90	475.0
176.80	824.0
177.80	260.0
178.90	3397.0
179.90	2644.0
180.90	1307.0
183.90	321.0
185.00	1670.0
186.00	11456.0
186.90	3484.0
188.00	523.0
188.90	819.0
190.90	552.0
191.90	1089.0
193.00	1536.0
194.00	281.0
195.00	158.0
196.00	2841.0
196.90	438.0
197.90	76032.0
198.90	5427.0
199.80	484.0
201.50	283.0
202.90	629.0
204.00	3259.0
205.00	5493.0
206.00	22944.0
207.00	4372.0
207.90	1028.0
208.90	746.0
209.90	370.0
211.00	896.0
211.90	200.0
215.00	343.0
215.90	515.0
216.90	6766.0
218.00	1079.0
219.90	183.0
221.00	3238.0
221.90	894.0
223.00	1107.0
224.00	13571.0
225.00	3037.0
226.00	314.0
227.00	5955.0
227.90	855.0
228.90	1152.0
231.00	497.0
233.80	294.0
234.90	492.0
235.80	506.0
236.90	619.0
237.90	172.0
238.80	367.0
240.00	150.0
240.90	296.0
241.90	551.0
242.90	860.0
244.00	10765.0
244.90	1244.0
245.90	2110.0
246.80	414.0
249.00	505.0
250.90	215.0
252.90	257.0
254.00	488.0
255.00	46640.0
255.90	6793.0
256.90	732.0
257.90	2886.0
258.90	498.0
265.00	1361.0
271.90	151.0
273.00	1346.0
273.90	2862.0
275.00	16944.0
276.00	2212.0

Instrument :
BNA_M
ClientSampleId :
DFTPP099

276.90	1850.0
278.00	368.0
281.00	232.0
282.90	275.0
292.90	399.0
294.90	203.0
295.90	6090.0
297.00	956.0
303.00	604.0
304.10	168.0
313.90	272.0
314.90	665.0
316.00	393.0
321.00	213.0
323.00	1758.0
324.00	359.0
327.00	245.0
331.90	212.0
334.00	861.0
334.90	310.0
345.90	259.0
351.80	468.0
353.00	347.0
354.00	407.0
354.80	156.0
365.00	2339.0
365.90	456.0
372.00	595.0
372.90	205.0
382.80	177.0
401.80	399.0
402.90	358.0
420.90	347.0
421.90	273.0
423.00	1792.0
424.00	803.0
441.00	7808.0
442.00	42456.0
443.00	8072.0
444.00	702.0

Instrument :
BNA_M
ClientSampleId :
DFTPP099

m/z	Abundance
36.90	381.0
38.00	1024.0
39.00	5658.0
39.90	478.0
41.00	247.0
44.00	201.0
45.00	232.0
49.00	782.0
50.00	21224.0
51.00	80608.0
52.00	4178.0
53.00	256.0
54.90	371.0
56.00	2130.0
57.00	4956.0
61.00	1098.0
62.00	1362.0
63.00	3341.0
63.90	419.0
65.10	1697.0
66.90	150.0
68.00	1156.0
69.00	80720.0
69.90	410.0
70.90	169.0
72.90	924.0
74.00	8886.0
75.00	13833.0
76.00	4535.0
77.00	89960.0
78.00	6577.0
79.00	5579.0
80.00	4451.0
81.00	6406.0
81.90	1625.0
82.90	1263.0
84.00	151.0
84.90	1083.0
85.90	1884.0
87.00	735.0
88.00	370.0
90.90	1427.0
91.90	1677.0
93.00	11369.0
94.00	889.0
94.80	177.0
96.10	466.0
96.90	259.0
98.00	8957.0
98.90	6365.0
100.00	450.0
100.90	3687.0
102.90	926.0
103.90	2172.0
104.90	2044.0
106.00	583.0
107.00	26744.0
108.00	3410.0
109.00	633.0
110.00	39392.0
111.00	6369.0
111.90	642.0
112.90	228.0
115.90	1299.0
117.00	25872.0
118.00	2218.0
118.80	262.0
120.00	446.0
121.90	1553.0
122.90	2283.0
123.90	1273.0
125.00	942.0
126.10	211.0
127.00	79056.0
128.00	5600.0
129.00	31848.0
130.00	2977.0
131.00	558.0
132.00	315.0
132.90	195.0
133.90	806.0
135.00	2780.0
136.00	1023.0
137.00	1772.0
138.00	242.0
139.80	395.0
140.90	4343.0
142.00	1377.0
142.90	816.0
143.80	151.0
145.00	348.0
145.90	818.0

Instrument :
BNA_M
ClientSampleId :
DFTPP099

147.00	2461.0
148.00	6153.0
148.90	1345.0
149.90	312.0
151.00	571.0
151.80	211.0
153.00	1253.0
153.90	1161.0
155.00	2565.0
156.00	3582.0
157.10	577.0
157.90	691.0
158.80	450.0
159.90	1373.0
160.90	2146.0
162.00	515.0
162.80	197.0
163.90	183.0
164.90	1607.0
165.90	1235.0
167.00	10962.0
168.00	5894.0
169.00	779.0
169.90	154.0
170.90	360.0
171.90	1258.0
173.00	963.0
173.90	2041.0
175.00	3366.0
176.00	931.0
176.90	1638.0
177.90	337.0
178.90	6631.0
180.00	4616.0
181.00	2176.0
181.80	404.0
183.00	246.0
184.00	434.0
185.00	3245.0
186.00	24064.0
187.00	6689.0
187.90	849.0
188.90	1977.0
189.80	326.0
190.90	591.0
191.90	2125.0
193.00	2895.0
193.80	457.0
194.90	334.0
195.90	4497.0
197.00	788.0
197.90	156608.0
198.90	10005.0
199.90	921.0
201.30	732.0
202.90	1450.0
204.00	7107.0
205.00	10831.0
206.00	46288.0
207.00	7523.0
208.00	2225.0
209.00	899.0
209.90	757.0
211.00	1809.0
211.50	494.0
214.90	502.0
215.90	967.0
216.90	13140.0
218.00	1929.0
221.00	5341.0
221.90	1784.0
222.90	2978.0
224.00	26792.0
225.00	7207.0
225.90	613.0
227.00	12474.0
227.90	1681.0
228.90	2347.0
229.80	306.0
230.90	856.0
231.90	175.0
232.80	181.0
233.90	858.0
234.90	704.0
235.90	638.0
236.90	1174.0
237.90	178.0
238.90	405.0
239.90	375.0
240.90	669.0
242.00	1308.0
243.00	1526.0
244.00	18928.0
245.00	2617.0
246.00	4418.0
246.90	764.0

Instrument :
BNA_M
ClientSampleId :
DFTPP099

247.70	160.0
248.90	615.0
250.90	237.0
251.90	290.0
253.00	489.0
254.00	410.0
255.00	98096.0
256.00	14059.0
256.90	1188.0
257.90	6307.0
258.90	1171.0
259.80	277.0
264.90	2431.0
265.90	253.0
267.00	152.0
270.90	394.0
272.10	247.0
272.90	3279.0
274.00	6402.0
275.00	36368.0
275.90	4926.0
277.00	3535.0
277.90	512.0
278.80	228.0
280.90	276.0
281.90	270.0
282.90	400.0
284.00	264.0
284.90	587.0
291.00	180.0
291.80	190.0
292.90	864.0
293.90	201.0
296.00	13617.0
296.90	1875.0
300.80	231.0
303.00	1479.0
303.80	291.0
308.90	172.0
310.00	202.0
314.00	559.0
314.90	1592.0
316.00	687.0
316.90	206.0
320.90	472.0
323.00	3100.0
324.00	708.0
326.90	649.0
327.90	379.0
332.00	302.0
333.00	285.0
334.00	2190.0
334.90	384.0
340.90	559.0
346.00	771.0
352.00	1031.0
352.90	679.0
354.00	919.0
355.00	161.0
364.90	4845.0
365.90	710.0
371.10	190.0
372.00	1426.0
372.90	436.0
383.00	567.0
389.90	226.0
390.80	150.0
401.90	673.0
402.90	1020.0
403.80	346.0
421.00	697.0
421.90	720.0
423.00	5164.0
424.00	1488.0
425.10	245.0
441.00	17672.0
442.00	98744.0
443.00	19544.0
444.00	1802.0

Instrument :
BNA_M
ClientSampleId :
DFTPP099

m/z	Abundance
37.10	236.0
37.90	846.0
39.00	4582.0
40.00	251.0
44.00	260.0
44.90	240.0
49.00	573.0
50.00	17672.0
51.00	63496.0
52.00	2939.0
52.90	244.0
54.90	327.0
56.00	1828.0
57.00	4056.0
57.90	190.0
60.90	829.0
62.00	1014.0
63.00	2623.0
64.00	476.0
65.00	1215.0
68.00	770.0
69.00	63368.0
70.00	427.0
72.90	1020.0
74.00	7053.0
75.00	11465.0
76.00	3975.0
77.00	75736.0
78.00	4691.0
79.00	4532.0
79.90	3396.0
80.90	5265.0
81.90	1422.0
83.00	1346.0
83.90	245.0
84.90	624.0
85.90	1474.0
86.90	732.0
88.00	239.0
90.90	1031.0
92.00	1132.0
93.00	8460.0
93.90	639.0
95.90	427.0
96.80	193.0
98.00	6422.0
99.00	5467.0
99.90	409.0
100.90	2521.0
102.90	762.0
103.90	1656.0
104.90	1560.0
105.90	479.0
107.00	22176.0
107.90	3216.0
108.90	418.0
110.00	32424.0
110.90	5467.0
112.00	717.0
112.80	176.0
115.90	1287.0
117.00	23784.0
117.90	1492.0
120.10	189.0
121.90	1155.0
122.90	1733.0
123.90	1138.0
124.90	1202.0
125.80	192.0
127.00	64288.0
128.00	4829.0
129.00	27184.0
129.90	2134.0
130.90	497.0
133.90	606.0
134.90	2303.0
135.90	992.0
136.90	1222.0
138.00	180.0
139.90	387.0
140.90	3832.0
141.80	955.0
142.90	1093.0
143.80	159.0
144.80	212.0
146.00	797.0
146.90	1926.0
148.00	5308.0
149.00	1064.0
150.00	252.0
151.00	623.0
152.00	293.0

Instrument :
BNA_M
ClientSampleId :
DFTPP099

152.90	1277.0
153.90	800.0
155.00	1934.0
156.00	3052.0
157.00	448.0
157.90	636.0
158.80	440.0
159.90	1131.0
161.00	1466.0
161.90	453.0
162.70	168.0
163.90	219.0
164.90	1652.0
165.90	1061.0
167.00	9324.0
168.00	5195.0
169.00	846.0
169.90	321.0
170.90	275.0
171.90	740.0
172.90	889.0
174.00	1653.0
175.00	2904.0
175.90	658.0
177.00	1350.0
177.80	419.0
178.90	6554.0
180.00	4290.0
181.00	1973.0
181.80	313.0
183.90	479.0
185.00	2906.0
186.00	22368.0
187.00	6550.0
188.00	582.0
188.90	1372.0
189.90	272.0
190.90	934.0
192.00	2104.0
192.90	2413.0
194.00	502.0
194.90	286.0
196.00	3756.0
196.90	729.0
197.90	141696.0
198.90	9866.0
199.90	735.0
201.50	499.0
202.90	1285.0
204.00	6424.0
205.00	10006.0
206.00	41064.0
207.00	6576.0
207.90	1708.0
209.00	683.0
210.90	1340.0
212.80	177.0
214.80	494.0
215.90	1066.0
216.90	12955.0
217.90	1529.0
221.00	4889.0
221.90	1594.0
223.00	2729.0
224.00	24616.0
225.00	6005.0
226.00	528.0
227.00	11399.0
227.90	1538.0
228.90	2251.0
229.80	266.0
230.90	1173.0
231.90	153.0
232.90	269.0
234.00	645.0
234.90	894.0
235.90	489.0
236.90	1123.0
237.90	174.0
239.00	555.0
239.90	257.0
240.90	502.0
241.90	1430.0
243.00	1200.0
244.00	19312.0
245.00	2687.0
245.90	3457.0
246.90	906.0
247.80	227.0
248.90	615.0
251.90	158.0
252.90	714.0
253.80	637.0
255.00	96544.0
256.00	12470.0
257.00	1033.0

Instrument :
BNA_M
ClientSampleId :
DFTPP099

258.00	5823.0
258.90	988.0
259.80	223.0
263.90	253.0
264.90	2501.0
265.90	453.0
267.00	164.0
270.90	179.0
271.90	296.0
272.90	2760.0
273.90	6958.0
275.00	37128.0
276.00	4844.0
277.00	3582.0
277.90	635.0
279.00	192.0
281.00	354.0
282.00	294.0
283.00	653.0
283.80	230.0
285.00	645.0
291.90	227.0
292.90	710.0
294.00	241.0
295.00	368.0
296.00	12532.0
297.00	1834.0
300.90	205.0
302.00	175.0
302.90	1429.0
303.90	316.0
313.90	677.0
314.90	1491.0
316.00	694.0
321.00	423.0
321.90	310.0
323.00	4064.0
324.00	716.0
326.90	589.0
327.90	340.0
331.90	294.0
333.00	322.0
334.00	2449.0
334.90	574.0
341.10	403.0
341.90	152.0
346.00	857.0
352.00	1182.0
353.00	805.0
354.00	971.0
355.00	317.0
365.00	5885.0
365.90	704.0
370.90	195.0
372.00	1918.0
372.90	397.0
383.00	486.0
389.90	177.0
390.90	208.0
391.90	164.0
401.90	757.0
403.00	1533.0
403.90	483.0
421.00	1036.0
422.00	985.0
423.00	5966.0
423.90	1397.0
441.00	21424.0
442.00	127872.0
443.00	24048.0
444.00	2139.0

Instrument :
BNA_M
ClientSampleId :
DFTPP099