

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
 Data File : BM043771.D
 Acq On : 05 Jan 2024 21:39
 Operator : MA/JU
 Sample : 05953-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCFB0

Quant Time: Jan 05 23:11:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 22:31:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	207403	20.000	ng/u1	0.00
20) Naphthalene-d8	10.769	136	813035	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.598	164	469040	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.351	188	942769	20.000	ng/u1	# 0.01
79) Chrysene-d12	21.533	240	862633	20.000	ng/u1	0.01
88) Perylene-d12	23.956	264	1034130	20.000	ng/u1	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	30486	4.777	ng/uL	0.00
4) Pyridine-d5	3.799	84	346845	18.884	ng/u1	0.01
7) Phenol-d5	7.134	99	614760	26.056	ng/u1	0.02
9) Bis-(2-Chloroethyl)eth...	7.293	67	367352	24.585	ng/u1	0.00
11) 2-Chlorophenol-d4	7.487	132	485106	26.929	ng/u1	0.00
15) 4-Methylphenol-d8	8.681	113	461226	25.192	ng/u1	0.01
21) Nitrobenzene-d5	9.134	128	243706	30.981	ng/u1	0.00
24) 2-Nitrophenol-d4	9.851	143	276998	34.081	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.398	165	470940	32.823	ng/u1	0.02
31) 4-Chloroaniline-d4	10.922	131	208117	9.860	ng/u1	0.01
46) Dimethylphthalate-d6	14.022	166	1414946	33.511	ng/u1	0.00
49) Acenaphthylene-d8	14.298	160	1726179	34.463	ng/u1	0.01
54) 4-Nitrophenol-d4	14.839	143	246825	30.886	ng/u1	0.05
60) Fluorene-d10	15.592	176	1235373	35.382	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.733	200	180341	28.923	ng/u1	0.02
73) Anthracene-d10	17.451	188	1819670	34.416	ng/u1	0.01
81) Pyrene-d10	19.739	212	2063258	30.296	ng/u1	0.01
92) Benzo(a)pyrene-d12	23.797	264	2175719	34.094	ng/u1	0.02
Target Compounds						
					Qvalue	
71) Pentachlorophenol	17.004	266	88502	11.440	ng/u1	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
Data File : BM043771.D
Acq On : 05 Jan 2024 21:39
Operator : MA/JU
Sample : 05953-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCFB0

Quant Time: Jan 05 23:11:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 22:31:57 2023
Response via : Initial Calibration

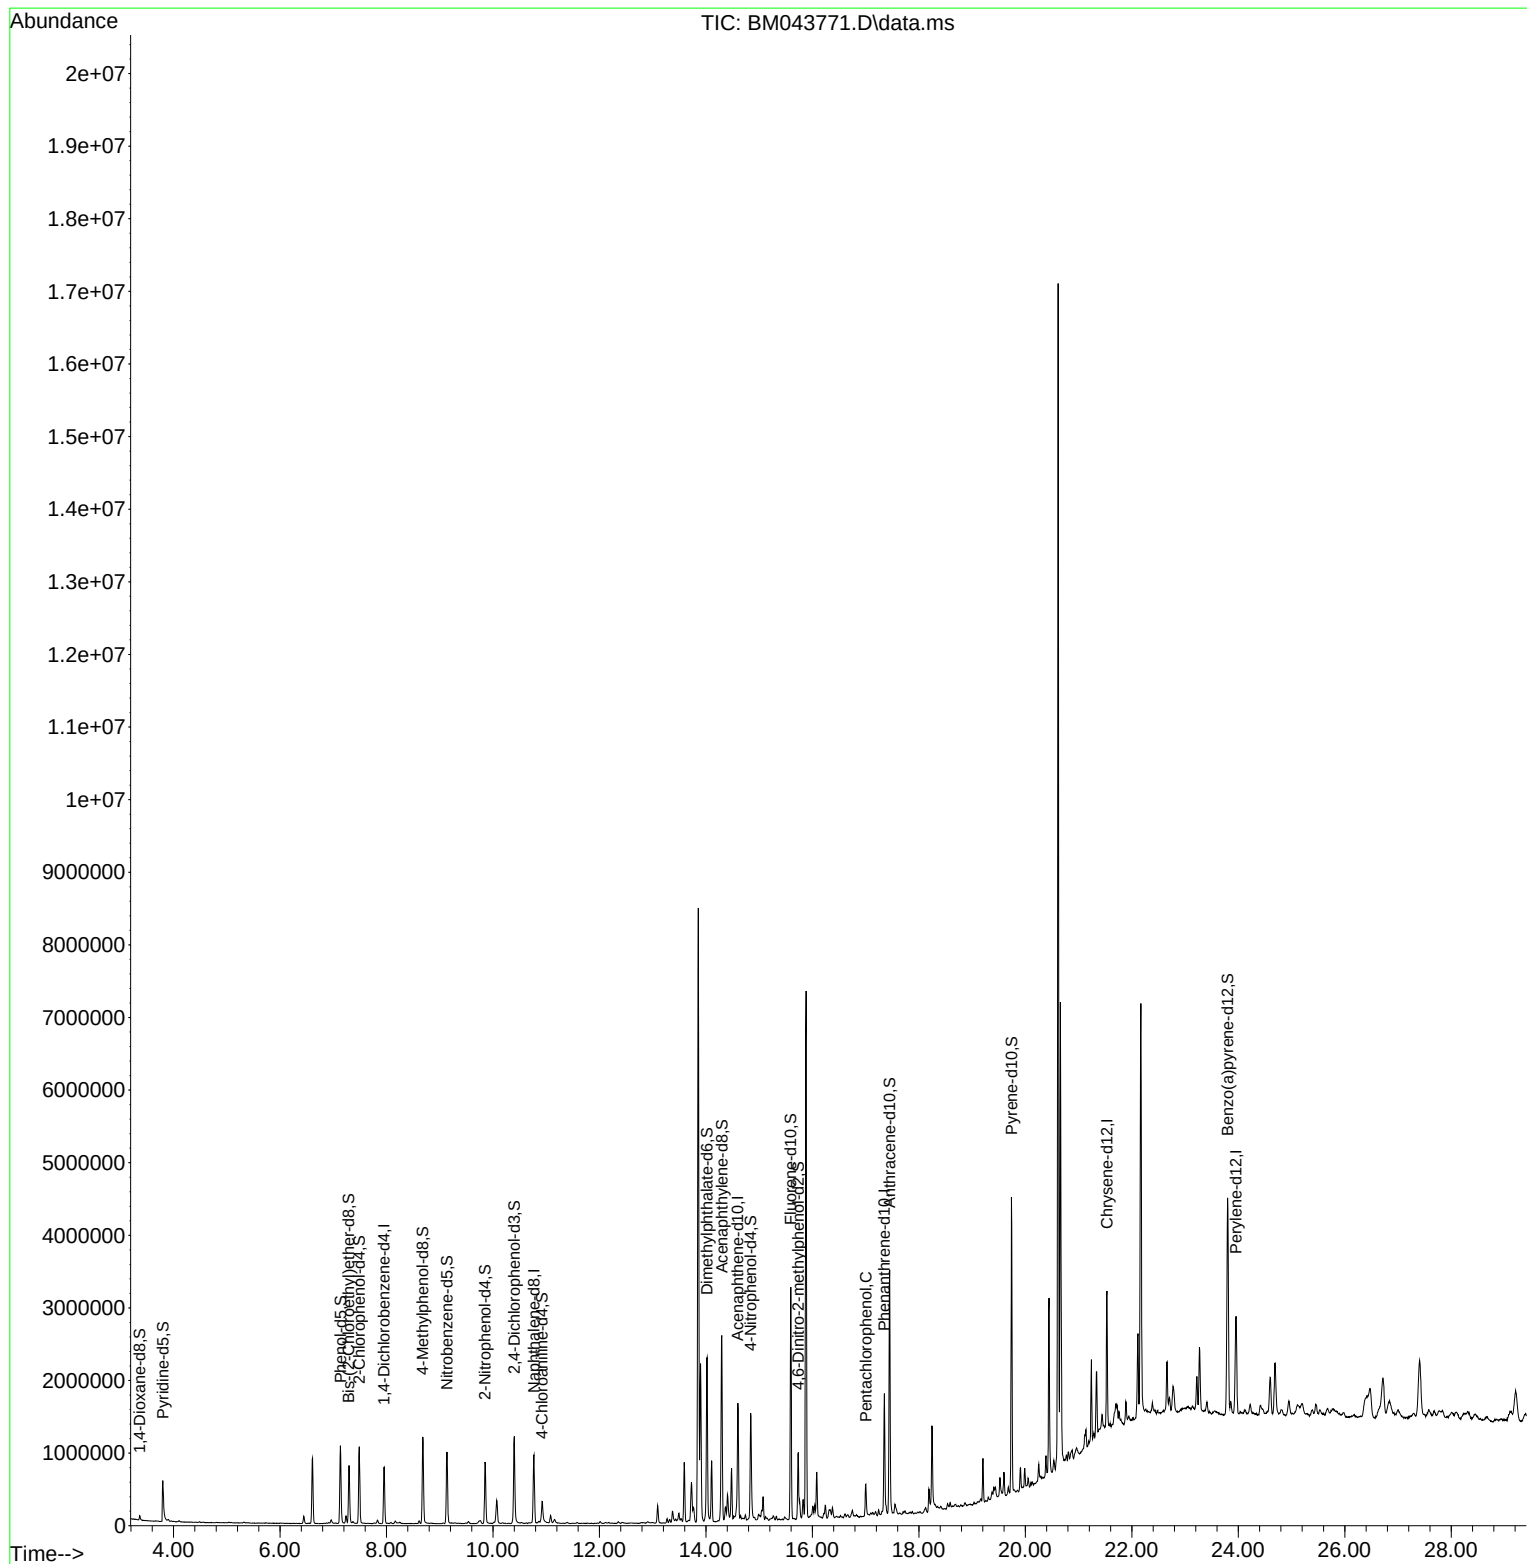

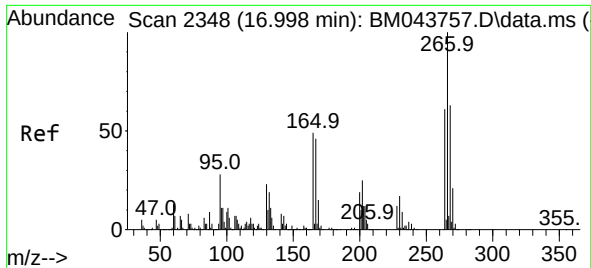

#71
 Pentachlorophenol
 Concen: 11.440 ng/ul
 RT: 17.004 min Scan# 21
 Delta R.T. 0.023 min
 Lab File: BM043771.D
 Acq: 05 Jan 2024 21:39

Instrument :
 BNA_M
 ClientSampleId :
 GCFB0

Tgt Ion	Ratio	Lower	Upper
266	100		
264	66.7	49.9	74.9
268	64.4	51.0	76.6

