

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
 Data File : BM043759.D
 Acq On : 05 Jan 2024 14:24
 Operator : MA/JU
 Sample : PB158241BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK241

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043759.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	26	29	38	rVB	97236	139945	2.32%	0.197%
2	3.787	98	102	123	rBV	1147551	1895636	31.48%	2.666%
3	4.105	152	156	162	rVB	19819	28519	0.47%	0.040%
4	7.052	653	657	659	rBV4	5648	7725	0.13%	0.011%
5	7.128	663	670	682	rBV	1334438	2174575	36.11%	3.058%
6	7.293	691	698	711	rBV	1067047	1706472	28.34%	2.400%
7	7.481	723	730	747	rVB	1346218	2188866	36.35%	3.078%
8	7.952	803	810	822	rBV	1141336	1827995	30.35%	2.571%
9	8.675	926	933	944	rBV	1528584	2525778	41.94%	3.552%
10	9.128	1003	1010	1021	rBV	1165404	2018021	33.51%	2.838%
11	9.722	1107	1111	1114	rVB6	4348	6105	0.10%	0.009%
12	9.851	1125	1133	1144	rBV	1007072	1723054	28.61%	2.423%
13	10.393	1217	1225	1237	rBV	1378640	2449447	40.67%	3.445%
14	10.763	1281	1288	1303	rBV	1453195	2476273	41.12%	3.482%
15	10.916	1306	1314	1335	rBV	1328656	2566915	42.62%	3.610%
16	12.357	1553	1559	1567	rBV2	21733	42983	0.71%	0.060%
17	13.492	1746	1752	1757	rBV2	29857	48152	0.80%	0.068%
18	13.563	1760	1764	1766	rBV5	6892	10391	0.17%	0.015%
19	14.016	1831	1841	1858	rBV	2287006	3271998	54.33%	4.601%
20	14.292	1878	1888	1901	rBV	2771496	4185259	69.50%	5.886%
21	14.475	1913	1919	1924	rBV8	11818	24071	0.40%	0.034%
22	14.598	1933	1940	1954	rVB	1966187	2945123	48.91%	4.142%
23	14.828	1973	1979	1997	rBV	895826	1738128	28.86%	2.444%
24	15.016	2007	2011	2017	rVB9	12198	22646	0.38%	0.032%
25	15.428	2076	2081	2093	rVB	89171	154010	2.56%	0.217%
26	15.592	2102	2109	2116	rBV	3415766	4853430	80.59%	6.825%
27	15.727	2126	2132	2143	rBV	907304	1385717	23.01%	1.949%
28	15.833	2146	2150	2155	rVB7	18677	30473	0.51%	0.043%
29	16.375	2238	2242	2249	rVB7	17111	28981	0.48%	0.041%
30	17.016	2345	2351	2355	rBV10	15456	33070	0.55%	0.047%
31	17.169	2373	2377	2384	rBV	37971	64990	1.08%	0.091%
32	17.345	2400	2407	2418	rBV	2274629	3277068	54.42%	4.609%
33	17.445	2418	2424	2437	rVV2	3586984	5155072	85.60%	7.250%
34	17.639	2455	2457	2460	rBV4	7719	9210	0.15%	0.013%
35	18.245	2555	2560	2569	rBV2	115086	242185	4.02%	0.341%
36	18.321	2570	2573	2583	rVB	43157	71521	1.19%	0.101%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
Data File : BM043759.D
Acq On : 05 Jan 2024 14:24
Operator : MA/JU
Sample : PB158241BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK241

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION

37	18.786	2648	2652	2655	rBV6	20965	31379	0.52%	0.044%
38	19.304	2736	2740	2748	rBV4	50688	71188	1.18%	0.100%
39	19.374	2749	2752	2755	rBV	40927	57196	0.95%	0.080%
40	19.521	2774	2777	2785	rBV6	48318	89506	1.49%	0.126%
41	19.739	2808	2814	2825	rBV	4334600	5967143	99.09%	8.392%
42	21.533	3113	3119	3130	rBV2	2557596	3717845	61.74%	5.228%
43	23.792	3497	3503	3510	rVB2	3153941	6022104	100.00%	8.469%
44	23.950	3523	3530	3540	rVB	1876567	3822590	63.48%	5.376%




Sum of corrected areas: 71108755

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
Data File : BM043759.D
Acq On : 05 Jan 2024 14:24
Operator : MA/JU
Sample : PB158241BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK241

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

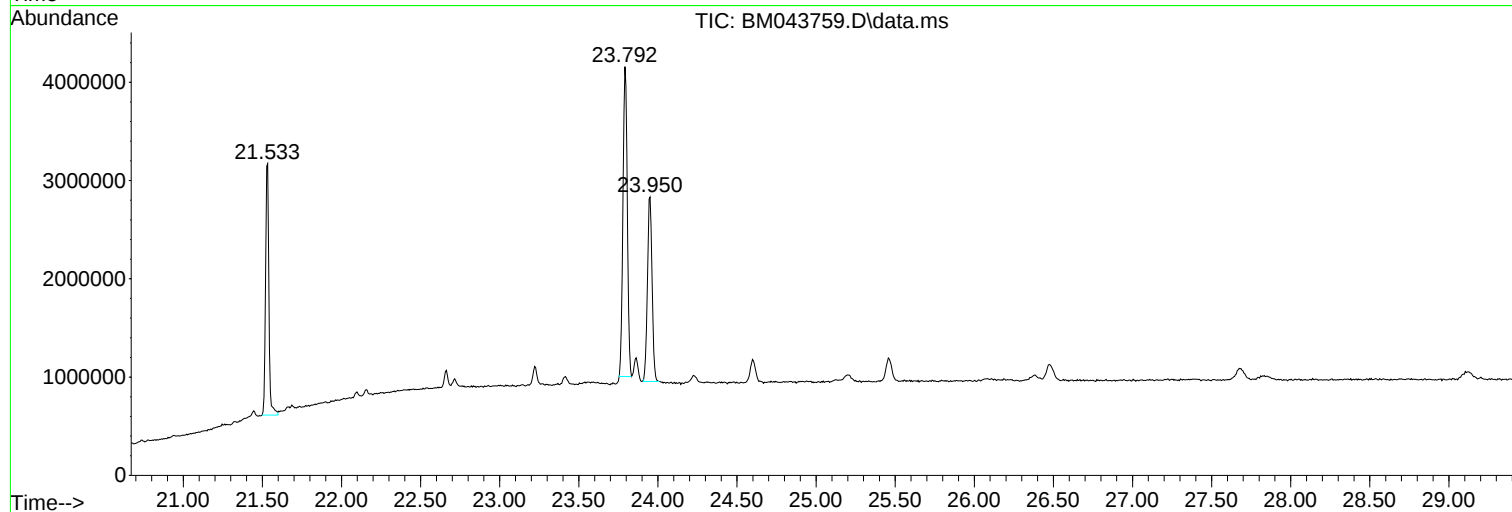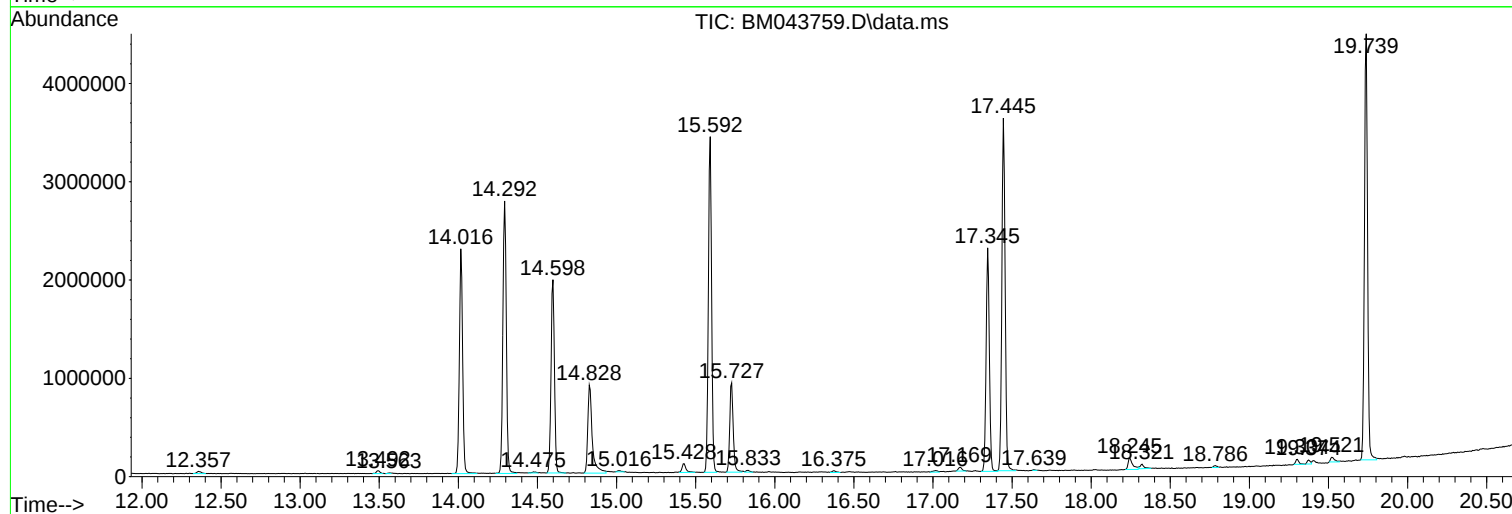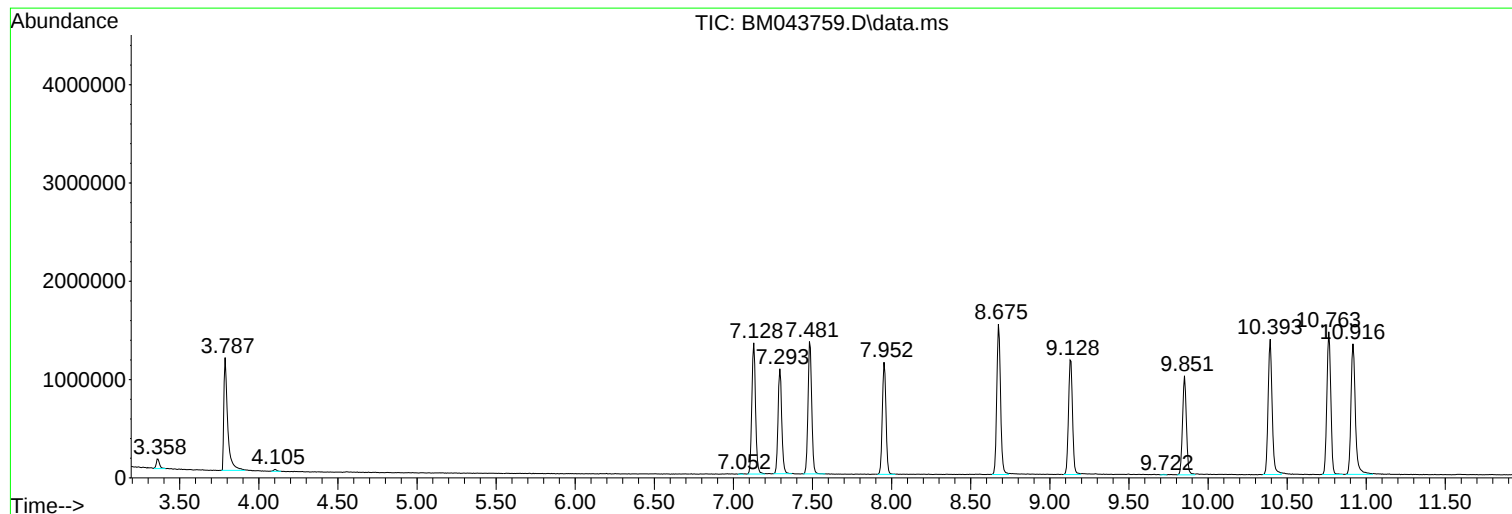

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
Data File : BM043759.D
Acq On : 05 Jan 2024 14:24
Operator : MA/JU
Sample : PB158241BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK241

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
Data File : BM043759.D
Acq On : 05 Jan 2024 14:24
Operator : MA/JU
Sample : PB158241BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK241

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc