

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
 Data File : BM043774.D
 Acq On : 06 Jan 2024 00:05
 Operator : MA/JU
 Sample : PB158241BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK241

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043774.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	26	30	38	rVB	104248	142130	2.13%	0.189%
2	3.793	99	103	128	rBV	1120630	1940204	29.03%	2.580%
3	4.104	152	156	162	rVB	25309	33108	0.50%	0.044%
4	7.134	661	671	685	rBV	1345581	2295351	34.35%	3.052%
5	7.293	692	698	712	rBV	1070496	1734435	25.96%	2.306%
6	7.487	723	731	741	rBV	1412299	2288608	34.25%	3.043%
7	7.951	803	810	818	rBV	1183051	1886505	28.23%	2.508%
8	8.681	926	934	950	rBV	1589077	2694469	40.32%	3.583%
9	9.134	1003	1011	1021	rBV	1249338	2113261	31.62%	2.810%
10	9.292	1034	1038	1042	rVB6	6854	10431	0.16%	0.014%
11	9.851	1126	1133	1146	rBV	1083320	1837433	27.50%	2.443%
12	10.392	1217	1225	1243	rBV	1468462	2698233	40.38%	3.588%
13	10.763	1281	1288	1297	rBV	1520513	2573613	38.51%	3.422%
14	10.916	1306	1314	1335	rBV	1340567	2710940	40.57%	3.605%
15	12.363	1555	1560	1569	rVB2	22104	42410	0.63%	0.056%
16	13.492	1747	1752	1760	rVB	31863	53952	0.81%	0.072%
17	13.574	1762	1766	1769	rBV5	5634	10011	0.15%	0.013%
18	14.016	1835	1841	1854	rBV	2301930	3430734	51.34%	4.562%
19	14.292	1882	1888	1901	rBV	2976378	4475018	66.97%	5.950%
20	14.486	1914	1921	1929	rBV2	15114	38348	0.57%	0.051%
21	14.598	1933	1940	1956	rVB	2204535	3171400	47.46%	4.217%
22	14.839	1974	1981	1998	rBV	930648	1860301	27.84%	2.474%
23	15.016	2007	2011	2017	rVB9	10287	16590	0.25%	0.022%
24	15.204	2040	2043	2046	rBV5	4866	7874	0.12%	0.010%
25	15.239	2046	2049	2056	rVB9	4724	7903	0.12%	0.011%
26	15.592	2102	2109	2125	rBV	3609729	5245759	78.50%	6.975%
27	15.727	2125	2132	2143	rBV	1048850	1598271	23.92%	2.125%
28	15.833	2146	2150	2154	rVB5	19103	35248	0.53%	0.047%
29	16.157	2203	2205	2210	rVB6	6374	7132	0.11%	0.009%
30	16.380	2238	2243	2246	rBV4	13979	21245	0.32%	0.028%
31	17.010	2344	2350	2359	rBV6	35540	83781	1.25%	0.111%
32	17.139	2369	2372	2375	rBV4	6932	8276	0.12%	0.011%
33	17.351	2401	2408	2418	rBV	2436141	3533616	52.88%	4.699%
34	17.451	2418	2425	2439	rBV	3791826	5599562	83.80%	7.446%
35	18.245	2556	2560	2569	rBV2	50837	102705	1.54%	0.137%
36	19.303	2737	2740	2748	rVB3	51067	69832	1.05%	0.093%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
Data File : BM043774.D
Acq On : 06 Jan 2024 00:05
Operator : MA/JU
Sample : PB158241BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK241

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION

37	19.374	2749	2752	2759	rBV	42959	70615	1.06%	0.094%
38	19.739	2808	2814	2823	rBV	4677778	6251447	93.55%	8.312%
39	21.533	3114	3119	3130	rBV	2811471	3692148	55.25%	4.909%
40	23.797	3497	3504	3511	rBV2	3417238	6682363	100.00%	8.885%
41	23.956	3524	3531	3541	rVB	1918114	4131874	61.83%	5.494%




Sum of corrected areas: 75207136

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
Data File : BM043774.D
Acq On : 06 Jan 2024 00:05
Operator : MA/JU
Sample : PB158241BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK241

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

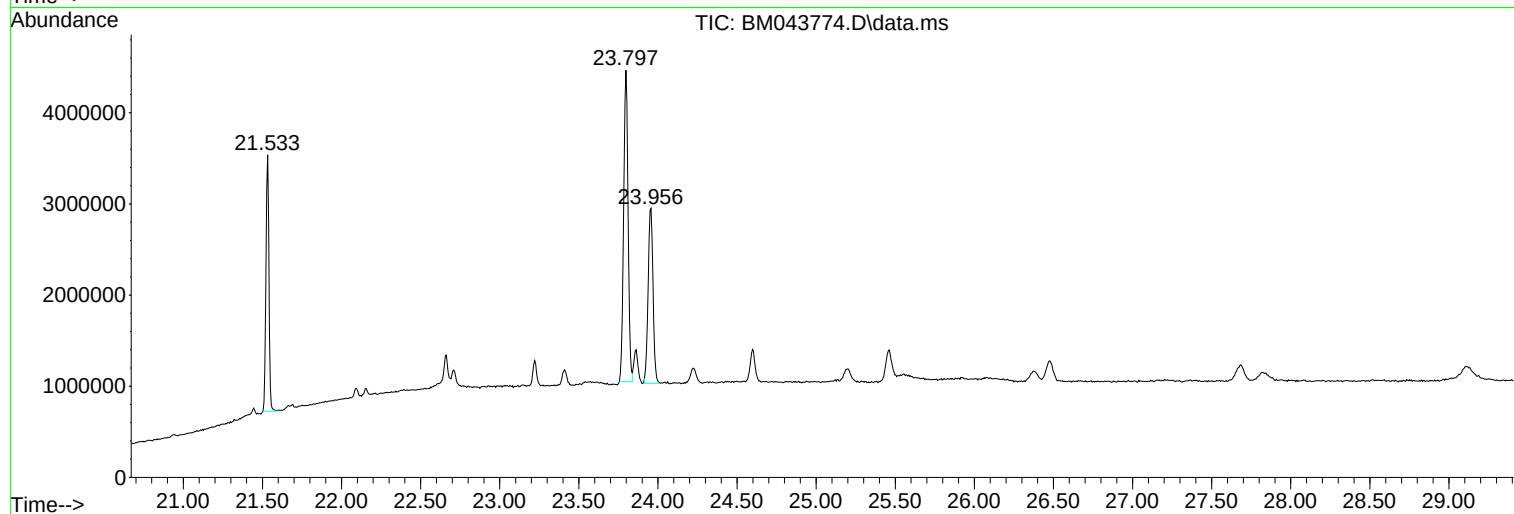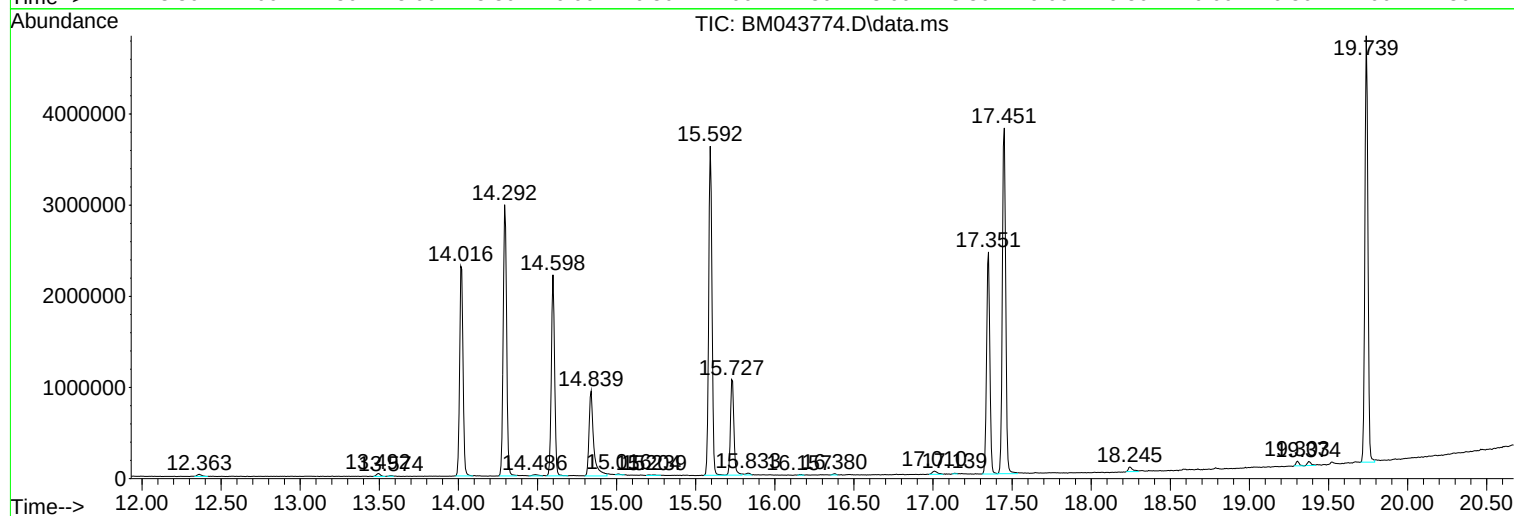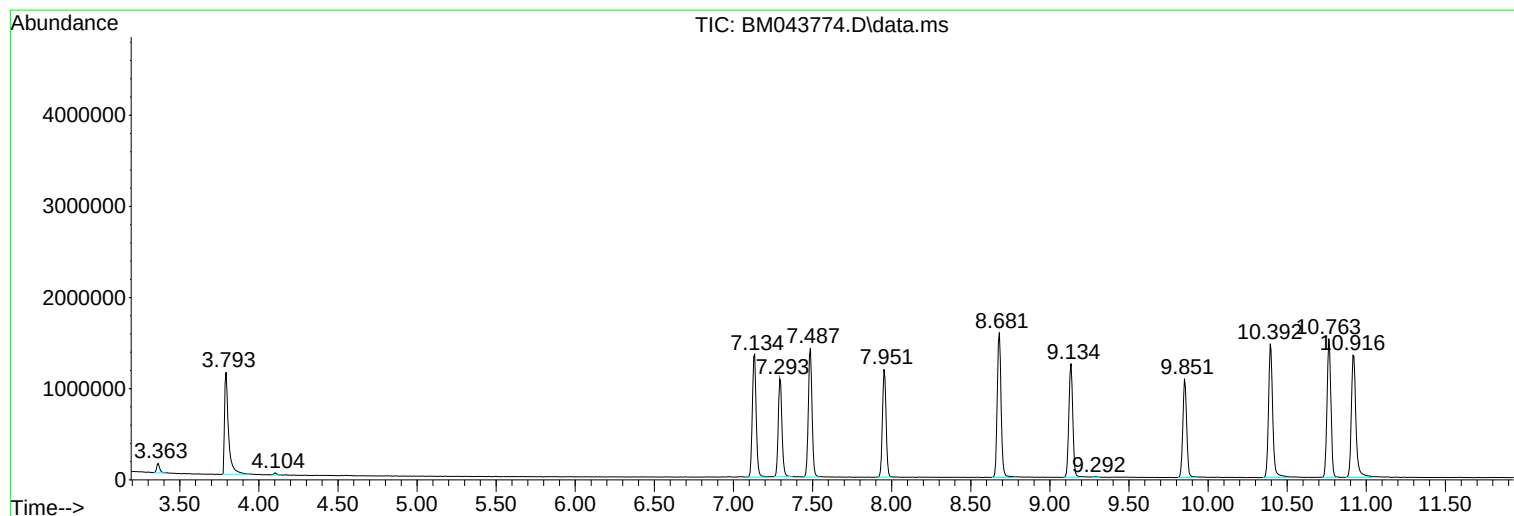

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
Data File : BM043774.D
Acq On : 06 Jan 2024 00:05
Operator : MA/JU
Sample : PB158241BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK241

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
Data File : BM043774.D
Acq On : 06 Jan 2024 00:05
Operator : MA/JU
Sample : PB158241BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK241

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------