

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
 Data File : BM043778.D
 Acq On : 06 Jan 2024 02:31
 Operator : MA/JU
 Sample : 05919-15MEDL2 200X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCF47MEDL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043778.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.105	153	156	163	rVB	20649	27171	0.69%	0.136%
2	6.816	613	617	620	rBV5	2974	3959	0.10%	0.020%
3	6.975	639	644	645	rBV5	2367	4050	0.10%	0.020%
4	7.010	647	650	653	rBV5	3176	5110	0.13%	0.026%
5	7.052	653	657	661	rVB6	7066	8478	0.21%	0.043%
6	7.305	697	700	705	rBV6	3918	7144	0.18%	0.036%
7	7.616	752	753	756	rBV2	4114	4823	0.12%	0.024%
8	7.952	801	810	823	rBV	1057258	1777280	44.92%	8.911%
9	8.099	833	835	840	rVB6	4163	6321	0.16%	0.032%
10	8.657	928	930	933	rBV4	3711	4857	0.12%	0.024%
11	8.693	933	936	942	rVB8	4246	7469	0.19%	0.037%
12	8.834	958	960	964	rVB5	3545	4351	0.11%	0.022%
13	9.093	1002	1004	1007	rBV4	3370	4160	0.11%	0.021%
14	9.487	1068	1071	1072	rBV3	5005	4674	0.12%	0.023%
15	10.440	1231	1233	1236	rBV4	3529	4251	0.11%	0.021%
16	10.763	1280	1288	1304	rBV	1356001	2485918	62.83%	12.465%
17	11.987	1493	1496	1500	rVB6	3483	4196	0.11%	0.021%
18	12.334	1551	1555	1559	rBV7	4131	4730	0.12%	0.024%
19	12.939	1655	1658	1661	rBV5	3694	4236	0.11%	0.021%
20	13.328	1720	1724	1728	rBV7	3578	5162	0.13%	0.026%
21	13.498	1746	1753	1760	rBV4	16790	33299	0.84%	0.167%
22	13.798	1801	1804	1808	rBV4	3680	5637	0.14%	0.028%
23	14.033	1840	1844	1847	rBV4	7831	9877	0.25%	0.050%
24	14.245	1876	1880	1881	rBV3	3840	5115	0.13%	0.026%
25	14.298	1884	1889	1892	rVB3	9313	15401	0.39%	0.077%
26	14.481	1916	1920	1926	rBV4	22623	39943	1.01%	0.200%
27	14.598	1933	1940	1957	rBV	2066075	3188839	80.59%	15.989%
28	15.110	2023	2027	2029	rBV4	6334	6716	0.17%	0.034%
29	15.163	2033	2036	2039	rBV5	3333	4442	0.11%	0.022%
30	15.375	2068	2072	2075	rBV5	4743	8838	0.22%	0.044%
31	15.428	2080	2081	2087	rVB6	10510	10720	0.27%	0.054%
32	15.533	2097	2099	2104	rVB6	3809	4329	0.11%	0.022%
33	15.598	2106	2110	2116	rBV5	14460	27263	0.69%	0.137%
34	15.704	2121	2128	2133	rBV	38060	61043	1.54%	0.306%
35	15.839	2148	2151	2158	rVV6	10561	17223	0.44%	0.086%
36	15.892	2158	2160	2163	rVB4	3885	4041	0.10%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
Data File : BM043778.D
Acq On : 06 Jan 2024 02:31
Operator : MA/JU
Sample : 05919-15MEDL2 200X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF47MEDL2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION

37	16.239	2217	2219	2224	rVB6	3968	4422	0.11%	0.022%
38	16.322	2226	2233	2238	rBV2	26247	50049	1.26%	0.251%
39	16.469	2256	2258	2260	rBV3	5923	4577	0.12%	0.023%
40	16.998	2343	2348	2361	rBV	376242	658467	16.64%	3.302%
41	17.145	2368	2373	2377	rBV2	28731	44195	1.12%	0.222%
42	17.351	2401	2408	2421	rBV	2315431	3634781	91.87%	18.225%
43	17.445	2422	2424	2429	rVB2	23263	37288	0.94%	0.187%
44	18.239	2556	2559	2565	rBV5	36336	62688	1.58%	0.314%
45	21.527	3114	3118	3127	rBV	2756191	3669562	92.74%	18.400%
46	23.950	3524	3530	3539	rVB	1924216	3956651	100.00%	19.839%




Sum of corrected areas: 19943746

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
Data File : BM043778.D
Acq On : 06 Jan 2024 02:31
Operator : MA/JU
Sample : 05919-15MEDL2 200X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF47MEDL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

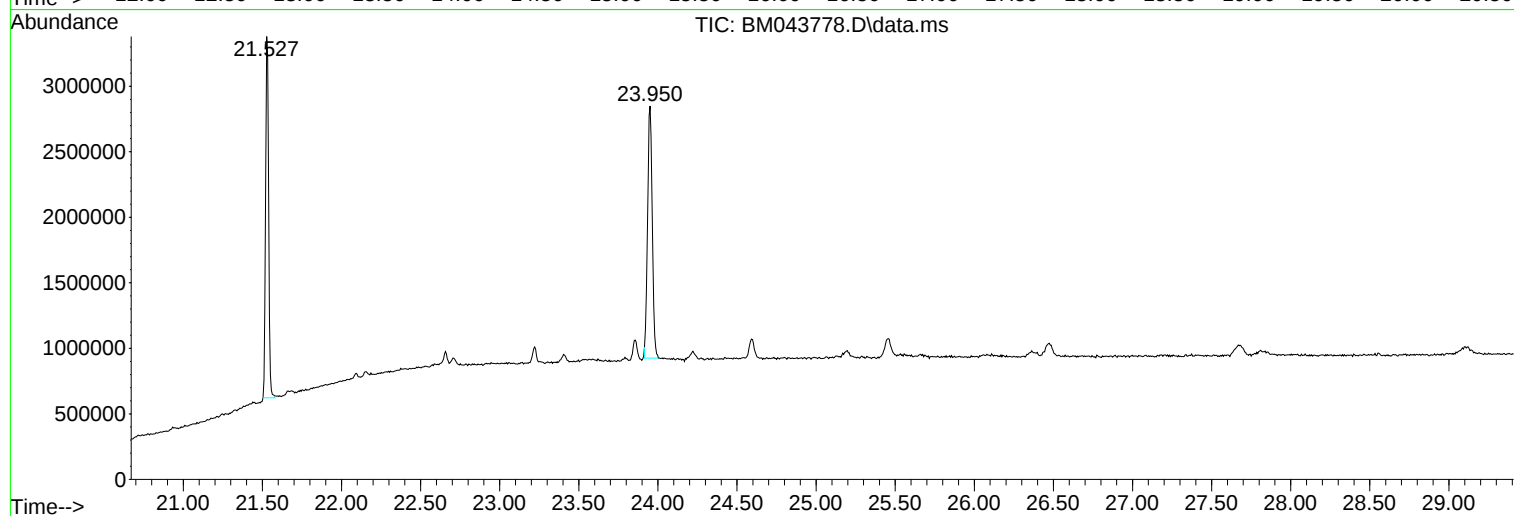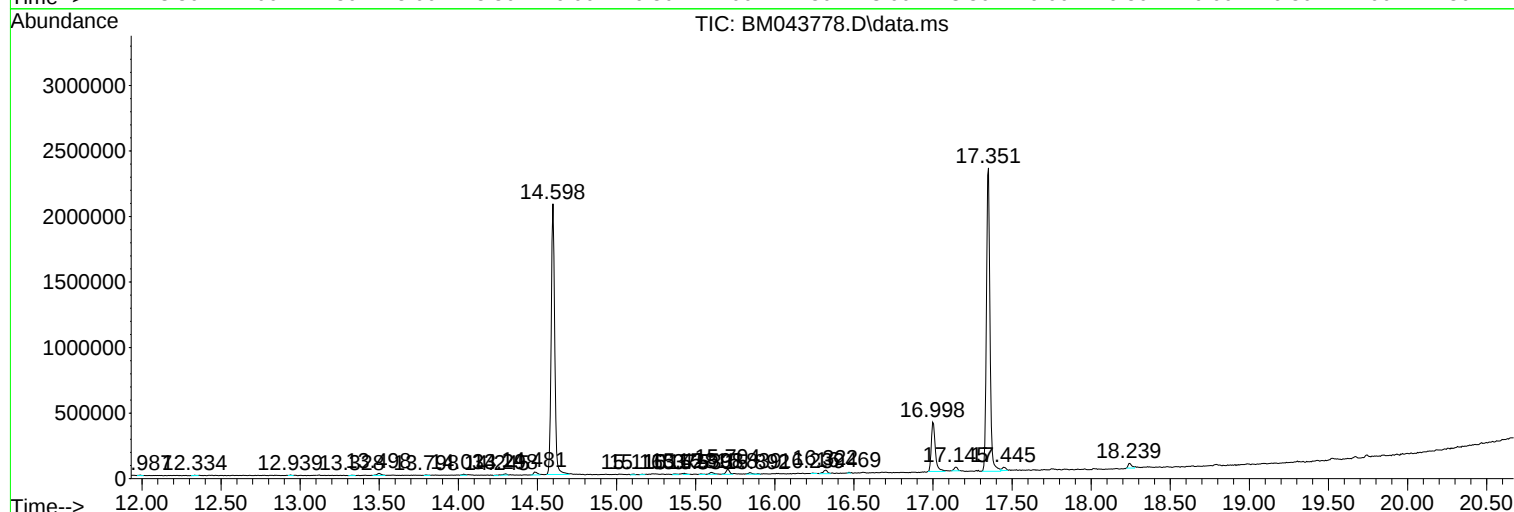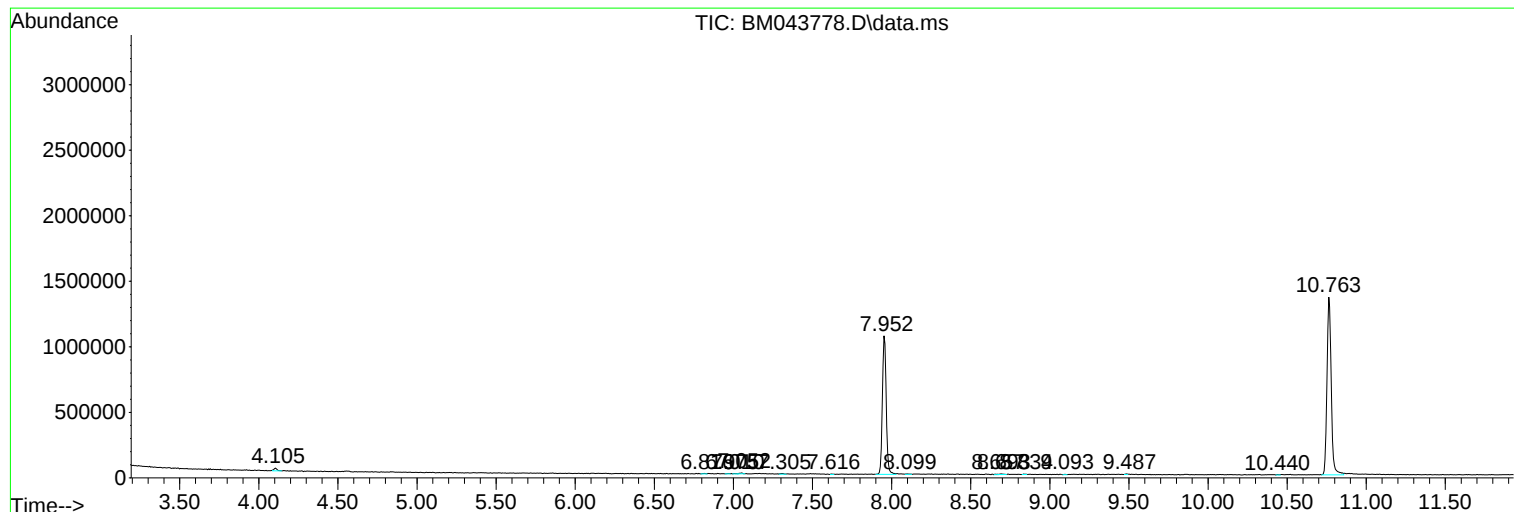

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
Data File : BM043778.D
Acq On : 06 Jan 2024 02:31
Operator : MA/JU
Sample : 05919-15MEDL2 200X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF47MEDL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
Data File : BM043778.D
Acq On : 06 Jan 2024 02:31
Operator : MA/JU
Sample : 05919-15MEDL2 200X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF47MEDL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc