

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
 Data File : BM043781.D
 Acq On : 06 Jan 2024 04:20
 Operator : MA/JU
 Sample : 05952-08MEDL 20X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCF91MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043781.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.846	110	112	113	rBV2	6330	5037	0.11%	0.020%
2	4.104	152	156	161	rVB	18586	25277	0.54%	0.102%
3	5.593	406	409	412	rVB5	4027	5731	0.12%	0.023%
4	7.051	653	657	661	rVB5	7708	9986	0.21%	0.040%
5	7.139	667	672	682	rVB	30486	68432	1.46%	0.276%
6	7.298	693	699	707	rVB	32169	58556	1.25%	0.236%
7	7.487	725	731	741	rBV2	39347	75445	1.61%	0.304%
8	7.951	803	810	820	rBV	1024019	1697527	36.17%	6.843%
9	8.686	930	935	942	rBV	32602	72831	1.55%	0.294%
10	9.145	1006	1013	1018	rBV	31067	61100	1.30%	0.246%
11	9.498	1066	1073	1077	rVB10	4668	10044	0.21%	0.040%
12	9.857	1129	1134	1143	rBV3	24257	52658	1.12%	0.212%
13	9.998	1155	1158	1162	rBV6	3181	5487	0.12%	0.022%
14	10.428	1224	1231	1239	rBV3	25634	74638	1.59%	0.301%
15	10.763	1280	1288	1303	rBV	1311953	2325667	49.55%	9.375%
16	10.957	1314	1321	1328	rBV4	13349	35302	0.75%	0.142%
17	11.992	1494	1497	1503	rVB8	5424	7321	0.16%	0.030%
18	13.368	1728	1731	1735	rVB6	5040	7002	0.15%	0.028%
19	13.498	1747	1753	1757	rBV5	15437	27182	0.58%	0.110%
20	13.851	1809	1813	1818	rBV5	38984	59818	1.27%	0.241%
21	14.021	1835	1842	1853	rBV	73164	138811	2.96%	0.560%
22	14.104	1853	1856	1862	rVV6	10687	20727	0.44%	0.084%
23	14.292	1882	1888	1900	rBV	100690	169495	3.61%	0.683%
24	14.404	1903	1907	1914	rVB9	14813	26194	0.56%	0.106%
25	14.480	1914	1920	1930	rBV10	35773	69399	1.48%	0.280%
26	14.598	1933	1940	1958	rBV	1833049	2940138	62.65%	11.852%
27	14.874	1980	1987	1991	rBV9	9717	26399	0.56%	0.106%
28	14.951	1997	2000	2004	rBV6	5084	6755	0.14%	0.027%
29	15.151	2031	2034	2038	rBV6	5824	8368	0.18%	0.034%
30	15.233	2040	2048	2055	rBV3	38597	86843	1.85%	0.350%
31	15.368	2068	2071	2072	rBV3	7798	7369	0.16%	0.030%
32	15.421	2076	2080	2086	rVB4	23206	38806	0.83%	0.156%
33	15.539	2095	2100	2103	rBV4	13487	22749	0.48%	0.092%
34	15.592	2104	2109	2120	rBV	127866	221186	4.71%	0.892%
35	15.698	2122	2127	2131	rBV	39561	62742	1.34%	0.253%
36	16.998	2342	2348	2359	rBV	3092042	4693108	100.00%	18.918%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
Data File : BM043781.D
Acq On : 06 Jan 2024 04:20
Operator : MA/JU
Sample : 05952-08MEDL 20X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF91MEDL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION

37	17.133	2368	2371	2376	rVB6	54070	81360	1.73%	0.328%
38	17.345	2401	2407	2415	rBV	2287664	3425354	72.99%	13.807%
39	17.445	2420	2424	2430	rBV2	147778	223556	4.76%	0.901%
40	19.739	2811	2814	2817	rBV	169919	201523	4.29%	0.812%
41	21.444	3101	3104	3110	rVB	230984	270774	5.77%	1.091%
42	21.527	3113	3118	3127	rVV2	2619996	3556553	75.78%	14.336%
43	23.950	3524	3530	3542	rVB	1893119	3824834	81.50%	15.418%




Sum of corrected areas: 24808084

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
Data File : BM043781.D
Acq On : 06 Jan 2024 04:20
Operator : MA/JU
Sample : 05952-08MEDL 20X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF91MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

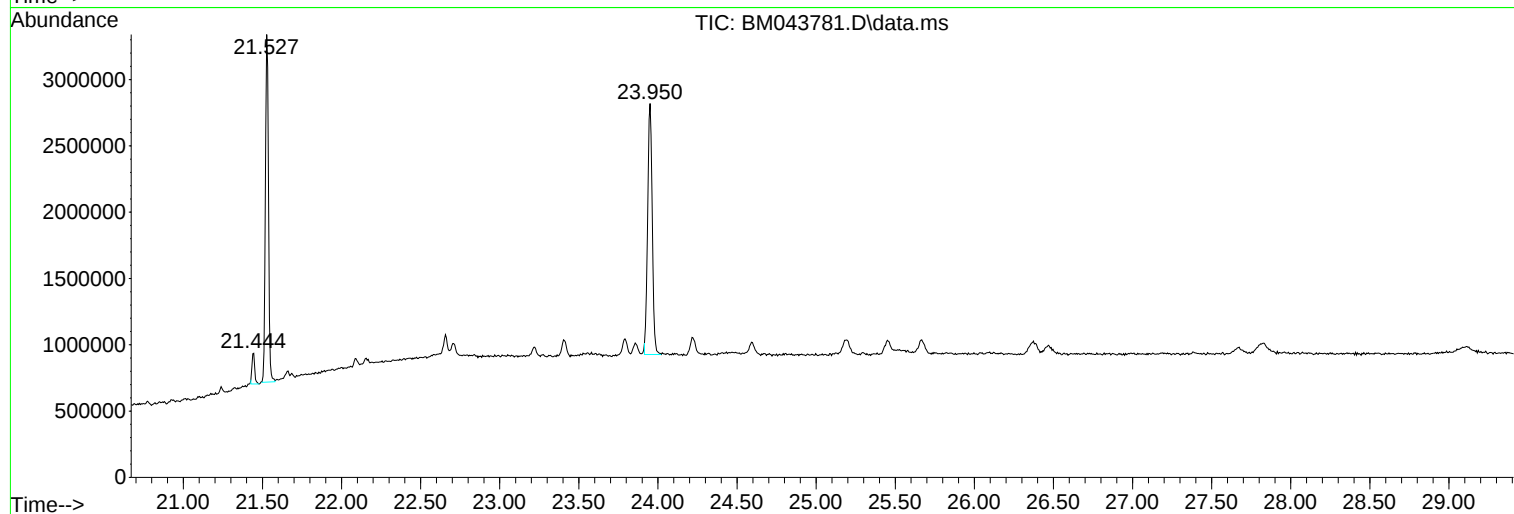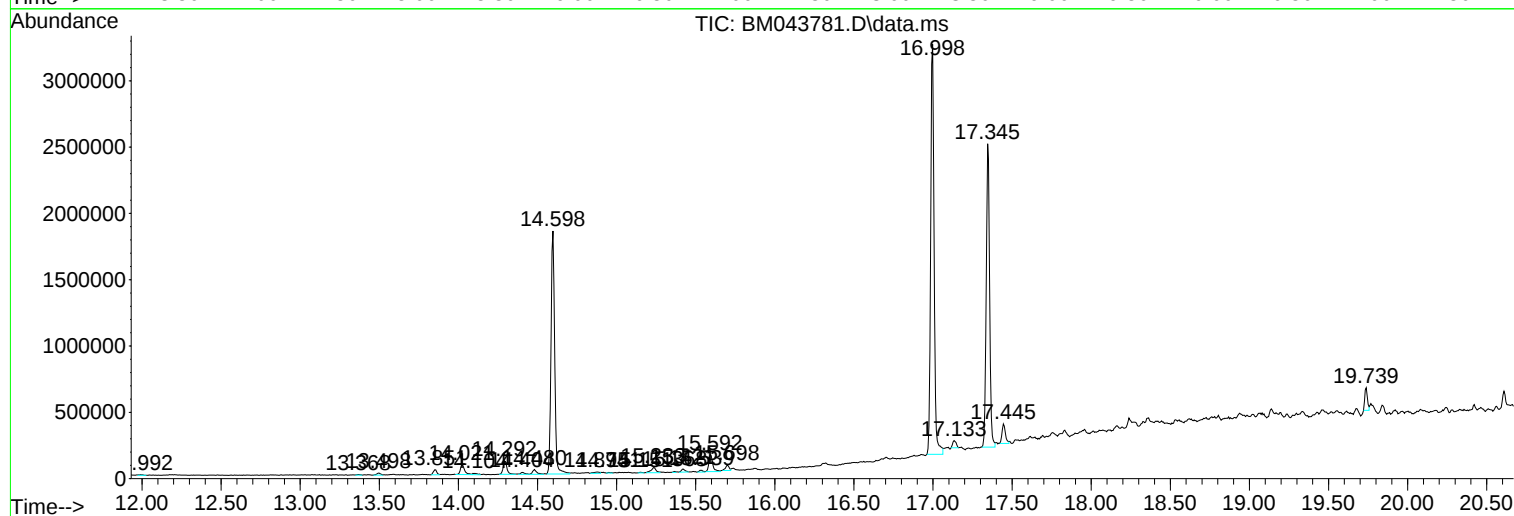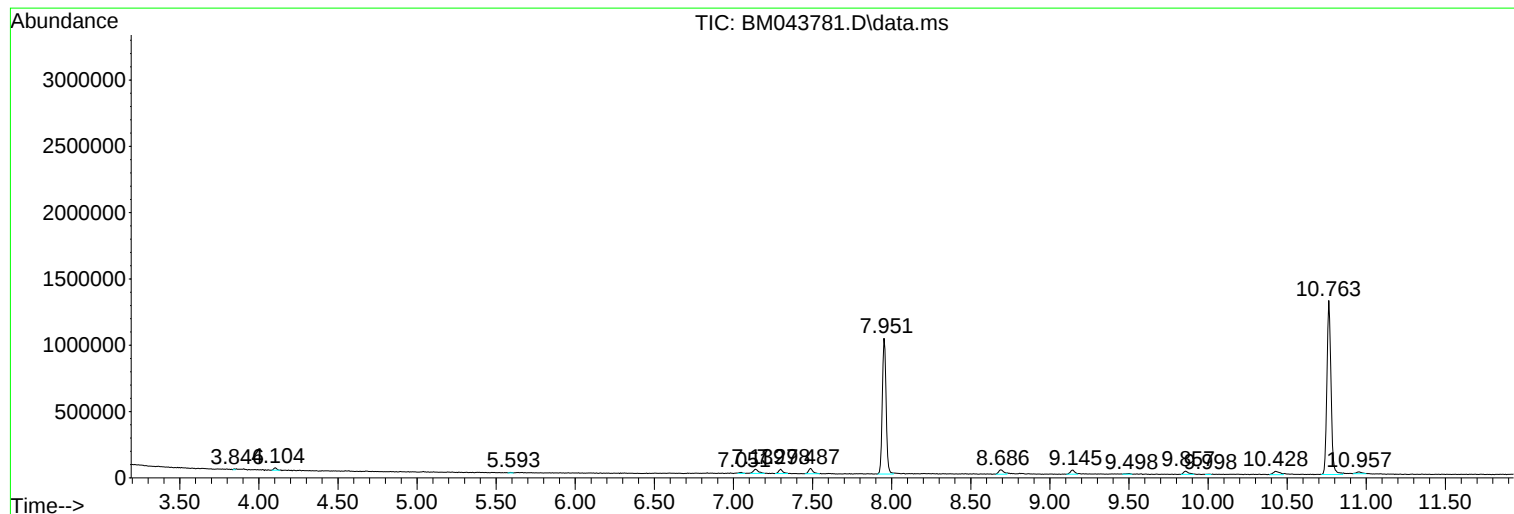

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
Data File : BM043781.D
Acq On : 06 Jan 2024 04:20
Operator : MA/JU
Sample : 05952-08MEDL 20X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF91MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
Data File : BM043781.D
Acq On : 06 Jan 2024 04:20
Operator : MA/JU
Sample : 05952-08MEDL 20X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF91MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------