

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
 Data File : BM043783.D
 Acq On : 06 Jan 2024 05:32
 Operator : MA/JU
 Sample : 05952-14MEDL2 200X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCF97MEDL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043783.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.105	152	156	160	rVB	19954	28619	0.71%	0.138%
2	5.940	466	468	472	rVB5	3739	4096	0.10%	0.020%
3	6.822	615	618	620	rBV4	3359	4049	0.10%	0.020%
4	7.046	653	656	660	rVB6	3995	5901	0.15%	0.029%
5	7.951	799	810	826	rBV	1036020	1742145	43.43%	8.430%
6	8.087	832	833	838	rVB5	3953	4928	0.12%	0.024%
7	8.692	934	936	938	rBV3	4515	4600	0.11%	0.022%
8	9.122	1005	1009	1011	rBV5	3860	5900	0.15%	0.029%
9	9.151	1011	1014	1017	rVV4	4800	4582	0.11%	0.022%
10	9.787	1120	1122	1127	rBV6	2688	5357	0.13%	0.026%
11	9.869	1133	1136	1140	rVB5	4010	5544	0.14%	0.027%
12	10.110	1174	1177	1179	rBV4	3655	4735	0.12%	0.023%
13	10.763	1281	1288	1309	rBV	1256166	2331709	58.13%	11.283%
14	11.545	1419	1421	1425	rBV4	3374	5313	0.13%	0.026%
15	12.286	1542	1547	1550	rBV7	2194	4135	0.10%	0.020%
16	13.498	1747	1753	1758	rBV3	23359	39704	0.99%	0.192%
17	13.857	1809	1814	1816	rBV6	3611	5181	0.13%	0.025%
18	13.969	1831	1833	1838	rBV6	4188	6406	0.16%	0.031%
19	14.027	1839	1843	1847	rVV2	7071	12508	0.31%	0.061%
20	14.063	1847	1849	1854	rVB5	10517	13168	0.33%	0.064%
21	14.292	1883	1888	1893	rBV3	12609	23448	0.58%	0.113%
22	14.374	1900	1902	1904	rVB3	5724	4611	0.11%	0.022%
23	14.398	1904	1906	1907	rBV2	4858	5015	0.13%	0.024%
24	14.421	1907	1910	1913	rVB5	6290	9253	0.23%	0.045%
25	14.492	1918	1922	1923	rVV4	4956	6350	0.16%	0.031%
26	14.510	1923	1925	1929	rVB4	5592	5964	0.15%	0.029%
27	14.598	1933	1940	1956	rVV	1837893	2934477	73.16%	14.200%
28	14.810	1973	1976	1979	rBV5	6265	10148	0.25%	0.049%
29	14.986	2002	2006	2010	rBV7	9460	14065	0.35%	0.068%
30	15.416	2077	2079	2084	rVB6	9419	12435	0.31%	0.060%
31	15.604	2106	2111	2114	rBV4	16235	27487	0.69%	0.133%
32	15.798	2142	2144	2145	rBV2	4831	4059	0.10%	0.020%
33	15.839	2145	2151	2161	rVB3	49236	109651	2.73%	0.531%
34	15.927	2164	2166	2168	rBV3	6743	5635	0.14%	0.027%
35	16.051	2185	2187	2191	rVB4	9836	10606	0.26%	0.051%
36	16.086	2191	2193	2194	rBV2	6268	4409	0.11%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
Data File : BM043783.D
Acq On : 06 Jan 2024 05:32
Operator : MA/JU
Sample : 05952-14MEDL2 200X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF97MEDL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION

37	16.151	2201	2204	2205	rBV3	10492	12216	0.30%	0.059%
38	16.321	2227	2233	2239	rBV2	112652	176372	4.40%	0.853%
39	16.421	2246	2250	2252	rBV5	10943	16065	0.40%	0.078%
40	16.451	2252	2255	2265	rVV5	16915	48722	1.21%	0.236%
41	16.998	2342	2348	2359	rBV	780733	1228157	30.62%	5.943%
42	17.145	2368	2373	2377	rBV	110446	167239	4.17%	0.809%
43	17.345	2401	2407	2420	rBV	2306869	3517561	87.70%	17.022%
44	17.751	2473	2476	2483	rBV4	23969	41133	1.03%	0.199%
45	18.239	2556	2559	2564	rBV5	33545	55037	1.37%	0.266%
46	19.062	2696	2699	2702	rBV	33768	36958	0.92%	0.179%
47	19.145	2709	2713	2717	rBV	26567	40195	1.00%	0.195%
48	21.527	3113	3118	3131	rBV	2778843	3888437	96.95%	18.816%
49	23.950	3523	3530	3539	rVB	1919222	4010926	100.00%	19.409%




Sum of corrected areas: 20665211

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
Data File : BM043783.D
Acq On : 06 Jan 2024 05:32
Operator : MA/JU
Sample : 05952-14MEDL2 200X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF97MEDL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

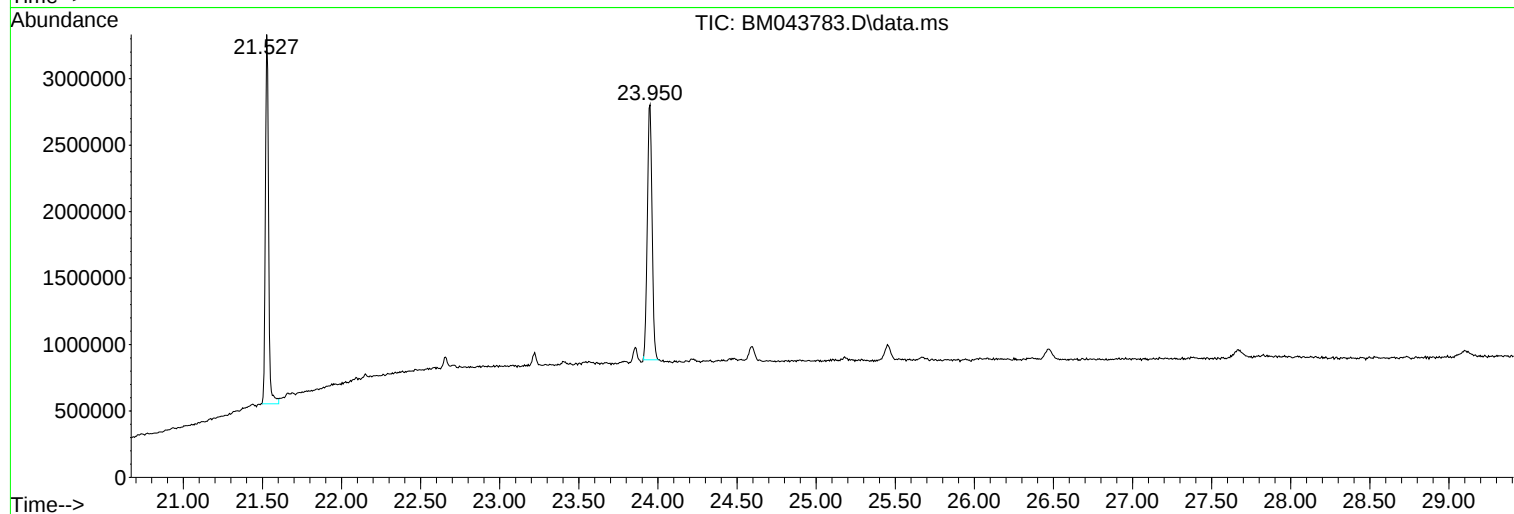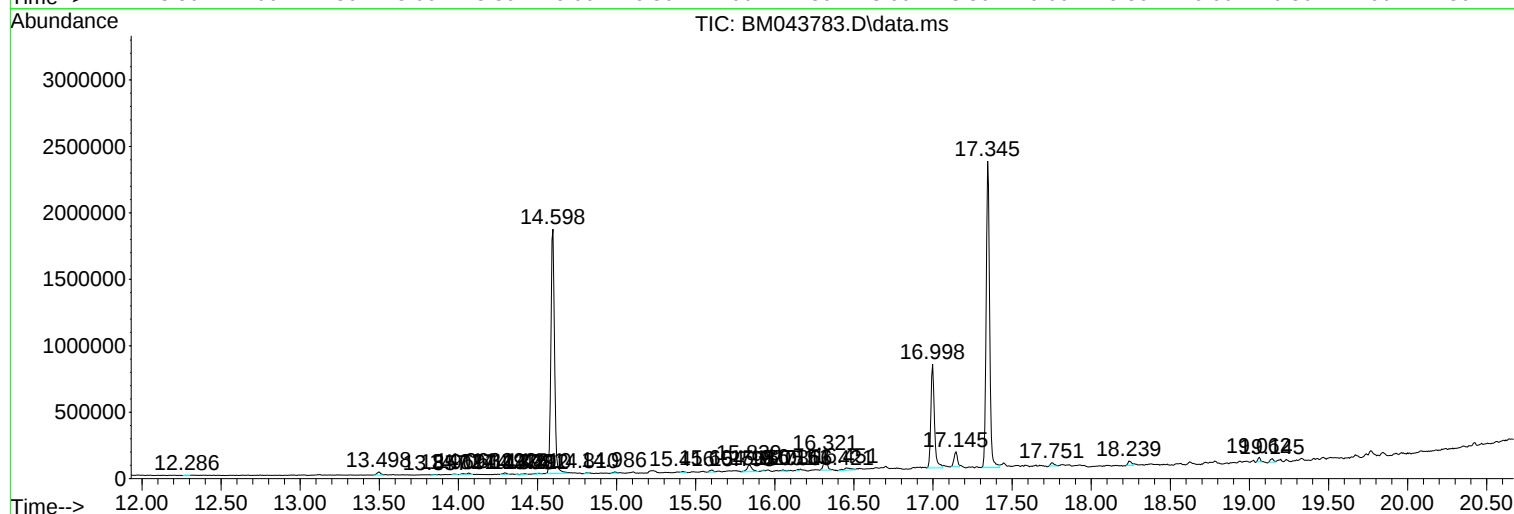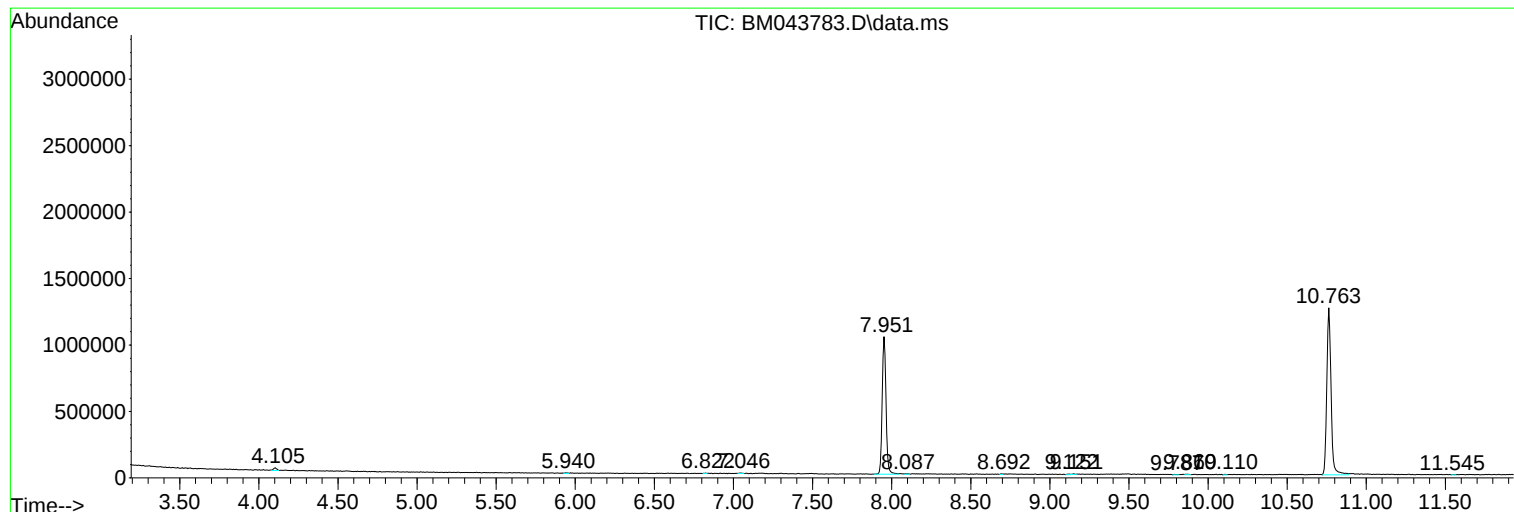

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
Data File : BM043783.D
Acq On : 06 Jan 2024 05:32
Operator : MA/JU
Sample : 05952-14MEDL2 200X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF97MEDL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010524\
Data File : BM043783.D
Acq On : 06 Jan 2024 05:32
Operator : MA/JU
Sample : 05952-14MEDL2 200X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF97MEDL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------