


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010719\
Data File : BM018451.D
Acq On : 07 Jan 2019 19:13
Operator : JU/SJ
Sample : K1048-05DL 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jan 08 00:54:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 07 23:55:53 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
C0950DL

Manual Integrations
APPROVED

Sohil
1/8/2019 5:39:04 PM

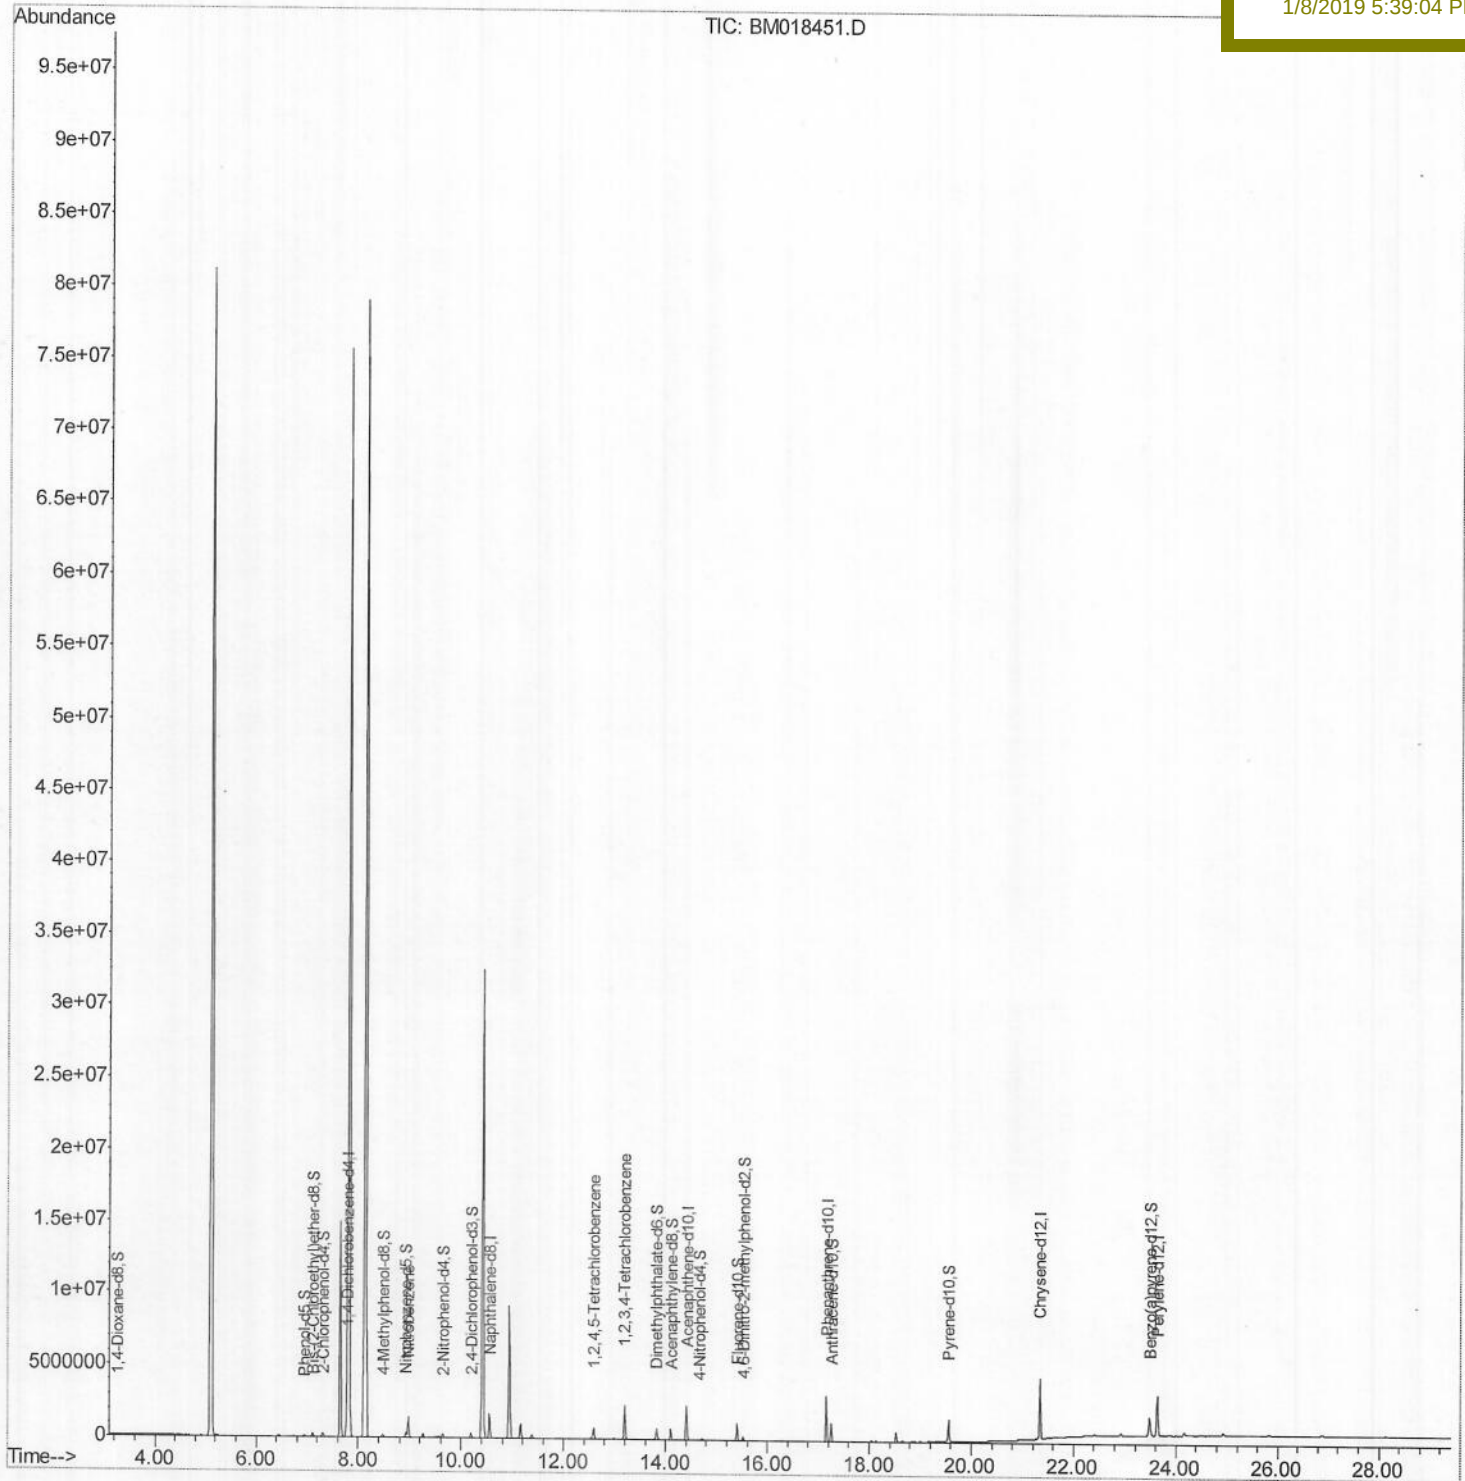

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010719\

Data File : BM018451.D

Acq On : 07 Jan 2019 19:13

Operator : JU/SJ

Sample : K1048-05DL 5X

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jan 08 00:08:05 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010719MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Mon Jan 07 23:55:53 2019

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




C0950DL

Manual Integrations

APPROVED

Sohil

1/8/2019 5:39:04 PM

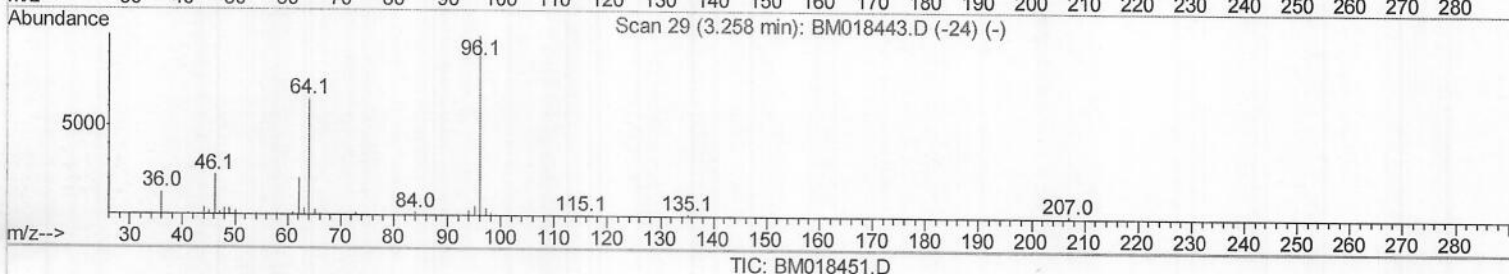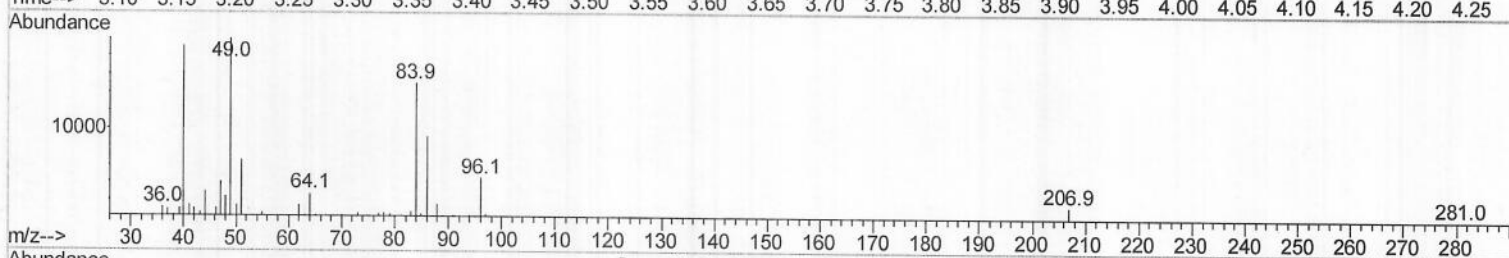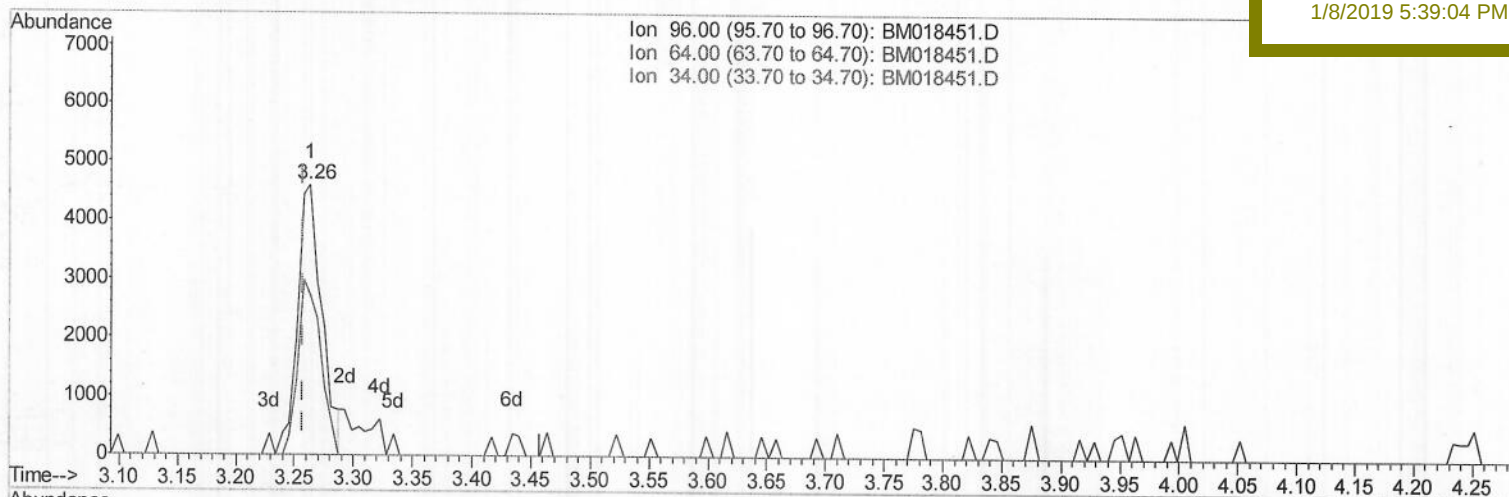

TIC: BM018451.D

(3) 1,4-Dioxane-d8 (S)

3.263min (+0.006) 0.89ng/uL

response 6534

Ion	Exp%	Act%
96.00	100	100
64.00	74.10	59.62
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010719\
 Data File : BM018451.D
 Acq On : 07 Jan 2019 19:13
 Operator : JU/SJ
 Sample : K1048-05DL 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jan 08 00:08:05 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 07 23:55:53 2019
 Response via : Initial Calibration

Instrument :
 BNA_M
ClientSampleId :
 C0950DL

Manual Integrations
APPROVED

Sohil
 1/8/2019 5:39:04 PM

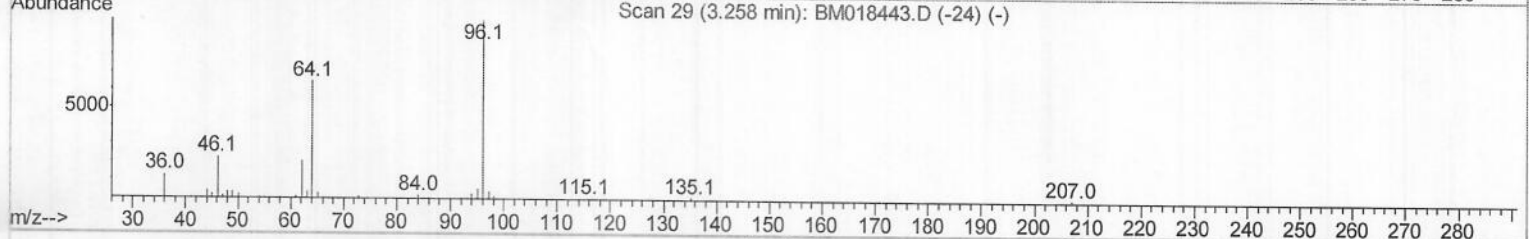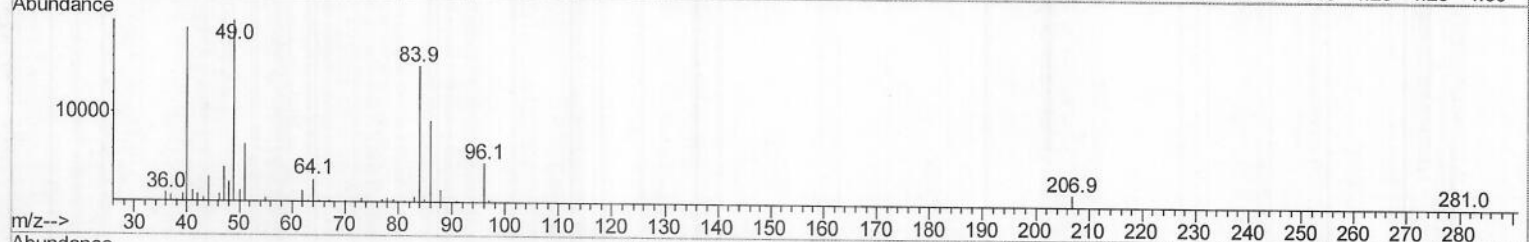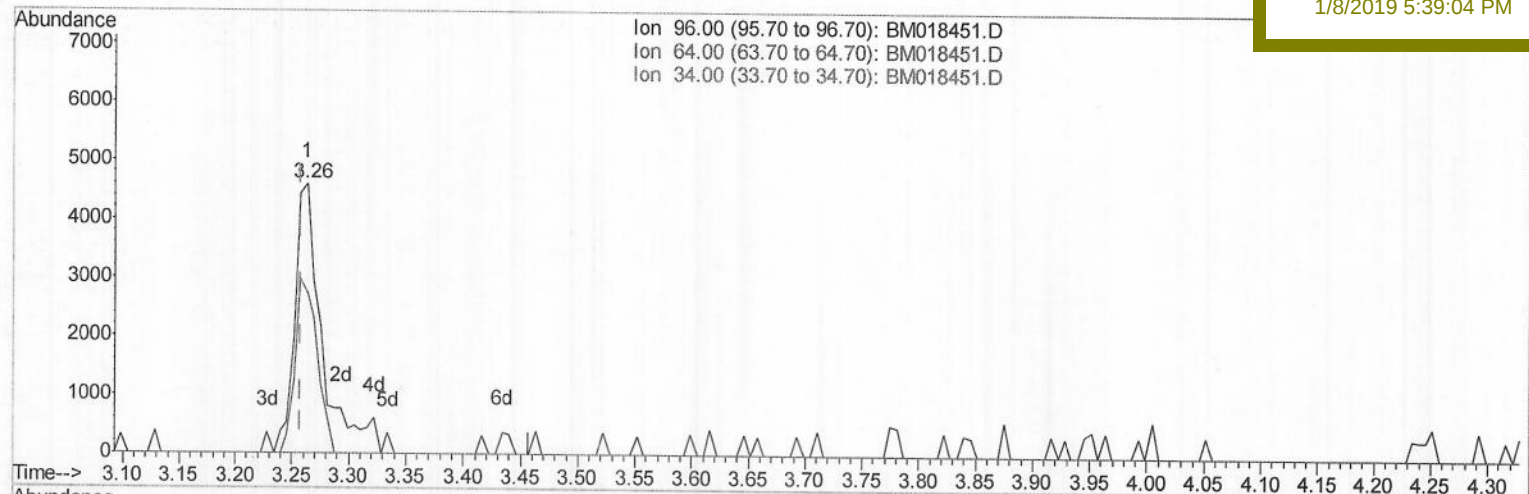

TIC: BM018451.D

(3) 1,4-Dioxane-d8 (S)
 3.263min (+0.006) 1.04ng/uL m
 response 7624

Ion	Exp%	Act%
96.00	100	100
64.00	74.10	59.62
34.00	0.00	0.00
0.00	0.00	0.00

SJ
1/8/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010719\

Data File : BM018451.D

Acq On : 07 Jan 2019 19:13

Operator : JU/SJ

Sample : K1048-05DL 5X

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jan 08 00:08:05 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010719MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Mon Jan 07 23:55:53 2019

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




C0950DL

Manual Integrations

APPROVED

Sohil

1/8/2019 5:39:04 PM

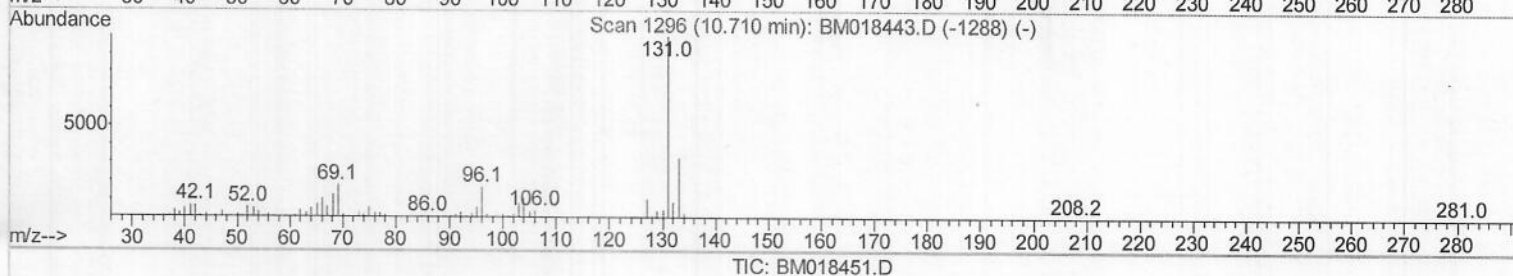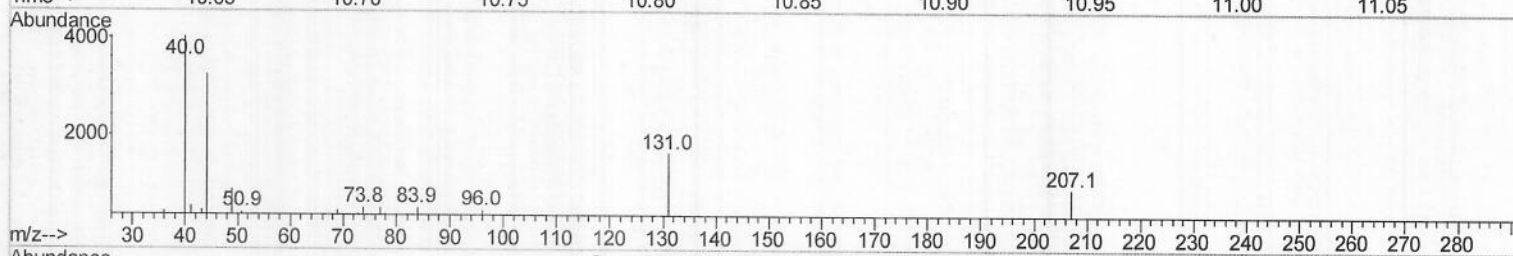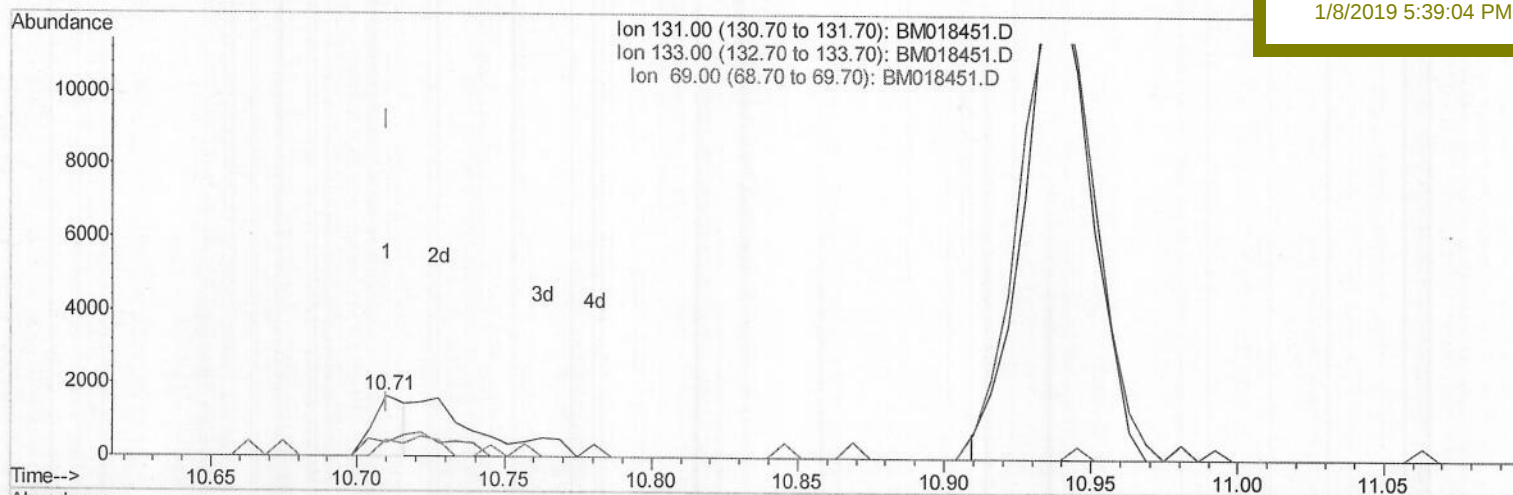

(29) 4-Chloroaniline-d4 (S)

10.710min (+0.000) 0.08ng/ul

response 1324

Ion	Exp%	Act%
131.00	100	100
133.00	32.30	21.68#
69.00	15.30	26.35#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010719\

Data File : BM018451.D

Acq On : 07 Jan 2019 19:13

Operator : JU/SJ

Sample : K1048-05DL 5X

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jan 08 00:08:05 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010719MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Mon Jan 07 23:55:53 2019

Response via : Initial Calibration

Instrument :

BNA_M

Client Sampled :




C0950DL

Manual Integrations

APPROVED

Sohil

1/8/2019 5:39:04 PM

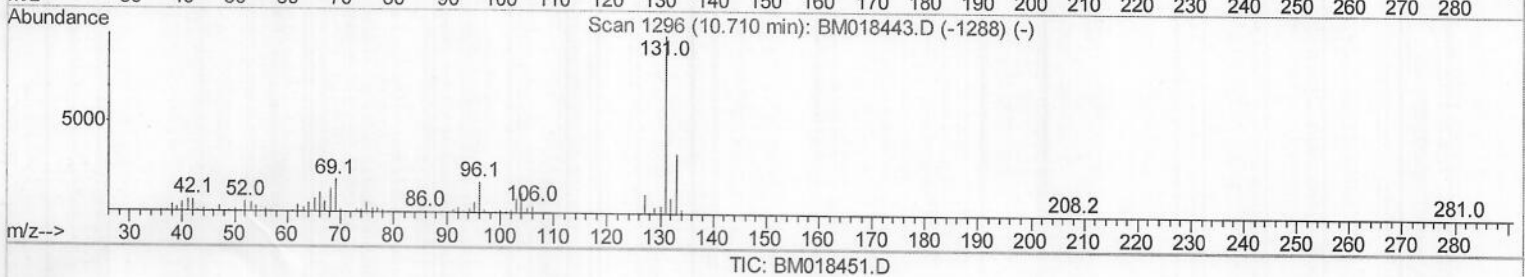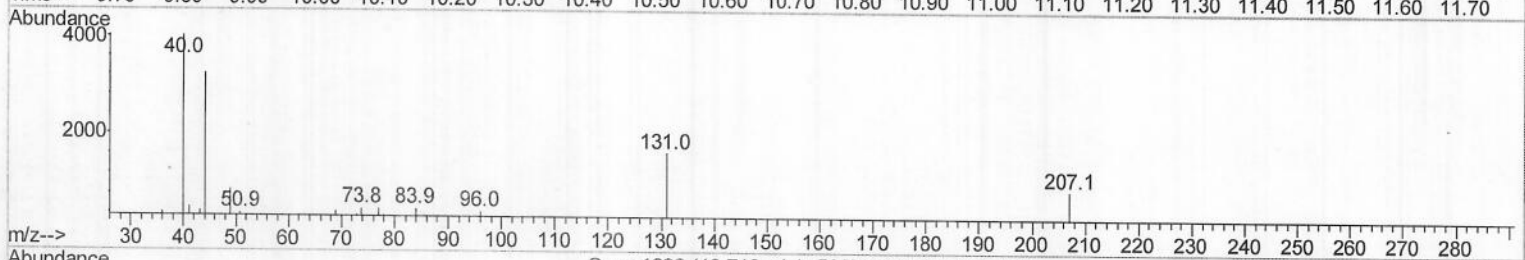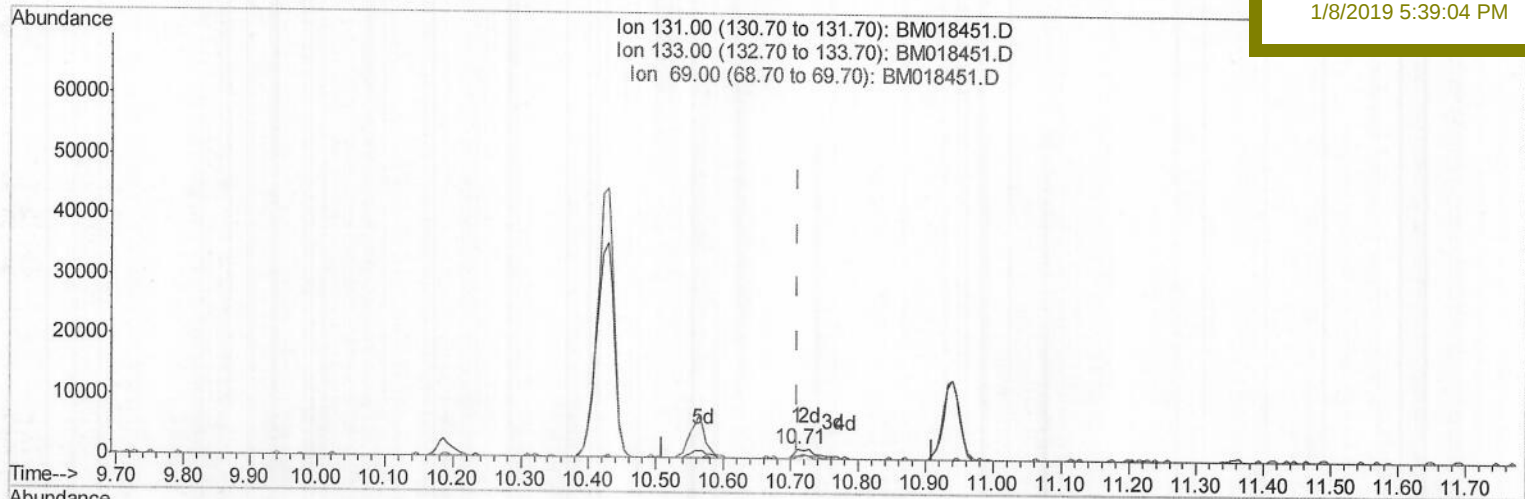

(29) 4-Chloroaniline-d4 (S)

10.710min (+0.000) 0.23ng/ul m

response 3753

Ion	Exp%	Act%
131.00	100	100
133.00	32.30	21.68#
69.00	15.30	26.35#
0.00	0.00	0.00

SJ
1/8/19

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010719\
 Data File : BM018451.D
 Acq On : 07 Jan 2019 19:13
 Operator : JU/SJ
 Sample : K1048-05DL 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jan 08 00:54:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 07 23:55:53 2019
 Response via : Initial Calibration

Instrument :
 BNA_M
 Client Sampled :
 C0950DL

Manual Integrations
 APPROVED

Sohil
 1/8/2019 5:39:04 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	341964	20.00	ng/ul	0.01
18) Naphthalene-d8	10.56	136	1363532	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.41	164	765366	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.16	188	1753201	20.00	ng/ul	0.00
77) Chrysene-d12	21.35	240	1915623	20.00	ng/ul	0.00
85) Perylene-d12	23.63	264	2009185	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	7624m →	1.04	ng/uL	0.00
5) Phenol-d5	6.95	99	36691	1.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	101273	6.67	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	121821	5.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	68736	3.14	ng/ul	0.00
19) Nitrobenzene-d5	8.93	128	74352	7.12	ng/ul	0.00
22) 2-Nitrophenol-d4	9.65	143	68803	6.46	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.19	165	130819	6.08	ng/ul	0.00
29) 4-Chloroaniline-d4	10.71	131	3753m →	0.23	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	495664	7.55	ng/ul	0.00
46) Acenaphthylene-d8	14.10	160	584290	7.17	ng/ul	0.00
51) 4-Nitrophenol-d4	14.66	143	11808	1.04	ng/ul	0.02
57) Fluorene-d10	15.40	176	431890	7.66	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	43179	4.50	ng/ul	0.00
70) Anthracene-d10	17.26	188	651071	7.63	ng/ul	0.00
78) Pyrene-d10	19.56	212	742022	7.62	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.49	264	827364	7.57	ng/ul	0.00

Target Compounds

						Ovalue
20) Nitrobenzene	8.97	77	733732	32.214	ng/ul	98
36) 1,2,4,5-Tetrachlorobenzene	12.59	216	263124	10.120	ng/ul	98
72) 1,2,3,4-Tetrachlorobenzene	13.20	216	671578	26.426	ng/uL	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed