

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010719\
 Data File : BM018447.D
 Acq On : 07 Jan 2019 16:50
 Operator : JU/SJ
 Sample : K1048-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0947

Quant Time: Jan 08 00:36:49 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 07 23:55:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	351082	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	1469270	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.41	164	846019	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.16	188	1944521	20.00	ng/ul	0.00
77) Chrysene-d12	21.35	240	2022145	20.00	ng/ul	0.00
85) Perylene-d12	23.63	264	2057912	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.26	96	32873	4.37	ng/uL	0.00
5) Phenol-d5	6.94	99	174812	6.31	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	469989	30.16	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	601356	24.80	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	345204	15.38	ng/ul	0.00
19) Nitrobenzene-d5	8.93	128	363784	32.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.65	143	385264	33.56	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.19	165	666072	28.75	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	2442511	33.64	ng/ul	0.00
46) Acenaphthylene-d8	14.10	160	2956433	32.82	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	69745	5.57	ng/ul	0.00
57) Fluorene-d10	15.40	176	2077358	33.34	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	295505	27.75	ng/ul	0.00
70) Anthracene-d10	17.26	188	3199613	33.83	ng/ul	0.00
78) Pyrene-d10	19.56	212	3510513	34.15	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.49	264	3816367	34.10	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
20) Nitrobenzene	8.97	77	689647	28.100	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010719\
Data File : BM018447.D
Acq On : 07 Jan 2019 16:50
Operator : JU/SJ
Sample : K1048-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0947

Quant Time: Jan 08 00:36:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 07 23:55:53 2019
Response via : Initial Calibration

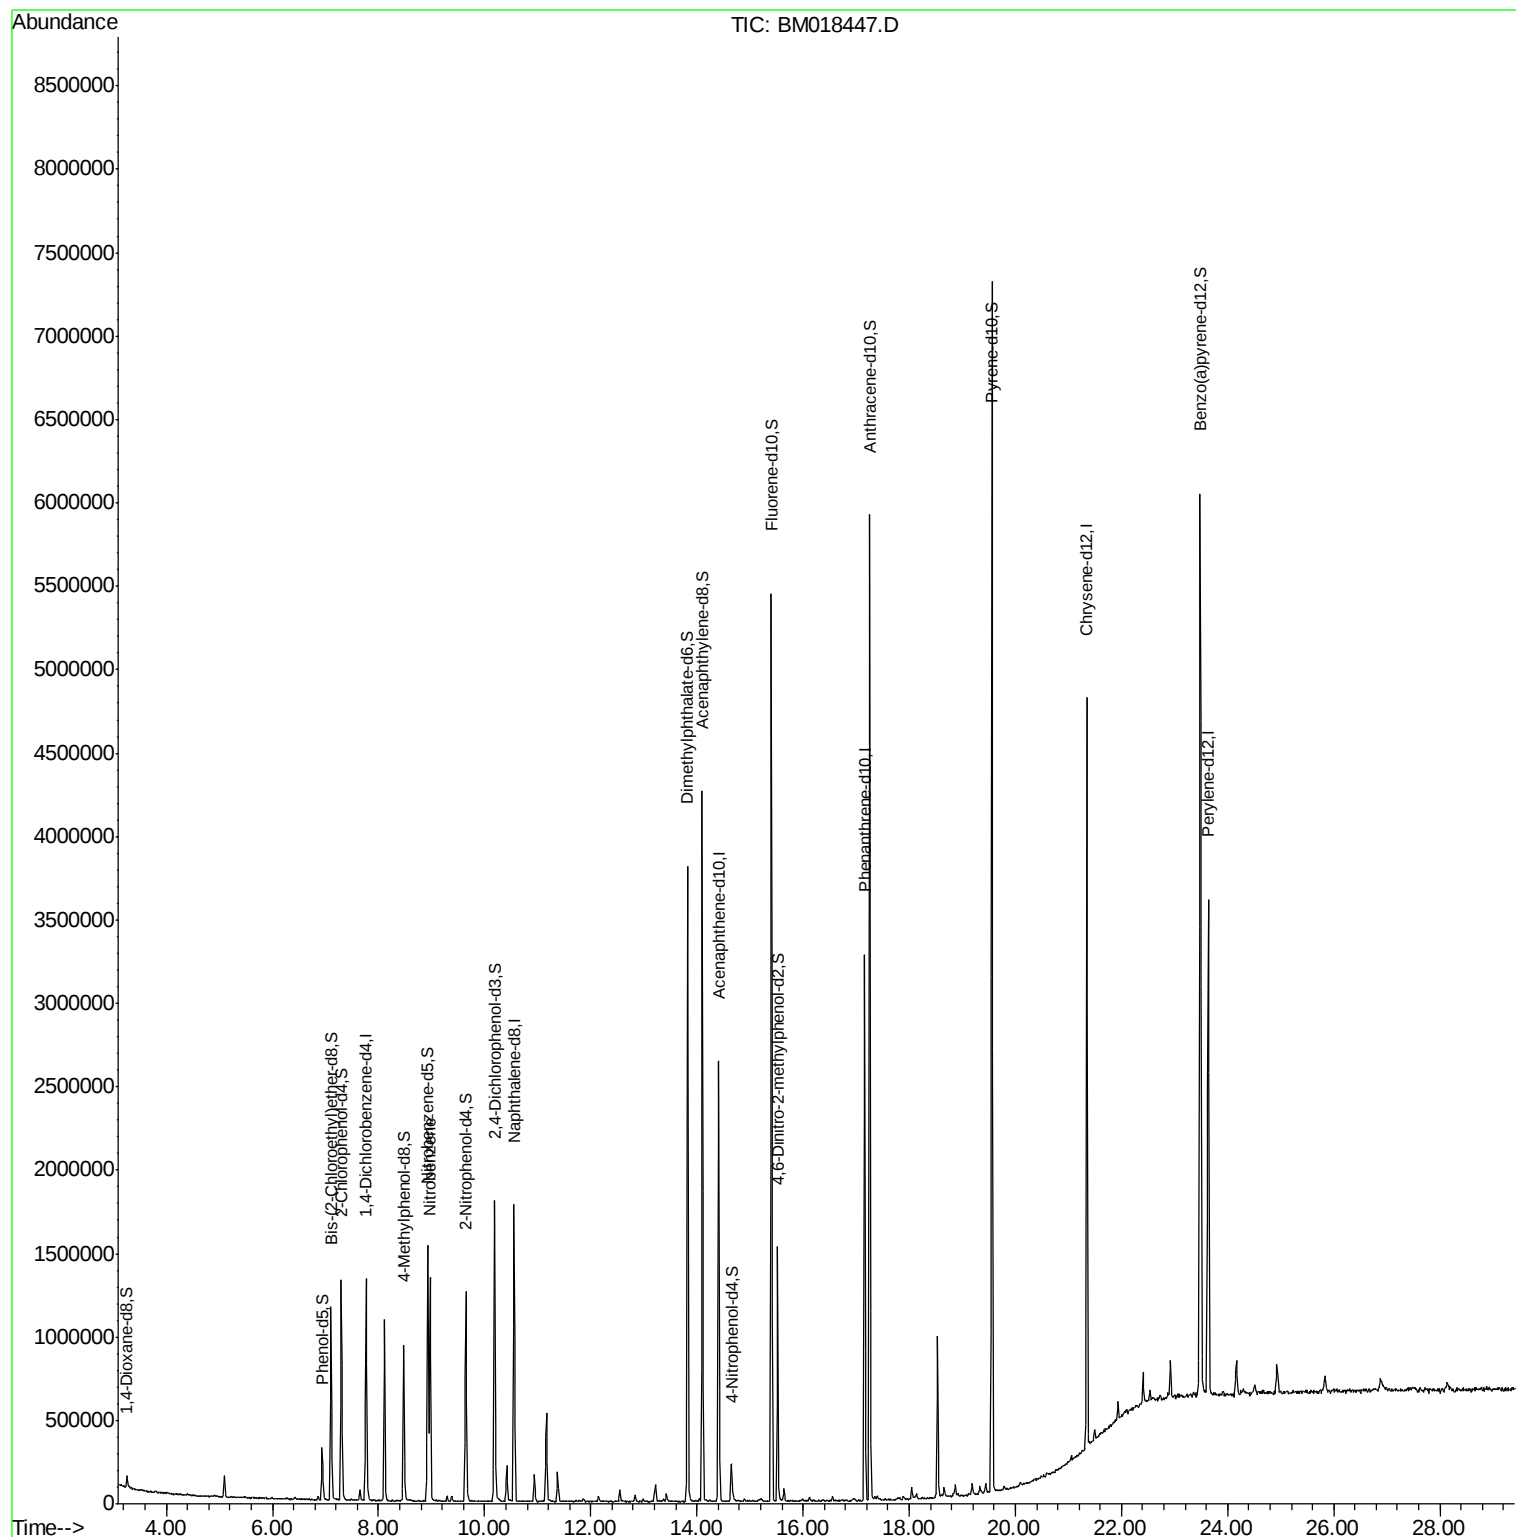

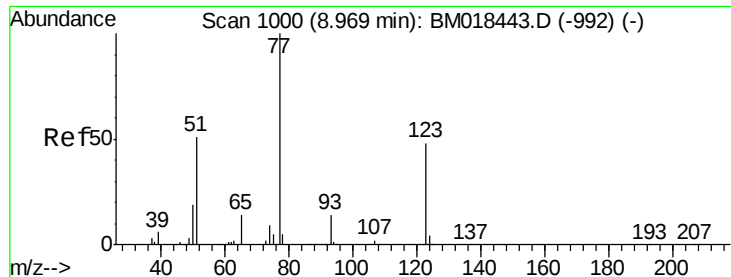

#20
 Nitrobenzene
 Concen: 28.100 ng/ul
 RT: 8.97 min Scan# 1000
 Delta R.T. -0.00 min
 Lab File: BM018447.D
 Acq: 07 Jan 2019 16:50

Instrument :
 BNA_M
 ClientSampleId :
 C0947

Tot Ion	Ion	Ratio	Lower	Upper
77	77	100		
123	123	47.7	39.5	59.3
65	65	13.7	10.9	16.3

