

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010719\
 Data File : BM018452.D
 Acq On : 07 Jan 2019 19:49
 Operator : JU/SJ
 Sample : K1048-02DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0947DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010719MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.093	338	341	346	rVB2	31335	41673	0.80%	0.115%
2	5.734	448	450	453	rBV4	4048	5272	0.10%	0.015%
3	6.057	502	505	508	rBV4	4489	6165	0.12%	0.017%
4	6.122	513	516	522	rVB6	4707	8097	0.15%	0.022%
5	6.939	650	655	665	rBV2	50963	99392	1.90%	0.274%
6	7.104	677	683	692	rBV	201710	324593	6.20%	0.895%
7	7.298	709	716	728	rBV	230346	391203	7.47%	1.078%
8	7.645	772	775	780	rVB5	12960	19266	0.37%	0.053%
9	7.763	788	795	808	rVB	1232352	1938922	37.01%	5.344%
10	8.110	844	854	862	rVB	214672	363796	6.94%	1.003%
11	8.475	910	916	925	rBV	143320	261766	5.00%	0.722%
12	8.928	987	993	997	rBV	275214	471758	9.01%	1.300%
13	8.969	997	1000	1008	rVB	234907	379075	7.24%	1.045%
14	9.292	1052	1055	1059	rVB4	5586	7544	0.14%	0.021%
15	9.380	1065	1070	1073	rBV5	7300	12800	0.24%	0.035%
16	9.645	1108	1115	1129	rVB	196839	334292	6.38%	0.921%
17	10.186	1200	1207	1220	rBV	266861	522346	9.97%	1.440%
18	10.416	1241	1246	1251	rVB3	44914	68358	1.30%	0.188%
19	10.557	1262	1270	1279	rVB	1578916	2615693	49.93%	7.210%
20	10.933	1328	1334	1341	rVB3	31735	53675	1.02%	0.148%
21	11.163	1367	1373	1380	rVB	96141	162151	3.10%	0.447%
22	11.380	1405	1410	1416	rVB4	31397	50924	0.97%	0.140%
23	11.722	1465	1468	1469	rBV2	5191	5317	0.10%	0.015%
24	12.151	1536	1541	1545	rBV4	6168	9406	0.18%	0.026%
25	12.404	1579	1584	1587	rBV5	3668	5575	0.11%	0.015%
26	12.551	1601	1609	1613	rBV5	12578	22098	0.42%	0.061%
27	12.839	1654	1658	1660	rBV5	6710	10520	0.20%	0.029%
28	13.227	1713	1724	1729	rBV7	16635	37215	0.71%	0.103%
29	13.368	1744	1748	1752	rBV5	3408	5837	0.11%	0.016%
30	13.427	1752	1758	1762	rVB7	10438	17578	0.34%	0.048%
31	13.463	1762	1764	1768	rBV4	5513	6661	0.13%	0.018%
32	13.821	1819	1825	1835	rBV	701842	966953	18.46%	2.665%
33	13.886	1835	1836	1842	rVB3	4695	6108	0.12%	0.017%
34	14.104	1867	1873	1880	rBV	724978	1061620	20.27%	2.926%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010719\
 Data File : BM018452.D
 Acq On : 07 Jan 2019 19:49
 Operator : JU/SJ
 Sample : K1048-02DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0947DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010719MA.M
 Title : SVOA CALIBRATION

35	14.410	1918	1925	1934	rBV2	2372600	3525278	67.29%	9.717%
36	14.668	1961	1969	1974	rBV5	22040	57775	1.10%	0.159%
37	15.162	2048	2053	2054	rBV2	3234	5332	0.10%	0.015%
38	15.198	2055	2059	2063	rVV2	18182	25233	0.48%	0.070%
39	15.233	2063	2065	2069	rVB3	8695	8775	0.17%	0.024%
40	15.404	2088	2094	2103	rBV	1064312	1476634	28.19%	4.070%
41	15.521	2108	2114	2123	rBV	168789	261466	4.99%	0.721%
42	15.645	2130	2135	2141	rBV6	9854	16659	0.32%	0.046%
43	16.357	2253	2256	2262	rVB6	7734	12271	0.23%	0.034%
44	16.945	2353	2356	2360	rBV	11675	14702	0.28%	0.041%
45	17.156	2386	2392	2399	rBV2	3033870	4296805	82.02%	11.843%
46	17.256	2403	2409	2423	rBV	1111807	1536879	29.34%	4.236%
47	17.668	2473	2479	2481	rBV4	6030	9588	0.18%	0.026%
48	18.051	2538	2544	2551	rBV8	26728	49063	0.94%	0.135%
49	18.127	2554	2557	2561	rVV5	6949	9239	0.18%	0.025%
50	18.192	2567	2568	2573	rBV6	5831	5627	0.11%	0.016%
51	18.321	2589	2590	2597	rBV7	4782	8748	0.17%	0.024%
52	18.533	2622	2626	2632	rBV4	148186	198920	3.80%	0.548%
53	18.862	2680	2682	2686	rVB5	8014	9624	0.18%	0.027%
54	18.915	2689	2691	2694	rBV4	7946	8033	0.15%	0.022%
55	19.139	2727	2729	2732	rBV4	5099	5461	0.10%	0.015%
56	19.198	2734	2739	2742	rBV6	12131	23011	0.44%	0.063%
57	19.339	2758	2763	2767	rBV8	17681	34144	0.65%	0.094%
58	19.415	2774	2776	2778	rBV3	10101	7214	0.14%	0.020%
59	19.556	2794	2800	2807	rBV	1368542	1816379	34.67%	5.007%
60	21.350	3100	3105	3111	rBV	4359164	5223382	99.71%	14.397%
61	23.485	3462	3468	3476	rVB	1006448	2101817	40.12%	5.793%
62	23.633	3486	3493	3509	rVB	2784360	5238576	100.00%	14.439%


Sum of corrected areas: 36280284

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010719\
Data File : BM018452.D
Acq On : 07 Jan 2019 19:49
Operator : JU/SJ
Sample : K1048-02DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0947DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

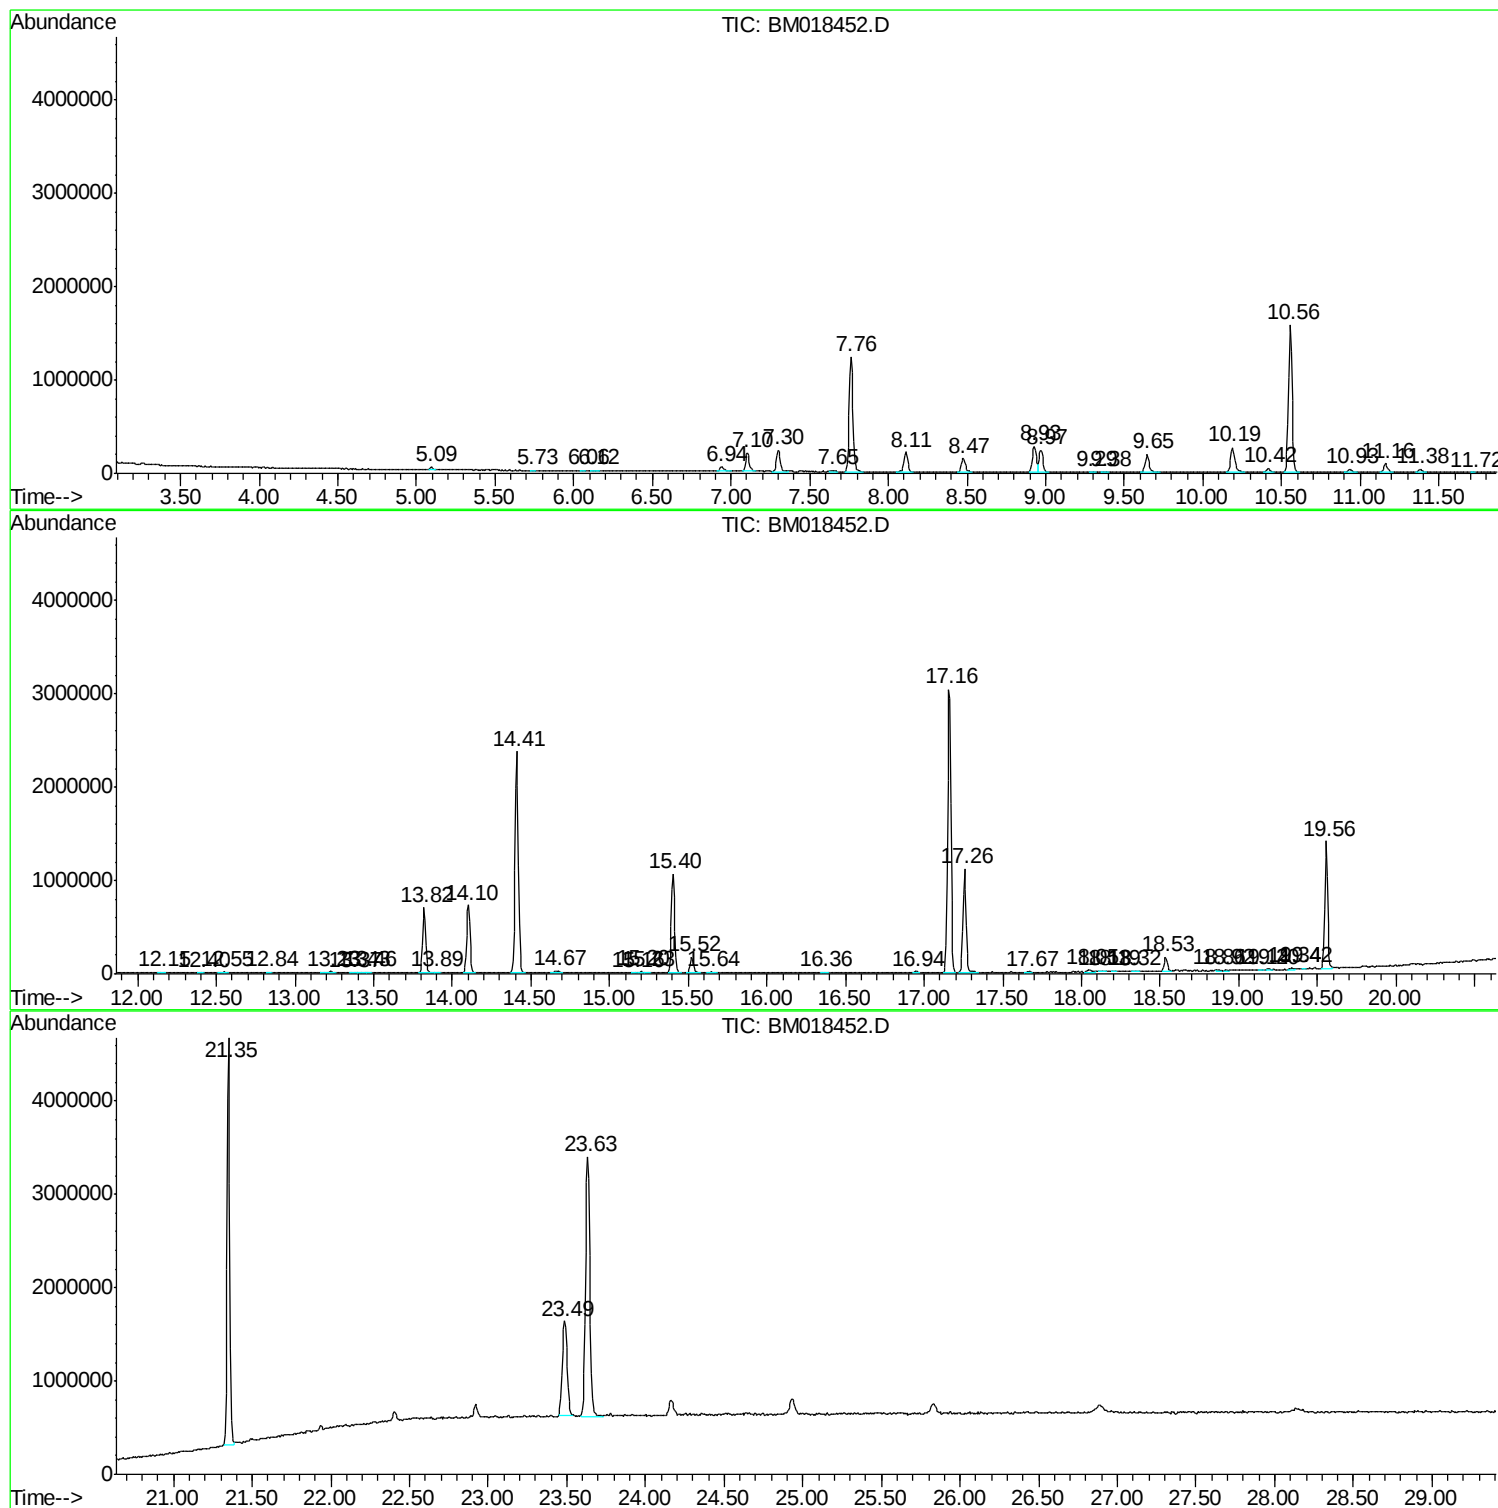

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM010719\
Data_File : BM018452.D
Acq_On : 07 Jan 2019 19:499
Operator : JU/SJJ
Sample : K1048-02DL_5XX
Misc :
ALS_Vial : 11 Sample_Multiplier: 11

Instrument :
BNA_M
ClientSampleId :
C0947DL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010719MA.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
