

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010722\
 Data File : BM033681.D
 Acq On : 07 Jan 2022 22:29
 Operator : CG/JU
 Sample : N1065-22
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 AMI-6

Quant Time: Jan 08 06:55:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 05 17:07:26 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.972	152	147741	20.000	ng	-0.01
21) Naphthalene-d8	10.790	136	622178	20.000	ng	-0.02
39) Acenaphthene-d10	14.613	164	415597	20.000	ng	-0.01
64) Phenanthrene-d10	17.348	188	934231	20.000	ng	-0.01
76) Chrysene-d12	21.512	240	1012973	20.000	ng	-0.01
86) Perylene-d12	23.936	264	1000091	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.519	112	868702	92.734	ng	0.00
7) Phenol-d6	7.131	99	1147233	90.867	ng	0.00
23) Nitrobenzene-d5	9.137	82	770044	57.158	ng	-0.02
42) 2,4,6-Tribromophenol	16.095	330	529751	122.040	ng	-0.01
45) 2-Fluorobiphenyl	13.242	172	1681157	52.983	ng	-0.02
79) Terphenyl-d14	19.960	244	2796601	49.694	ng	-0.01
Target Compounds						
9) Benzaldehyde	7.131	77	2866	Below Cal	Qvalue #	7

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010722\
Data File : BM033681.D
Acq On : 07 Jan 2022 22:29
Operator : CG/JU
Sample : N1065-22
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
AMI-6

Quant Time: Jan 08 06:55:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 05 17:07:26 2022
Response via : Initial Calibration




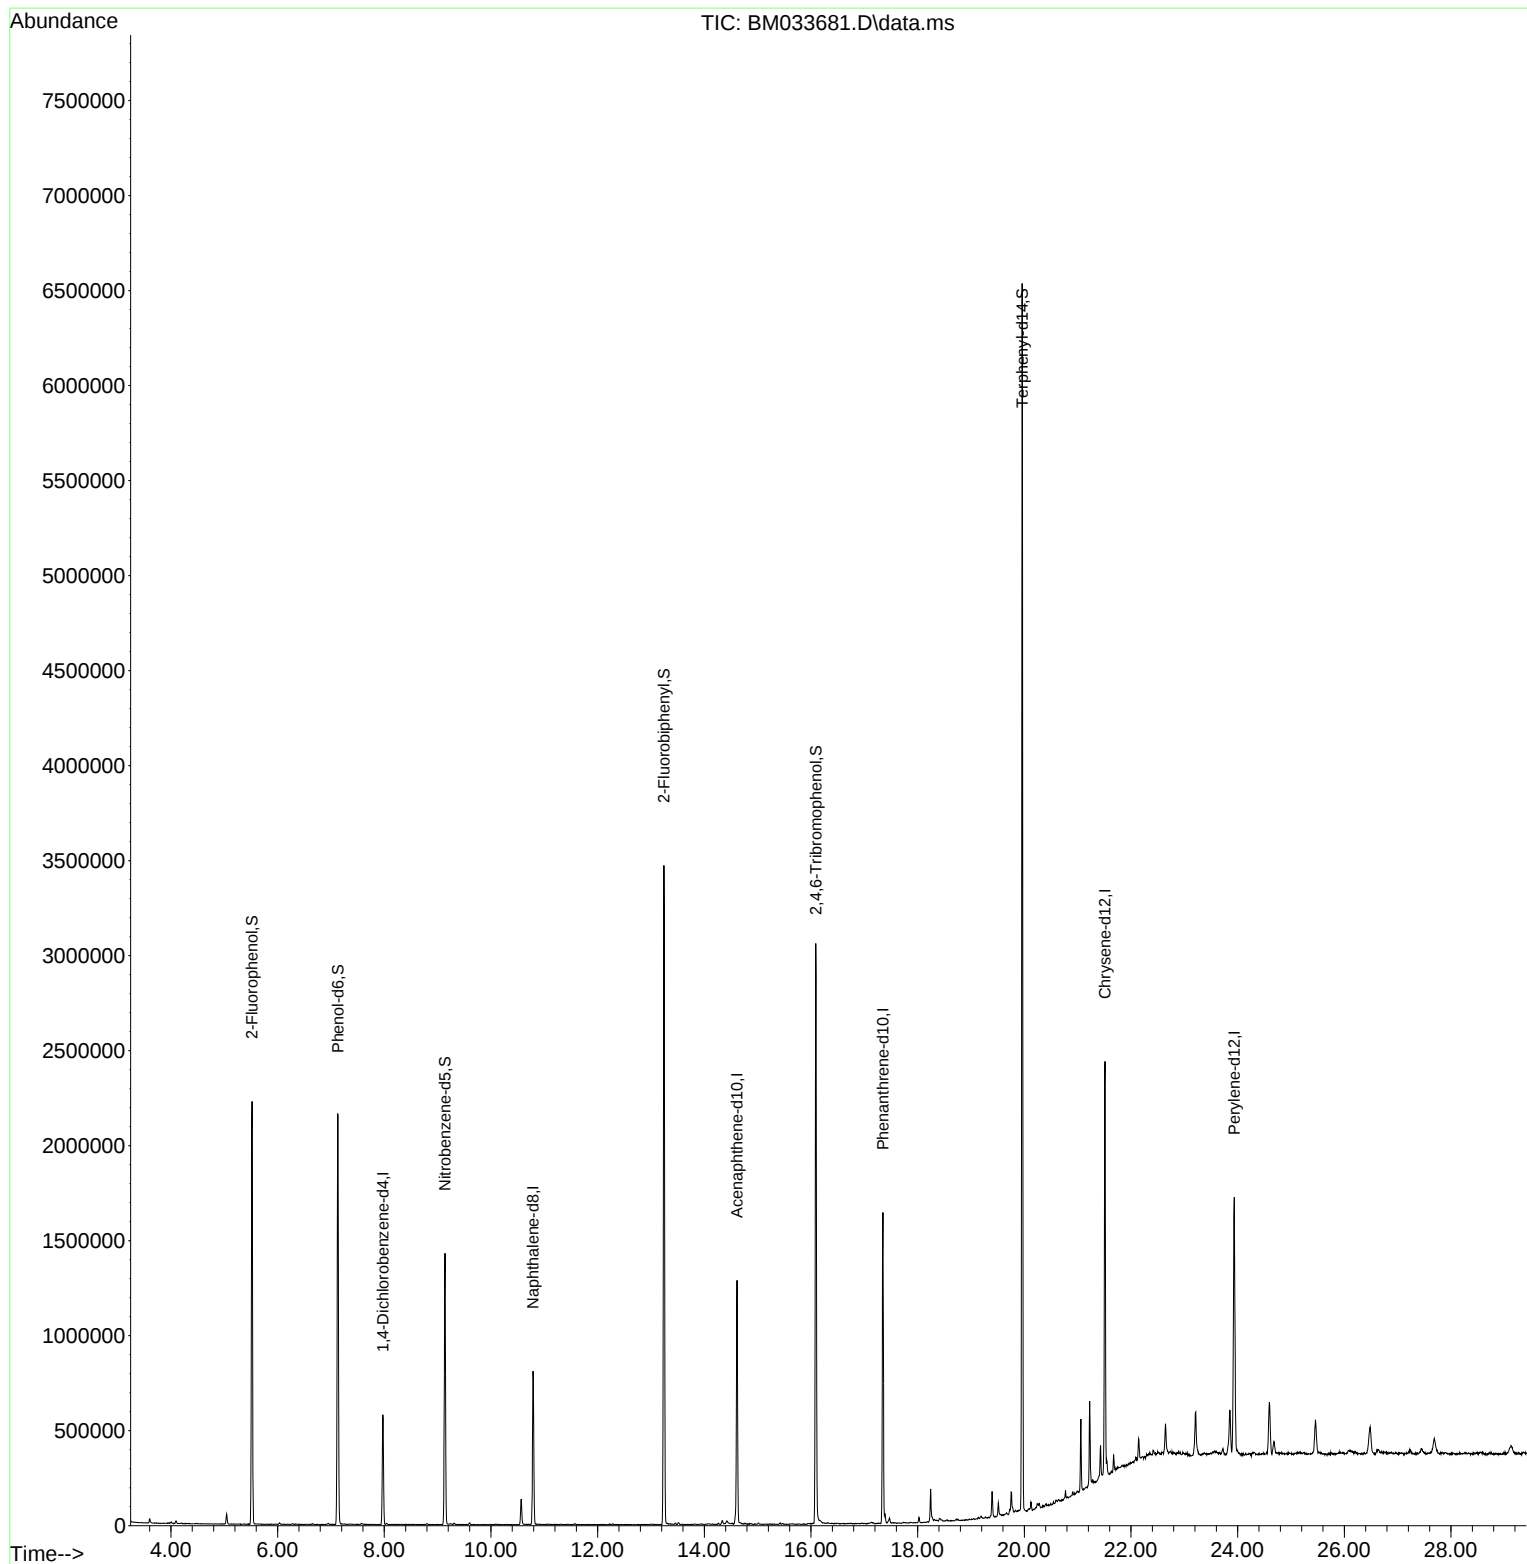




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.972 min Scan# 807
Delta R.T. -0.012 min
Lab File: BM033681.D
Acq: 07 Jan 2022 22:29




Instrument :
BNA_M
ClientSampleId :
AMI-6


Tgt Ion:152 Resp: 147741
Ion Ratio Lower Upper
152 100
150 155.1 128.9 193.3
115 66.8 53.0 79.6

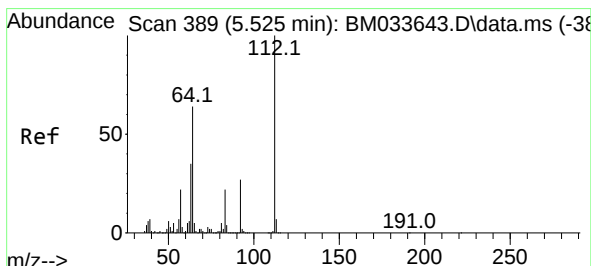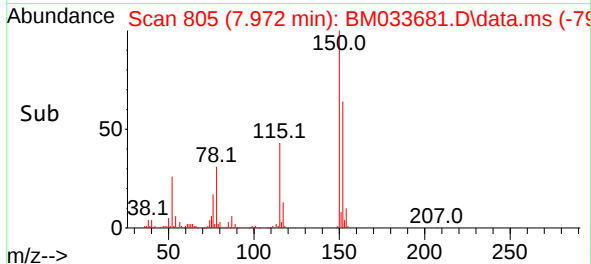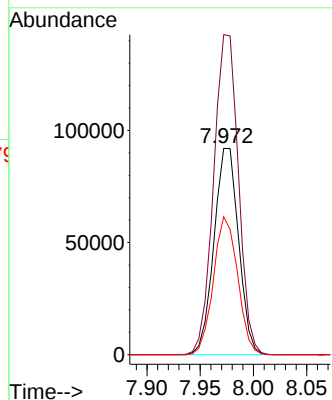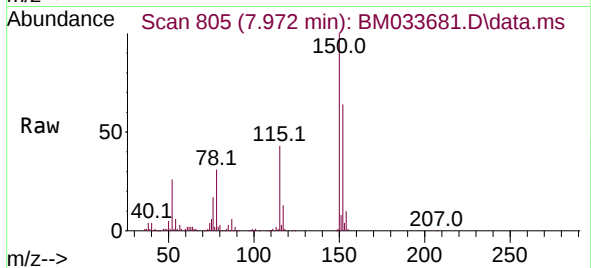

#5
2-Fluorophenol
Concen: 92.734 ng
RT: 5.519 min Scan# 388
Delta R.T. -0.006 min
Lab File: BM033681.D
Acq: 07 Jan 2022 22:29

Tgt Ion:112 Resp: 868702
Ion Ratio Lower Upper
112 100
64 61.5 55.5 83.3
63 33.7 31.3 46.9


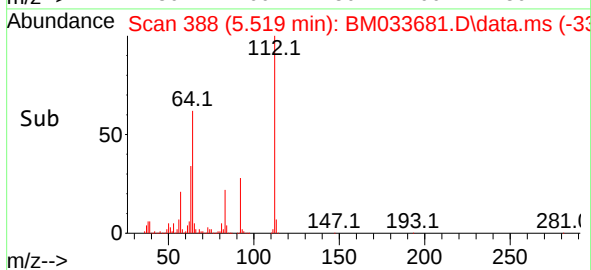
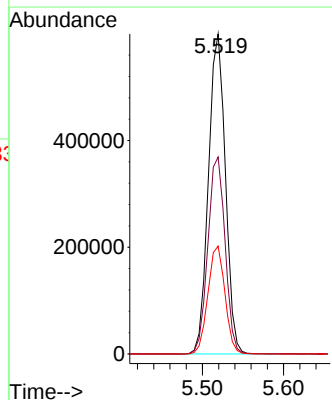
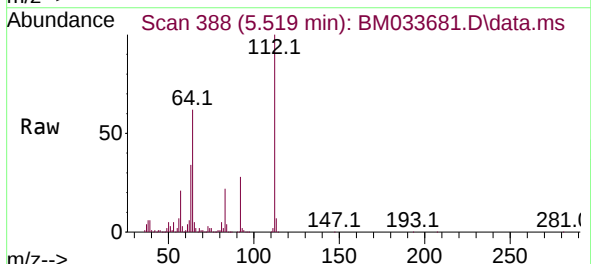


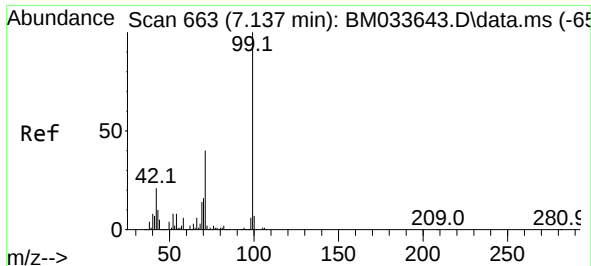

#7
Phenol-d6
Concen: 90.867 ng
RT: 7.131 min Scan# 662
Delta R.T. -0.006 min
Lab File: BM033681.D
Acq: 07 Jan 2022 22:29




Instrument :
BNA_M
ClientSampleId :
AMI-6


Tgt Ion: 99 Resp: 1147233
Ion Ratio Lower Upper
99 100
42 19.2 20.3 30.5#
71 40.2 34.5 51.7

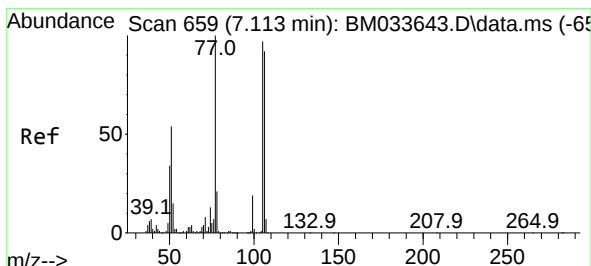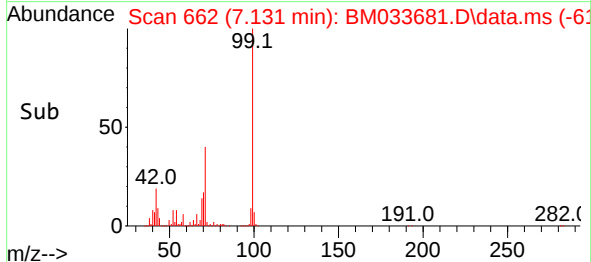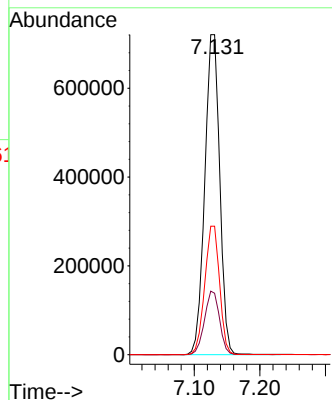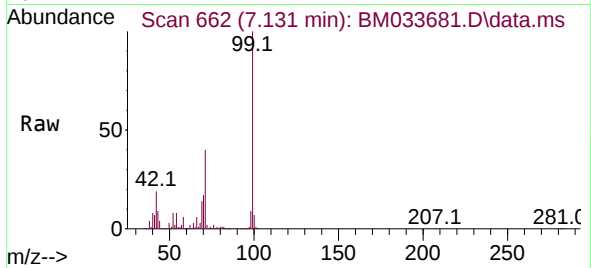

#9
Benzaldehyde
Concen: Below Cal
RT: 7.131 min Scan# 662
Delta R.T. 0.018 min
Lab File: BM033681.D
Acq: 07 Jan 2022 22:29

Tgt Ion: 77 Resp: 2866
Ion Ratio Lower Upper
77 100
105 0.0 67.1 107.1#
106 0.0 64.3 104.3#


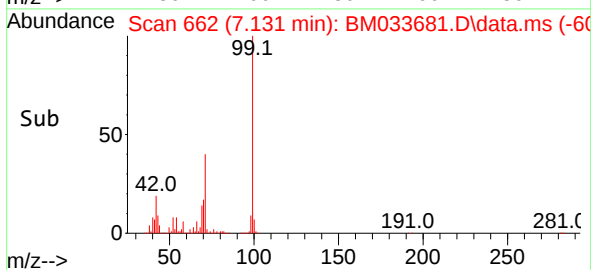
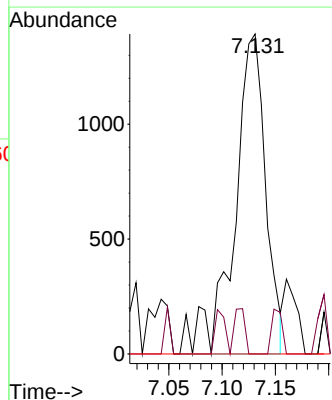
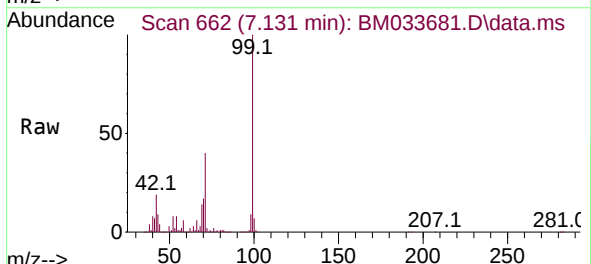


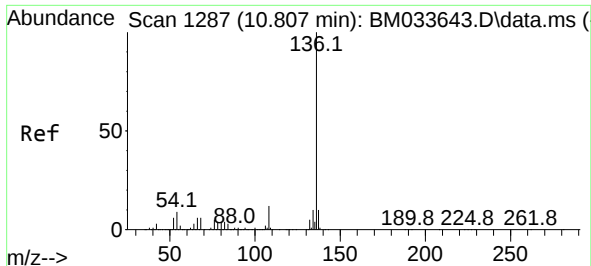

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.790 min Scan# 1003
Delta R.T. -0.018 min
Lab File: BM033681.D
Acq: 07 Jan 2022 22:29




Instrument :
BNA_M
ClientSampleId :
AMI-6


Tgt Ion:	136	Resp:	622178
Ion Ratio	Lower	Upper	
136	100		
137	10.9	8.6	13.0
54	8.8	8.3	12.5
68	5.3	5.0	7.6

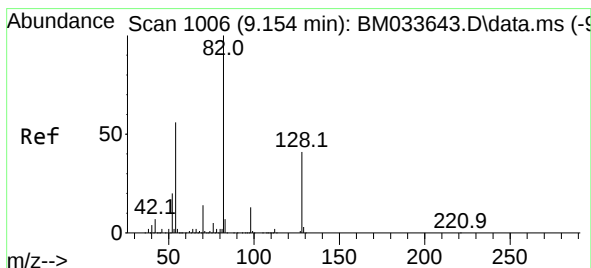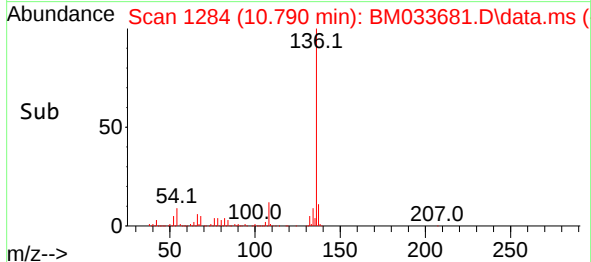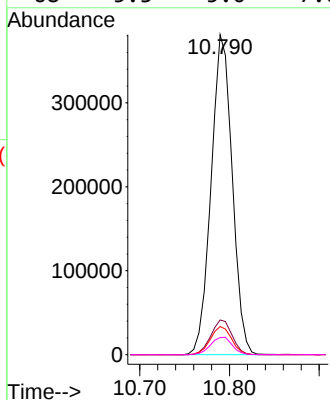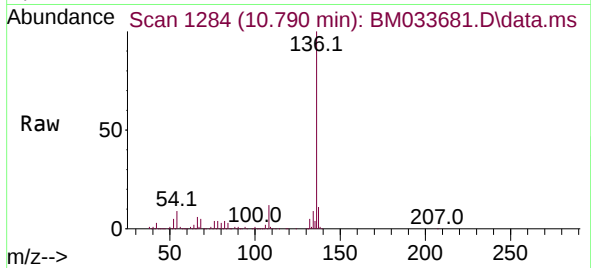

#23
Nitrobenzene-d5
Concen: 57.158 ng
RT: 9.137 min Scan# 1003
Delta R.T. -0.018 min
Lab File: BM033681.D
Acq: 07 Jan 2022 22:29


Tgt Ion:	82	Resp:	770044
Ion Ratio	Lower	Upper	
82	100		
128	41.7	28.1	42.1
54	55.4	46.1	69.1

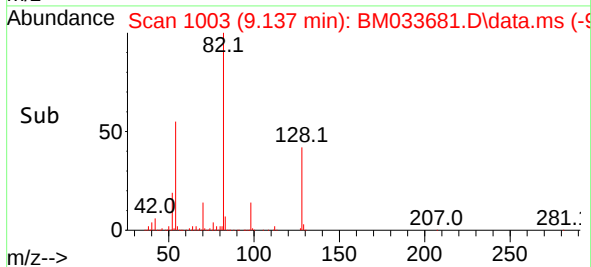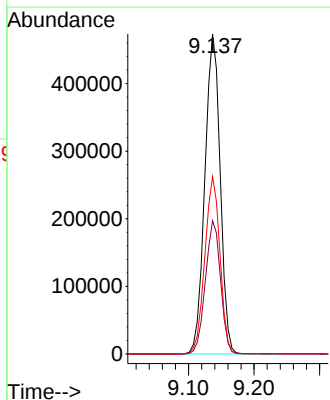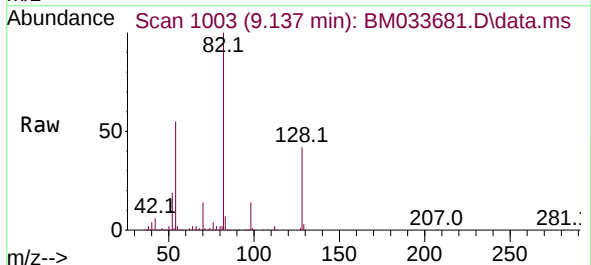



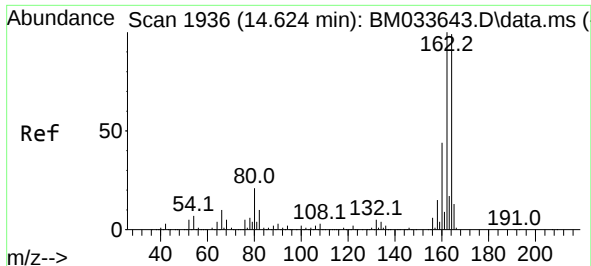


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.613 min Scan# 1934
Delta R.T. -0.012 min
Lab File: BM033681.D
Acq: 07 Jan 2022 22:29

Instrument :
BNA_M
ClientSampleId :
AMI-6



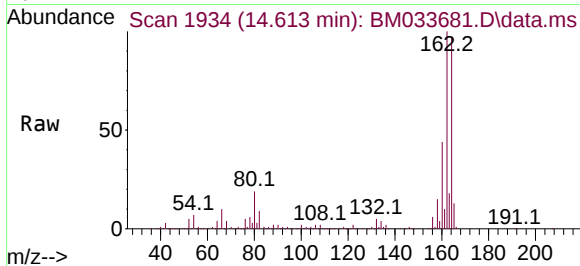



Tgt Ion:164 Resp: 415597
Ion Ratio Lower Upper
164 100
162 103.1 79.7 119.5
160 45.4 34.2 51.4

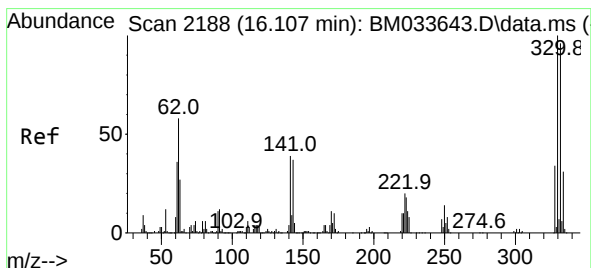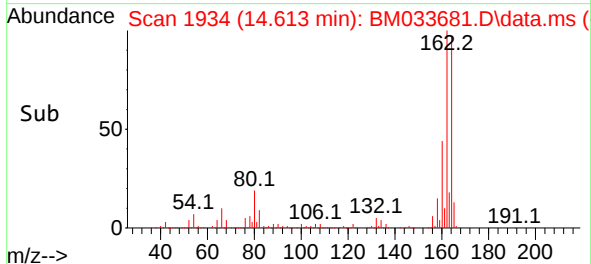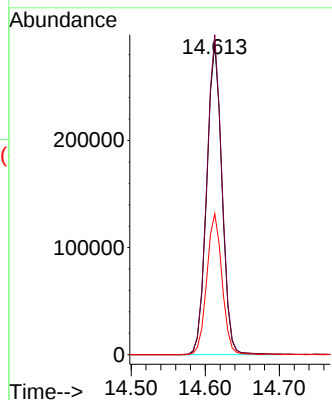

#42
2,4,6-Tribromophenol
Concen: 122.040 ng
RT: 16.095 min Scan# 2186
Delta R.T. -0.012 min
Lab File: BM033681.D
Acq: 07 Jan 2022 22:29

Tgt Ion:330 Resp: 529751
Ion Ratio Lower Upper
330 100
332 97.0 76.5 114.7
141 40.5 35.9 53.9


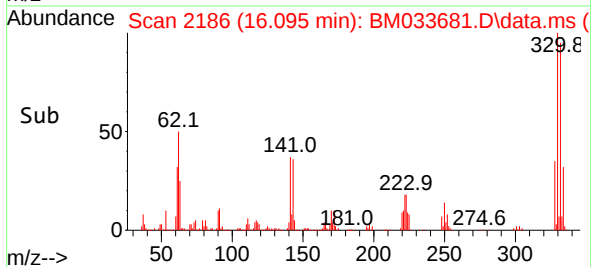
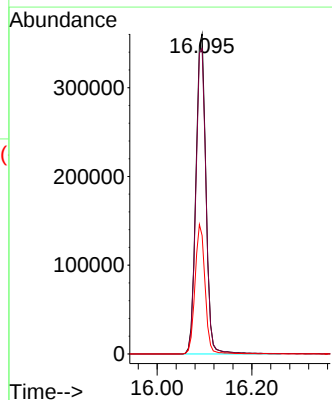
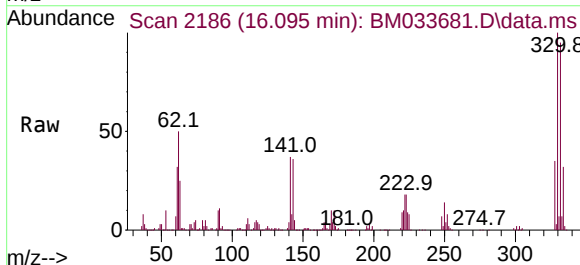


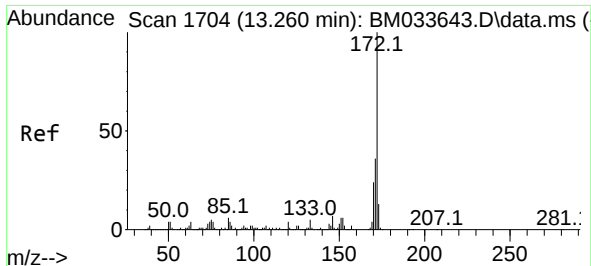

#45
2-Fluorobiphenyl
Concen: 52.983 ng
RT: 13.242 min Scan# 1
Delta R.T. -0.018 min
Lab File: BM033681.D
Acq: 07 Jan 2022 22:29




Instrument :
BNA_M
ClientSampleId :
AMI-6


Tgt Ion:172 Resp: 1681157
Ion Ratio Lower Upper
172 100
171 35.2 27.2 40.8
170 23.3 18.7 28.1

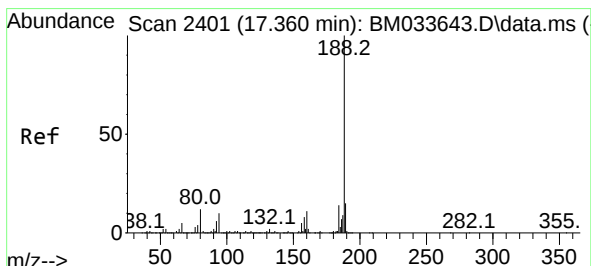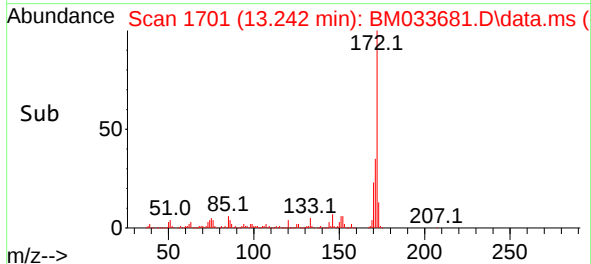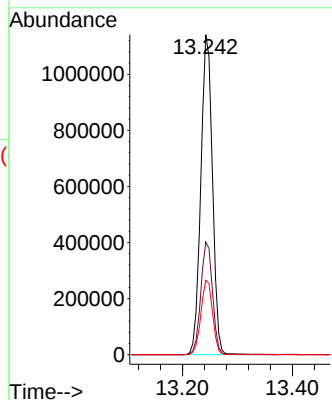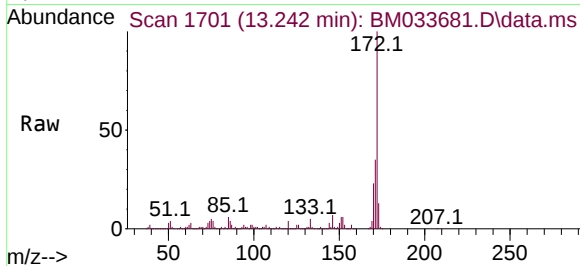

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.348 min Scan# 2399
Delta R.T. -0.012 min
Lab File: BM033681.D
Acq: 07 Jan 2022 22:29

Tgt Ion:188 Resp: 934231
Ion Ratio Lower Upper
188 100
94 8.8 7.5 11.3
80 9.9 8.9 13.3


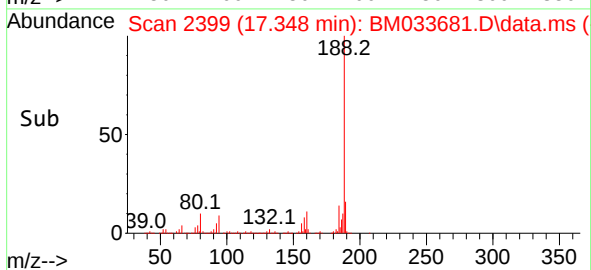
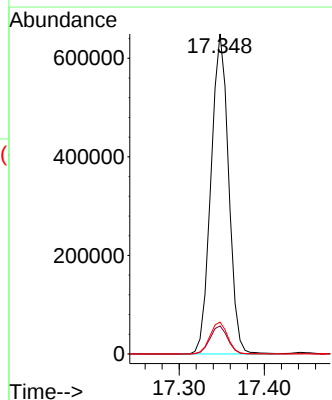
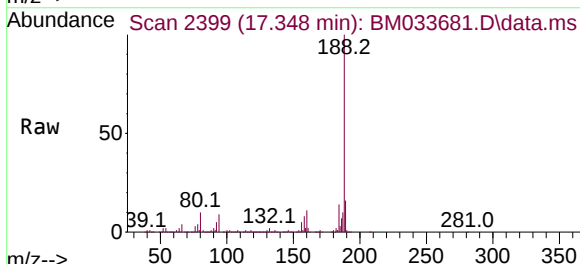


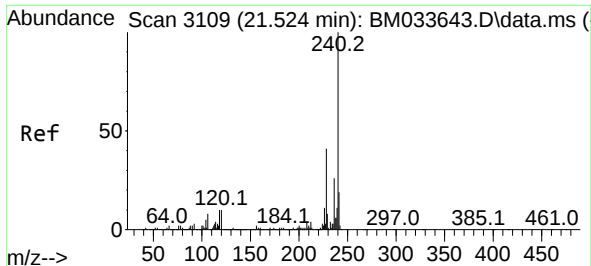

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.512 min Scan# 3109
Delta R.T. -0.012 min
Lab File: BM033681.D
Acq: 07 Jan 2022 22:29




Instrument :
BNA_M
ClientSampleId :
AMI-6


Tgt Ion:240 Resp: 1012973
Ion Ratio Lower Upper
240 100
120 9.7 7.8 11.6
236 25.8 20.3 30.5

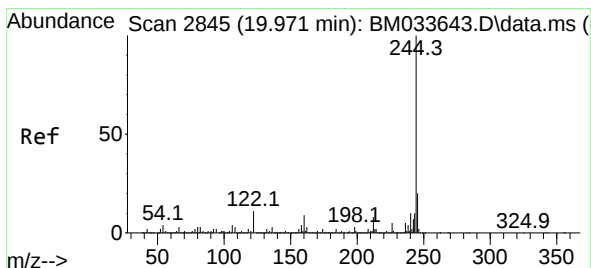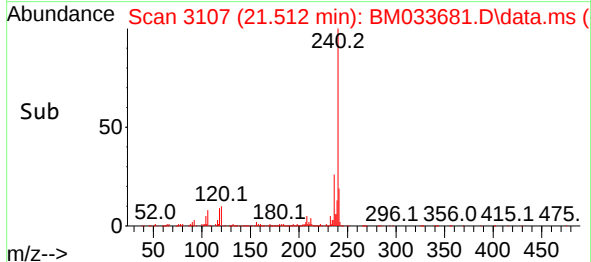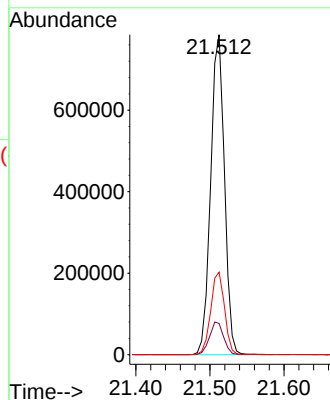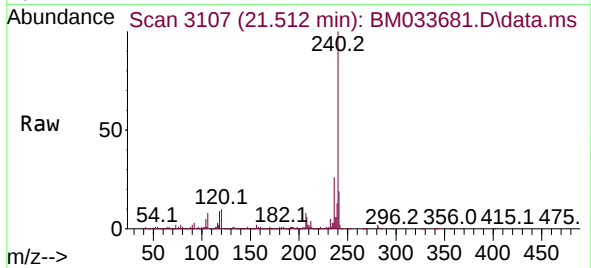

#79
Terphenyl-d14
Concen: 49.694 ng
RT: 19.960 min Scan# 2843
Delta R.T. -0.012 min
Lab File: BM033681.D
Acq: 07 Jan 2022 22:29

Tgt Ion:244 Resp: 2796601
Ion Ratio Lower Upper
244 100
212 8.2 5.9 8.9
122 10.6 8.4 12.6

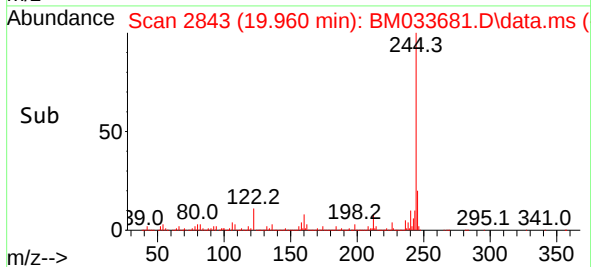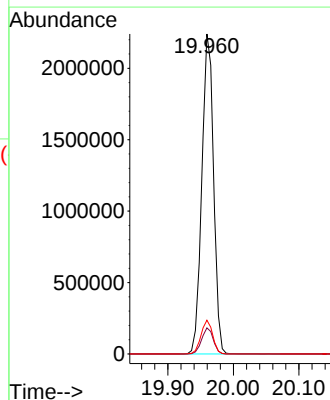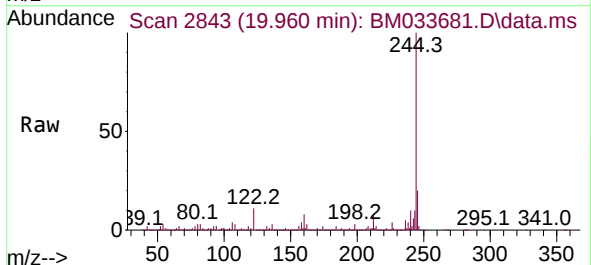

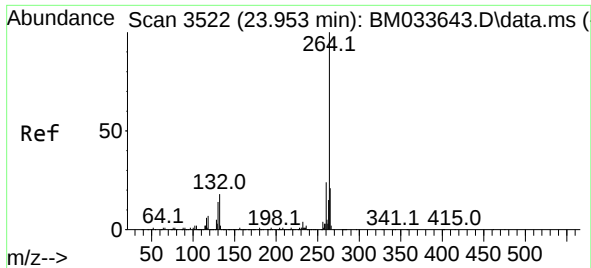

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.936 min Scan# 31
 Delta R.T. -0.018 min
 Lab File: BM033681.D
 Acq: 07 Jan 2022 22:29

Instrument :
 BNA_M
 ClientSampleId :
 AMI-6

Tgt Ion:264 Resp: 1000091
 Ion Ratio Lower Upper
 264 100
 260 23.5 17.7 26.5
 265 21.1 17.7 26.5

