
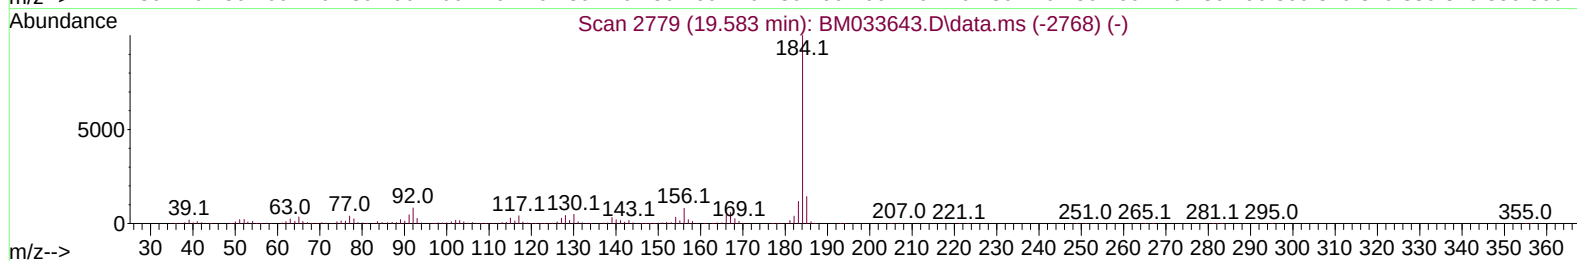
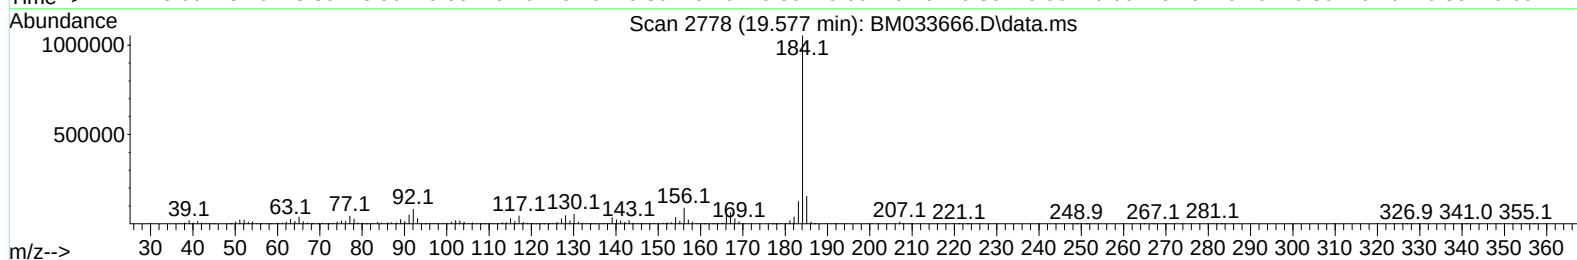


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010722\
 Data File : BM033666.D
 Acq On : 07 Jan 2022 12:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 09 23:55:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 05 17:07:26 2022
 Response via : Initial Calibration

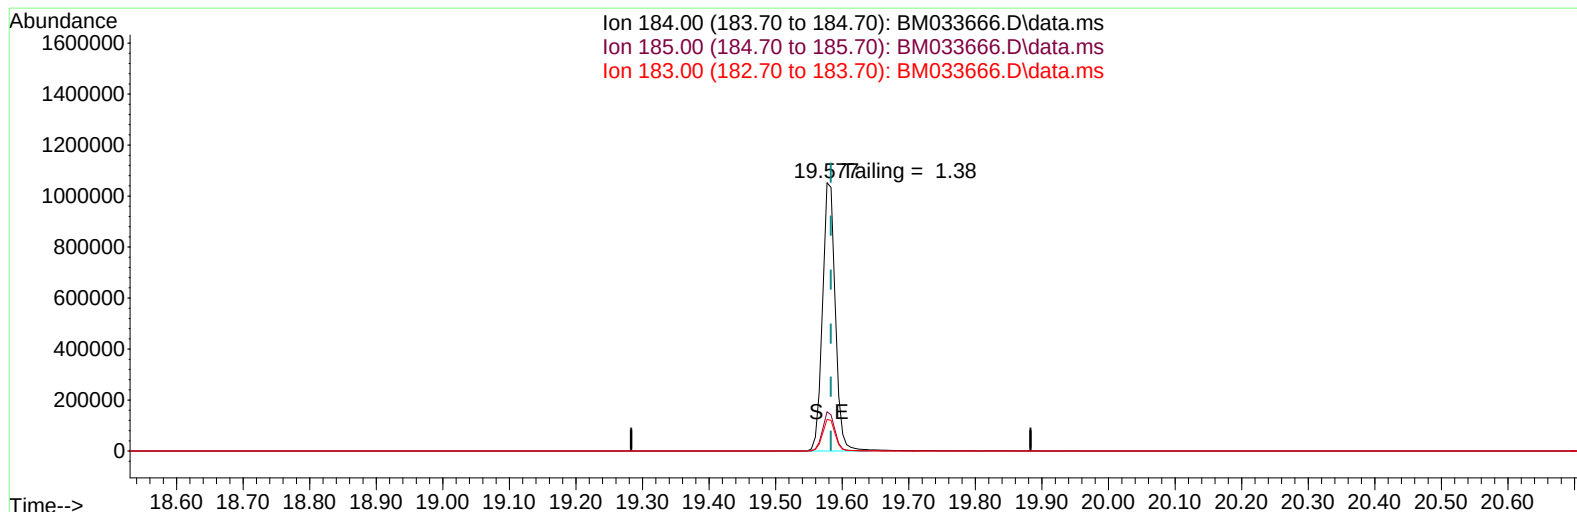




TIC: BM033666.D\data.ms

(77) Benzidine**19.577min (-0.006) 82410.75 ng****response 1412304**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.60
183.00	12.10	11.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010722\
Data File : BM033666.D
Acq On : 07 Jan 2022 12:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 09 23:55:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 05 17:07:26 2022
Response via : Initial Calibration

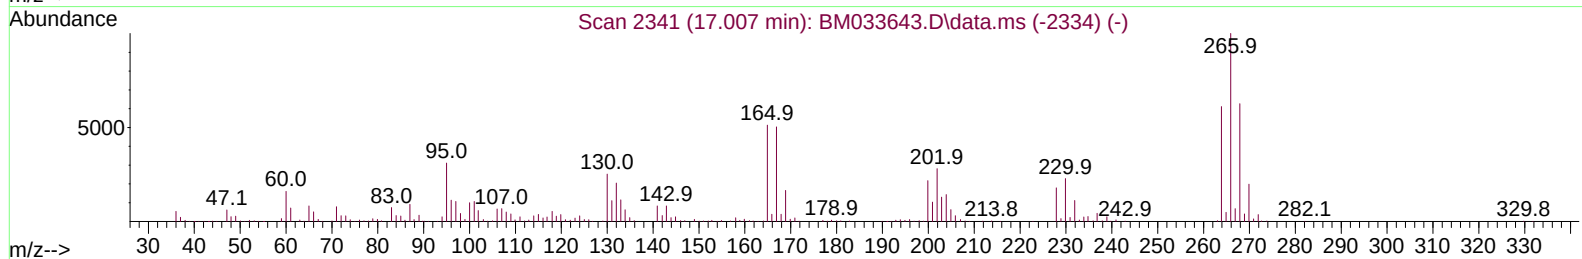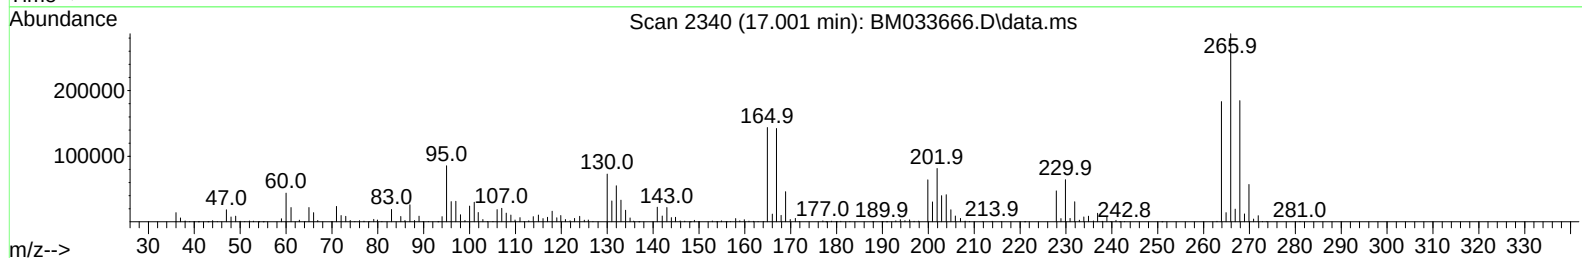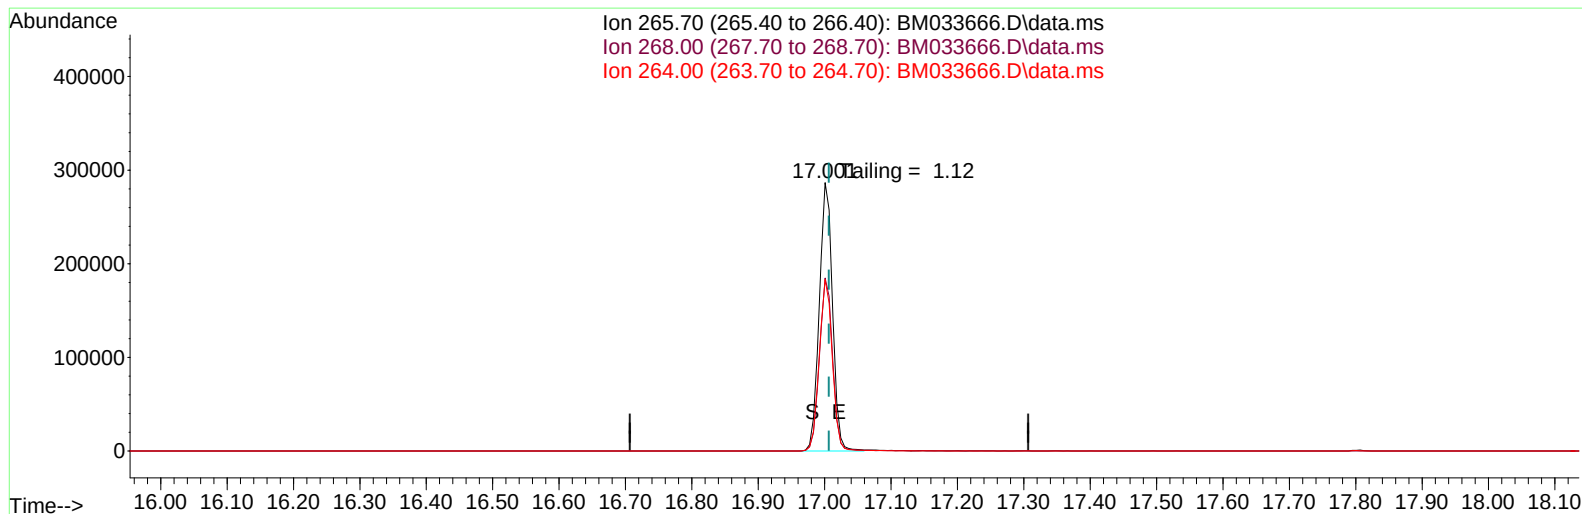

TIC: BM033666.D\data.ms

(70) Pentachlorophenol (C)

17.001min (-0.006) 229125.78 ng

response 398448

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.43
264.00	61.40	63.94
0.00	0.00	0.00