


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010722\
 Data File : BM033666.D
 Acq On : 07 Jan 2022 12:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 05 17:07:26 2022

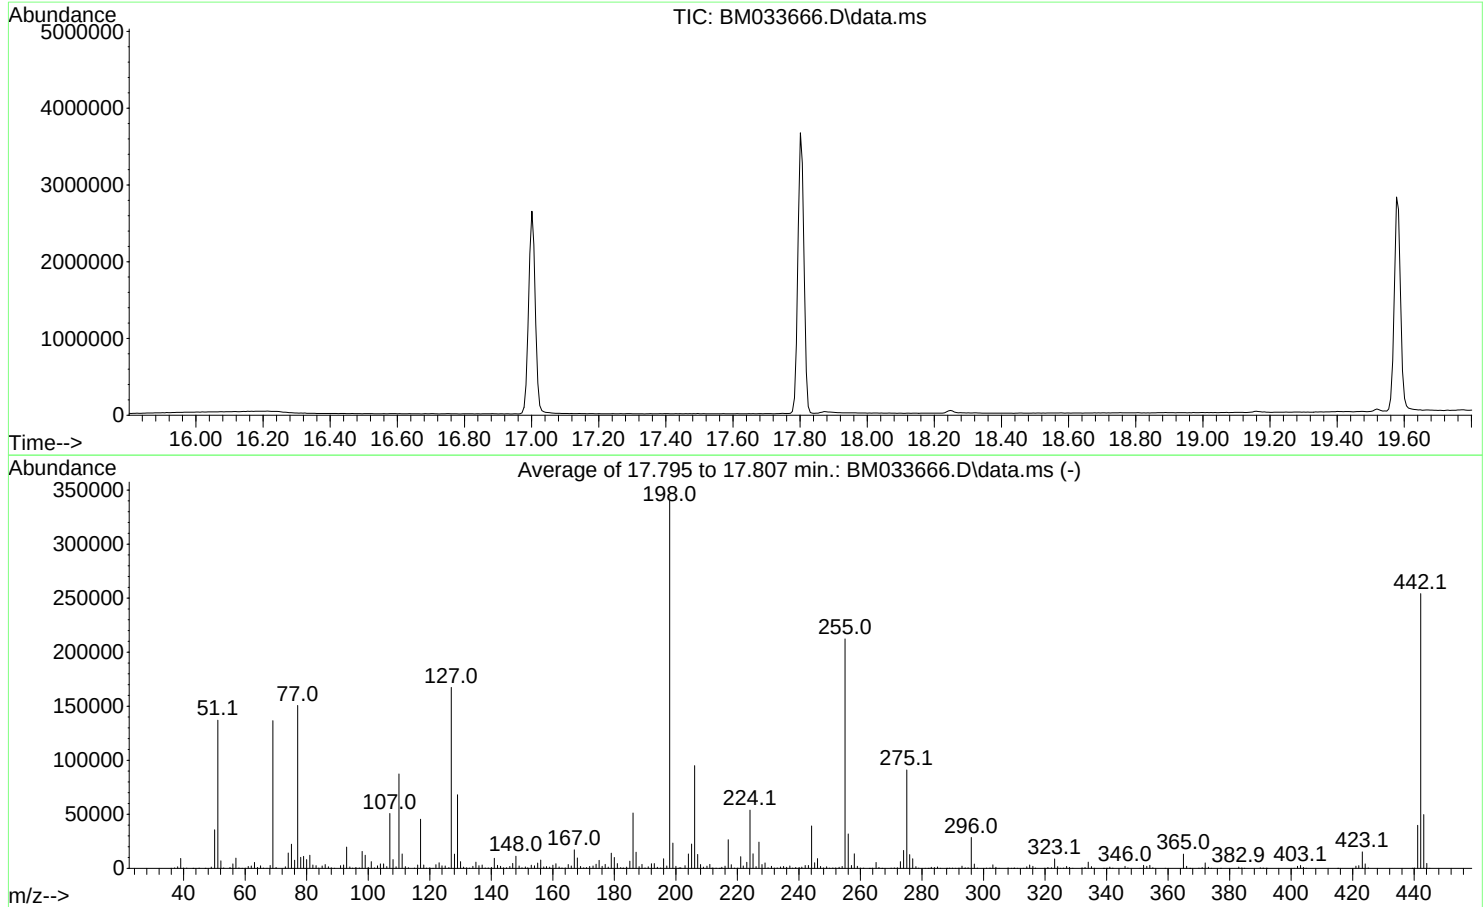

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	137118	PASS
68	69	0.00	2	2.0	2690	PASS
69	198	0.00	100	40.1	136589	PASS
70	69	0.00	2	0.6	872	PASS
127	198	10	80	49.2	167360	PASS
197	198	0.00	2	0.7	2238	PASS
198	198	100	100	100.0	340352	PASS
199	198	5	9	6.9	23328	PASS
275	198	10	60	26.7	91027	PASS
365	198	1	100	3.9	13134	PASS
441	198	0.01	100	11.7	39883	PASS
442	442	50	100	100.0	254144	PASS
443	442	15	24	19.6	49723	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/7/2022	BNA_M	<u>BM033666.D</u>
Compound Name	Response	Retention Time
DDT	1021406	20.818
DDD	16574	20.377
DDE	443	19.871
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17017	1038423	1.64

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010722\
 Data File : BM033666.D
 Acq On : 07 Jan 2022 12:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jan 09 23:55:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 05 17:07:26 2022
 Response via : Initial Calibration

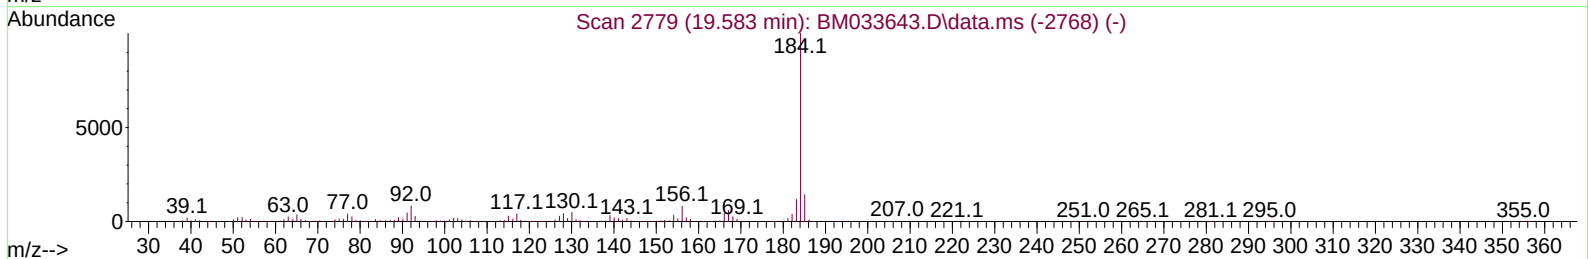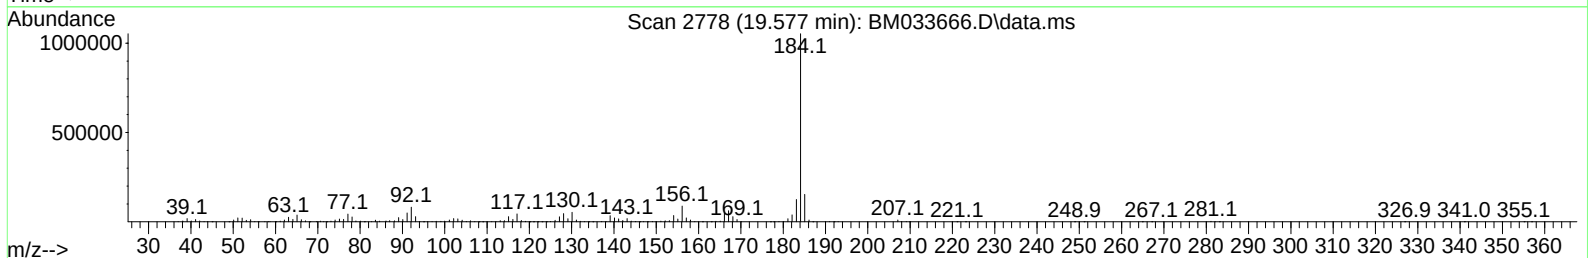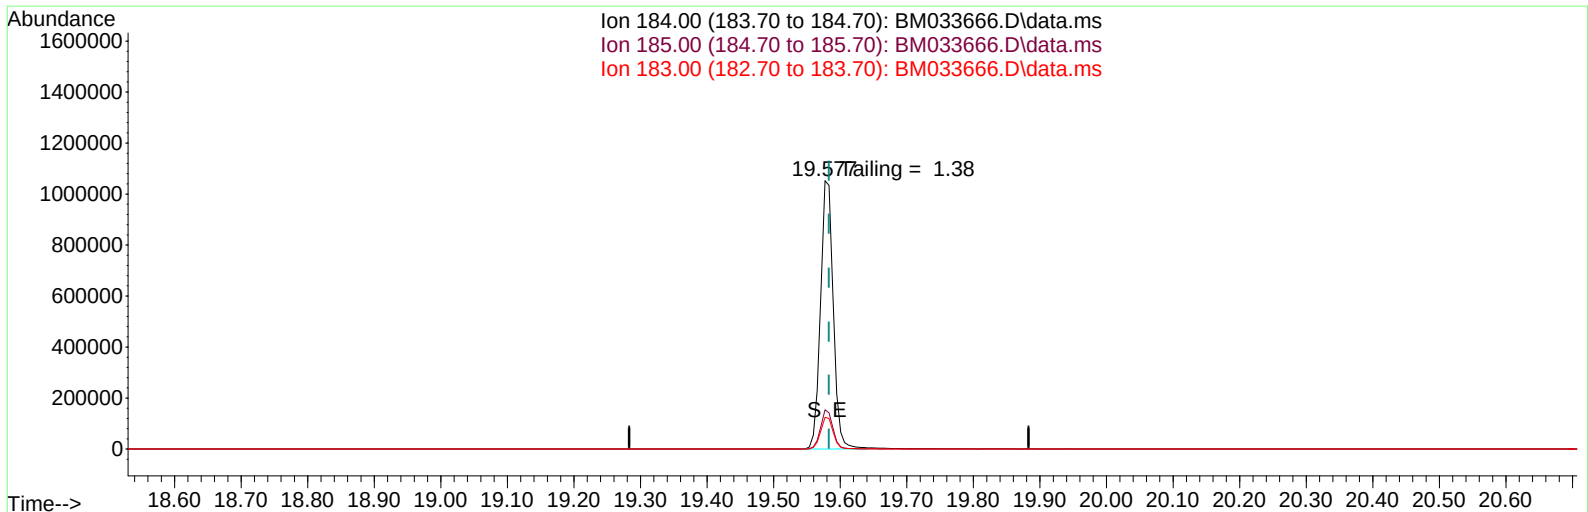

TIC: BM033666.D\data.ms

(77) Benzidine

19.577min (-0.006) 82410.75 ng


response 1412304

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.60
183.00	12.10	11.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010722\
Data File : BM033666.D
Acq On : 07 Jan 2022 12:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jan 09 23:55:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 05 17:07:26 2022
Response via : Initial Calibration

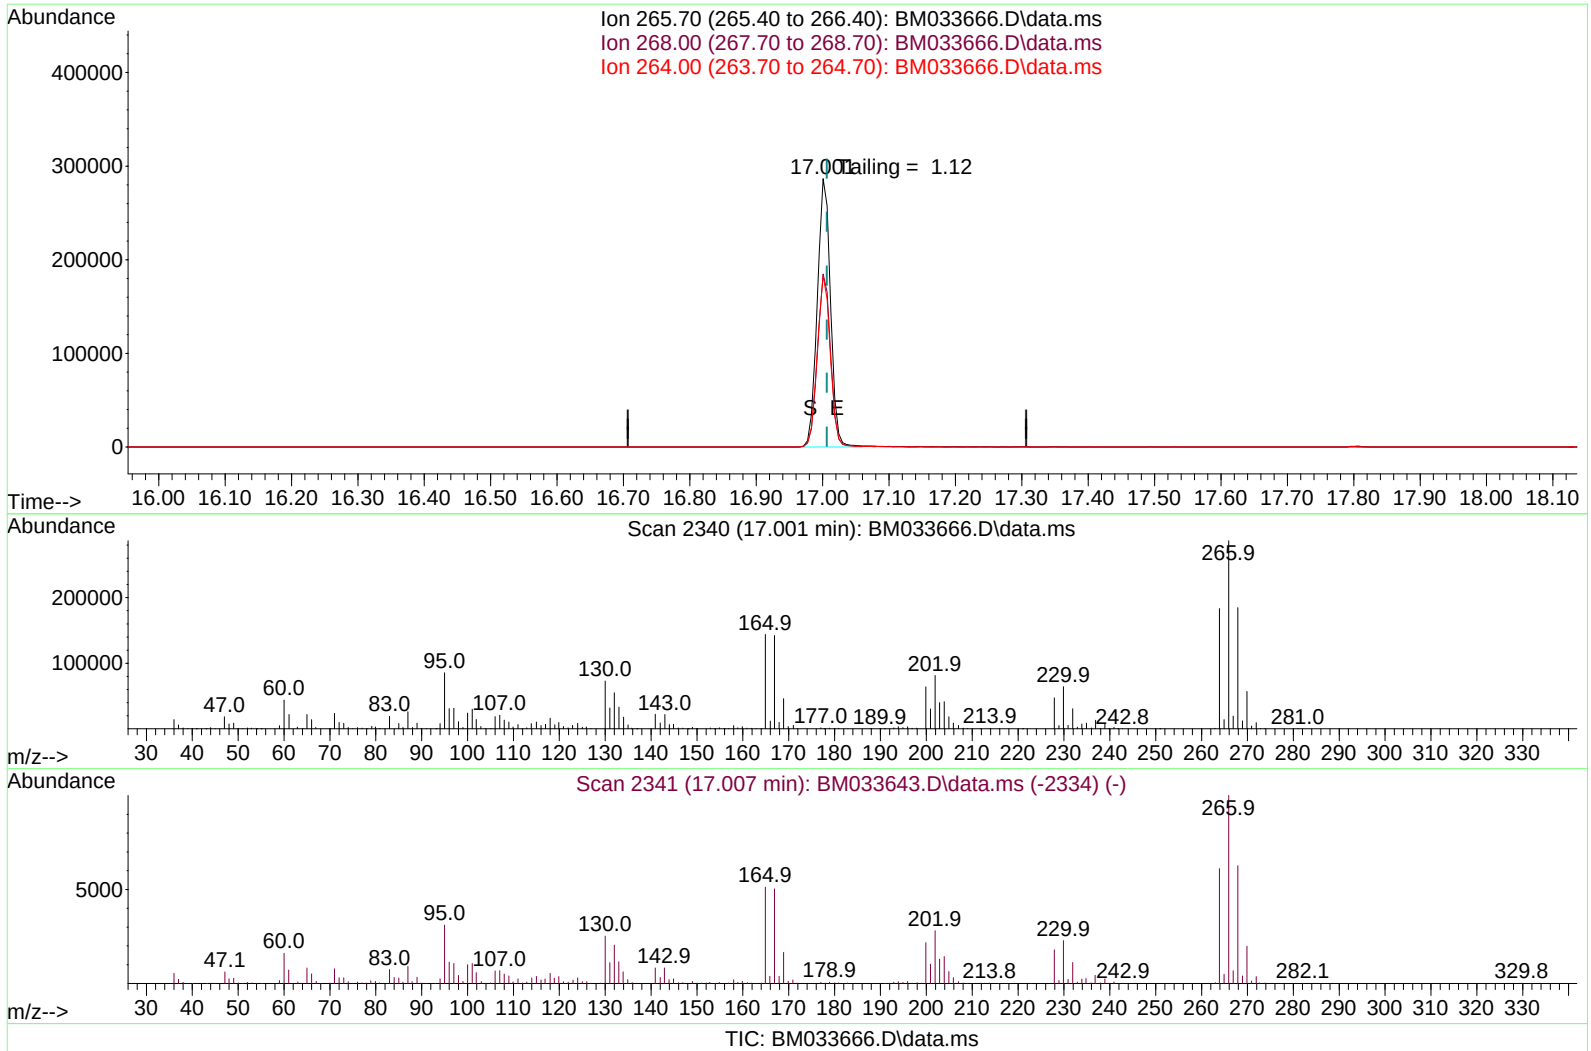

(70) Pentachlorophenol (C)

17.001min (-0.006) 229125.78 ng

response 398448

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.43
264.00	61.40	63.94
0.00	0.00	0.00