


Data Path : Z:\HPCHEM1\BNA\_M\Data\BM010815\  
Data File : BM000144.D  
Acq On : 08 Jan 2015 14:45  
Operator : TP/IZ  
Sample : DFTPP05  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM02.2-EPA-SIM-BM010715.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Thu Jan 08 10:41:47 2015

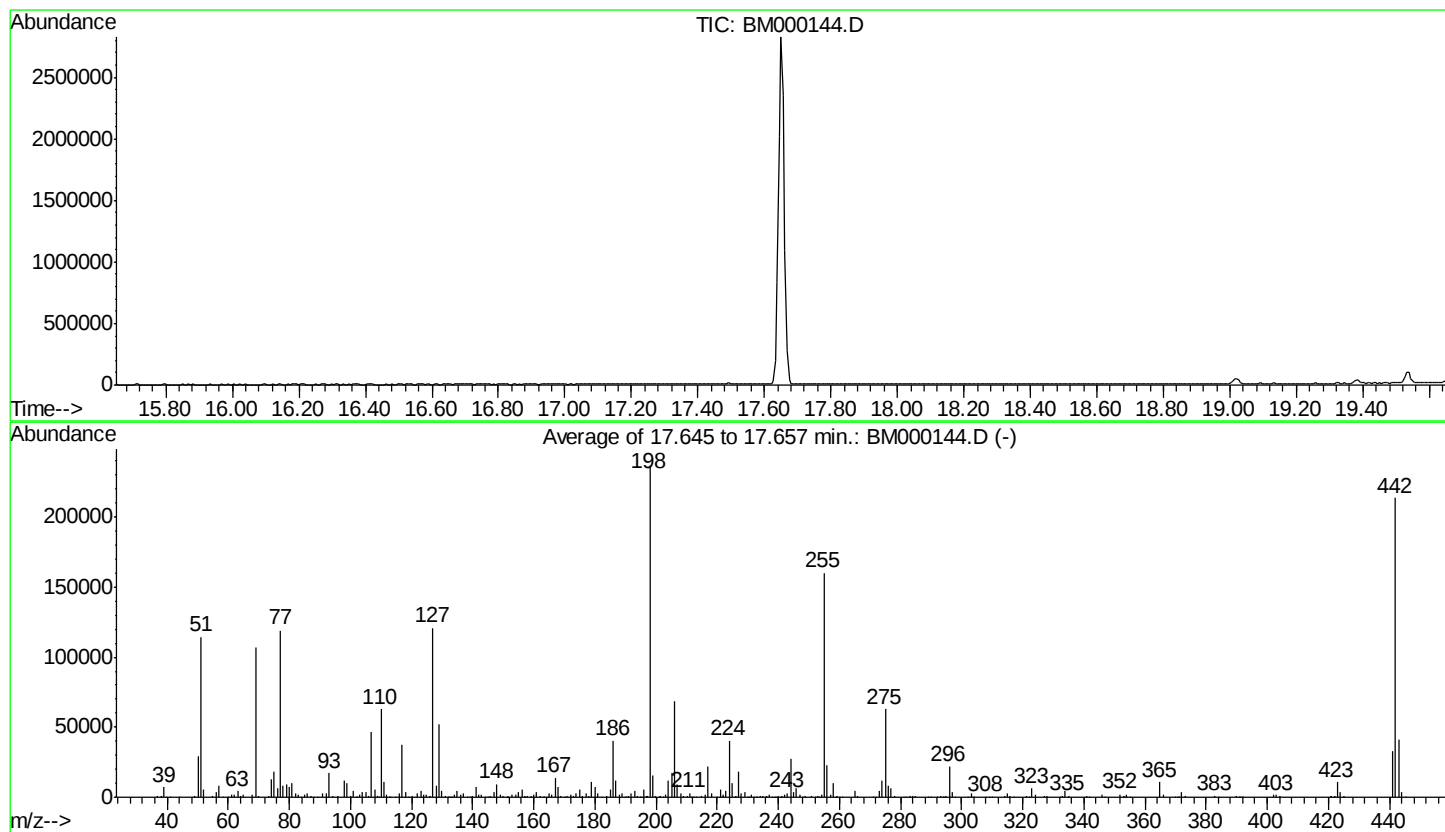

AutoFind: Scans 2543, 2544, 2545; Background Corrected with Scan 2536

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 48.4         | 114586     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.6          | 1696       | PASS                |
| 69             | 198             | 0.00            | 100             | 45.3         | 107144     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 547        | PASS                |
| 127            | 198             | 10              | 80              | 51.1         | 120952     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.4          | 987        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 236714     | PASS                |
| 199            | 198             | 5               | 9               | 6.6          | 15636      | PASS                |
| 275            | 198             | 10              | 60              | 26.5         | 62749      | PASS                |
| 365            | 198             | 1               | 100             | 4.5          | 10657      | PASS                |
| 441            | 443             | 0.01            | 100             | 80.1         | 33189      | PASS                |
| 442            | 198             | 50              | 100             | 90.3         | 213781     | PASS                |
| 443            | 442             | 15              | 24              | 19.4         | 41429      | PASS                |