


```
Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010820\  
Data File : BM024418.D  
Acq On    : 08 Jan 2020 13:37  
Operator  : JU  
Sample    : SSTD16003  
Misc      :  
ALS Vial  : 7      Sample Multiplier: 1
```

**Instrument :**  
BNA\_M  
**ClientSampleId :**  
SSTD16003

## Manual Integrations APPROVED

mohammad  
1/9/2020 12:12:35 PM

Quant Time: Jan 08 14:25:14 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM010820MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Jan 08 12:28:28 2020  
Response via : Initial Calibration

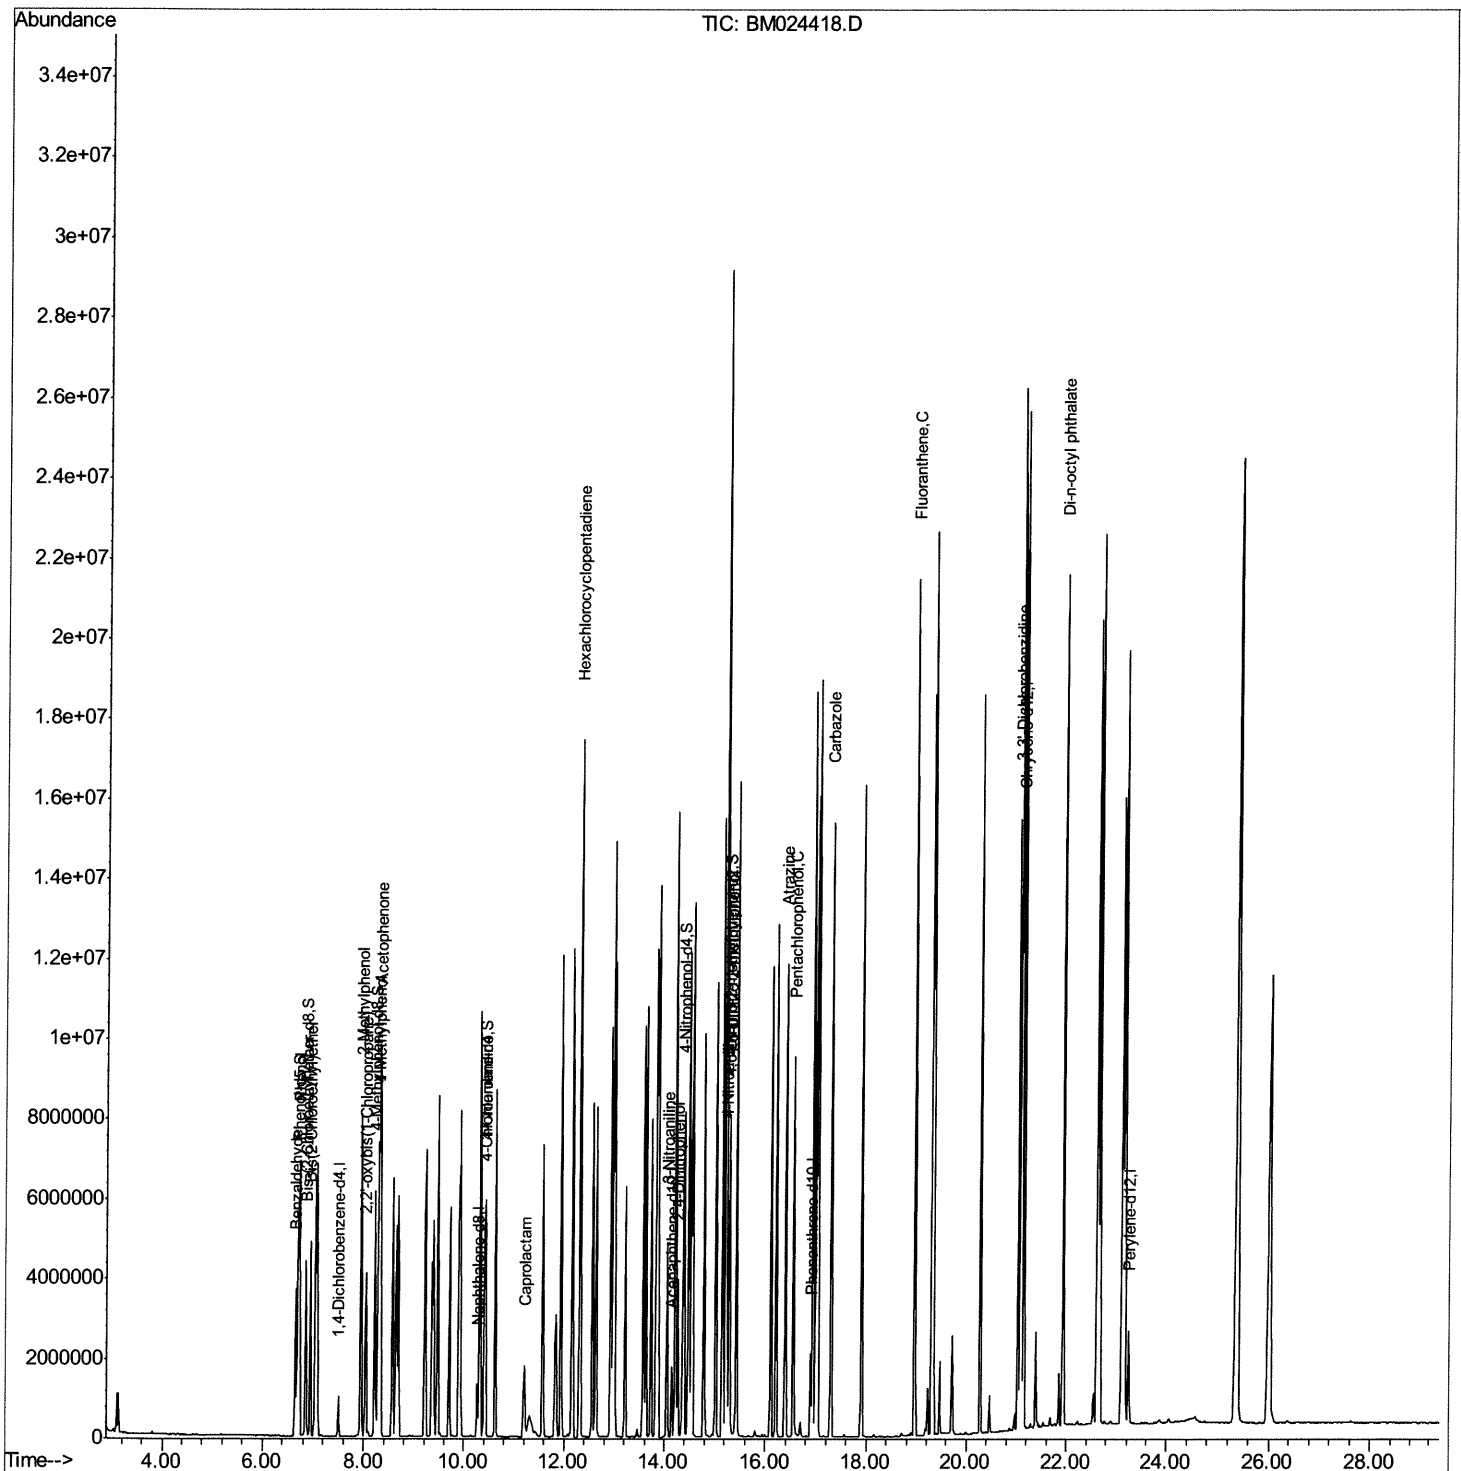

## Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM010820\  
Data File : BM024418.D  
Acq On : 08 Jan 2020 13:37  
Operator : JU  
Sample : SSTD16003  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SSTD16003

Manual Integrations  
APPROVED

mohammad  
1/9/2020 12:12:35 PM

Quant Time: Jan 08 14:17:49 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM010820MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Jan 08 12:28:28 2020  
Response via : Initial Calibration

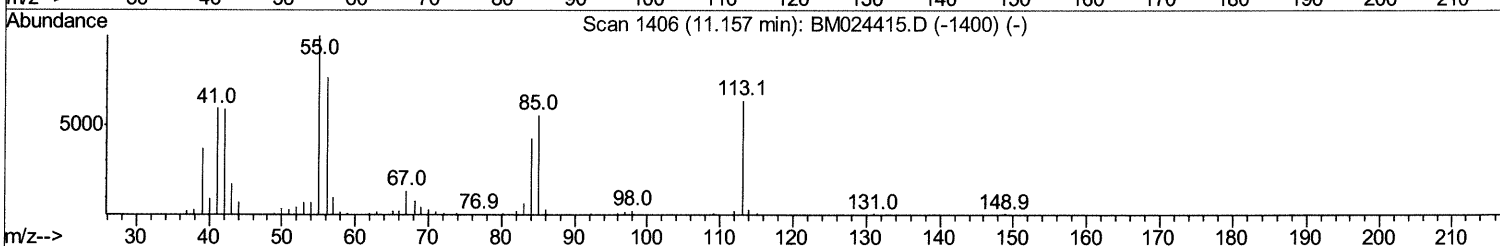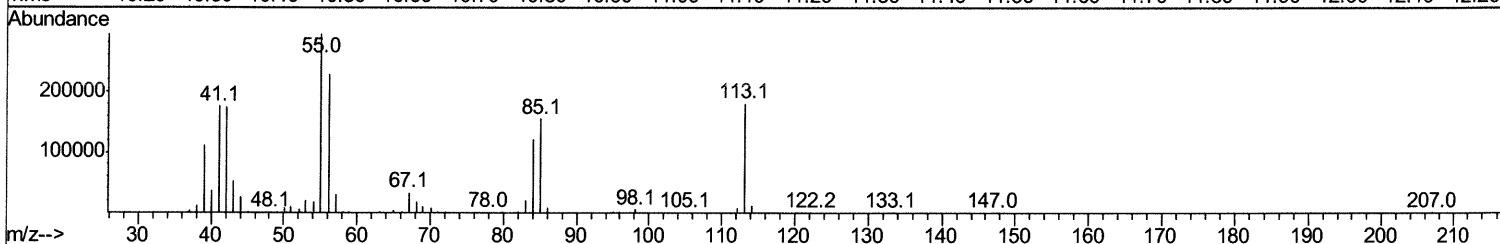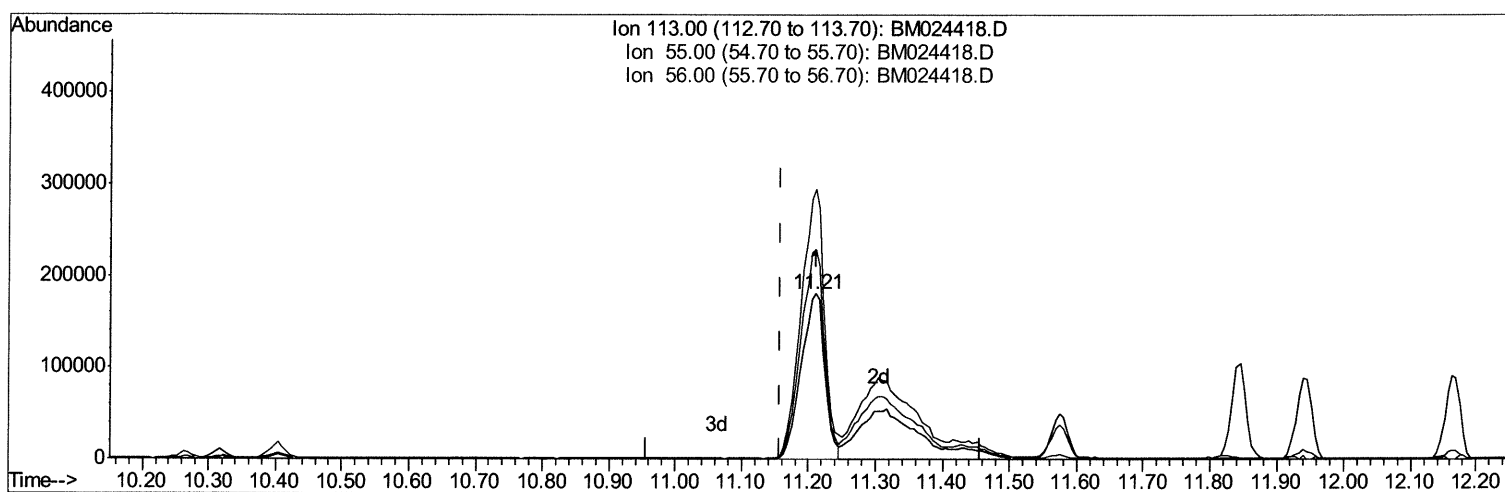

TIC: BM024418.D

(32) Caprolactam

11.210min (+0.053) 101.68ng/ul

response 442030

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 113.00 | 100    | 100    |
| 55.00  | 161.50 | 163.32 |
| 56.00  | 122.30 | 126.85 |
| 0.00   | 0.00   | 0.00   |

# Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM010820\  
 Data File : BM024418.D  
 Acq On : 08 Jan 2020 13:37  
 Operator : JU  
 Sample : SSTD16003  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 SSTD16003

Manual Integrations  
 APPROVED

mohammad  
 1/9/2020 12:12:35 PM

Quant Time: Jan 08 14:18:55 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM010820MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Jan 08 12:28:28 2020  
 Response via : Initial Calibration

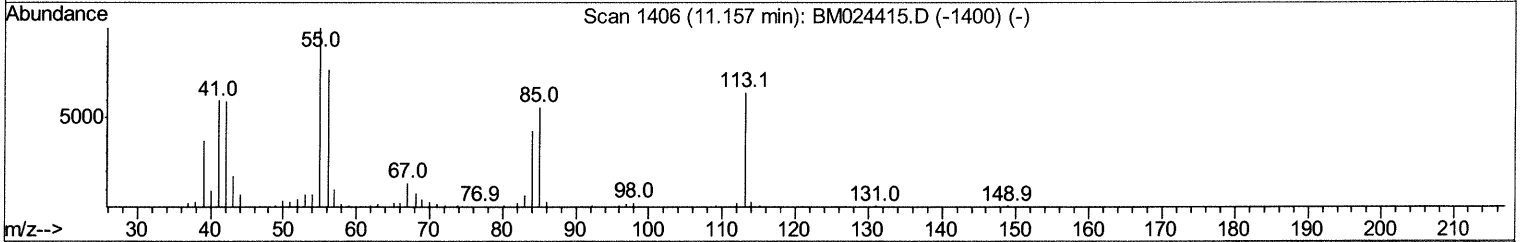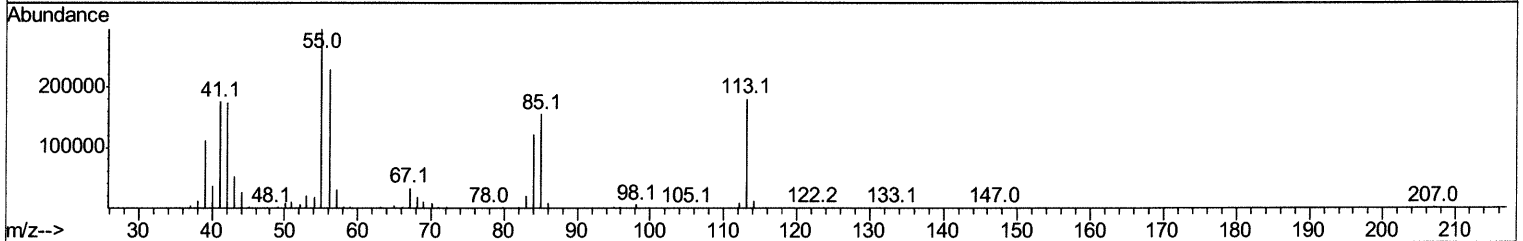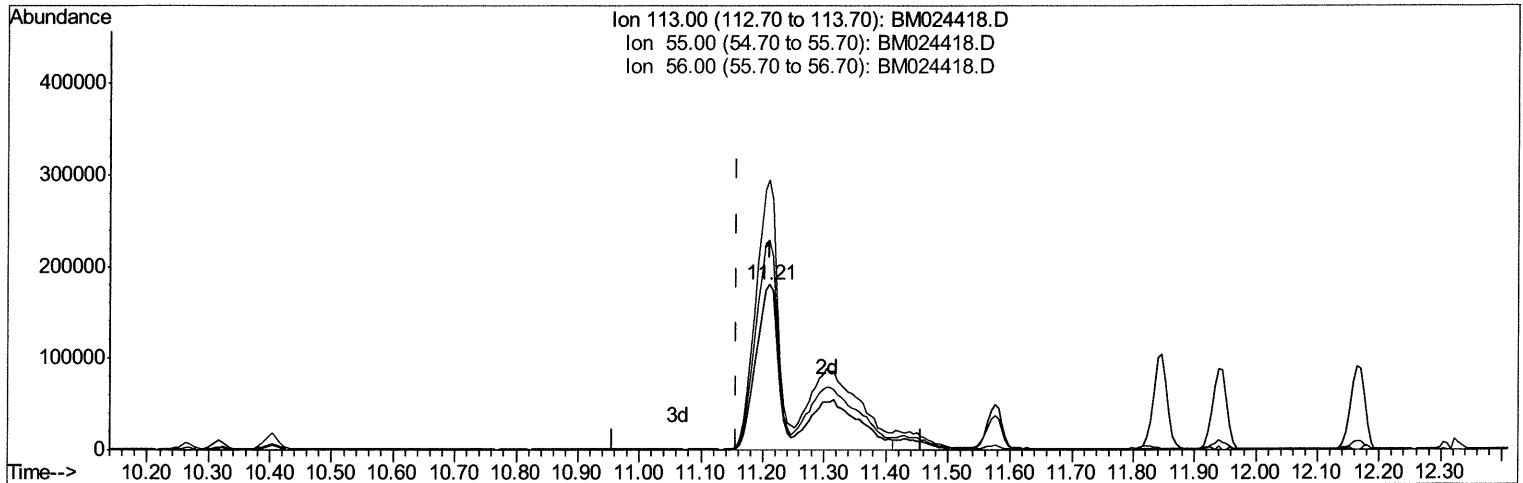

TIC: BM024418.D

(32) Caprolactam

11.210min (+0.053) 173.67ng/ul m JU 01/09/20

response 754957

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 113.00 | 100    | 100    |
| 55.00  | 161.50 | 163.32 |
| 56.00  | 122.30 | 126.85 |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010820\  
 Data File : BM024418.D  
 Acq On : 08 Jan 2020 13:37  
 Operator : JU  
 Sample : SSTD16003  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 SSTD16003

Manual Integrations  
 APPROVED

mohammad  
 1/9/2020 12:12:35 PM

Quant Time: Jan 08 14:25:14 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM010820MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Jan 08 12:28:28 2020  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 7.50  | 152  | 256806   | 20.00 | ng/ul | 0.00     |
| 18) Naphthalene-d8        | 10.26 | 136  | 1019804  | 20.00 | ng/ul | 0.00     |
| 36) Acenaphthene-d10      | 14.15 | 164  | 589868   | 20.00 | ng/ul | 0.00     |
| 62) Phenanthrene-d10      | 16.90 | 188  | 1231850  | 20.00 | ng/ul | 0.00     |
| 78) Chrysene-d12          | 21.11 | 240  | 1189367  | 20.00 | ng/ul | 0.00     |
| 86) Perylene-d12          | 23.24 | 264  | 1453080  | 20.00 | ng/ul | 0.00     |

## System Monitoring Compounds

|                                |       |     |         |        |       |      |
|--------------------------------|-------|-----|---------|--------|-------|------|
| 3) 1,4-Dioxane-d8              | 0.00  | 96  | 0d      | 0.00   | ng/ul |      |
| 5) Phenol-d5                   | 6.70  | 99  | 3235844 | 142.93 | ng/ul | 0.02 |
| 7) Bis-(2-Chloroethyl)ether-d  | 6.86  | 67  | 1855840 | 118.63 | ng/ul | 0.01 |
| 9) 2-Chlorophenol-d4           | 0.00  | 132 | 0d      | 0.00   | ng/ul |      |
| 13) 4-Methylphenol-d8          | 8.22  | 113 | 2557294 | 148.66 | ng/ul | 0.02 |
| 19) Nitrobenzene-d5            | 0.00  | 128 | 0d      | 0.00   | ng/ul |      |
| 22) 2-Nitrophenol-d4           | 0.00  | 143 | 0d      | 0.00   | ng/ul |      |
| 26) 2,4-Dichlorophenol-d3      | 0.00  | 165 | 0d      | 0.00   | ng/ul |      |
| 29) 4-Chloroaniline-d4         | 10.40 | 131 | 2449723 | 143.64 | ng/ul | 0.01 |
| 44) Dimethylphthalate-d6       | 0.00  | 166 | 0d      | 0.00   | ng/ul |      |
| 47) Acenaphthylene-d8          | 0.00  | 160 | 0d      | 0.00   | ng/ul |      |
| 52) 4-Nitrophenol-d4           | 14.37 | 143 | 1341679 | 230.85 | ng/ul | 0.03 |
| 58) Fluorene-d10               | 0.00  | 176 | 0d      | 0.00   | ng/ul |      |
| 63) 4,6-Dinitro-2-methylphenol | 15.28 | 200 | 1174745 | 167.83 | ng/ul | 0.02 |
| 71) Anthracene-d10             | 0.00  | 188 | 0d      | 0.00   | ng/ul |      |
| 79) Pyrene-d10                 | 0.00  | 212 | 0d      | 0.00   | ng/ul |      |
| 90) Benzo(a)pyrene-d12         | 0.00  | 264 | 0d      | 0.00   | ng/ul |      |

## Target Compounds

|                                |       |     |          |         | Ovalue |     |
|--------------------------------|-------|-----|----------|---------|--------|-----|
| 4) Benzaldehyde                | 6.65  | 77  | 1167277  | 87.022  | ng/ul  | 96  |
| 6) Phenol                      | 6.73  | 94  | 3268286  | 136.387 | ng/ul  | 99  |
| 8) Bis(2-Chloroethyl)ether     | 6.95  | 93  | 2532003  | 130.833 | ng/ul  | 100 |
| 11) 2-Methylphenol             | 7.95  | 108 | 2451474  | 145.331 | ng/ul  | 99  |
| 12) 2,2'-oxybis(1-Chloropropan | 8.05  | 45  | 3339107  | 139.997 | ng/ul  | 99  |
| 14) Acetophenone               | 8.32  | 105 | 3867897  | 138.083 | ng/ul  | 99  |
| 16) 4-Methylphenol             | 8.29  | 108 | 2598514  | 142.501 | ng/ul  | 97  |
| 30) 4-Chloroaniline            | 10.43 | 127 | 2411856  | 141.261 | ng/ul  | 99  |
| 32) Caprolactam                | 11.21 | 113 | 754957m  | 173.667 | ng/ul  | >   |
| 38) Hexachlorocyclopentadiene  | 12.32 | 237 | 2401750  | 351.399 | ng/ul  | 98  |
| 49) 3-Nitroaniline             | 14.06 | 138 | 1173717  | 170.482 | ng/ul# | 92  |
| 51) 2,4-Dinitrophenol          | 14.26 | 184 | 775097   | 197.588 | ng/ul  | 91  |
| 53) 4-Nitrophenol              | 14.39 | 109 | 1119016  | 216.863 | ng/ul  | 98  |
| 61) 4-Nitroaniline             | 15.24 | 138 | 1518896  | 222.254 | ng/ul  | 98  |
| 64) 4,6-Dinitro-2-methylphenol | 15.30 | 198 | 1246085  | 167.324 | ng/ul# | 93  |
| 68) Atrazine                   | 16.40 | 200 | 2171247  | 166.442 | ng/ul  | 98  |
| 69) Pentachlorophenol          | 16.56 | 266 | 1594808  | 226.194 | ng/ul  | 98  |
| 75) Carbazole                  | 17.30 | 167 | 9487611  | 161.657 | ng/ul  | 99  |
| 77) Fluoranthene               | 18.97 | 202 | 12232394 | 156.600 | ng/ul# | 95  |
| 82) 3,3'-Dichlorobenzidine     | 21.03 | 252 | 4240576  | 174.317 | ng/ul  | 100 |
| 87) Di-n-octyl phthalate       | 21.93 | 149 | 11851908 | 132.211 | ng/ul  | 100 |

Ju 01/09/20

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010820\  
Data File : BM024418.D  
Acq On : 08 Jan 2020 13:37  
Operator : JU  
Sample : SSTD16003  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SSTD16003

Manual Integrations  
APPROVED

mohammad  
1/9/2020 12:12:35 PM

Quant Time: Jan 08 14:25:14 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM010820MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Jan 08 12:28:28 2020  
Response via : Initial Calibration

| Internal Standards                                                         | R.T. | QIon | Response | Conc | Units | Dev(Min) |
|----------------------------------------------------------------------------|------|------|----------|------|-------|----------|
| -----                                                                      |      |      |          |      |       |          |
| (#) = qualifier out of range (m) = manual integration (+) = signals summed |      |      |          |      |       |          |