

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010824\
 Data File : BM043791.D
 Acq On : 08 Jan 2024 11:23
 Operator : MA/JU
 Sample : PB158128BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK128

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043791.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	26	29	39	rVB	106774	147565	2.55%	0.211%
2	3.787	99	102	128	rBV	1130672	1982970	34.27%	2.832%
3	4.099	153	155	161	rVB2	22986	30411	0.53%	0.043%
4	7.122	662	669	682	rBV	1345734	2273856	39.30%	3.247%
5	7.287	691	697	707	rBV	1058676	1740620	30.08%	2.486%
6	7.481	722	730	741	rBV	1374369	2276705	39.35%	3.252%
7	7.810	781	786	788	rBV6	3658	5954	0.10%	0.009%
8	7.946	802	809	818	rBV	1134113	1888049	32.63%	2.696%
9	8.669	926	932	948	rBV	1477008	2605409	45.03%	3.721%
10	9.128	1002	1010	1026	rBV	1220157	2110379	36.47%	3.014%
11	9.487	1068	1071	1075	rVB5	4215	6592	0.11%	0.009%
12	9.845	1124	1132	1143	rBV	1030346	1769372	30.58%	2.527%
13	10.387	1217	1224	1241	rBV	1324077	2566968	44.36%	3.666%
14	10.757	1280	1287	1298	rBV	1464788	2501149	43.22%	3.572%
15	10.916	1306	1314	1339	rBV	1227692	2605262	45.02%	3.721%
16	12.363	1555	1560	1568	rVB3	18860	41014	0.71%	0.059%
17	13.492	1745	1752	1754	rBV7	9930	15992	0.28%	0.023%
18	13.581	1760	1767	1770	rBV7	6009	13644	0.24%	0.019%
19	14.016	1834	1841	1856	rBV	2169359	3223369	55.71%	4.603%
20	14.286	1880	1887	1900	rBV	2715503	4223834	72.99%	6.032%
21	14.592	1932	1939	1949	rBV	2028163	2953339	51.04%	4.218%
22	14.833	1972	1980	2005	rBV	668965	1613159	27.88%	2.304%
23	15.586	2102	2108	2121	rBV	3328356	4896112	84.61%	6.992%
24	15.727	2125	2132	2146	rVV	718013	1178885	20.37%	1.684%
25	15.827	2146	2149	2157	rVB6	20243	34984	0.60%	0.050%
26	16.157	2203	2205	2211	rVB6	5055	7635	0.13%	0.011%
27	16.369	2236	2241	2245	rBV6	12691	18672	0.32%	0.027%
28	16.474	2256	2259	2263	rVB6	4326	6448	0.11%	0.009%
29	17.016	2346	2351	2356	rVB8	11435	24091	0.42%	0.034%
30	17.345	2400	2407	2416	rBV	2208016	3268384	56.48%	4.668%
31	17.445	2417	2424	2438	rVV	3407110	5167626	89.31%	7.380%
32	18.251	2557	2561	2568	rBV9	12604	26402	0.46%	0.038%
33	18.321	2570	2573	2575	rBV2	11843	12759	0.22%	0.018%
34	18.998	2686	2688	2690	rBV3	7867	7978	0.14%	0.011%
35	19.298	2735	2739	2743	rBV4	41664	62177	1.07%	0.089%
36	19.368	2748	2751	2755	rVV2	34249	45658	0.79%	0.065%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010824\
Data File : BM043791.D
Acq On : 08 Jan 2024 11:23
Operator : MA/JU
Sample : PB158128BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK128

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION

37	19.733	2807	2813	2824	rBV	4163703	5769711	99.71%	8.240%
38	21.439	3100	3103	3110	rBV	160933	212050	3.66%	0.303%
39	21.527	3113	3118	3126	rBV	2538893	3368737	58.22%	4.811%
40	23.792	3496	3503	3511	rBV2	2865877	5786473	100.00%	8.264%
41	23.945	3523	3529	3539	rVB	1683211	3529711	61.00%	5.041%




Sum of corrected areas: 70020105

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010824\
Data File : BM043791.D
Acq On : 08 Jan 2024 11:23
Operator : MA/JU
Sample : PB158128BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK128

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

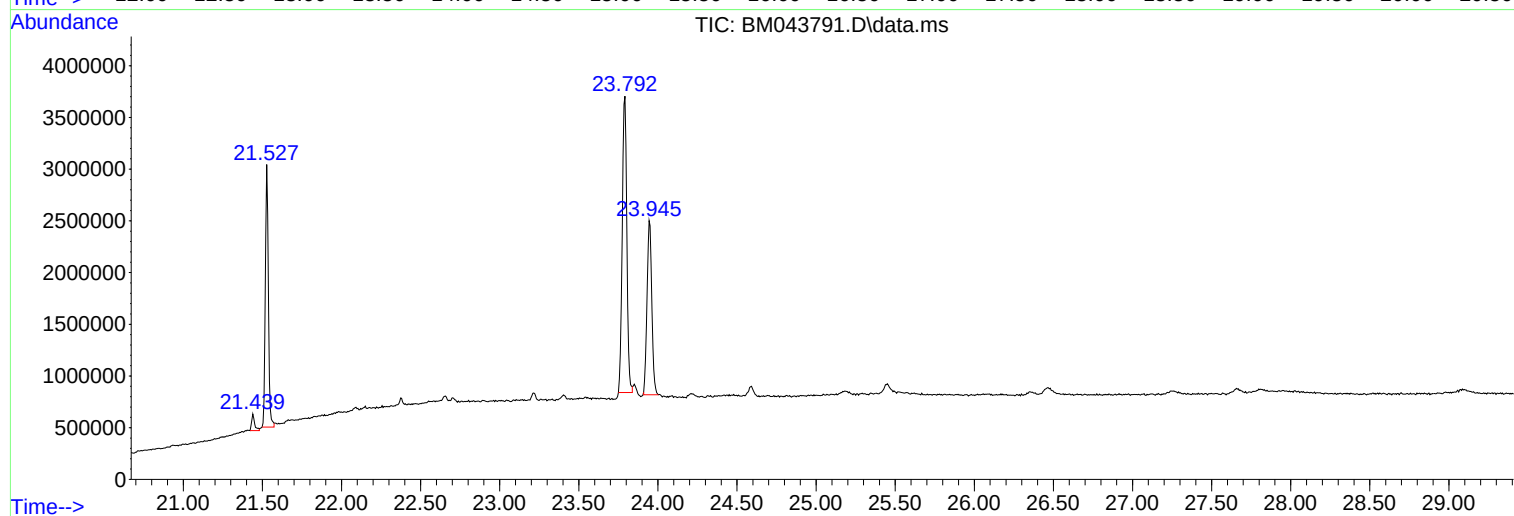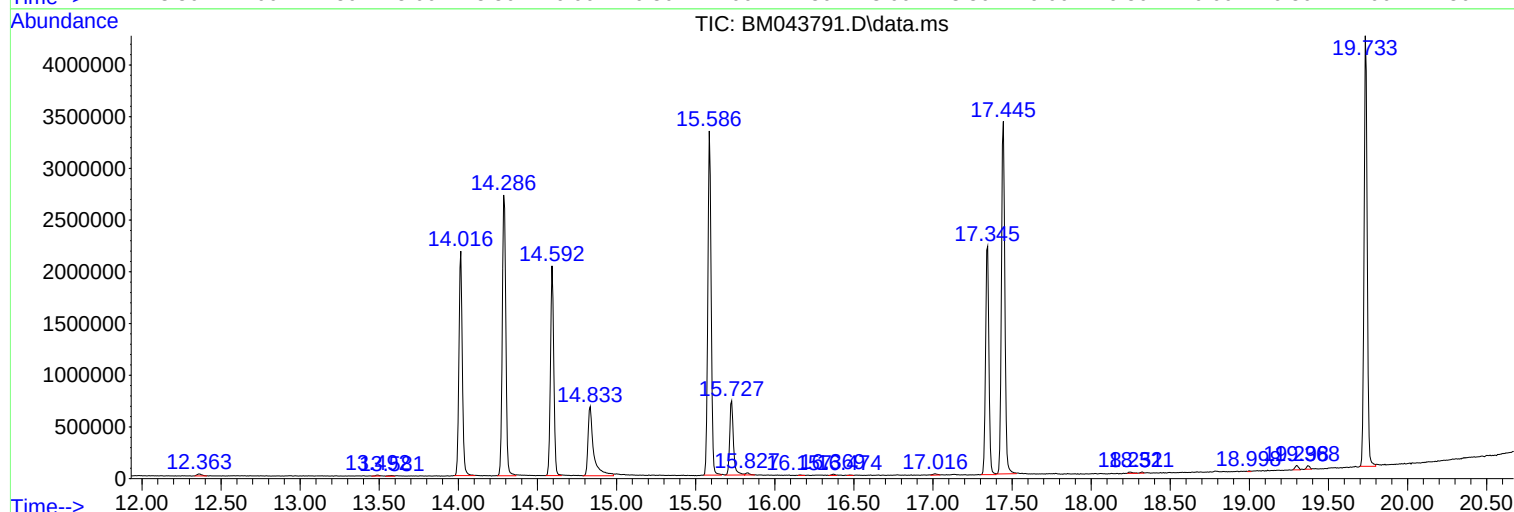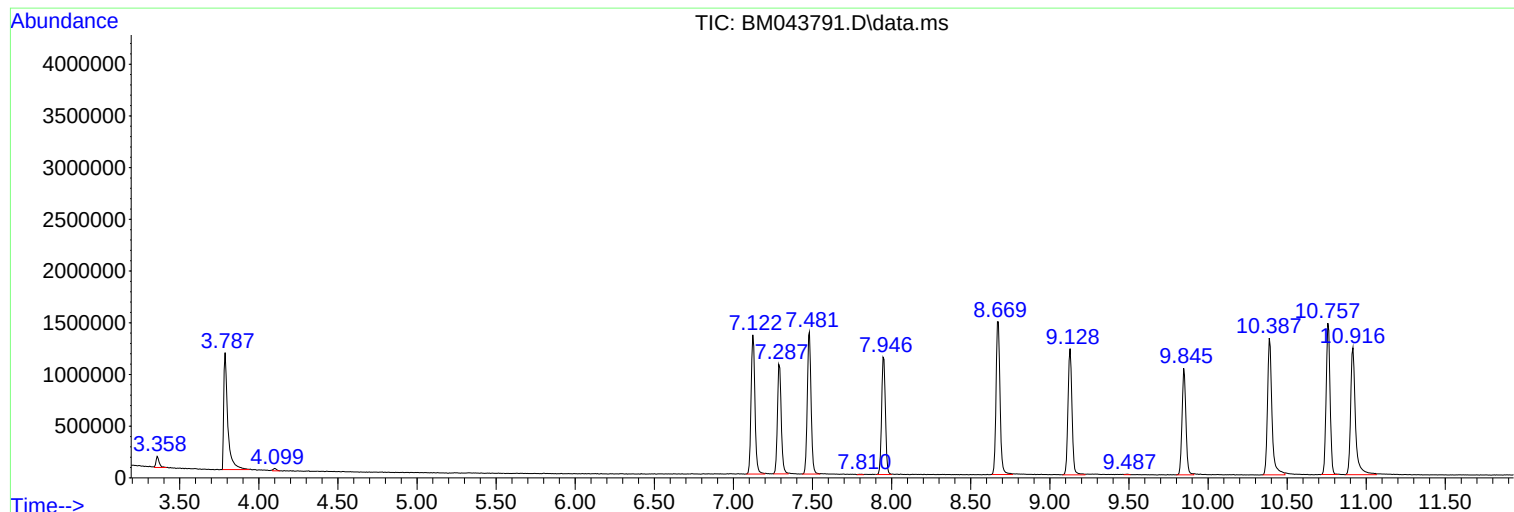

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010824\
Data File : BM043791.D
Acq On : 08 Jan 2024 11:23
Operator : MA/JU
Sample : PB158128BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK128

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010824\
Data File : BM043791.D
Acq On : 08 Jan 2024 11:23
Operator : MA/JU
Sample : PB158128BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK128

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc