

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010824\
 Data File : BM043796.D
 Acq On : 08 Jan 2024 16:26
 Operator : MA/JU
 Sample : 05952-13DL 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCF96DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043796.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.099	152	155	159	rVB	19253	22380	0.48%	0.069%
2	4.922	291	295	300	rVB7	5016	7634	0.17%	0.024%
3	5.034	310	314	316	rBV	9158	12087	0.26%	0.037%
4	5.793	441	443	449	rBV7	4287	4646	0.10%	0.014%
5	6.904	630	632	634	rBV3	5014	4986	0.11%	0.015%
6	6.969	637	643	647	rBV8	6433	15397	0.33%	0.048%
7	7.122	663	669	682	rVB	115232	227233	4.91%	0.703%
8	7.287	692	697	707	rVB	141883	227463	4.92%	0.704%
9	7.475	723	729	737	rVB	144984	249647	5.40%	0.772%
10	7.945	796	809	820	rBV	1250063	2016882	43.61%	6.240%
11	8.045	823	826	831	rBV6	5873	10440	0.23%	0.032%
12	8.151	839	844	849	rBV6	10187	19165	0.41%	0.059%
13	8.404	883	887	890	rBV5	3215	4627	0.10%	0.014%
14	8.463	892	897	899	rBV5	6395	9097	0.20%	0.028%
15	8.598	916	920	925	rVB4	8772	13087	0.28%	0.040%
16	8.681	927	934	948	rVV2	60725	130511	2.82%	0.404%
17	8.798	948	954	958	rBV7	7298	16133	0.35%	0.050%
18	9.128	1002	1010	1022	rBV	134588	263345	5.69%	0.815%
19	9.851	1126	1133	1141	rBV	86338	160523	3.47%	0.497%
20	9.987	1151	1156	1158	rVB6	2932	4741	0.10%	0.015%
21	10.404	1220	1227	1240	rBV	92218	252136	5.45%	0.780%
22	10.622	1259	1264	1269	rVB6	11411	21223	0.46%	0.066%
23	10.757	1275	1287	1298	rBV	1581794	2709552	58.58%	8.383%
24	11.804	1459	1465	1466	rBV5	4759	8118	0.18%	0.025%
25	12.163	1521	1526	1532	rBV10	2660	5440	0.12%	0.017%
26	12.586	1597	1598	1603	rVB5	6162	7228	0.16%	0.022%
27	13.063	1676	1679	1680	rBV3	5710	6148	0.13%	0.019%
28	13.075	1680	1681	1685	rVB4	5843	6851	0.15%	0.021%
29	13.410	1731	1738	1739	rBV6	9948	15095	0.33%	0.047%
30	13.486	1744	1751	1756	rVV3	24751	40530	0.88%	0.125%
31	13.592	1764	1769	1775	rVV10	16175	27495	0.59%	0.085%
32	13.639	1775	1777	1780	rVB4	6035	5865	0.13%	0.018%
33	13.722	1786	1791	1796	rBV8	20112	32277	0.70%	0.100%
34	13.769	1796	1799	1804	rVB6	9219	14591	0.32%	0.045%
35	13.845	1807	1812	1817	rBV4	101914	170150	3.68%	0.526%
36	13.898	1817	1821	1828	rVB6	29103	56450	1.22%	0.175%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010824\
Data File : BM043796.D
Acq On : 08 Jan 2024 16:26
Operator : MA/JU
Sample : 05952-13DL 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF96DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION

37	14.016	1836	1841	1852	rBV	203920	322173	6.97%	0.997%
38	14.186	1867	1870	1874	rVB6	4583	5661	0.12%	0.018%
39	14.227	1874	1877	1879	rBV4	6176	7581	0.16%	0.023%
40	14.286	1881	1887	1898	rVV	351091	573001	12.39%	1.773%
41	14.404	1903	1907	1913	rVV9	10929	20480	0.44%	0.063%
42	14.480	1915	1920	1926	rVB3	31431	54396	1.18%	0.168%
43	14.527	1926	1928	1930	rBV2	6407	6433	0.14%	0.020%
44	14.592	1932	1939	1958	rVB	2293378	3431801	74.20%	10.618%
45	14.904	1989	1992	1999	rVB8	7618	14091	0.30%	0.044%
46	14.980	2002	2005	2007	rBV4	8792	10498	0.23%	0.032%
47	15.045	2013	2016	2023	rVB8	11724	18881	0.41%	0.058%
48	15.098	2023	2025	2029	rVB5	5934	7768	0.17%	0.024%
49	15.151	2030	2034	2035	rVV4	9733	12182	0.26%	0.038%
50	15.169	2035	2037	2039	rVV3	10999	12855	0.28%	0.040%
51	15.198	2039	2042	2043	rVV2	21468	23402	0.51%	0.072%
52	15.227	2043	2047	2058	rVB2	59958	115446	2.50%	0.357%
53	15.363	2066	2070	2075	rVB8	9850	17899	0.39%	0.055%
54	15.433	2078	2082	2086	rVB	45050	57235	1.24%	0.177%
55	15.474	2086	2089	2091	rBV4	7364	10241	0.22%	0.032%
56	15.521	2093	2097	2101	rVV4	16074	29423	0.64%	0.091%
57	15.586	2103	2108	2117	rVB	447221	720307	15.57%	2.229%
58	15.727	2129	2132	2139	rBV5	28896	52352	1.13%	0.162%
59	15.839	2144	2151	2153	rBV3	27948	59368	1.28%	0.184%
60	15.868	2153	2156	2162	rVB2	82864	121743	2.63%	0.377%
61	15.927	2164	2166	2168	rBV3	6840	7005	0.15%	0.022%
62	16.068	2185	2190	2194	rBV7	15162	27762	0.60%	0.086%
63	16.298	2224	2229	2240	rBV2	122024	282797	6.11%	0.875%
64	16.457	2253	2256	2260	rBV6	22705	32996	0.71%	0.102%
65	16.698	2295	2297	2303	rVB6	30162	39442	0.85%	0.122%
66	16.992	2341	2347	2359	rBV	2120582	3263815	70.57%	10.098%
67	17.092	2360	2364	2367	rVV	206515	278755	6.03%	0.862%
68	17.139	2367	2372	2383	rVB4	119375	281976	6.10%	0.872%
69	17.345	2401	2407	2418	rBV	2750184	3990527	86.28%	12.347%
70	17.445	2419	2424	2434	rVB	430369	711976	15.39%	2.203%
71	17.792	2481	2483	2486	rBV4	32698	39854	0.86%	0.123%
72	17.833	2486	2490	2498	rVB	258822	334119	7.22%	1.034%
73	18.233	2554	2558	2562	rVB3	130693	212272	4.59%	0.657%
74	18.527	2605	2608	2614	rBV	221142	274435	5.93%	0.849%
75	19.162	2713	2716	2719	rVB	135192	141386	3.06%	0.437%
76	19.739	2809	2814	2819	rBV	700537	984736	21.29%	3.047%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010824\
Data File : BM043796.D
Acq On : 08 Jan 2024 16:26
Operator : MA/JU
Sample : 05952-13DL 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF96DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Title : SVOA CALIBRATION

77	21.533	3114	3119	3130	rVB	3101399	4287116	92.69%	13.264%
78	23.950	3524	3530	3539	rVB	2269500	4625199	100.00%	14.310%




Sum of corrected areas: 32320558

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010824\
Data File : BM043796.D
Acq On : 08 Jan 2024 16:26
Operator : MA/JU
Sample : 05952-13DL 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF96DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

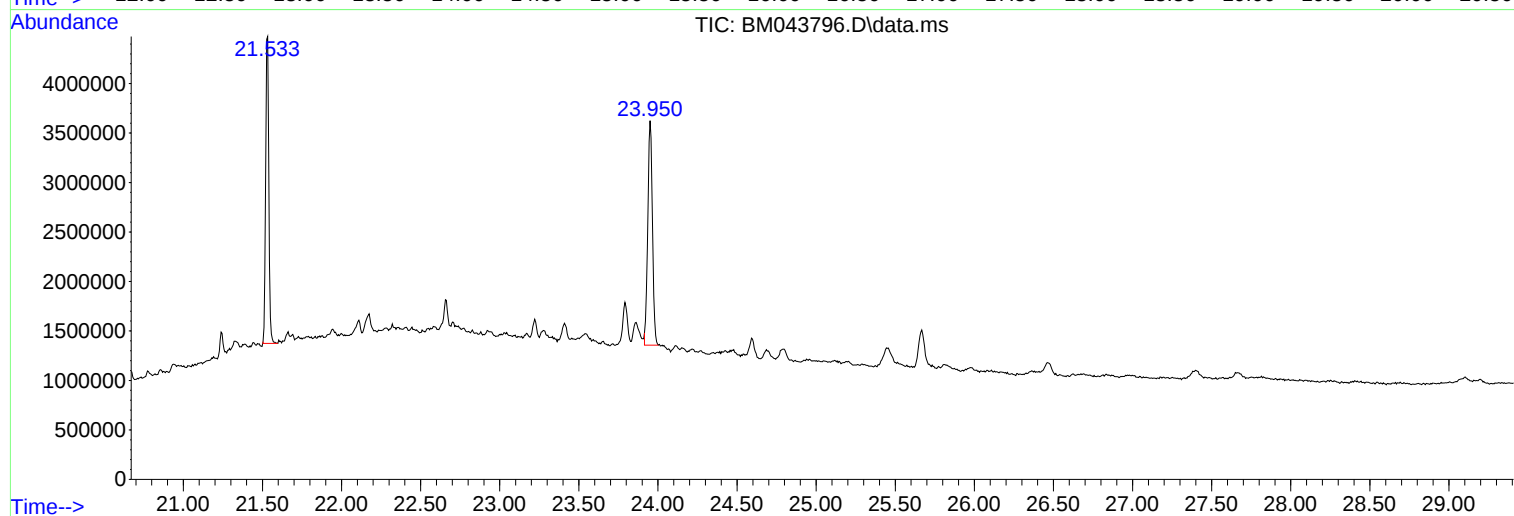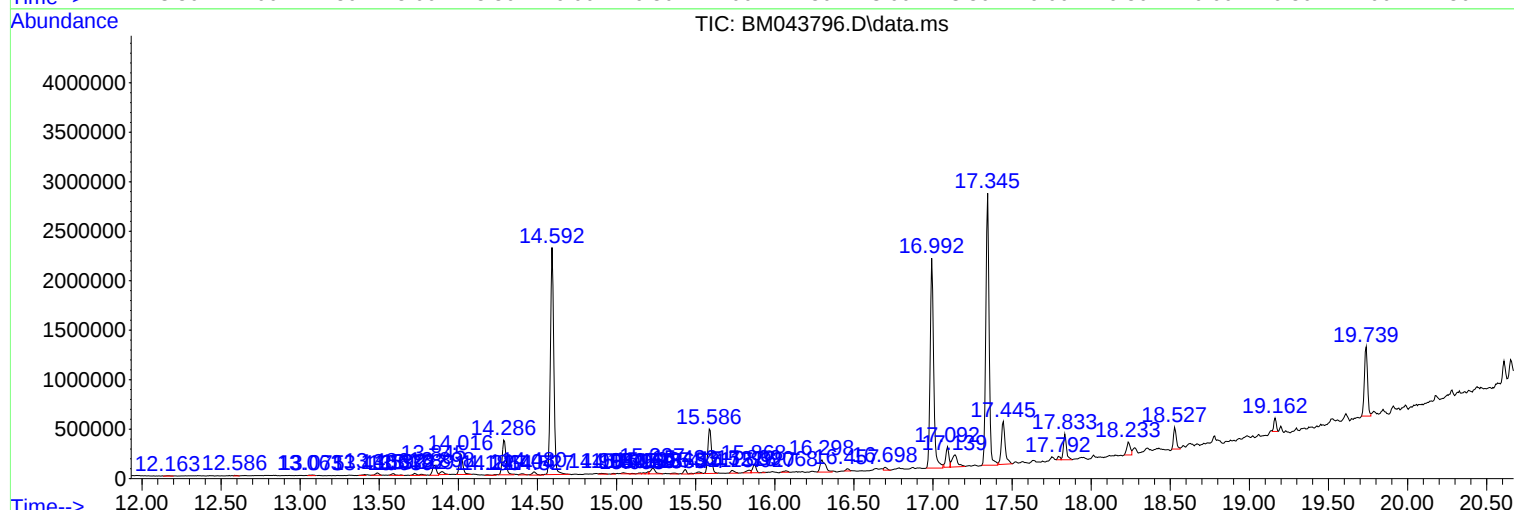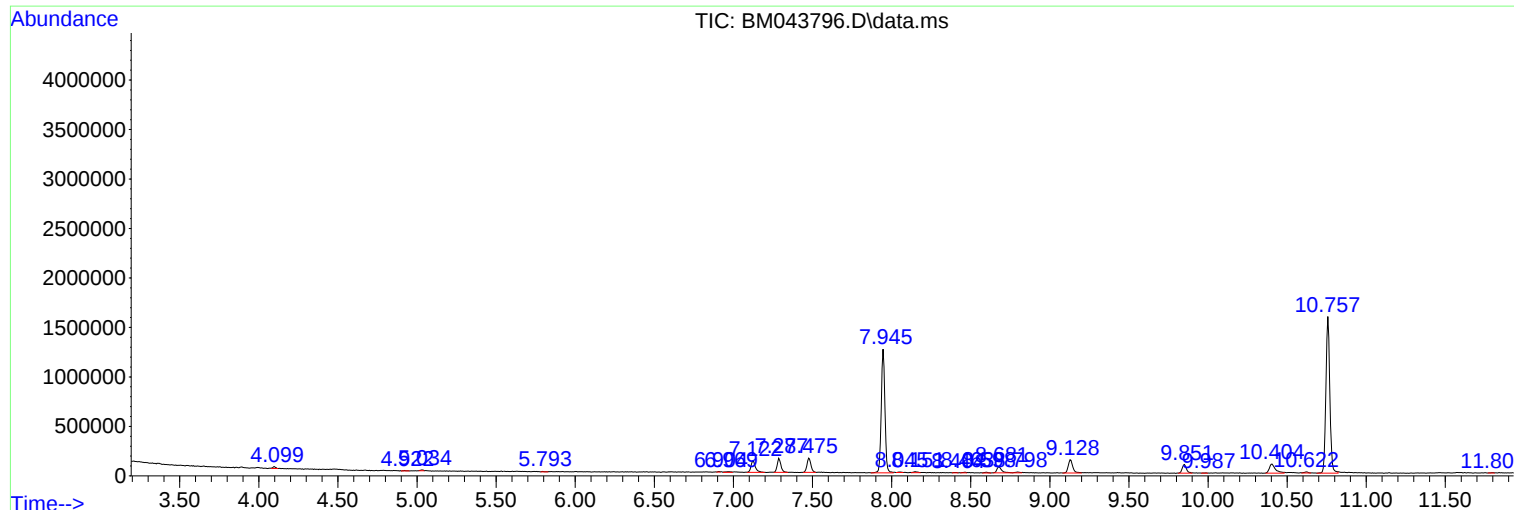

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010824\
Data File : BM043796.D
Acq On : 08 Jan 2024 16:26
Operator : MA/JU
Sample : 05952-13DL 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF96DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010824\
Data File : BM043796.D
Acq On : 08 Jan 2024 16:26
Operator : MA/JU
Sample : 05952-13DL 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCF96DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------