

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010919\
 Data File : BM018495.D
 Acq On : 10 Jan 2019 05:45
 Operator : JU/SJ
 Sample : K1006-20
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JC-03-010819-J

Quant Time: Jan 10 08:22:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 10 05:57:41 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	561418	20.00	ng	0.00
21) Naphthalene-d8	10.56	136	2365340	20.00	ng	0.00
39) Acenaphthene-d10	14.41	164	1358957	20.00	ng	0.00
64) Phenanthrene-d10	17.16	188	3018223	20.00	ng	0.00
76) Chrysene-d12	21.36	240	2212651	20.00	ng	0.00
87) Perylene-d12	23.64	264	2131236	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.36	112	3083330	101.41	ng	0.00
7) Phenol-d6	6.94	99	3556514	92.10	ng	0.00
23) Nitrobenzene-d5	8.93	82	2909194	71.30	ng	0.00
42) 2,4,6-Tribromophenol	15.91	330	1980490	114.46	ng	0.00
45) 2-Fluorobiphenyl	13.03	172	7502897	72.04	ng	0.00
79) Terphenyl-d14	19.79	244	9513707	90.64	ng	0.00
Target Compounds						
32) Benzoic acid	9.90	122	110	6.507	ng	Qvalue # 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010919\
Data File : BM018495.D
Acq On : 10 Jan 2019 05:45
Operator : JU/SJ
Sample : K1006-20
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JC-03-010819-J

Quant Time: Jan 10 08:22:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 10 05:57:41 2019
Response via : Initial Calibration

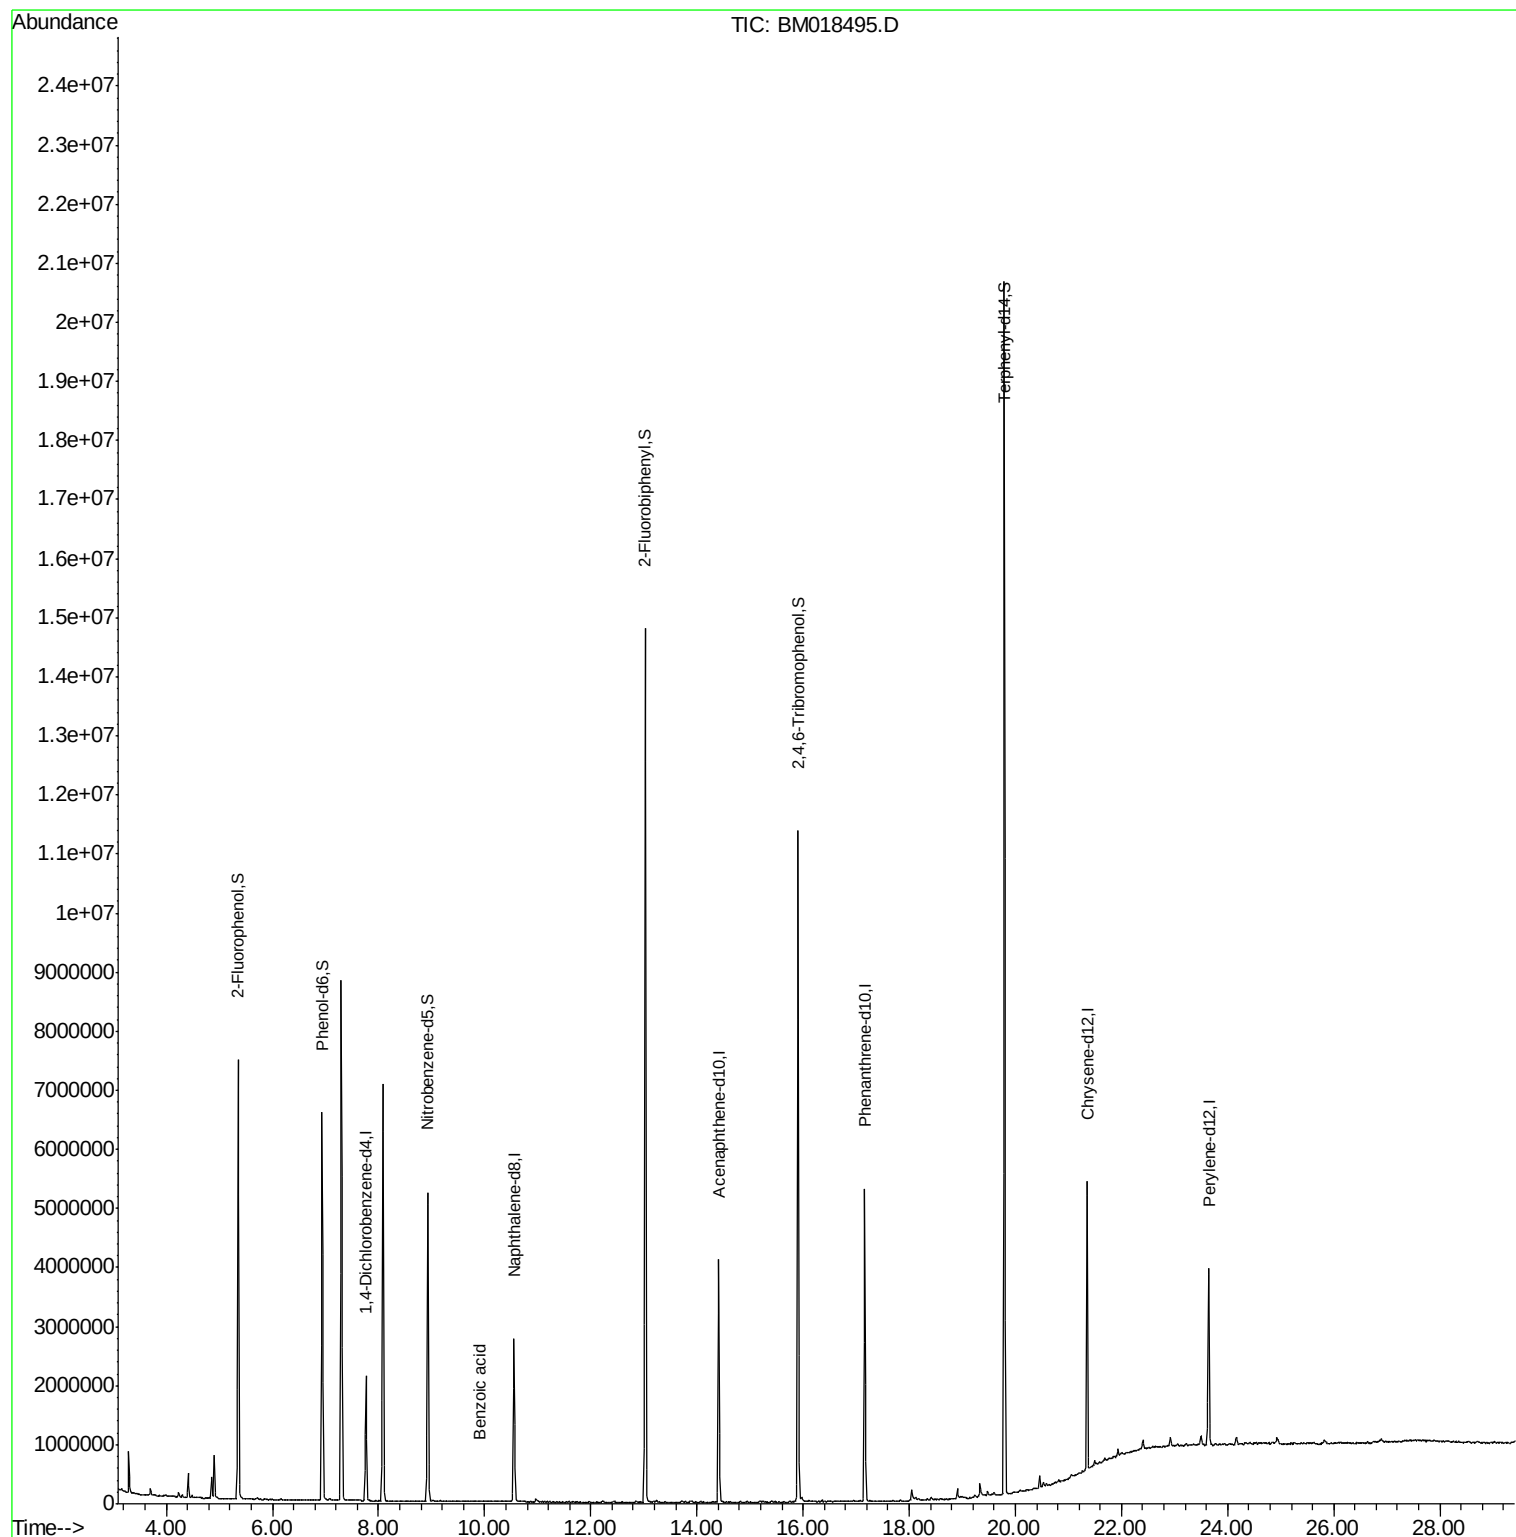




#1


1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.76 min Scan# 795
Delta R.T. 0.00 min
Lab File: BM018495.D
Acq: 10 Jan 2019 05:45

Instrument :
BNA_M
ClientSampleId :
JC-03-010819-J



Tot Ion	Ratio	Lower	Upper
152	100		
150	153.5	126.9	190.3
115	56.7	45.5	68.3

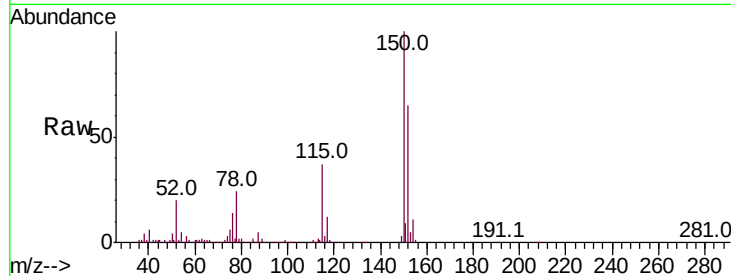

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

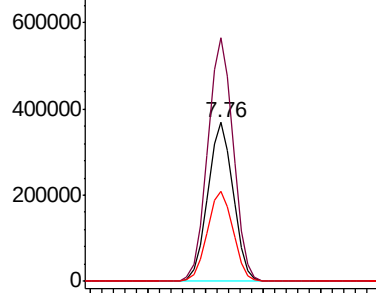


Time-->

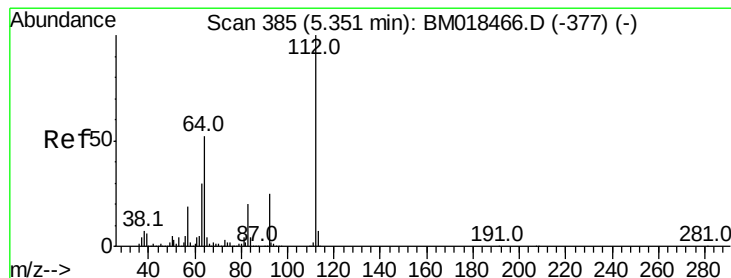


#5

2-Fluorophenol
Concen: 101.410 ng
RT: 5.36 min Scan# 386
Delta R.T. 0.01 min
Lab File: BM018495.D
Acq: 10 Jan 2019 05:45


Tgt Ion	Ratio	Lower	Upper
112	100		
64	53.5	46.5	69.7
63	28.8	25.2	37.8

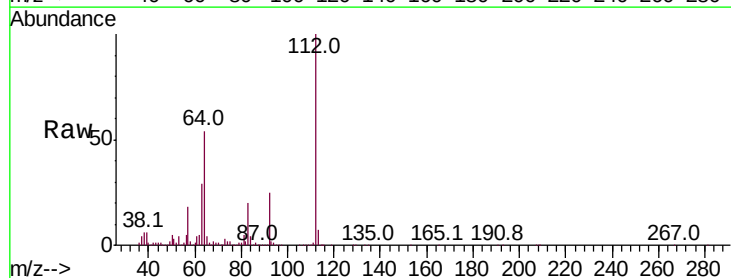


Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

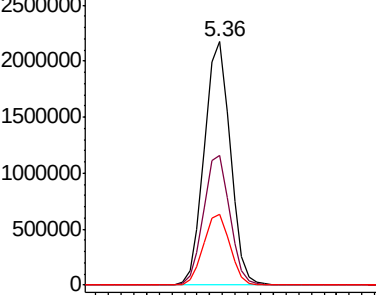

Time-->





#7

Phenol-d6

Concen: 92.096 ng

RT: 6.94 min Scan# 655

Delta R.T. 0.01 min

Lab File: BM018495.D

Acq: 10 Jan 2019 05:45

Instrument :

BNA_M

ClientSampleId :

JC-03-010819-J


Tot Ion: 99 Resp: 3556514

Ion Ratio Lower Upper

99 100

42 20.0 17.3 25.9




71 36.7 28.0 42.0

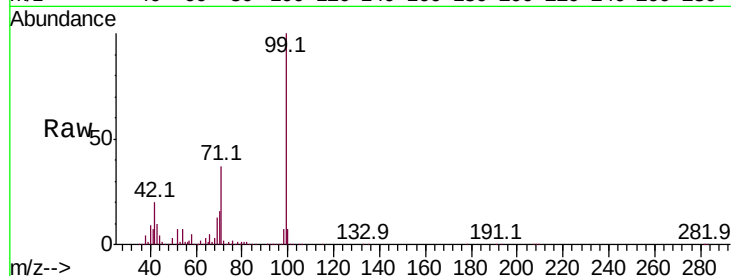

Abundance Ion 99.00 (98.70 to 99.70): BM018466.D (-646) (-)

Ion 42.00 (41.70 to 42.70): BM018466.D (-646) (-)

Ion 71.00 (70.70 to 71.70): BM018466.D (-646) (-)

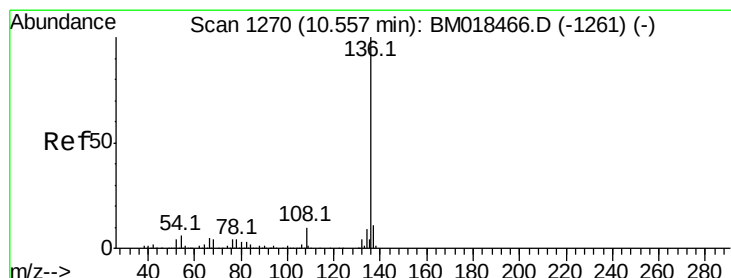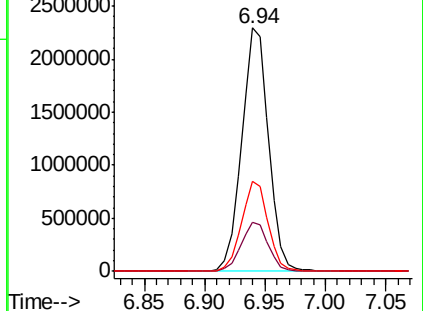

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.56 min Scan# 1270

Delta R.T. 0.01 min

Lab File: BM018495.D

Acq: 10 Jan 2019 05:45

Tgt Ion: 136 Resp: 2365340


Ion Ratio Lower Upper

136 100

137 10.8 8.5 12.7

54 6.2 6.0 9.0

68 4.4 4.5 6.7#


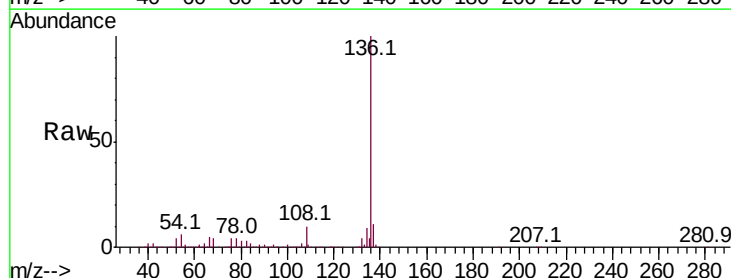



Abundance Ion 136.00 (135.70 to 136.70): BM018466.D (-1261) (-)

Ion 137.00 (136.70 to 137.70): BM018466.D (-1261) (-)

Ion 54.00 (53.70 to 54.70): BM018466.D (-1261) (-)

Ion 68.00 (67.70 to 68.70): BM018466.D (-1261) (-)




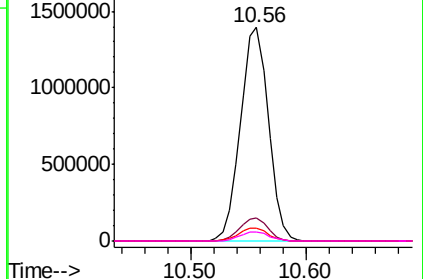


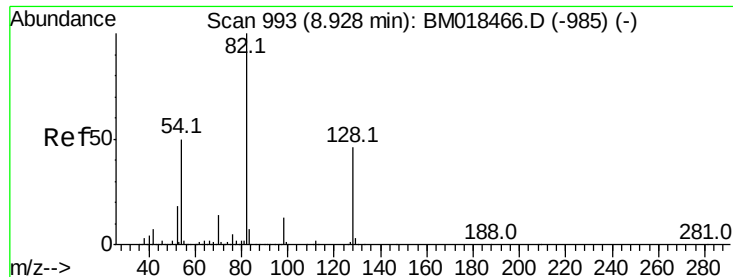

#23
 Nitrobenzene-d5
 Concen: 71.300 ng
 RT: 8.93 min Scan# 993
 Delta R.T. 0.01 min
 Lab File: BM018495.D
 Acq: 10 Jan 2019 05:45




Instrument :
 BNA_M
 ClientSampleId :
 JC-03-010819-J


Tot Ion: 82 Resp: 2909194
 Ion Ratio Lower Upper
 82 100
 128 46.2 36.3 54.5
 54 50.4 41.7 62.5

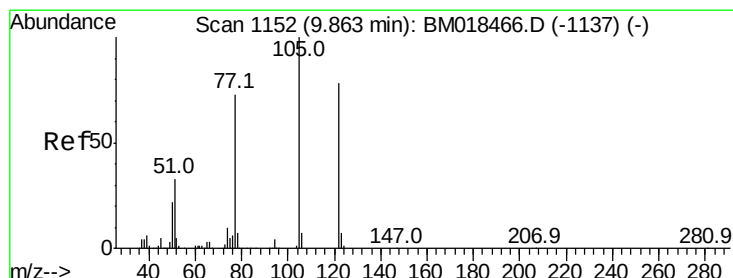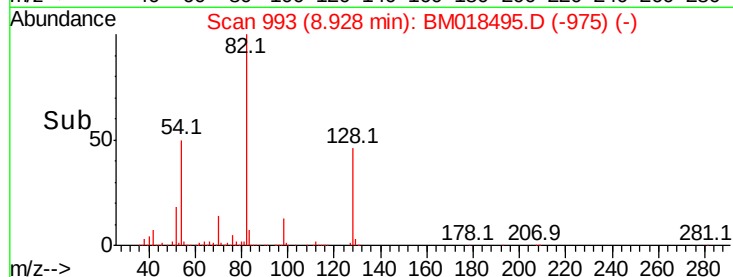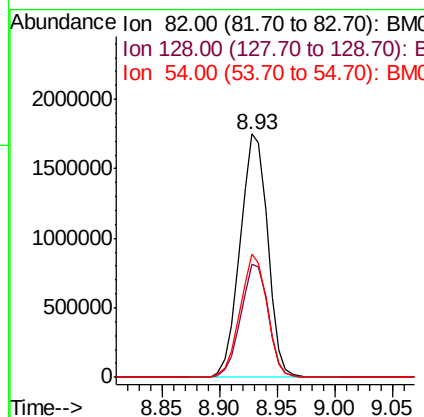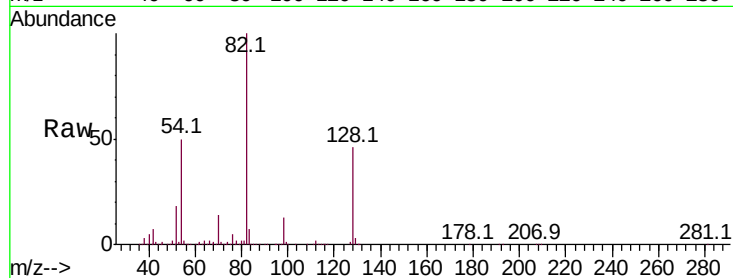

#32
 Benzoic acid
 Concen: 6.507 ng
 RT: 9.90 min Scan# 1159
 Delta R.T. 0.00 min
 Lab File: BM018495.D
 Acq: 10 Jan 2019 05:45

Tgt Ion: 122 Resp: 110
 Ion Ratio Lower Upper
 122 100
 105 231.6 100.4 140.4#
 77 393.9 71.7 111.7#

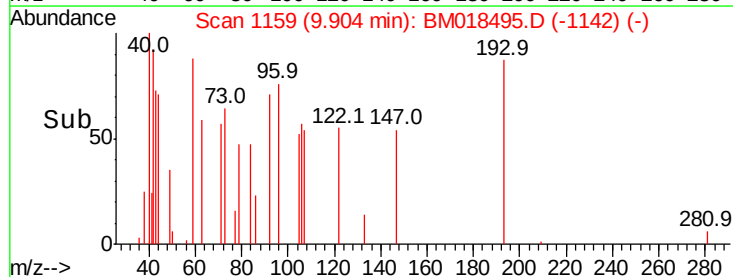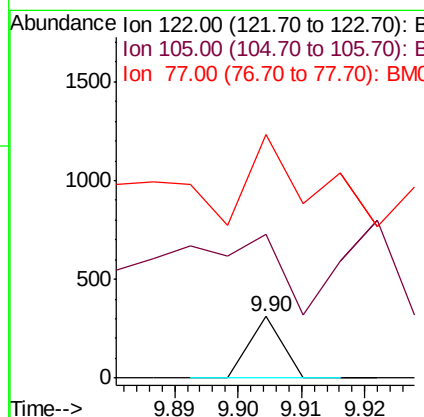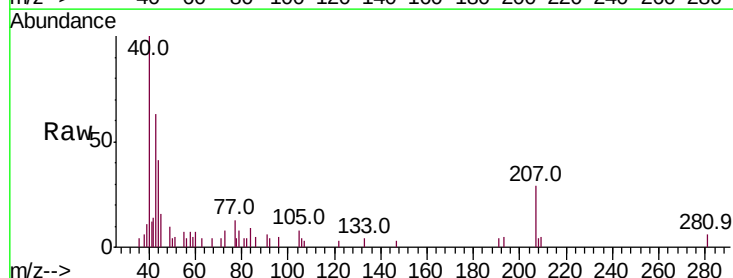




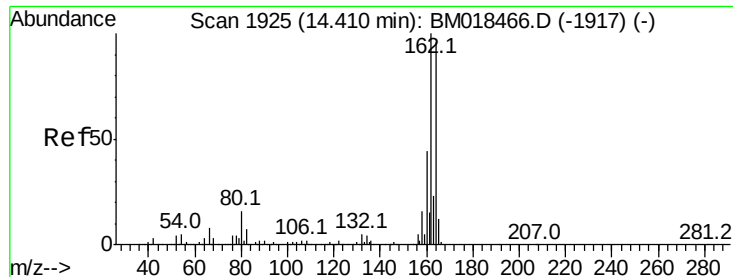


#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.41 min Scan# 1925
 Delta R.T. 0.00 min
 Lab File: BM018495.D
 Acq: 10 Jan 2019 05:45

Instrument :
 BNA_M
 ClientSampleId :
 JC-03-010819-J

Tot Ion:164 Resp: 1358957




Ion	Ratio	Lower	Upper
164	100		
162	104.9	83.0	124.4
160	45.9	37.1	55.7

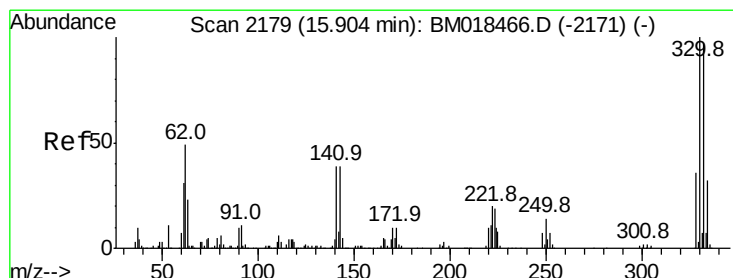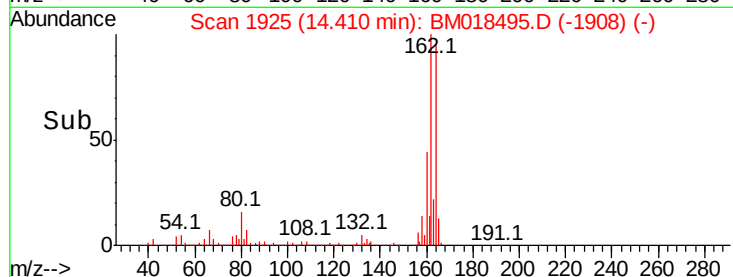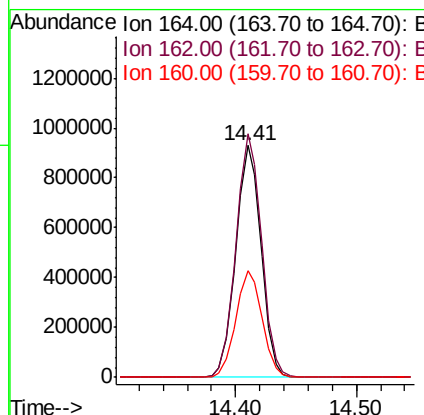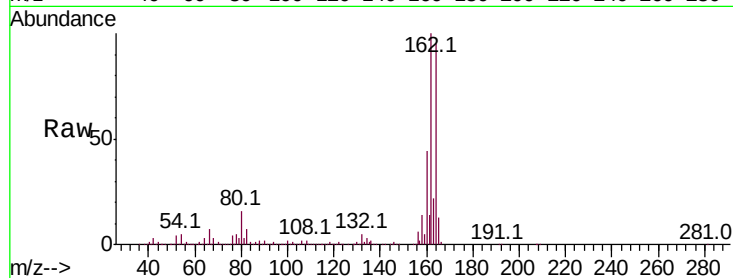


#42
 2,4,6-Tribromophenol
 Concen: 114.457 ng
 RT: 15.91 min Scan# 2180
 Delta R.T. 0.01 min
 Lab File: BM018495.D
 Acq: 10 Jan 2019 05:45

Tgt Ion:330 Resp: 1980490

Ion	Ratio	Lower	Upper
330	100		
332	96.8	77.6	116.4
141	38.5	31.7	47.5


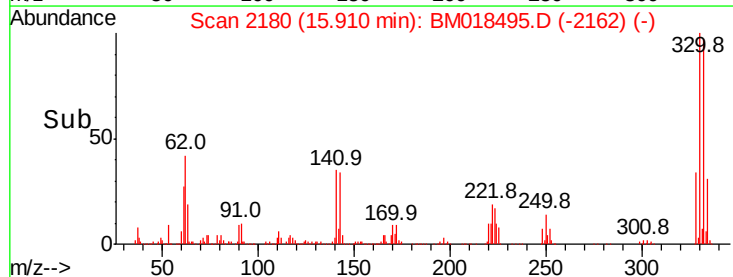
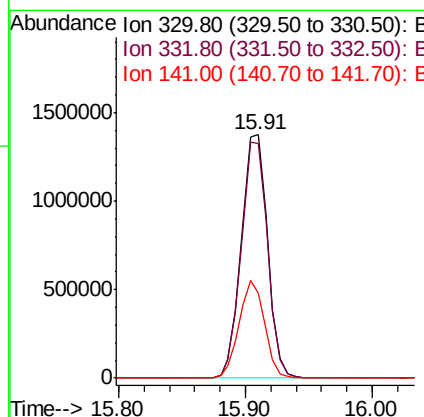
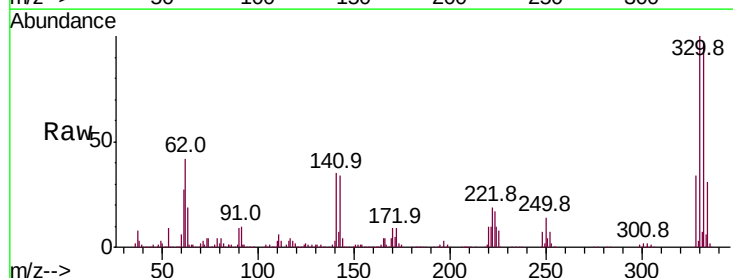




#45
2-Fluorobiphenyl
Concen: 72.042 ng
RT: 13.03 min Scan# 1690
Delta R.T. 0.01 min
Lab File: BM018495.D
Acq: 10 Jan 2019 05:45




Instrument :
BNA_M
ClientSampleId :
JC-03-010819-J


Tot Ion:172 Resp: 7502897
Ion Ratio Lower Upper
172 100
171 35.7 28.2 42.4
170 23.6 18.9 28.3

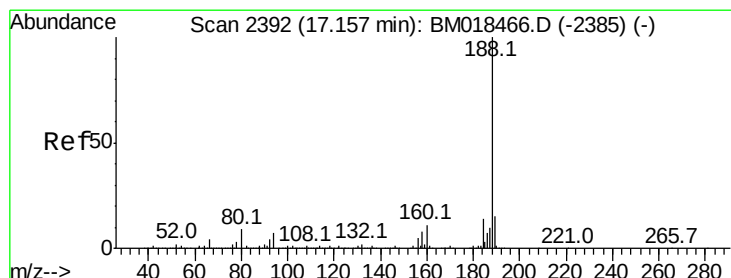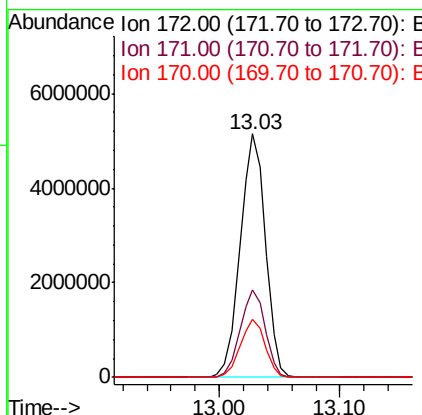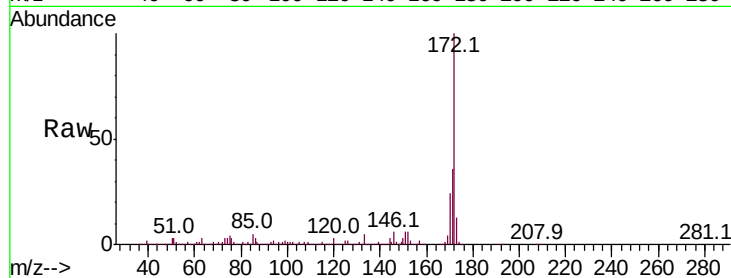

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.16 min Scan# 2393
Delta R.T. 0.01 min
Lab File: BM018495.D
Acq: 10 Jan 2019 05:45

Tgt Ion:188 Resp: 3018223
Ion Ratio Lower Upper
188 100
94 7.4 7.1 10.7
80 8.3 7.6 11.4



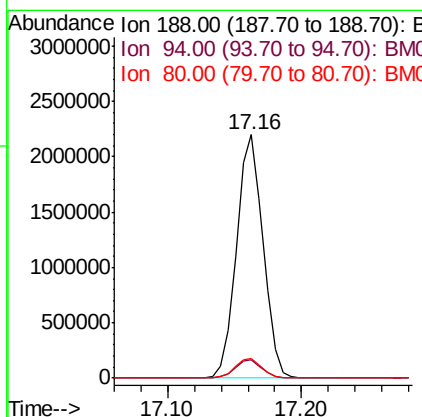
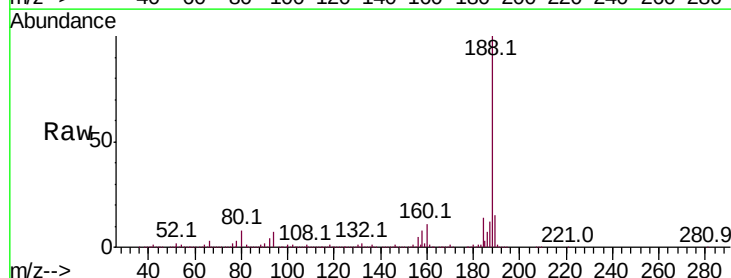


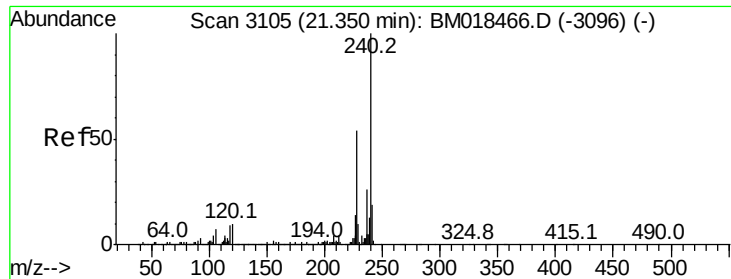

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.36 min Scan# 3106
Delta R.T. 0.01 min
Lab File: BM018495.D
Acq: 10 Jan 2019 05:45




Instrument :
BNA_M
ClientSampleId :
JC-03-010819-J


Tot Ion:240 Resp: 2212651
Ion Ratio Lower Upper
240 100
120 9.1 8.4 12.6
236 25.8 20.7 31.1

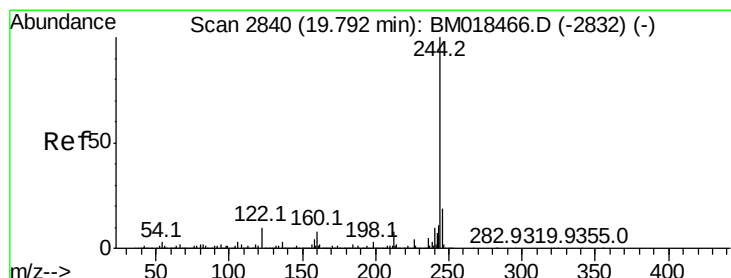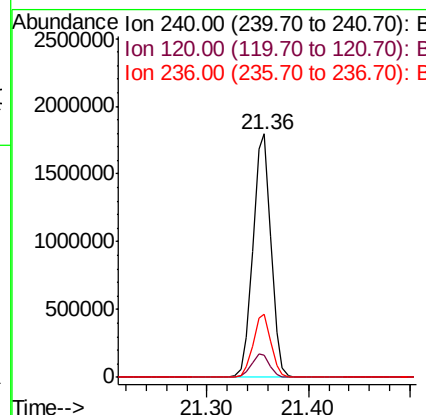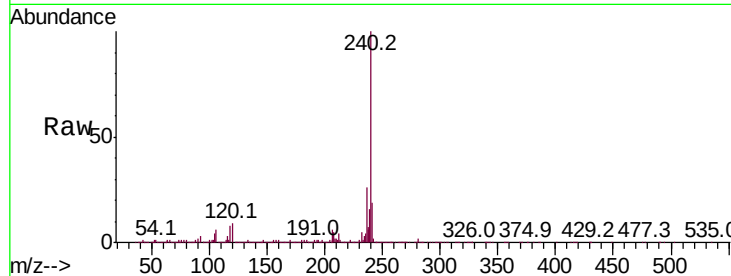

#79
Terphenyl-d14
Concen: 90.639 ng
RT: 19.79 min Scan# 2840
Delta R.T. 0.01 min
Lab File: BM018495.D
Acq: 10 Jan 2019 05:45

Tgt Ion:244 Resp: 9513707
Ion Ratio Lower Upper
244 100
212 7.9 5.9 8.9
122 10.4 9.0 13.4

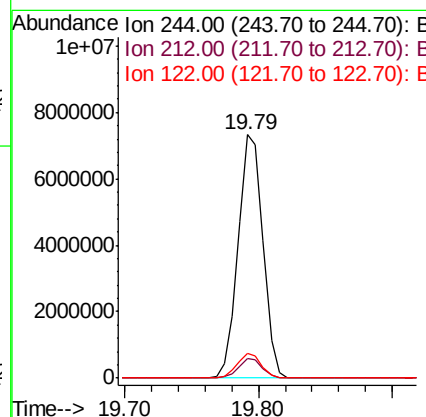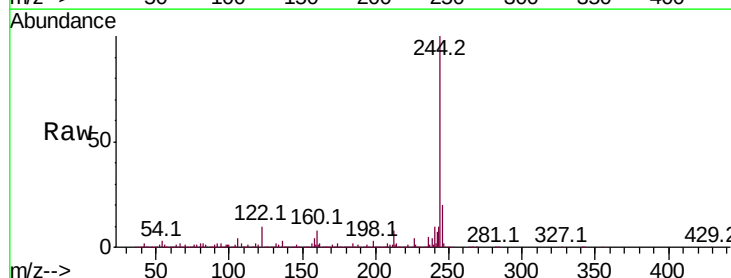



#87
Pervlene-d12
Concen: 20.000 ng
RT: 23.64 min Scan# 3495
Delta R.T. 0.01 min
Lab File: BM018495.D
Acq: 10 Jan 2019 05:45

Instrument :
BNA_M
ClientSampleId :
JC-03-010819-J

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.8	18.9	28.3
265	22.0	16.8	25.2

