




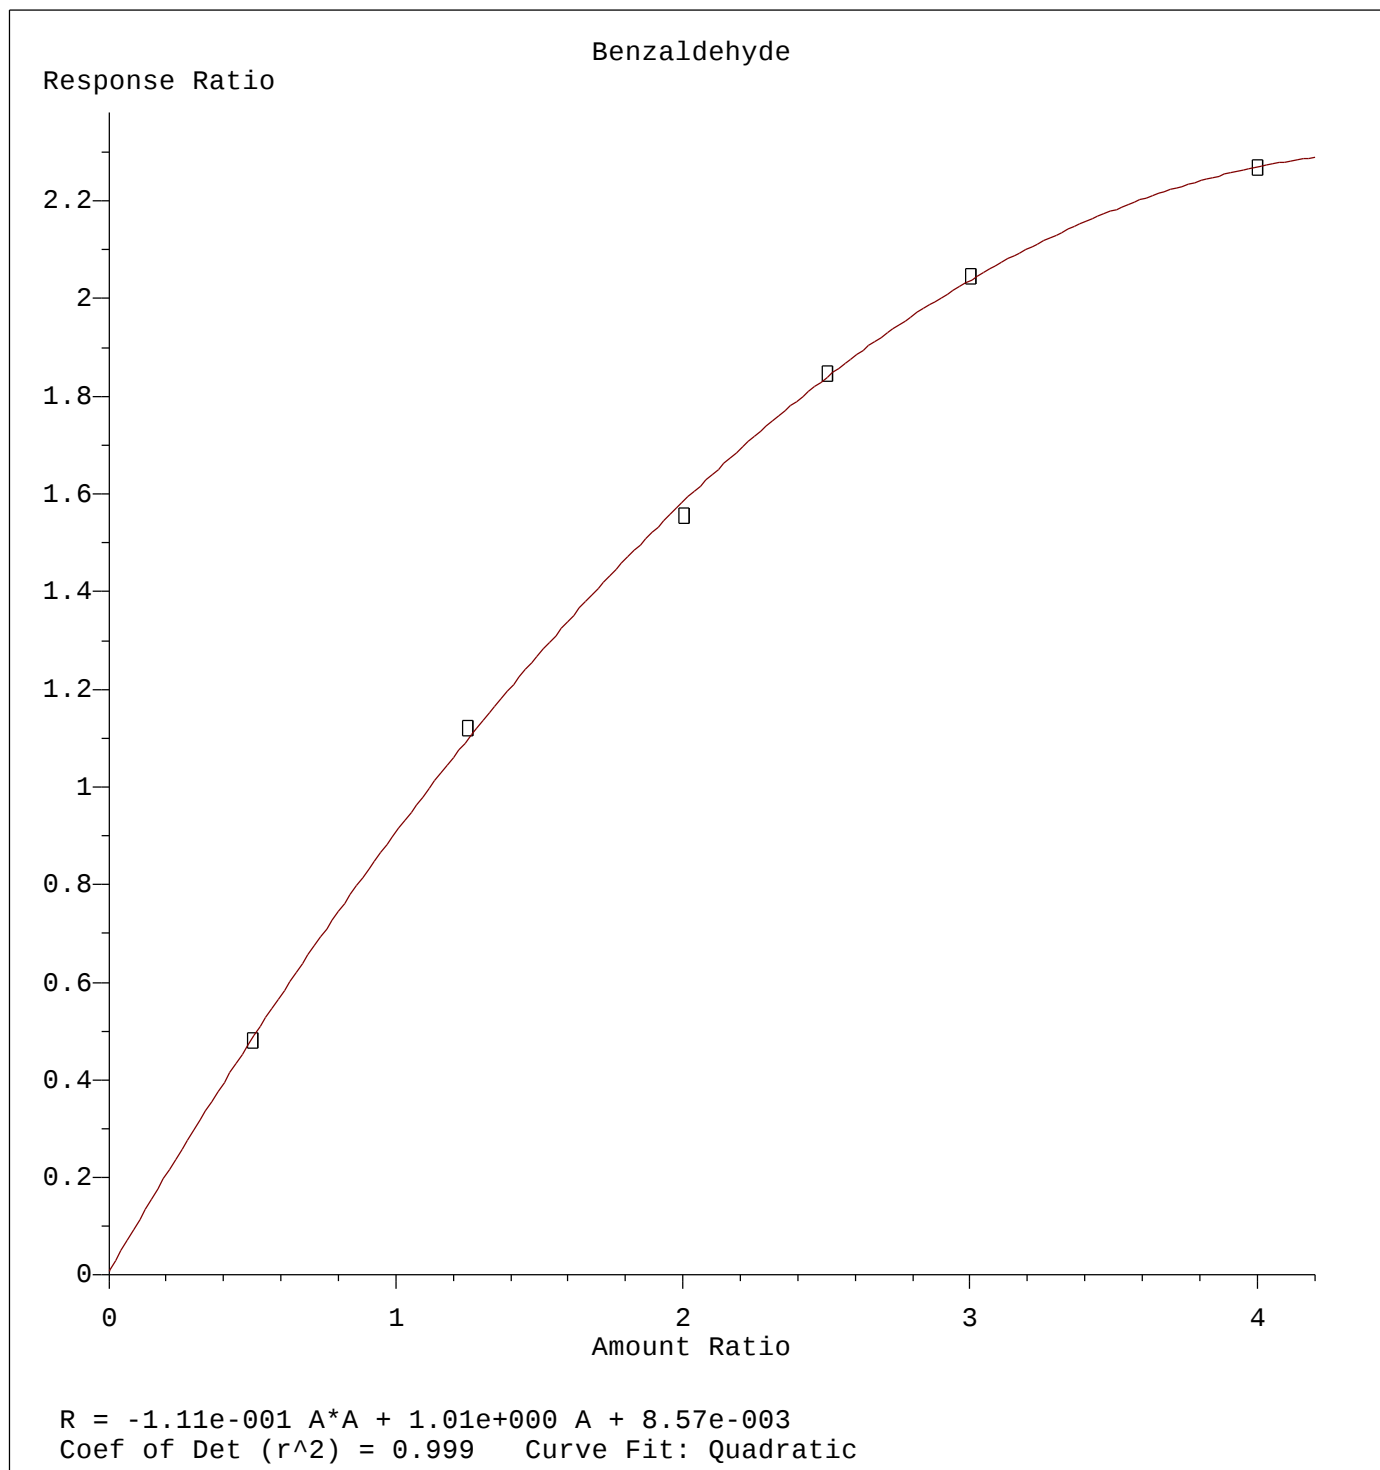

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
Calibration Table Last Updated: Thu Jan 10 05:57:41 2019

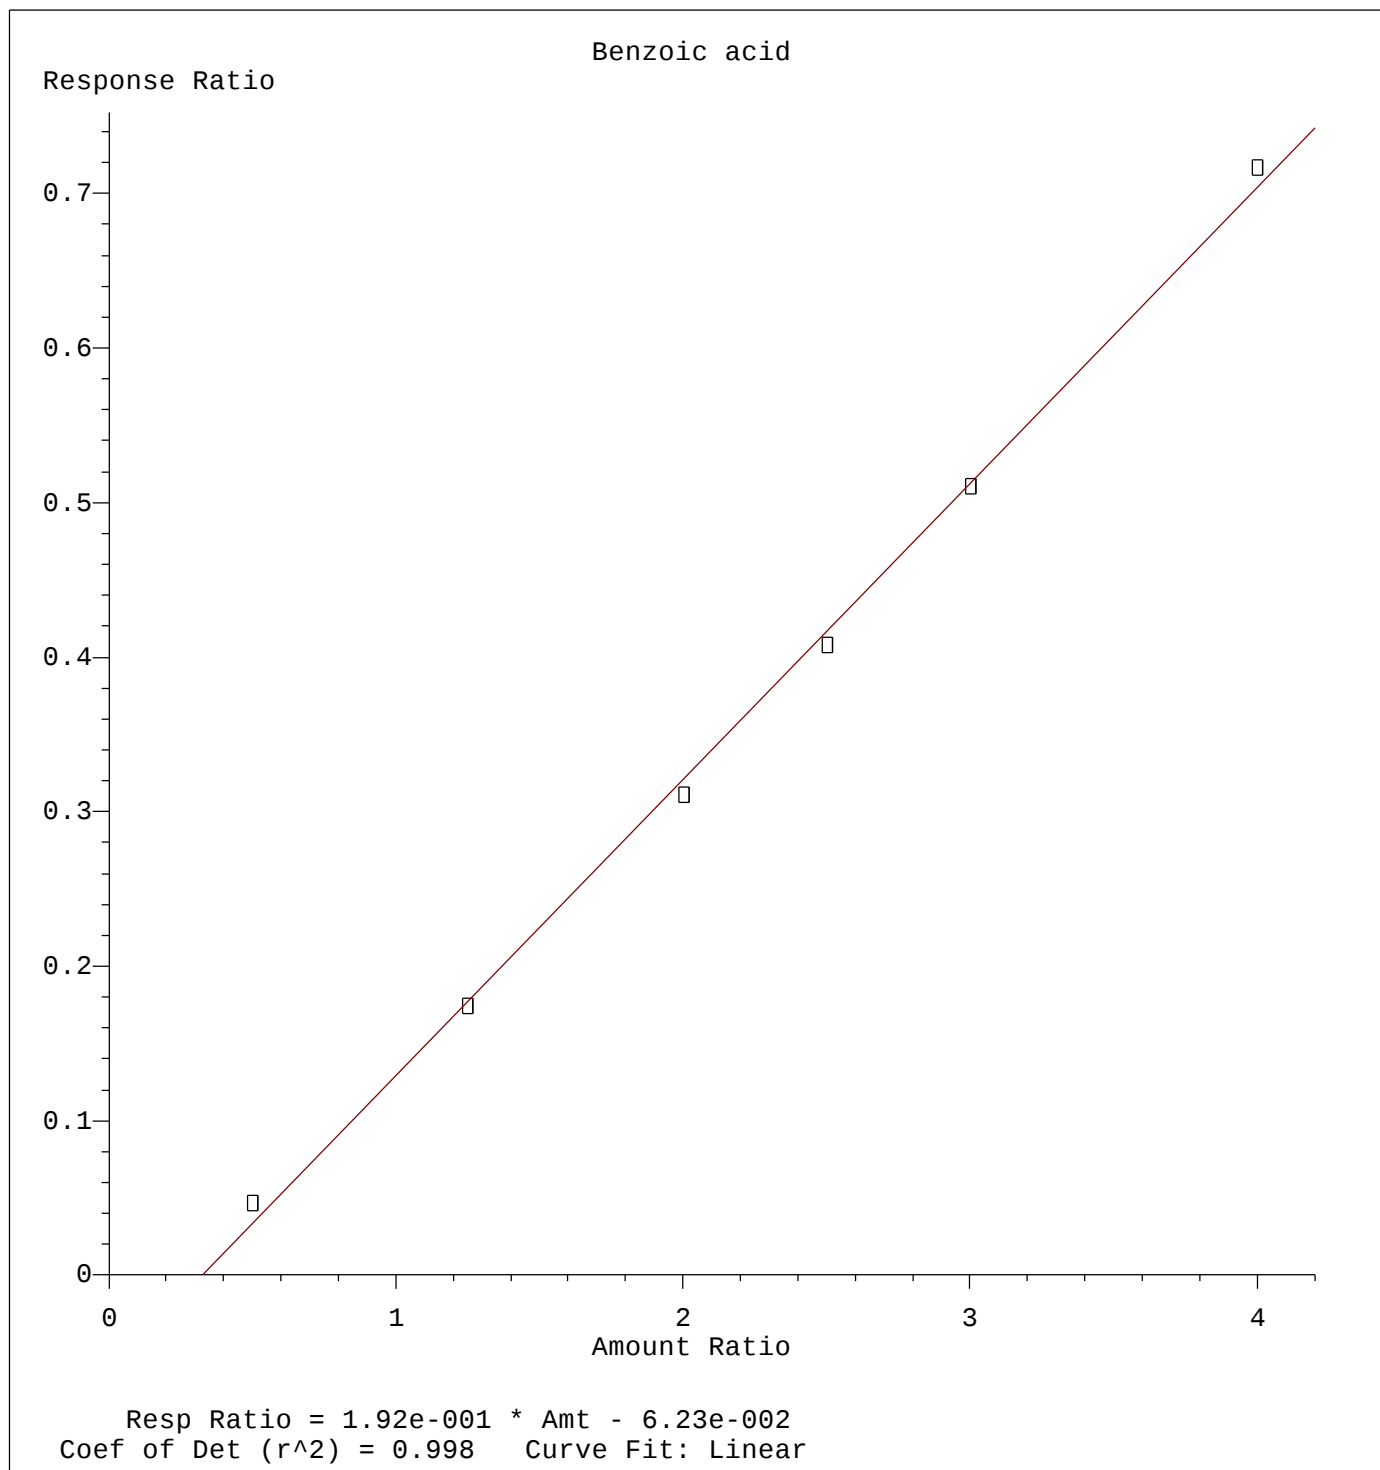


Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
Calibration Table Last Updated: Thu Jan 10 05:57:41 2019

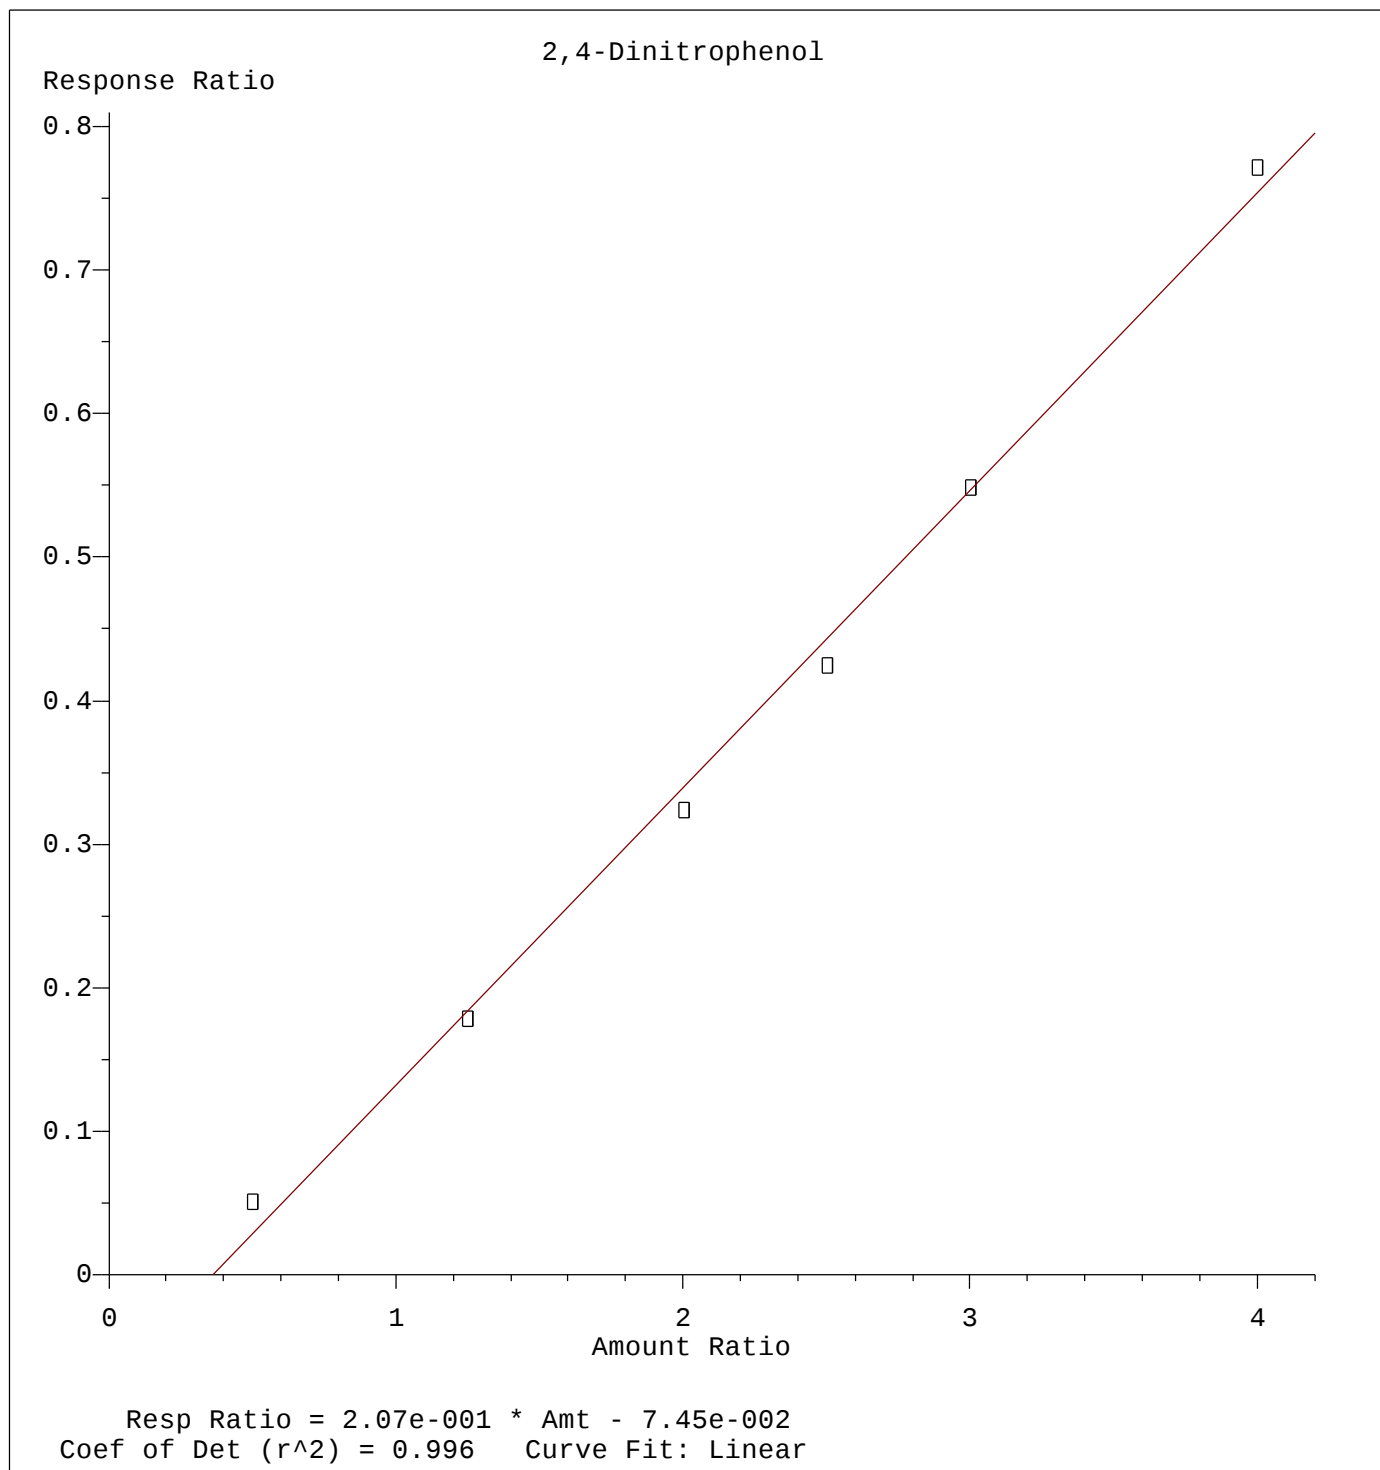

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
Calibration Table Last Updated: Thu Jan 10 05:57:41 2019

4,6-Dinitro-2-methylphenol

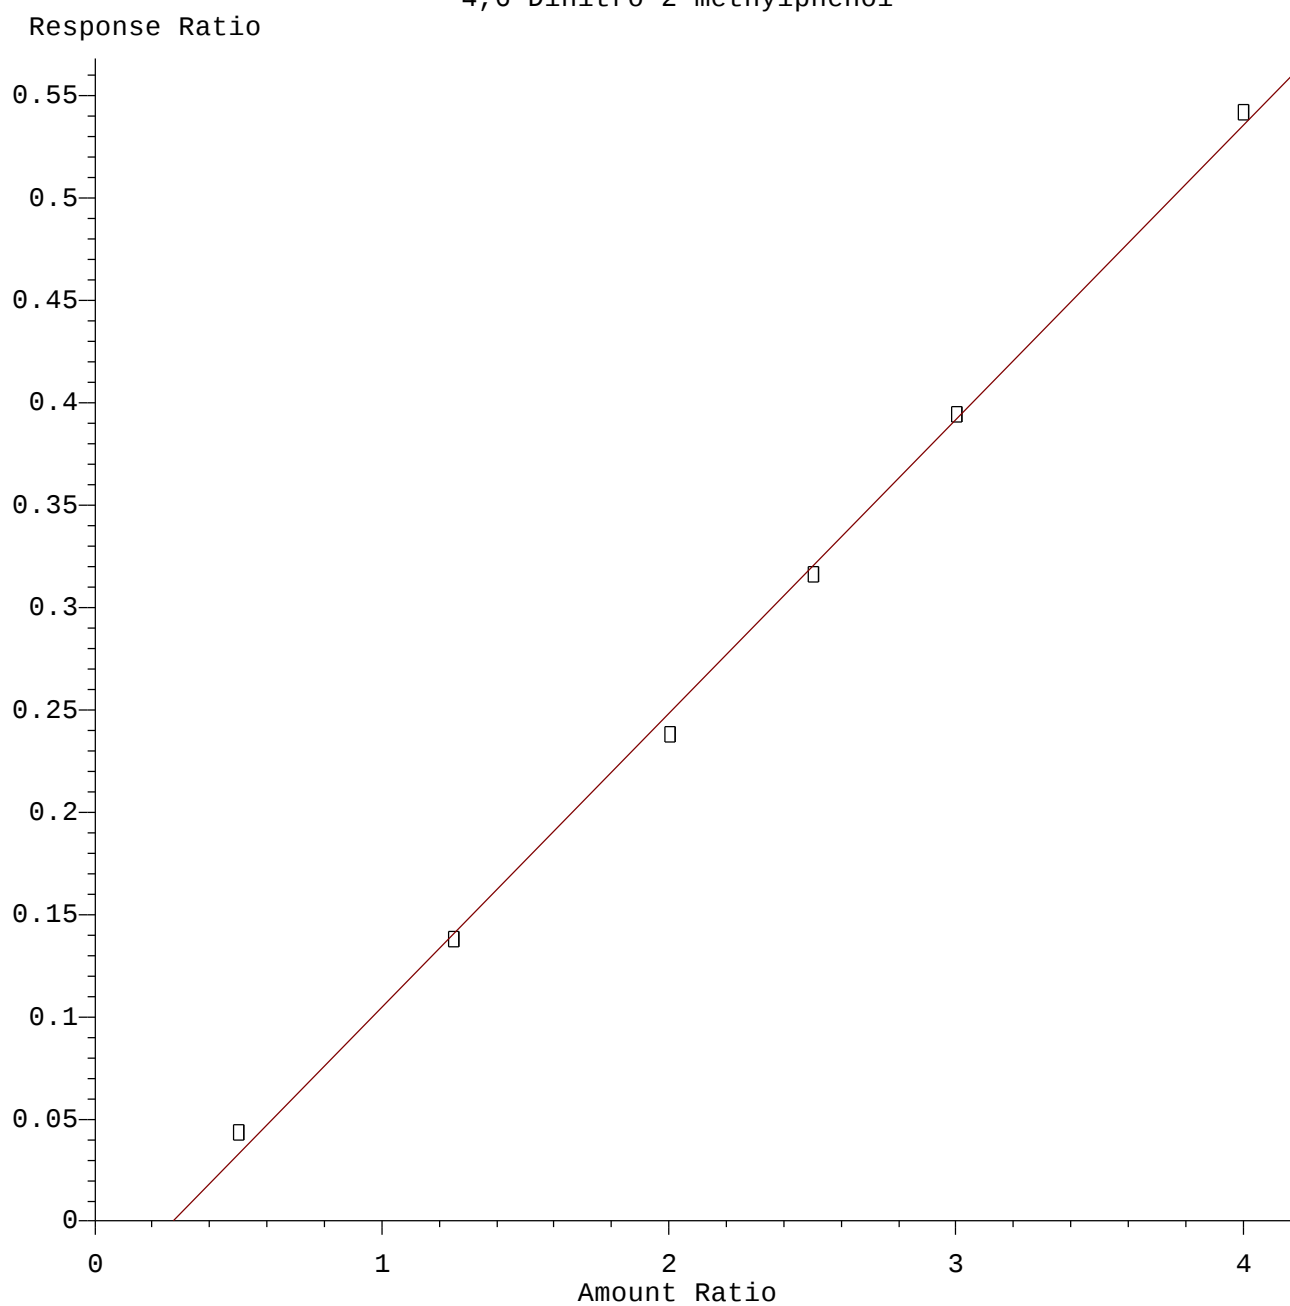

Resp Ratio = $1.44 \times 10^{-1} \times \text{Amt} - 3.87 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
Calibration Table Last Updated: Thu Jan 10 05:57:41 2019