


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010919\
 Data File : BM018491.D
 Acq On : 10 Jan 2019 03:20
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 10 05:57:41 2019

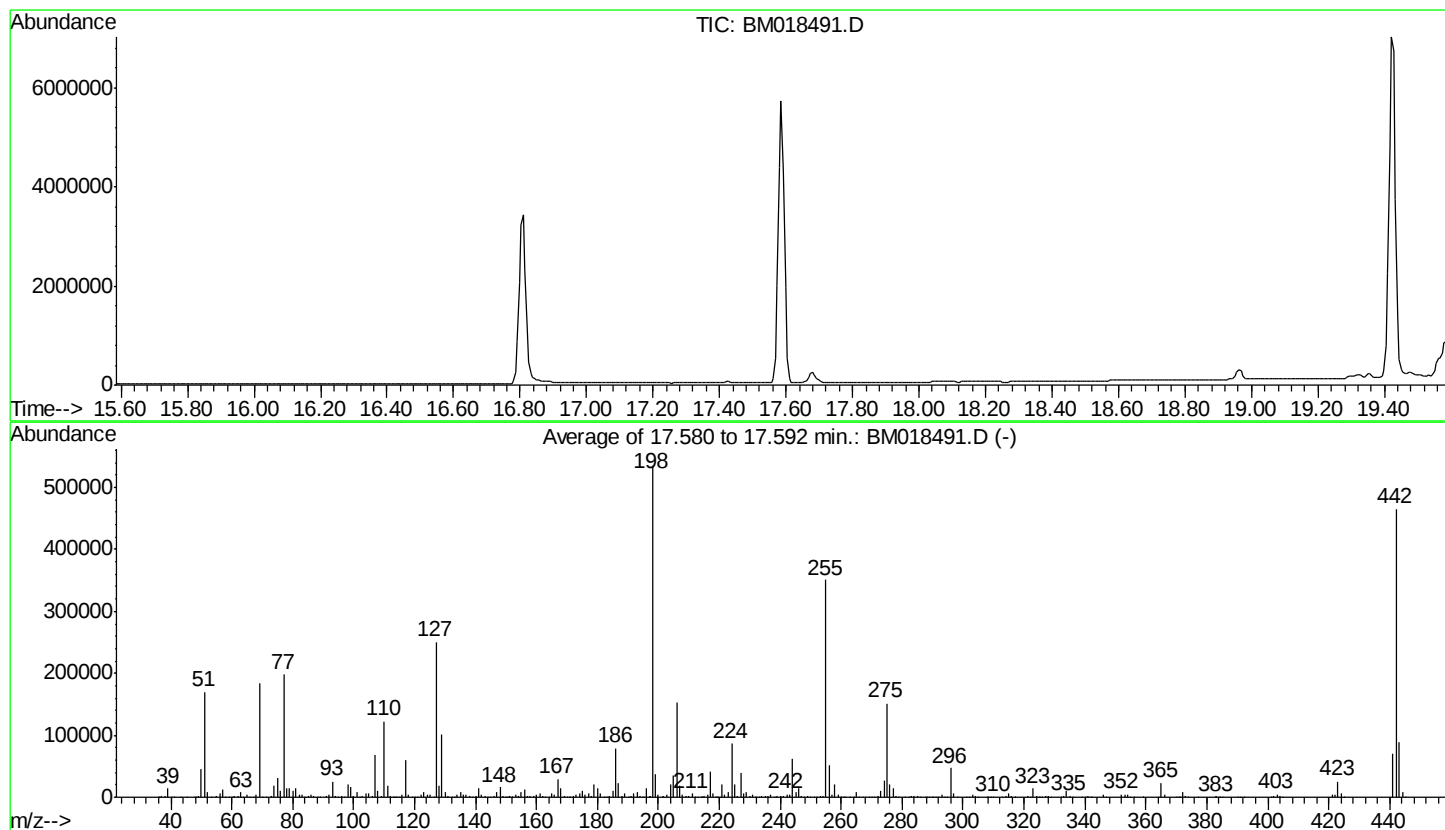

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.7	169765	PASS
68	69	0.00	2	1.8	3251	PASS
69	198	0.00	100	34.2	183147	PASS
70	69	0.00	2	0.4	669	PASS
127	198	10	80	46.8	250261	PASS
197	198	0.00	2	0.4	1954	PASS
198	198	100	100	100.0	535232	PASS
199	198	5	9	6.9	36912	PASS
275	198	10	60	28.3	151634	PASS
365	198	1	100	4.3	23016	PASS
441	198	0.01	100	13.0	69805	PASS
442	198	50	100	86.9	464896	PASS
443	442	15	24	19.3	89850	PASS