

Data File : BM018514.D
Acq On : 10 Jan 2019 18:28
Operator : JU/SJ
Sample : K1082-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP-1-1

Quant Time: Jan 11 03:26:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 10 05:57:41 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	415269	20.00	ng	0.00
21) Naphthalene-d8	10.55	136	1676330	20.00	ng	0.00
39) Acenaphthene-d10	14.41	164	1024800	20.00	ng	0.00
64) Phenanthrene-d10	17.16	188	2606188	20.00	ng	0.00
76) Chrysene-d12	21.36	240	2975293	20.00	ng	0.00
87) Perylene-d12	23.64	264	3080104	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.35	112	3067624	136.40	ng	0.00
7) Phenol-d6	6.94	99	3573777	125.11	ng	0.00
23) Nitrobenzene-d5	8.93	82	2796515	96.71	ng	0.00
42) 2,4,6-Tribromophenol	15.90	330	2234386	171.24	ng	0.00
45) 2-Fluorobiphenyl	13.03	172	7445049	94.80	ng	0.00
79) Terphenyl-d14	19.79	244	12325619	87.33	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM018514.D
Acq On : 10 Jan 2019 18:28
Operator : JU/SJ
Sample : K1082-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP-1-1

Quant Time: Jan 11 03:26:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 10 05:57:41 2019
Response via : Initial Calibration

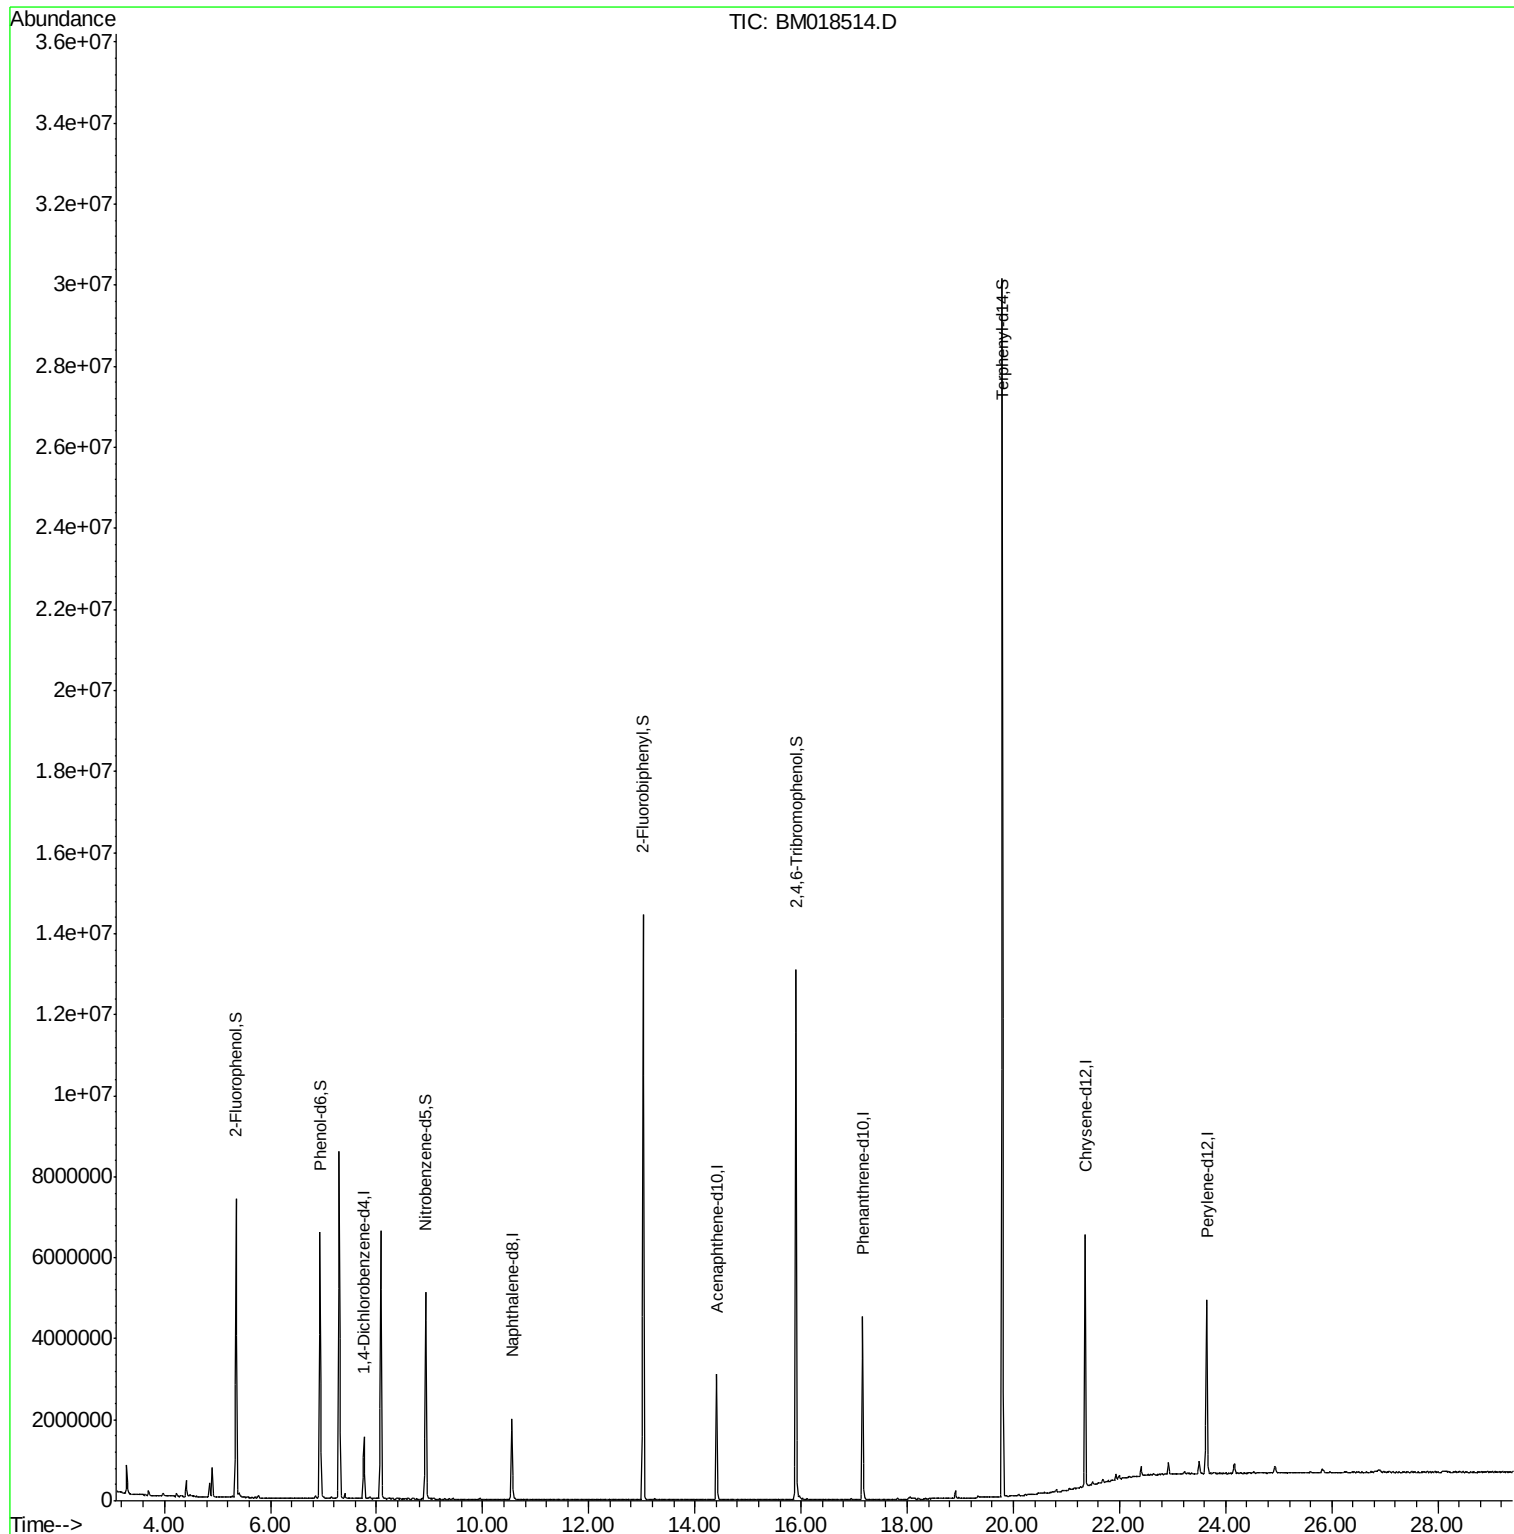

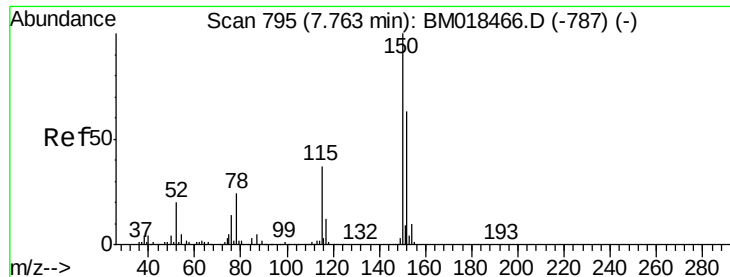


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.76 min Scan# 795
Delta R.T. 0.00 min
Lab File: BM018514.D
Acq: 10 Jan 2019 18:28

Instrument :
BNA_M
ClientSampleId :
SP-1-1

Tgt Ion:152 Resp: 415269
Ion Ratio Lower Upper
152 100
150 154.1 126.9 190.3
115 57.8 45.5 68.3

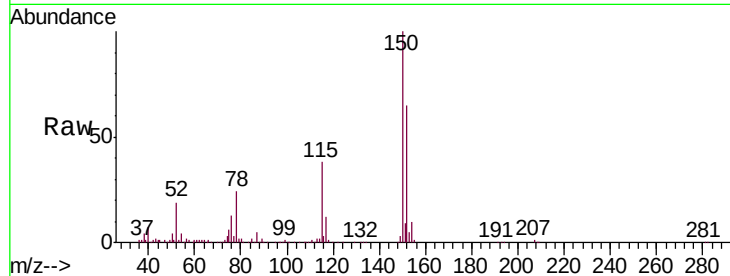


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

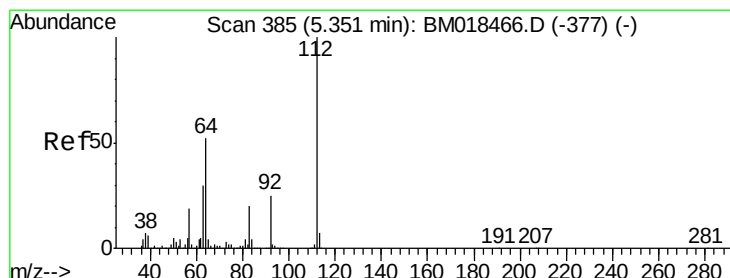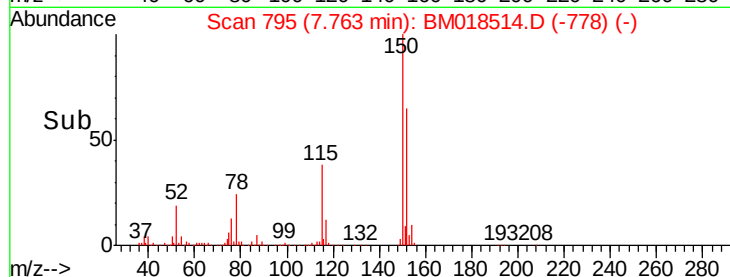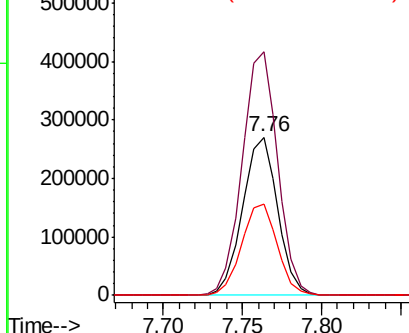



#5


2-Fluorophenol
Concen: 136.402 ng
RT: 5.35 min Scan# 385
Delta R.T. 0.00 min
Lab File: BM018514.D
Acq: 10 Jan 2019 18:28

Tgt Ion:112 Resp: 3067624
Ion Ratio Lower Upper
112 100
64 54.6 46.5 69.7
63 30.4 25.2 37.8

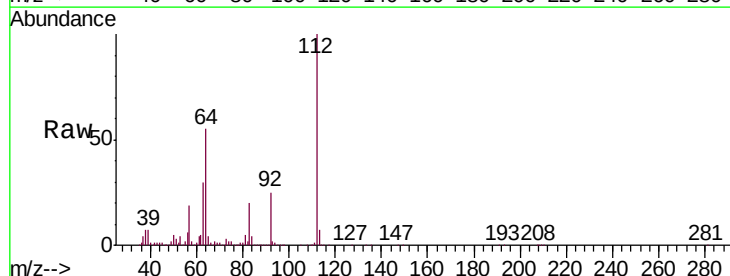

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

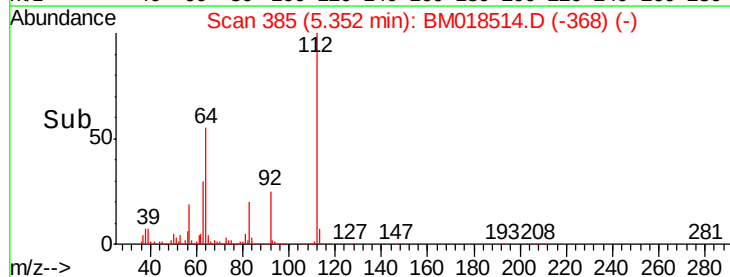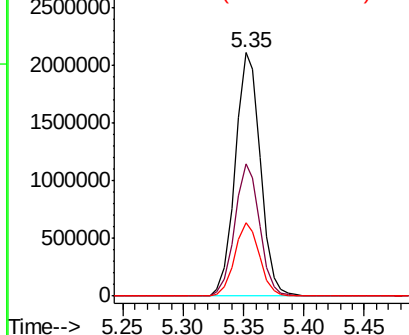

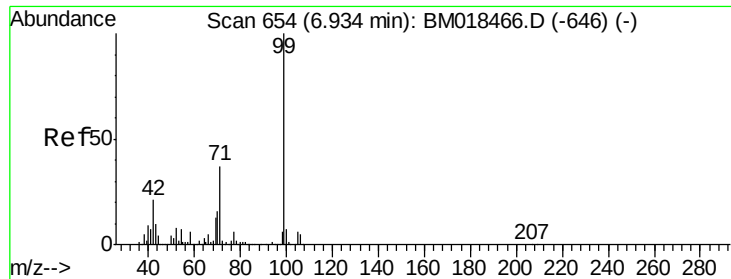

#7

Phenol-d6

Concen: 125.113 ng

RT: 6.94 min Scan# 655

Delta R.T. 0.01 min

Lab File: BM018514.D

Acq: 10 Jan 2019 18:28

Instrument :


BNA_M

ClientSampleId :

SP-1-1

Tgt Ion: 99 Resp: 3573777

Ion	Ratio	Lower	Upper
99	100		
42	20.1	17.3	25.9
71	36.6	28.0	42.0



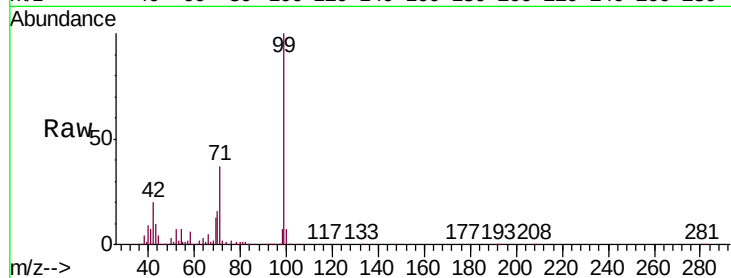


Abundance

Ion 99.00 (98.70 to 99.70): BM018514.D (-637) (-)

Ion 42.00 (41.70 to 42.70): BM018514.D (-637) (-)

Ion 71.00 (70.70 to 71.70): BM018514.D (-637) (-)

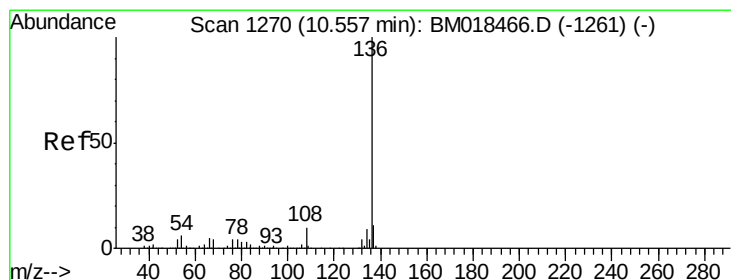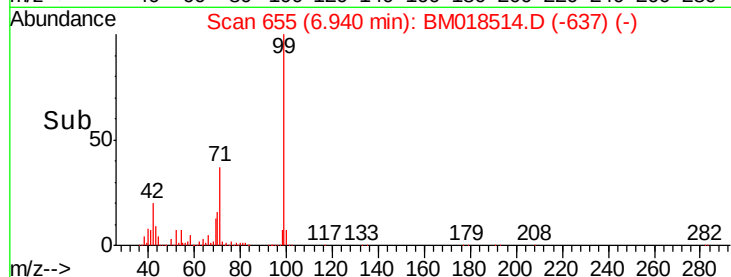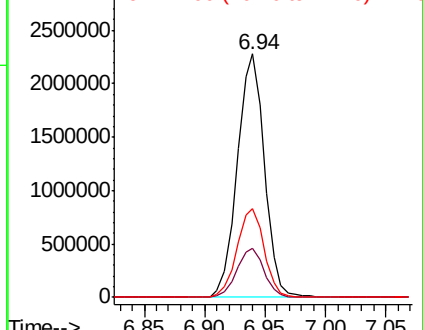

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.55 min Scan# 1269


Delta R.T. 0.00 min

Lab File: BM018514.D

Acq: 10 Jan 2019 18:28

Tgt Ion: 136 Resp: 1676330

Ion	Ratio	Lower	Upper
136	100		
137	10.6	8.5	12.7
54	6.3	6.0	9.0
68	4.6	4.5	6.7

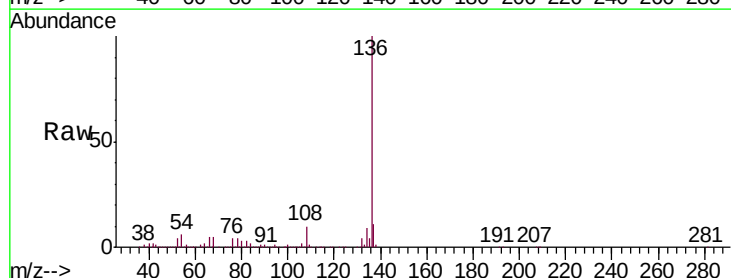



Abundance


Ion 136.00 (135.70 to 136.70): BM018514.D (-1252) (-)

Ion 137.00 (136.70 to 137.70): BM018514.D (-1252) (-)

Ion 54.00 (53.70 to 54.70): BM018514.D (-1252) (-)

Ion 68.00 (67.70 to 68.70): BM018514.D (-1252) (-)



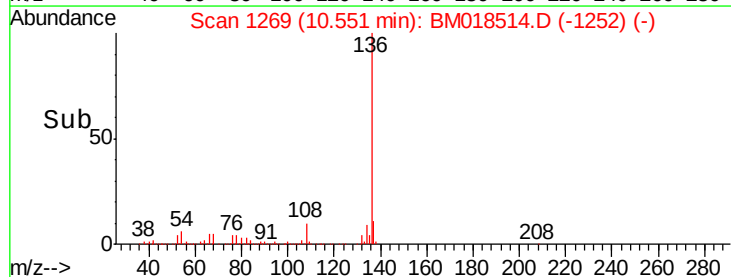
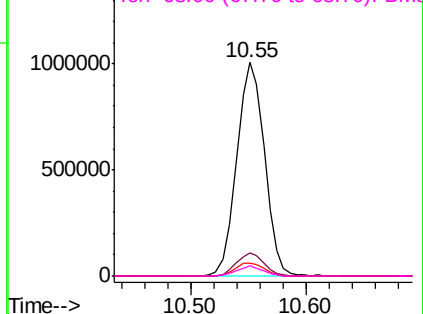


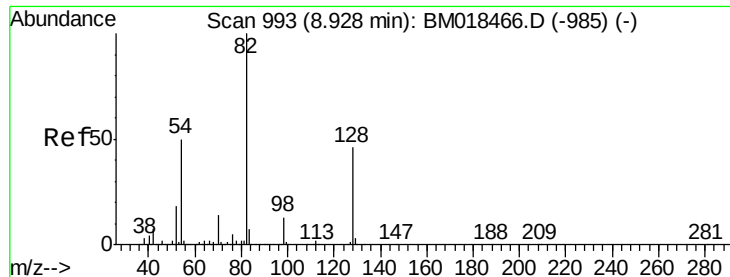

#23
 Nitrobenzene-d5
 Concen: 96.709 ng
 RT: 8.93 min Scan# 993
 Delta R.T. 0.01 min
 Lab File: BM018514.D
 Acq: 10 Jan 2019 18:28




Instrument :
 BNA_M
 ClientSampled :
 SP-1-1


Tgt Ion: 82 Resp: 2796515
 Ion Ratio Lower Upper
 82 100
 128 47.0 36.3 54.5
 54 49.7 41.7 62.5

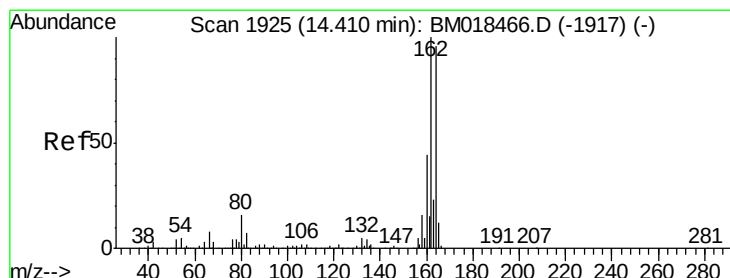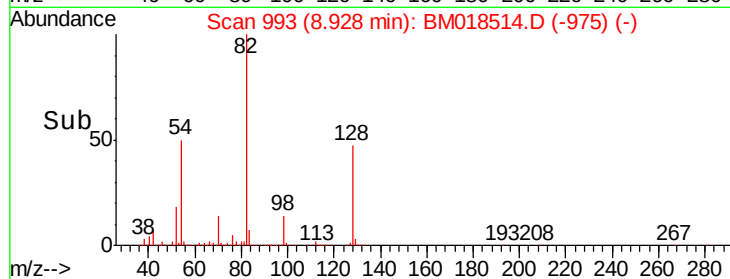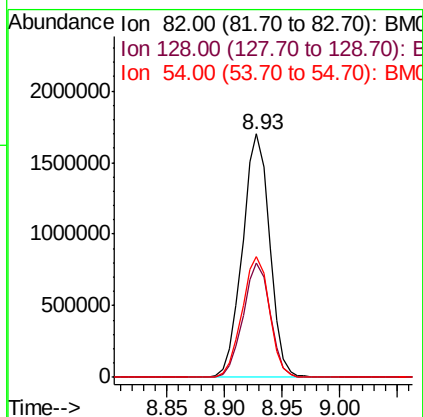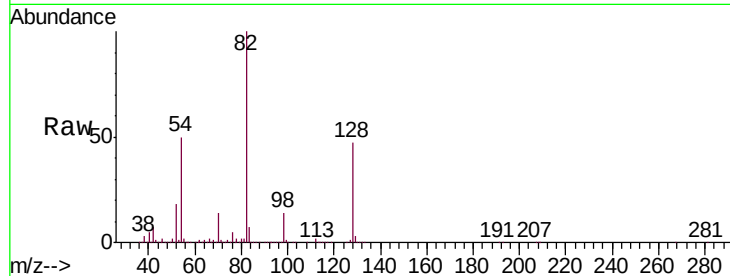

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.41 min Scan# 1925
 Delta R.T. 0.00 min
 Lab File: BM018514.D
 Acq: 10 Jan 2019 18:28

Tgt Ion: 164 Resp: 1024800
 Ion Ratio Lower Upper
 164 100
 162 104.6 83.0 124.4
 160 46.0 37.1 55.7

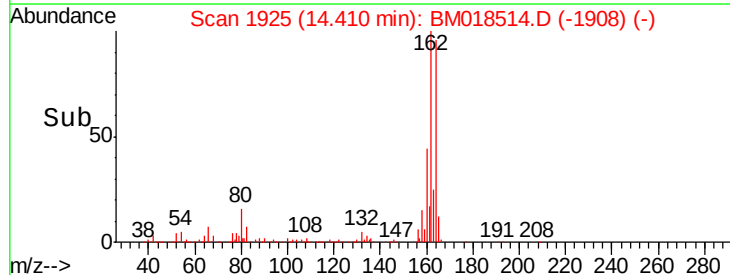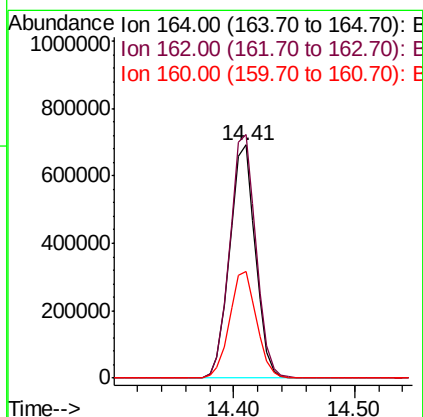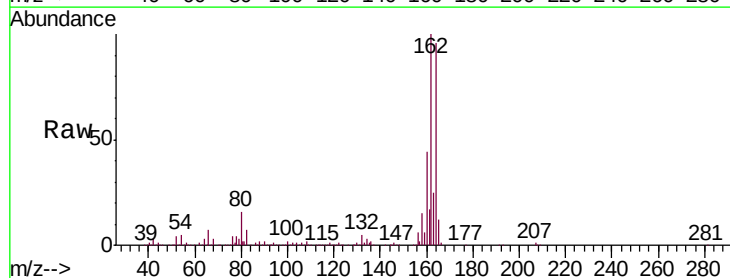


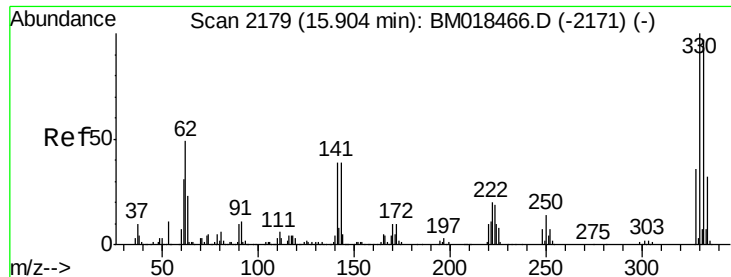




#42
 2,4,6-Tribromophenol
 Concen: 171.236 ng
 RT: 15.90 min Scan# 2179
 Delta R.T. 0.00 min
 Lab File: BM018514.D
 Acq: 10 Jan 2019 18:28

Instrument :
 BNA_M
 ClientSampleId :
 SP-1-1

Tgt Ion:330 Resp: 2234386
 Ion Ratio Lower Upper
 330 100
 332 97.2 77.6 116.4
 141 39.2 31.7 47.5

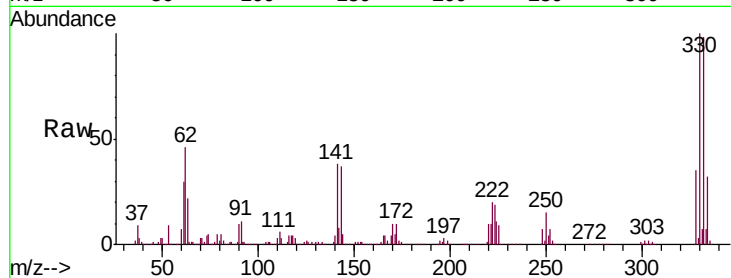


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

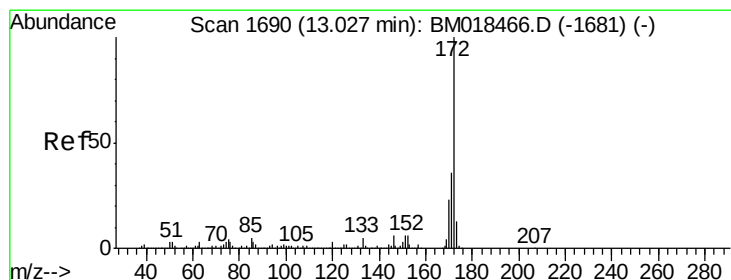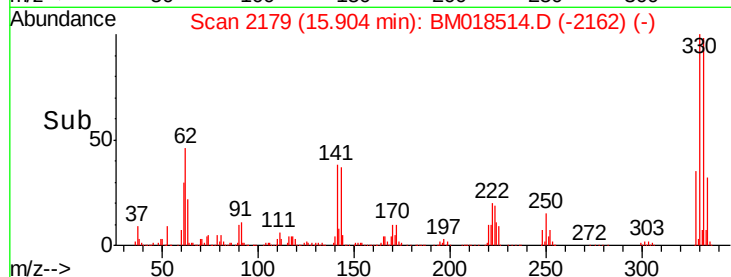
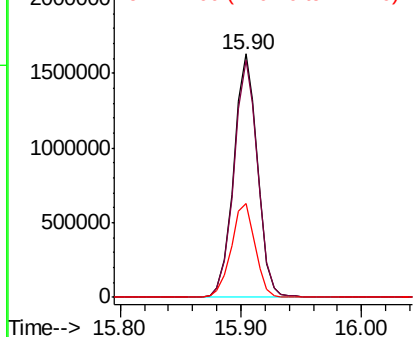



#45
 2-Fluorobiphenyl
 Concen: 94.797 ng
 RT: 13.03 min Scan# 1690
 Delta R.T. 0.01 min
 Lab File: BM018514.D
 Acq: 10 Jan 2019 18:28

Tgt Ion:172 Resp: 7445049
 Ion Ratio Lower Upper
 172 100
 171 35.6 28.2 42.4
 170 23.7 18.9 28.3

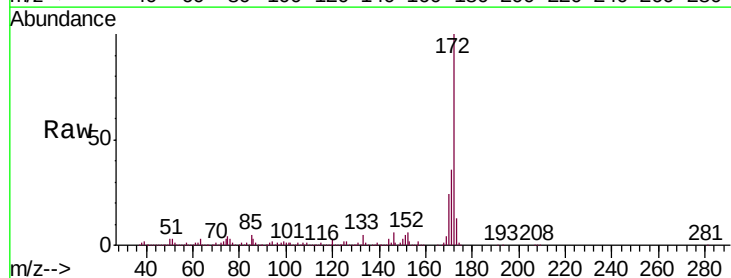

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

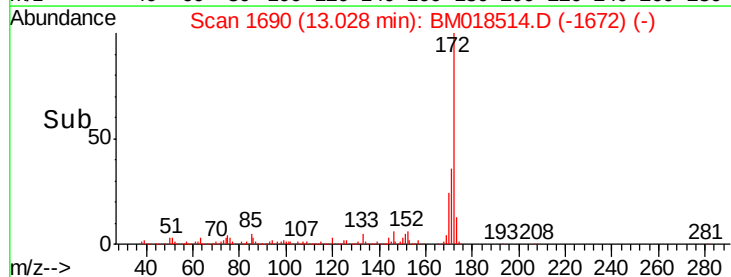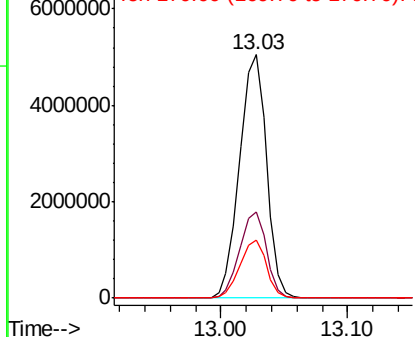

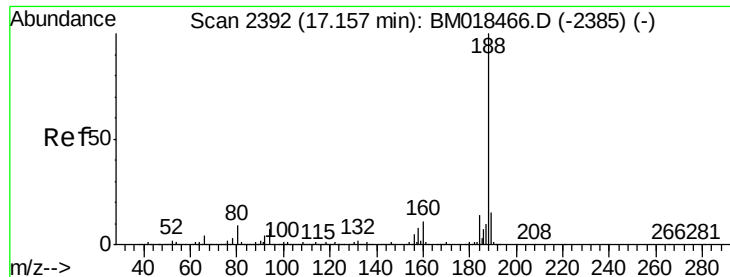

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.16 min Scan# 2392

Delta R.T. 0.00 min

Lab File: BM018514.D

Acq: 10 Jan 2019 18:28

Instrument :

BNA_M

ClientSampled :

SP-1-1


Tgt Ion:188 Resp: 2606188

Ion Ratio Lower Upper

188 100

94 7.2 7.1 10.7




80 8.1 7.6 11.4

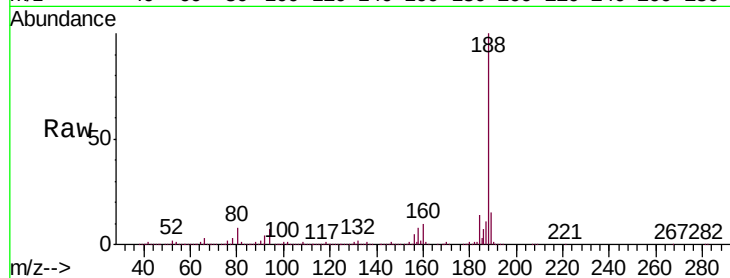

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM

Ion 80.00 (79.70 to 80.70): BM

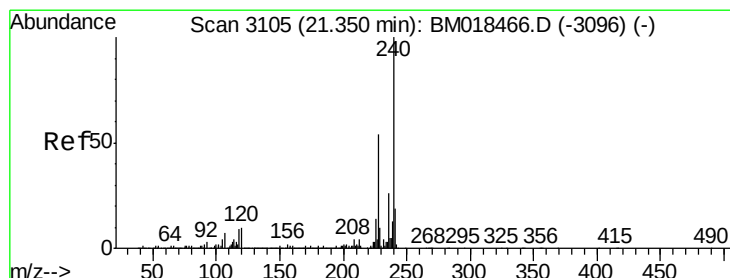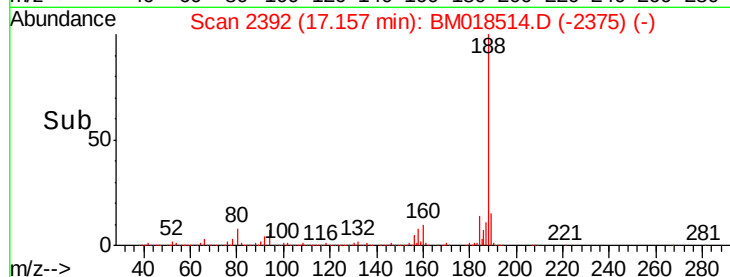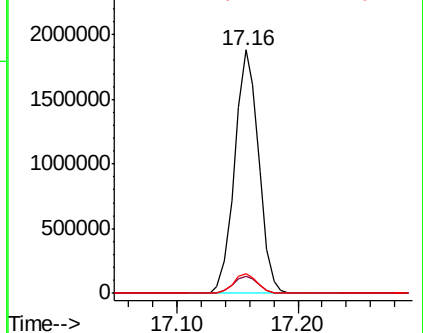

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.36 min Scan# 3106

Delta R.T. 0.01 min

Lab File: BM018514.D

Acq: 10 Jan 2019 18:28


Tgt Ion:240 Resp: 2975293

Ion Ratio Lower Upper

240 100

120 9.1 8.4 12.6



236 25.8 20.7 31.1

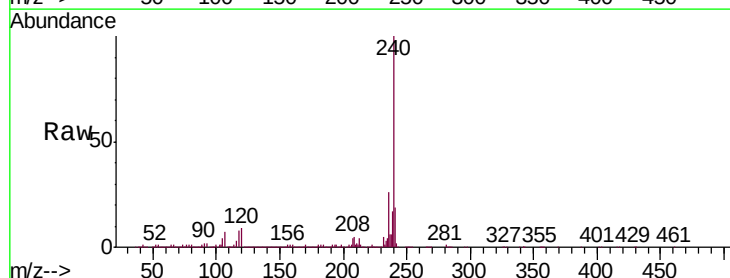


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

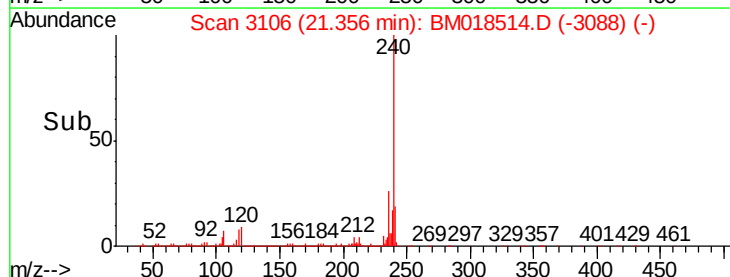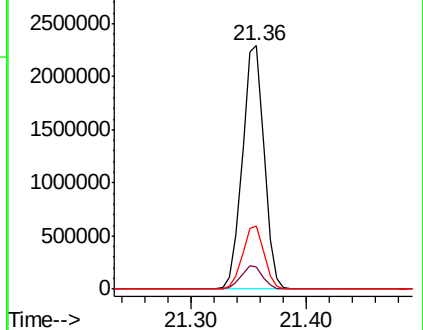

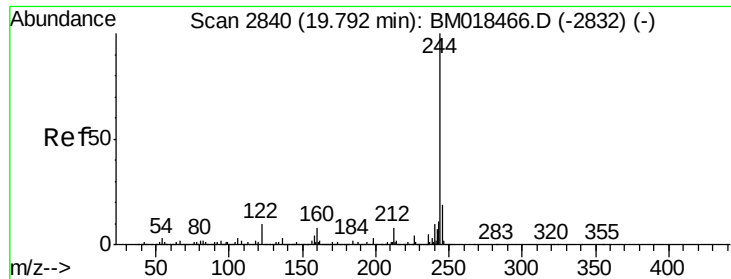

#79

Terphenyl-d14

Concen: 87.329 ng

RT: 19.79 min Scan# 2840

Delta R.T. 0.01 min

Lab File: BM018514.D

Acq: 10 Jan 2019 18:28

Instrument :

BNA_M

ClientSampled :

SP-1-1


Tgt Ion:244 Resp:12325619

Ion Ratio Lower Upper

244 100

212 10.4 5.9 8.9#




122 13.3 9.0 13.4

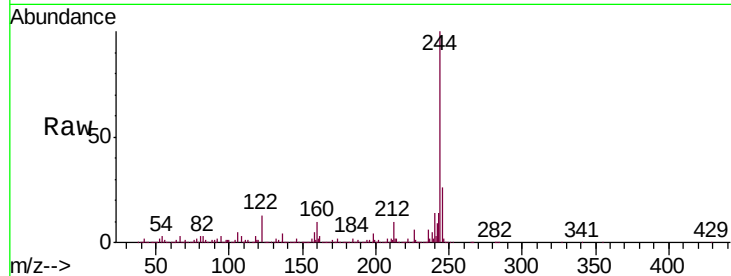

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

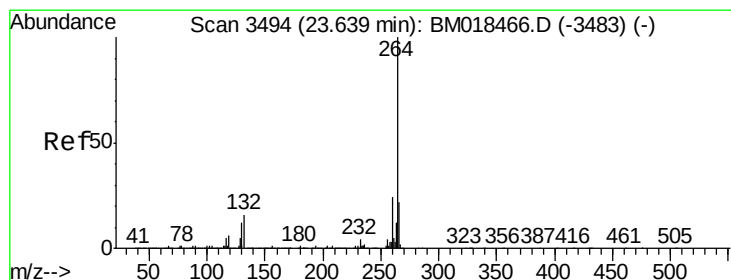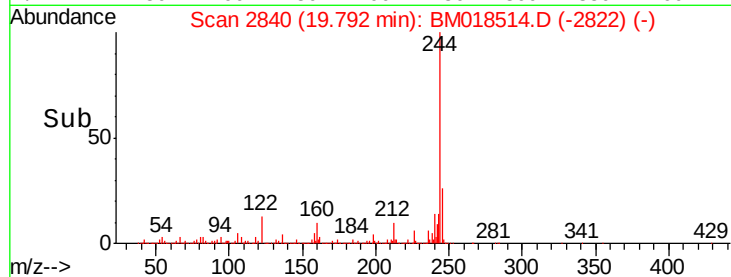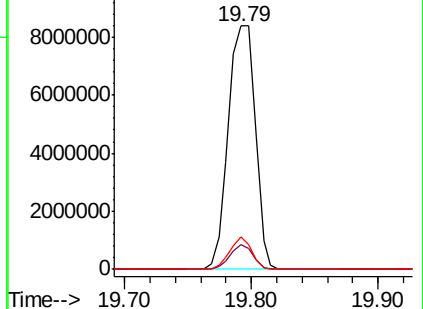

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.64 min Scan# 3495

Delta R.T. 0.01 min

Lab File: BM018514.D

Acq: 10 Jan 2019 18:28


Tgt Ion:264 Resp: 3080104

Ion Ratio Lower Upper

264 100

260 23.6 18.9 28.3

265 21.8 16.8 25.2

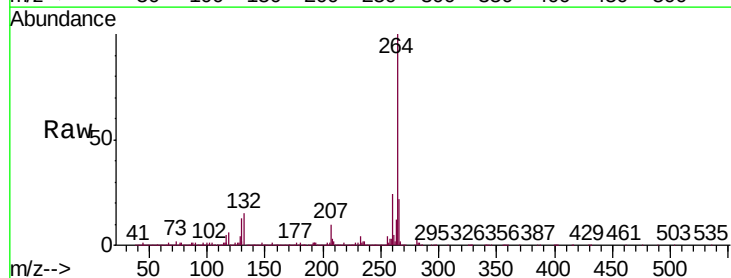

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

