

Data File : BM018517.D
Acq On : 10 Jan 2019 20:17
Operator : JU/SJ
Sample : K1082-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP-1-4

Quant Time: Jan 11 03:27:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 10 05:57:41 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	375579	20.00	ng	0.00
21) Naphthalene-d8	10.55	136	1484186	20.00	ng	0.00
39) Acenaphthene-d10	14.41	164	921765	20.00	ng	0.00
64) Phenanthrene-d10	17.16	188	2356009	20.00	ng	0.00
76) Chrysene-d12	21.35	240	2694621	20.00	ng	0.00
87) Perylene-d12	23.64	264	2796289	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.35	112	2834421	139.35	ng	0.00
7) Phenol-d6	6.94	99	3340462	129.30	ng	0.00
23) Nitrobenzene-d5	8.93	82	2536568	99.08	ng	0.00
42) 2,4,6-Tribromophenol	15.90	330	2111396	179.90	ng	0.00
45) 2-Fluorobiphenyl	13.03	172	6790280	96.12	ng	0.00
79) Terphenyl-d14	19.79	244	12196646	95.42	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM018517.D
Acq On : 10 Jan 2019 20:17
Operator : JU/SJ
Sample : K1082-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP-1-4

Quant Time: Jan 11 03:27:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 10 05:57:41 2019
Response via : Initial Calibration

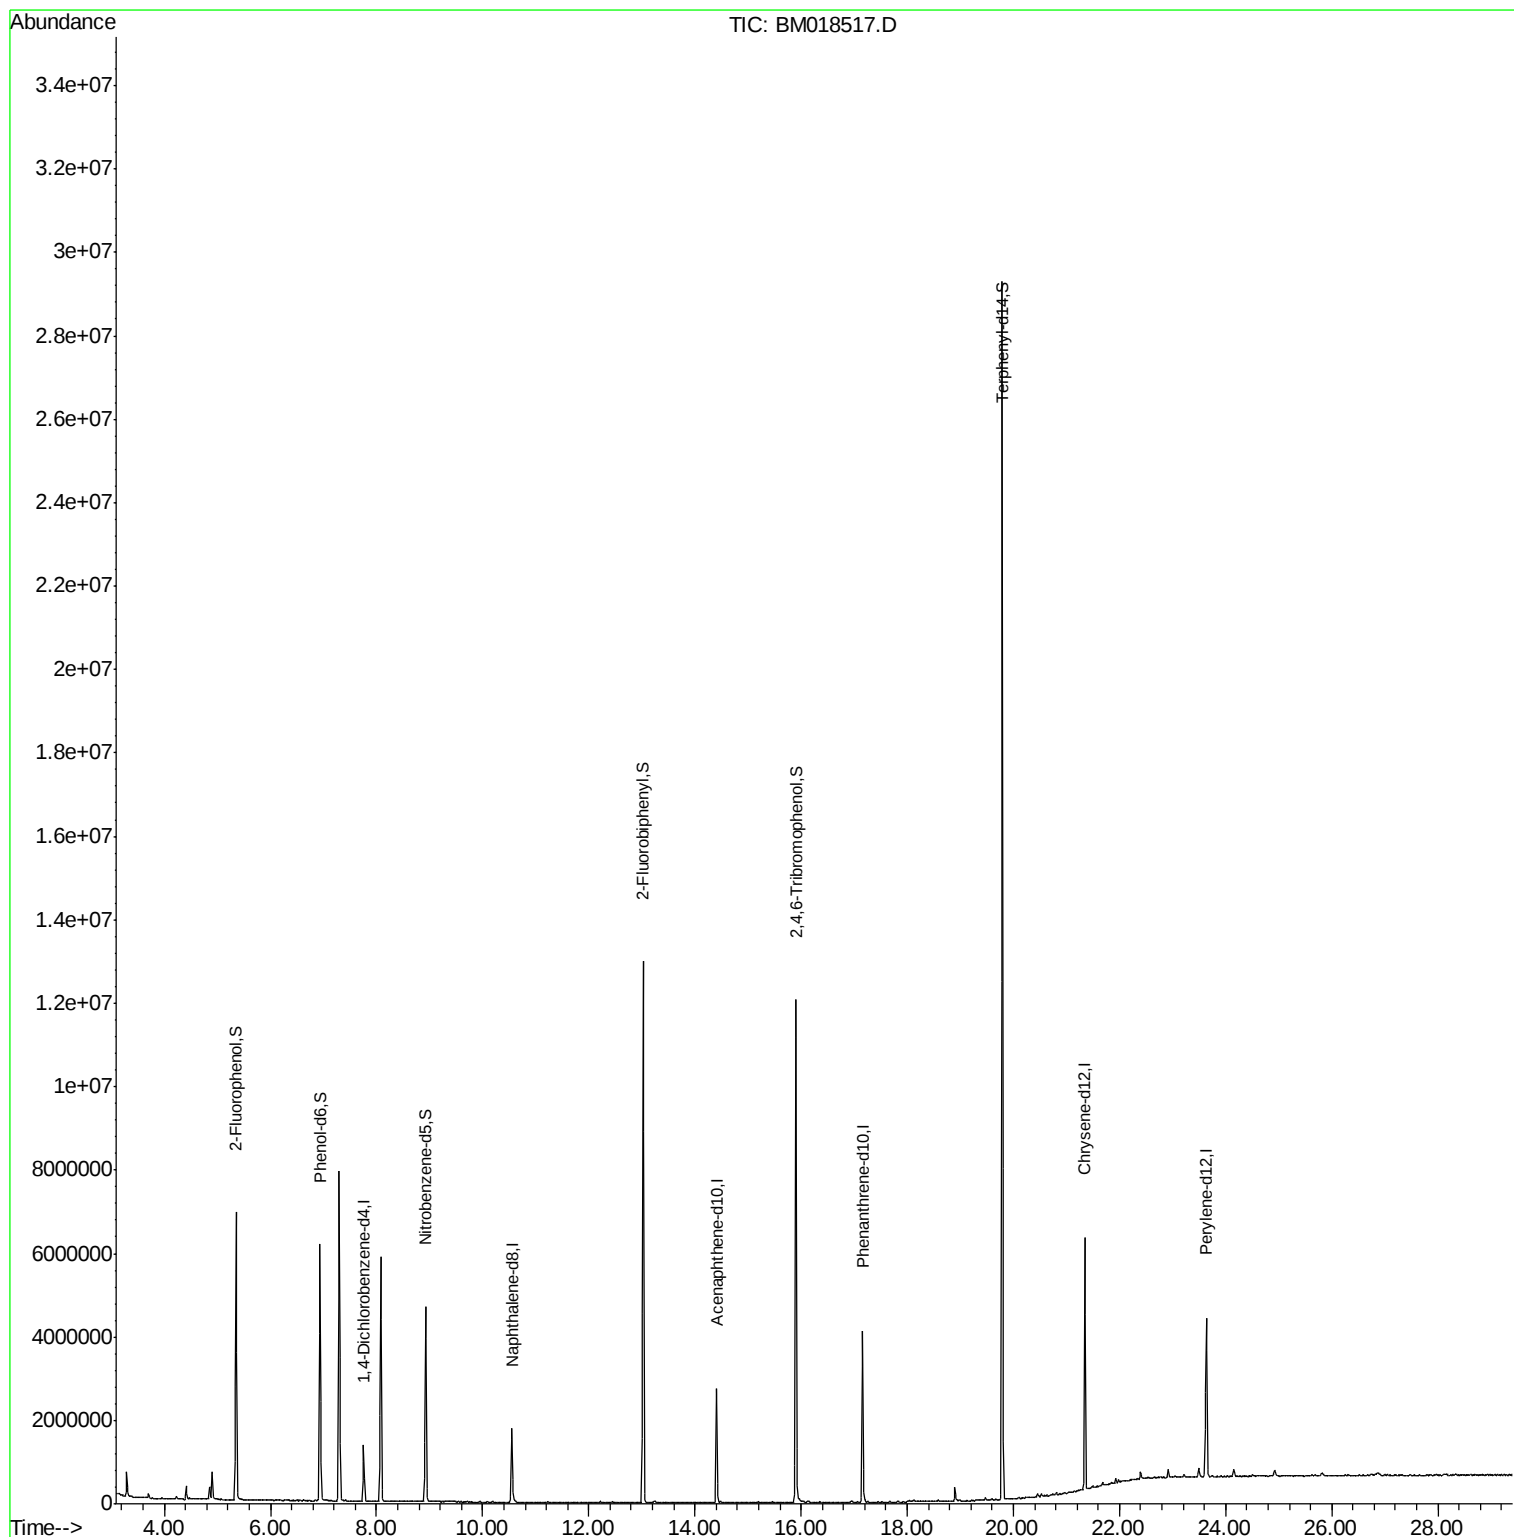

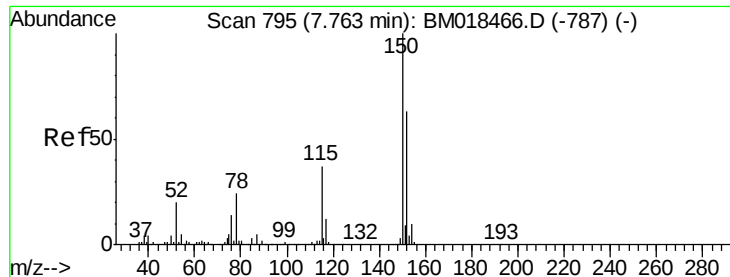


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.76 min Scan# 794
Delta R.T. -0.01 min
Lab File: BM018517.D
Acq: 10 Jan 2019 20:17

Instrument :
BNA_M
ClientSampleId :
SP-1-4

Tgt Ion	Ratio	Lower	Upper
152	100		
150	156.8	126.9	190.3
115	59.0	45.5	68.3

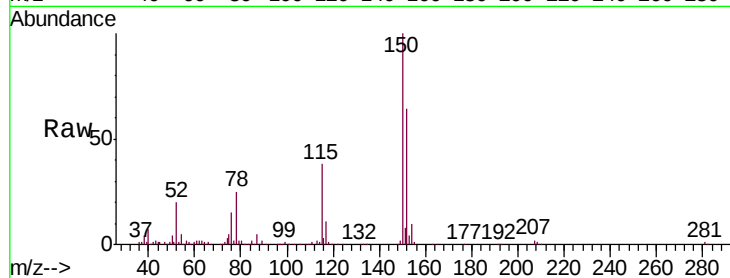


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

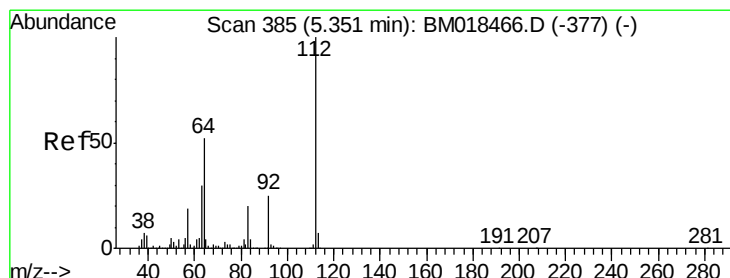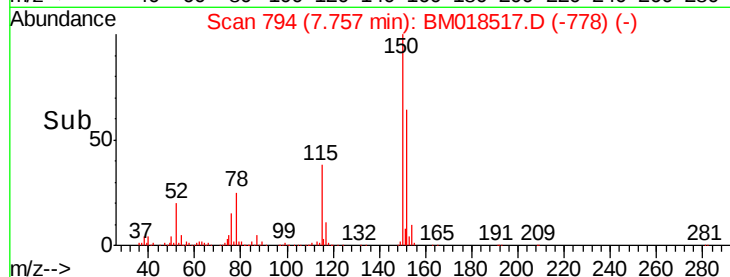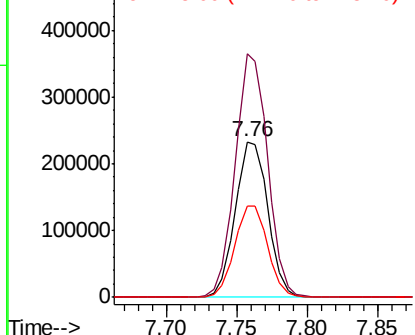



#5


2-Fluorophenol
Concen: 139.351 ng
RT: 5.35 min Scan# 385
Delta R.T. -0.00 min
Lab File: BM018517.D
Acq: 10 Jan 2019 20:17

Tgt Ion	Ratio	Lower	Upper
112	100		
64	53.8	46.5	69.7
63	30.4	25.2	37.8

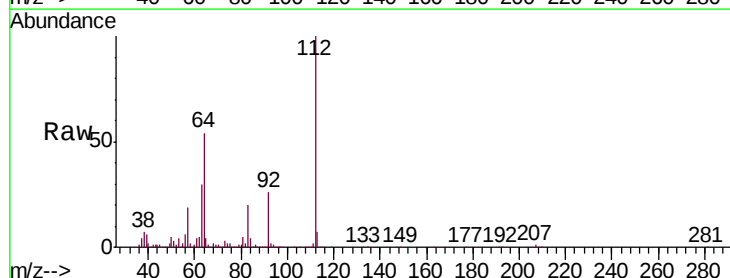

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

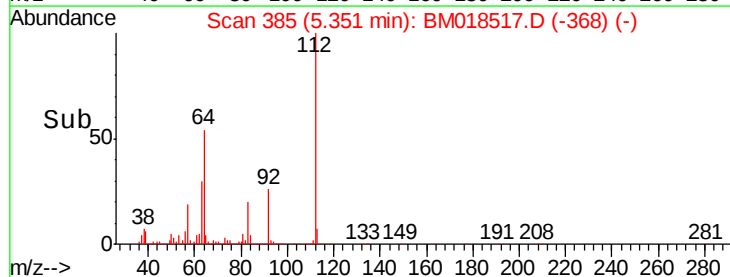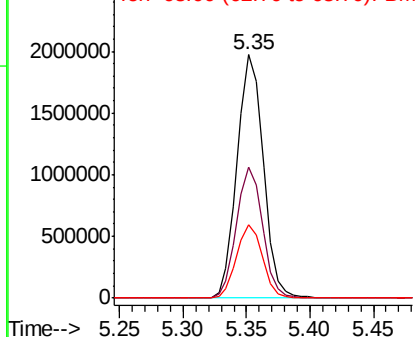

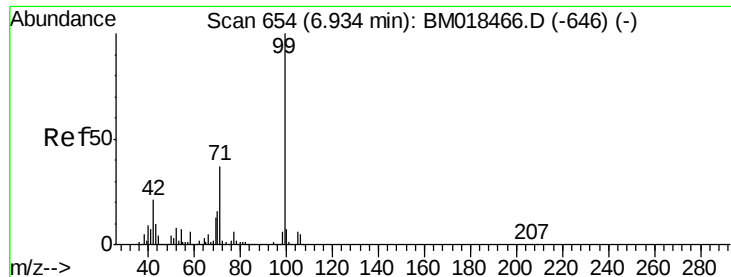

#7

Phenol-d6

Concen: 129.303 ng

RT: 6.94 min Scan# 655

Delta R.T. 0.01 min

Lab File: BM018517.D

Acq: 10 Jan 2019 20:17

Instrument :

BNA_M

ClientSampled :

SP-1-4


Tgt Ion: 99 Resp: 3340462

Ion Ratio Lower Upper

99 100

42 19.8 17.3 25.9




71 36.3 28.0 42.0

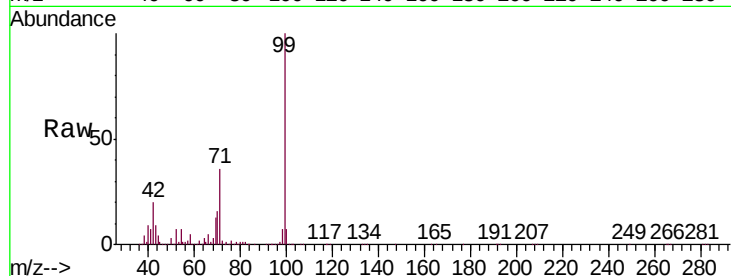

Abundance Ion 99.00 (98.70 to 99.70): BM018517.D (-637) (-)

Ion 42.00 (41.70 to 42.70): BM018517.D (-637) (-)

Ion 71.00 (70.70 to 71.70): BM018517.D (-637) (-)

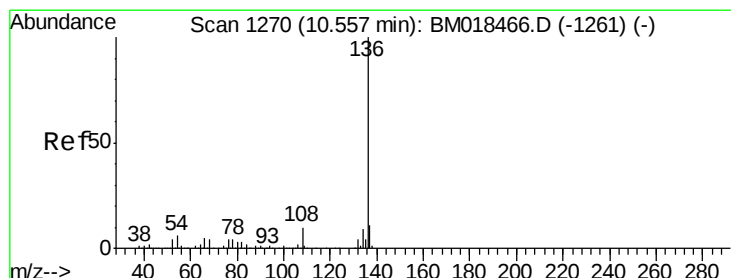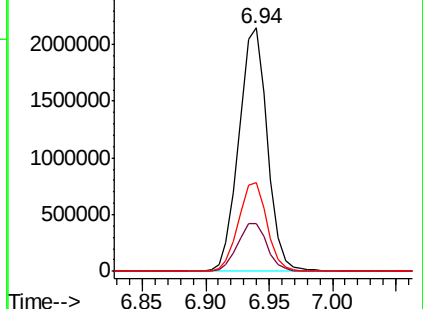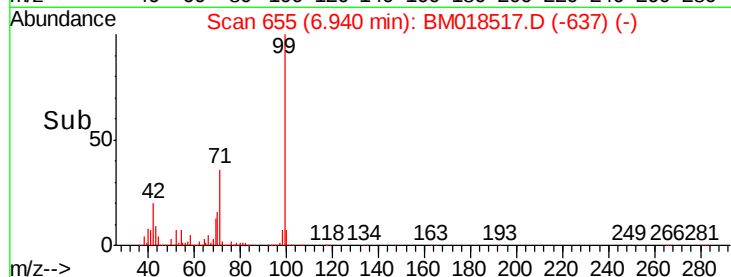

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.55 min Scan# 1269

Delta R.T. -0.00 min

Lab File: BM018517.D

Acq: 10 Jan 2019 20:17

Tgt Ion: 136 Resp: 1484186


Ion Ratio Lower Upper

136 100

137 10.5 8.5 12.7

54 6.5 6.0 9.0

68 4.5 4.5 6.7


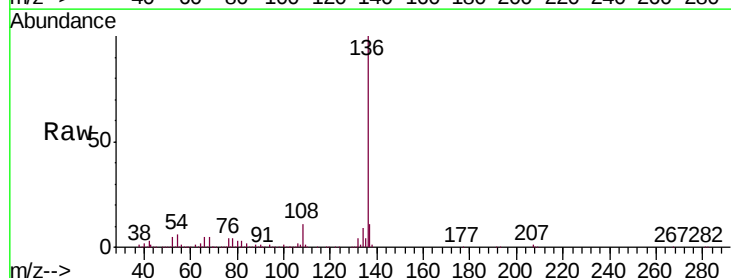



Abundance Ion 136.00 (135.70 to 136.70): BM018517.D (-1252) (-)

Ion 137.00 (136.70 to 137.70): BM018517.D (-1252) (-)

Ion 54.00 (53.70 to 54.70): BM018517.D (-1252) (-)

Ion 68.00 (67.70 to 68.70): BM018517.D (-1252) (-)



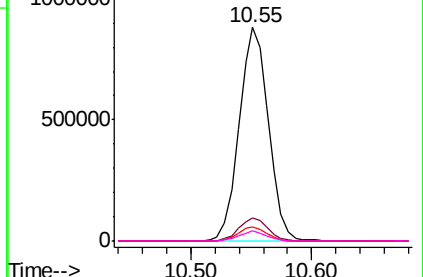
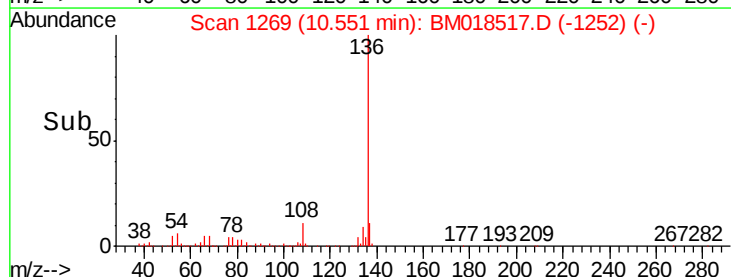


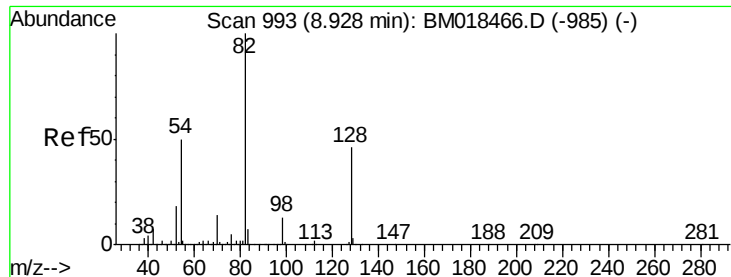

#23
Nitrobenzene-d5
Concen: 99.076 ng
RT: 8.93 min Scan# 993
Delta R.T. 0.01 min
Lab File: BM018517.D
Acq: 10 Jan 2019 20:17




Instrument :
BNA_M
ClientSampled :
SP-1-4


Tgt Ion: 82 Resp: 2536568
Ion Ratio Lower Upper
82 100
128 46.4 36.3 54.5
54 49.5 41.7 62.5

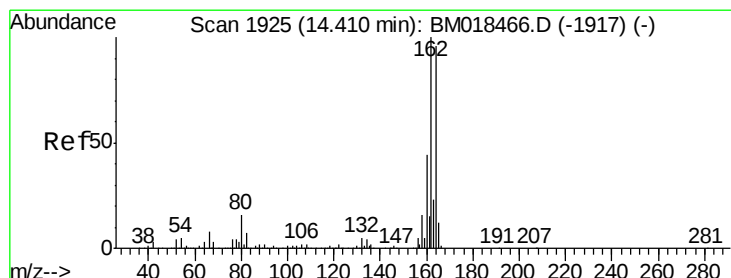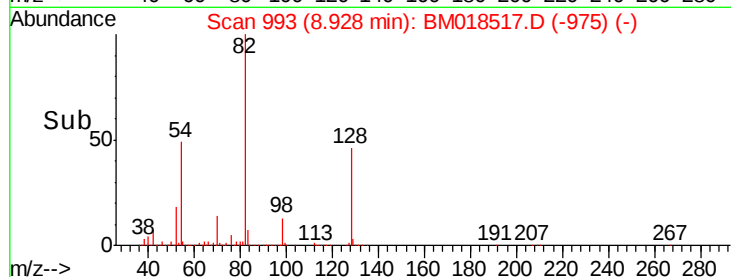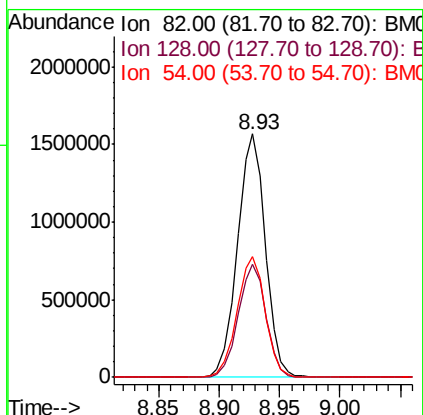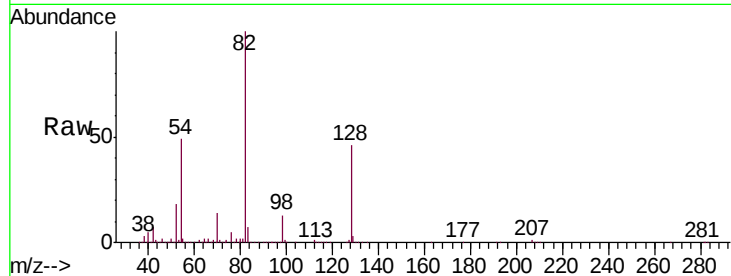

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.41 min Scan# 1925
Delta R.T. -0.00 min
Lab File: BM018517.D
Acq: 10 Jan 2019 20:17

Tgt Ion: 164 Resp: 921765
Ion Ratio Lower Upper
164 100
162 105.2 83.0 124.4
160 45.9 37.1 55.7

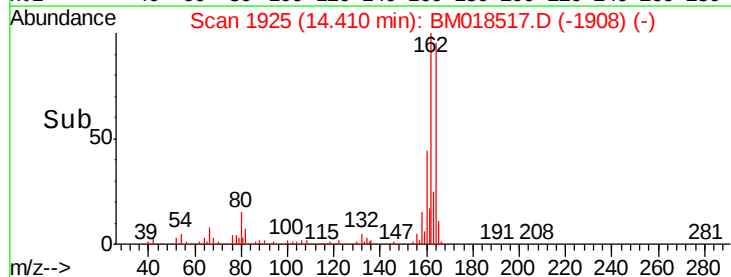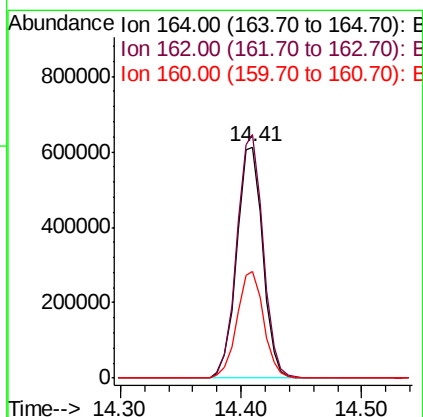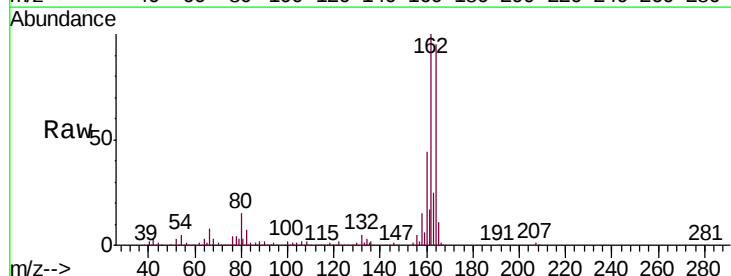

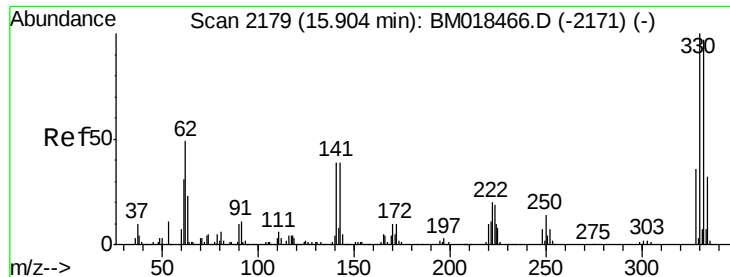

#42

2,4,6-Tribromophenol

Concen: 179.898 ng

RT: 15.90 min Scan# 2179

Delta R.T. -0.00 min

Lab File: BM018517.D

Acq: 10 Jan 2019 20:17

Instrument :

BNA_M

ClientSampleId :

SP-1-4


Tgt Ion:330 Resp: 2111396

Ion Ratio Lower Upper

330 100

332 97.3 77.6 116.4

141 39.2 31.7 47.5



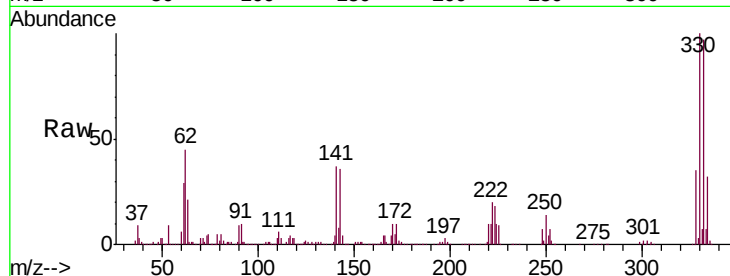


Abundance

Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

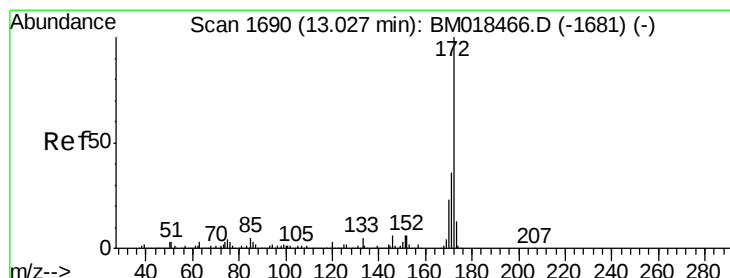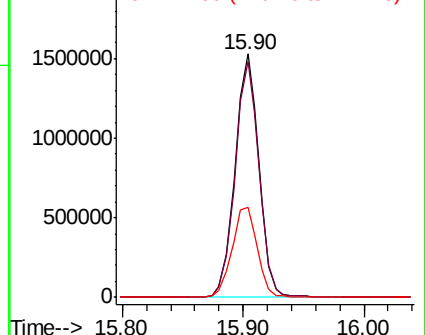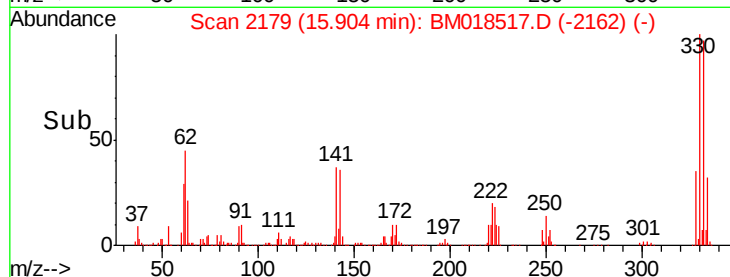

#45

2-Fluorobiphenyl

Concen: 96.124 ng

RT: 13.03 min Scan# 1690

Delta R.T. 0.01 min

Lab File: BM018517.D

Acq: 10 Jan 2019 20:17


Tgt Ion:172 Resp: 6790280

Ion Ratio Lower Upper

172 100

171 35.7 28.2 42.4

170 23.3 18.9 28.3


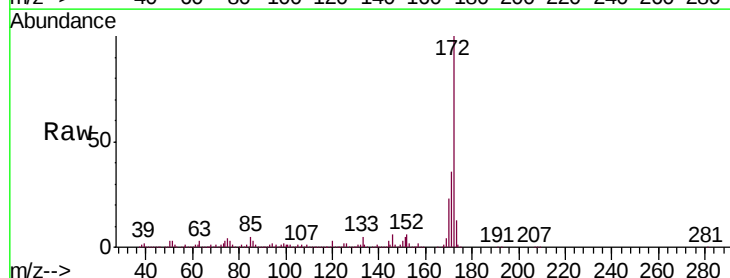



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

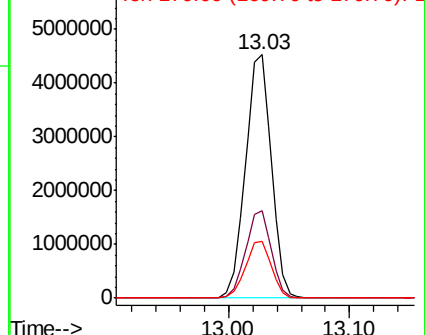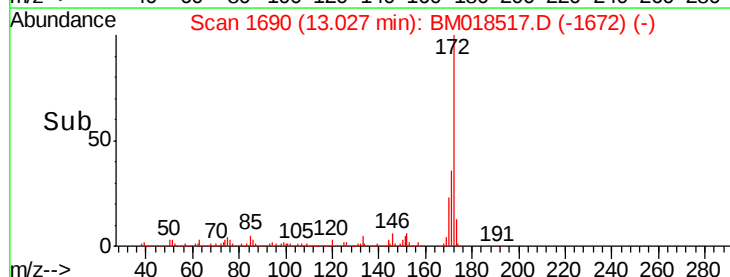

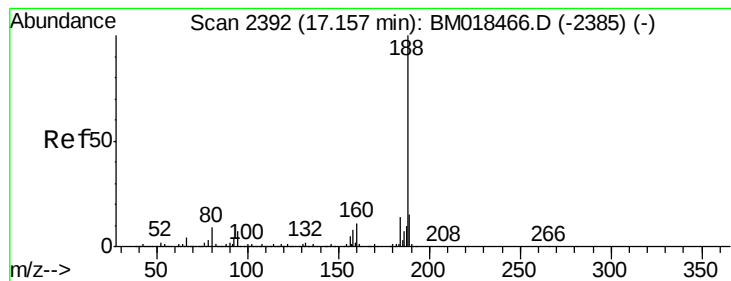

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.16 min Scan# 2392

Delta R.T. -0.00 min

Lab File: BM018517.D

Acq: 10 Jan 2019 20:17

Instrument :

BNA_M

ClientSampleId :

SP-1-4


Tgt Ion:188 Resp: 2356009

Ion Ratio Lower Upper

188 100

94 7.2 7.1 10.7




80 8.0 7.6 11.4

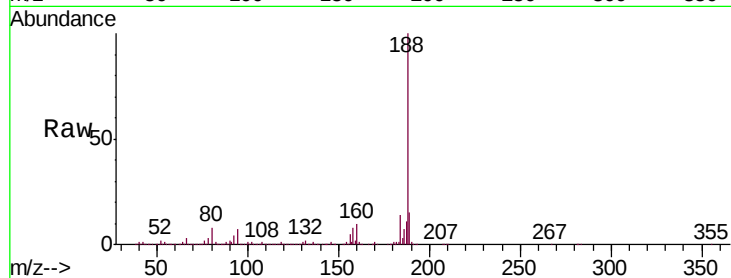

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM

Ion 80.00 (79.70 to 80.70): BM

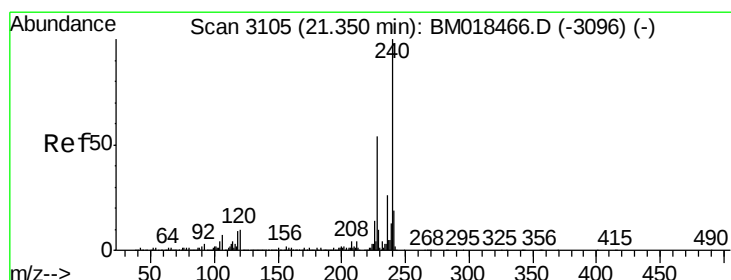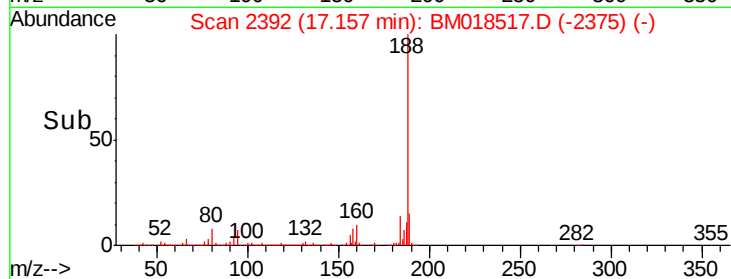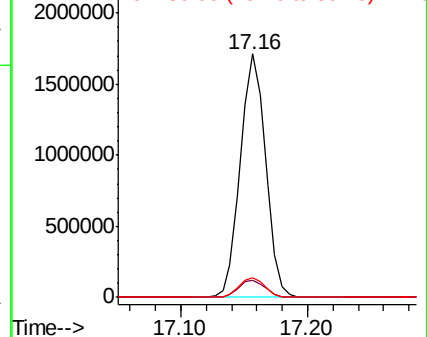

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.35 min Scan# 3105

Delta R.T. -0.00 min

Lab File: BM018517.D

Acq: 10 Jan 2019 20:17


Tgt Ion:240 Resp: 2694621

Ion Ratio Lower Upper

240 100

120 9.5 8.4 12.6



236 25.8 20.7 31.1

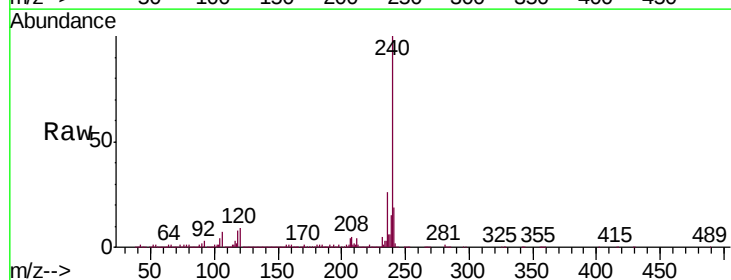


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

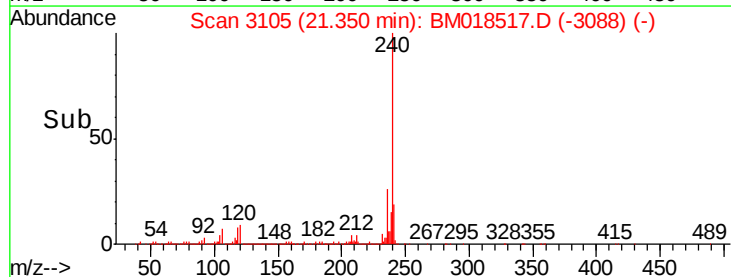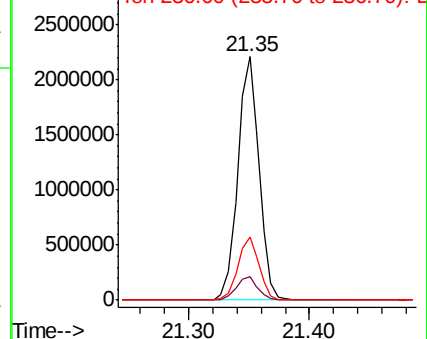

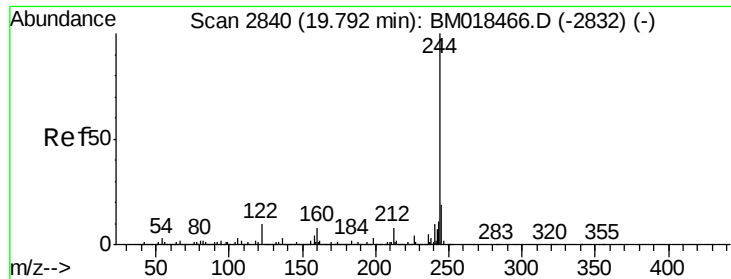

#79

Terphenyl-d14

Concen: 95.416 ng

RT: 19.79 min Scan# 2840

Delta R.T. 0.01 min

Lab File: BM018517.D

Acq: 10 Jan 2019 20:17

Instrument :

BNA_M

ClientSampled :

SP-1-4


Tgt Ion:244 Resp:12196646

Ion Ratio Lower Upper

244 100

212 10.0 5.9 8.9#




122 12.6 9.0 13.4

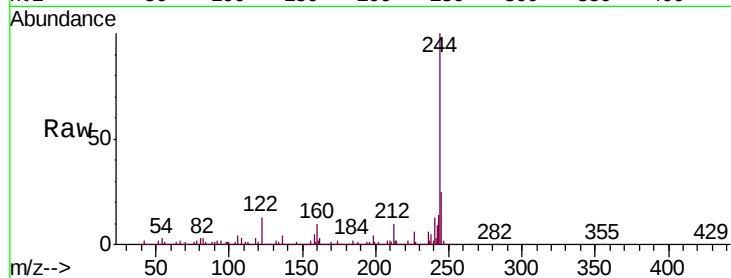

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

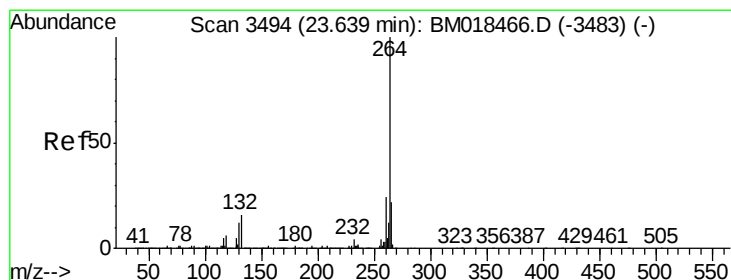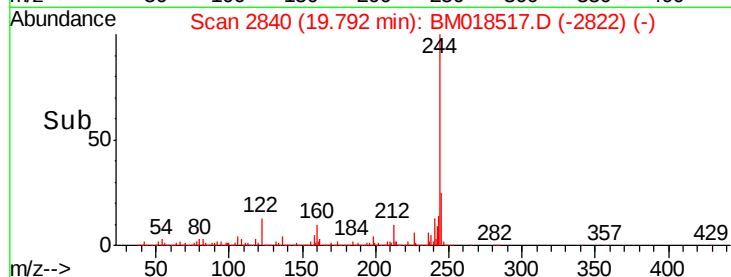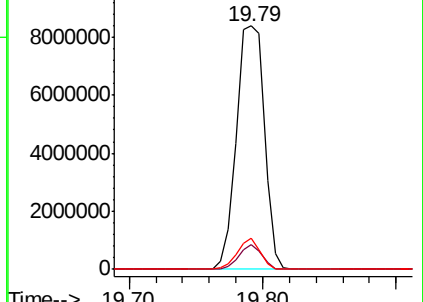

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.64 min Scan# 3494

Delta R.T. 0.01 min

Lab File: BM018517.D

Acq: 10 Jan 2019 20:17


Tgt Ion:264 Resp: 2796289

Ion Ratio Lower Upper

264 100

260 23.6 18.9 28.3

265 21.5 16.8 25.2

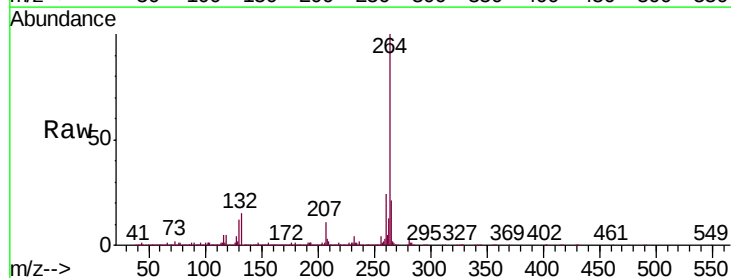

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

